

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040980.D
 Acq On : 11 Apr 2024 17:02
 Operator : JC/MD
 Sample : P2048-06 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R54

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M

Title : VOC Analysis

Signal : TIC: VX040980.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	24	28	32	rBV2	4356	5913	0.16%	0.040%
2	1.368	43	46	59	rBV	76699	117116	3.22%	0.801%
3	1.648	88	92	109	rVB	47518	93588	2.57%	0.640%
4	2.294	192	198	210	rVB	195673	302943	8.32%	2.073%
5	2.550	238	240	241	rBV2	339	296	0.01%	0.002%
6	2.782	274	278	284	rBV3	1137	1935	0.05%	0.013%
7	2.947	296	305	315	rBV	6517	16603	0.46%	0.114%
8	3.050	320	322	324	rBV2	134	125	0.00%	0.001%
9	3.111	330	332	333	rBV2	151	124	0.00%	0.001%
10	3.209	345	348	352	rBB2	138	207	0.01%	0.001%
11	3.483	390	393	396	rBV2	138	187	0.01%	0.001%
12	3.611	409	414	415	rBV2	132	193	0.01%	0.001%
13	3.709	427	430	432	rVB2	117	114	0.00%	0.001%
14	3.824	446	449	453	rBV2	129	219	0.01%	0.001%
15	3.879	456	458	461	rVB2	161	173	0.00%	0.001%
16	3.910	461	463	465	rBV	182	183	0.01%	0.001%
17	4.288	524	525	528	rVB	238	147	0.00%	0.001%
18	4.385	540	541	543	rVB2	212	117	0.00%	0.001%
19	4.471	546	555	578	rBV2	58775	220593	6.06%	1.510%
20	4.843	614	616	617	rBV	185	116	0.00%	0.001%
21	5.056	638	651	668	rBV	123682	383398	10.53%	2.624%
22	5.227	678	679	682	rVB	327	224	0.01%	0.002%
23	5.385	699	705	713	rVB4	547	1450	0.04%	0.010%
24	5.470	716	719	721	rVB	318	307	0.01%	0.002%
25	5.556	727	733	739	rBV3	631	1435	0.04%	0.010%
26	5.635	745	746	750	rBV2	163	207	0.01%	0.001%
27	5.861	780	783	786	rVB2	164	165	0.00%	0.001%
28	5.964	788	800	805	rBV2	335343	972691	26.70%	6.657%
29	6.031	806	811	831	rVB	1061854	2728207	74.90%	18.671%
30	6.263	848	849	853	rVB3	689	579	0.02%	0.004%
31	6.489	884	886	887	rBV	204	110	0.00%	0.001%
32	6.537	893	894	895	rBV	294	156	0.00%	0.001%
33	6.641	907	911	915	rVB2	152	229	0.01%	0.002%
34	6.757	921	930	945	rBV	257239	618691	16.99%	4.234%
35	7.123	984	990	997	rVB8	1331	3450	0.09%	0.024%
36	7.202	1001	1003	1005	rBV3	525	502	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040980.D
 Acq On : 11 Apr 2024 17:02
 Operator : JC/MD
 Sample : P2048-06 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R54

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	7.306	1011	1020	1035	rBV	195263	429145	11.78%	2.937%
38	7.488	1048	1050	1053	rVB3	483	414	0.01%	0.003%
39	7.629	1071	1073	1077	rBV2	144	209	0.01%	0.001%
40	7.696	1082	1084	1086	rBV2	164	162	0.00%	0.001%
41	7.726	1086	1089	1092	rVB2	157	217	0.01%	0.001%
42	7.958	1121	1127	1131	rBV5	665	1343	0.04%	0.009%
43	8.135	1154	1156	1161	rVB2	101	140	0.00%	0.001%
44	8.324	1180	1187	1208	rBV	121543	205485	5.64%	1.406%
45	8.598	1228	1232	1233	rBV2	210	245	0.01%	0.002%
46	8.647	1233	1240	1256	rBV	485992	788034	21.63%	5.393%
47	8.952	1284	1290	1304	rBV	85187	130767	3.59%	0.895%
48	9.092	1311	1313	1315	rVB2	238	200	0.01%	0.001%
49	9.183	1327	1328	1331	rBV2	177	197	0.01%	0.001%
50	9.275	1339	1343	1348	rVB5	1372	2021	0.06%	0.014%
51	9.391	1356	1362	1379	rBV	284125	478775	13.14%	3.277%
52	9.640	1401	1403	1409	rVB2	320	461	0.01%	0.003%
53	9.805	1428	1430	1433	rBV2	145	192	0.01%	0.001%
54	9.915	1446	1448	1450	rBV	137	109	0.00%	0.001%
55	9.964	1453	1456	1458	rBV	134	170	0.00%	0.001%
56	10.079	1465	1475	1493	rBV2	2139172	3642543	100.00%	24.928%
57	10.299	1509	1511	1516	rVB4	882	1254	0.03%	0.009%
58	10.342	1516	1518	1520	rBV2	244	253	0.01%	0.002%
59	10.598	1559	1560	1563	rVB2	147	109	0.00%	0.001%
60	10.646	1565	1568	1574	rVV4	682	954	0.03%	0.007%
61	10.695	1574	1576	1579	rVB	198	180	0.00%	0.001%
62	10.890	1606	1608	1611	rVV	129	116	0.00%	0.001%
63	10.970	1618	1621	1625	rBV3	523	729	0.02%	0.005%
64	11.091	1637	1641	1649	rVB4	1128	2305	0.06%	0.016%
65	11.195	1652	1658	1670	rVV	388483	521585	14.32%	3.569%
66	11.311	1674	1677	1681	rVB	2838	3445	0.09%	0.024%
67	11.451	1697	1700	1706	rVB2	482	820	0.02%	0.006%
68	11.549	1713	1716	1719	rBV2	104	153	0.00%	0.001%
69	11.707	1740	1742	1744	rBV2	510	450	0.01%	0.003%
70	11.756	1748	1750	1754	rVB2	562	541	0.01%	0.004%
71	11.786	1754	1755	1759	rVB2	138	118	0.00%	0.001%
72	11.969	1781	1785	1789	rBV	28803	36744	1.01%	0.251%
73	12.036	1789	1796	1808	rVB2	713862	1554392	42.67%	10.638%
74	12.225	1825	1827	1829	rVB3	264	174	0.00%	0.001%
75	12.323	1837	1843	1858	rBV2	718775	1286575	35.32%	8.805%
76	12.548	1878	1880	1881	rBV2	140	127	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040980.D
Acq On : 11 Apr 2024 17:02
Operator : JC/MD
Sample : P2048-06 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R54

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Title : VOC Analysis

77	12.762	1911	1915	1920	rVV	3538	4573	0.13%	0.031%
78	12.817	1923	1924	1926	rBV	307	170	0.00%	0.001%
79	12.994	1951	1953	1957	rBV2	170	156	0.00%	0.001%
80	13.122	1969	1974	1980	rBV3	382	636	0.02%	0.004%
81	13.201	1984	1987	1989	rBV2	183	182	0.00%	0.001%
82	13.268	1995	1998	1999	rBV	107	121	0.00%	0.001%
83	13.311	2003	2005	2006	rBV	273	157	0.00%	0.001%
84	13.335	2006	2009	2012	rBV	99	113	0.00%	0.001%
85	13.445	2026	2027	2031	rBV2	161	204	0.01%	0.001%
86	13.493	2033	2035	2036	rBV2	253	189	0.01%	0.001%
87	13.591	2046	2051	2063	rVB	16618	22398	0.61%	0.153%
88	13.719	2068	2072	2074	rBV3	132	164	0.00%	0.001%
89	13.780	2079	2082	2087	rBV2	583	967	0.03%	0.007%
90	13.884	2096	2099	2101	rBV2	110	127	0.00%	0.001%
91	13.963	2109	2112	2119	rVB3	1594	2387	0.07%	0.016%
92	14.018	2119	2121	2122	rBV	246	132	0.00%	0.001%
93	14.127	2135	2139	2144	rVB	4682	6129	0.17%	0.042%
94	14.323	2169	2171	2174	rVB2	250	218	0.01%	0.001%
95	14.384	2179	2181	2184	rVB2	296	292	0.01%	0.002%
96	14.621	2219	2220	2223	rBV2	291	249	0.01%	0.002%
97	14.938	2271	2272	2273	rBV	426	229	0.01%	0.002%
98	15.139	2304	2305	2309	rBV2	407	383	0.01%	0.003%
99	15.176	2309	2311	2312	rVB2	380	157	0.00%	0.001%
100	15.396	2342	2347	2353	rVB2	4350	7471	0.21%	0.051%




Sum of corrected areas: 14612350

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040980.D
Acq On : 11 Apr 2024 17:02
Operator : JC/MD
Sample : P2048-06 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R54

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

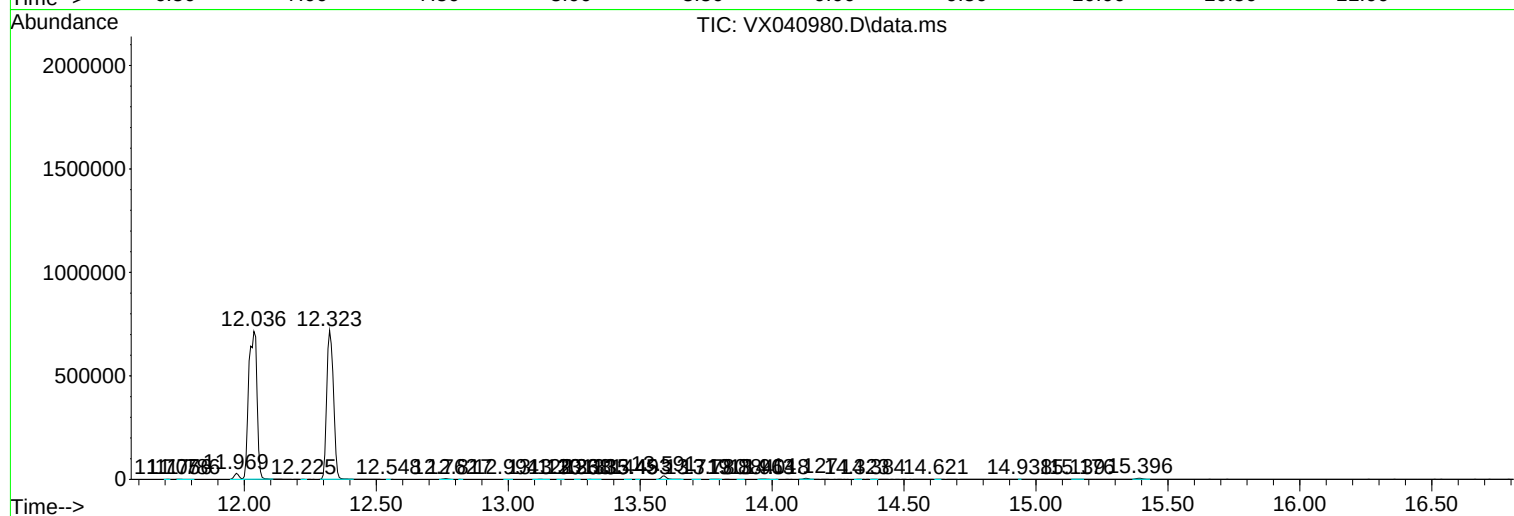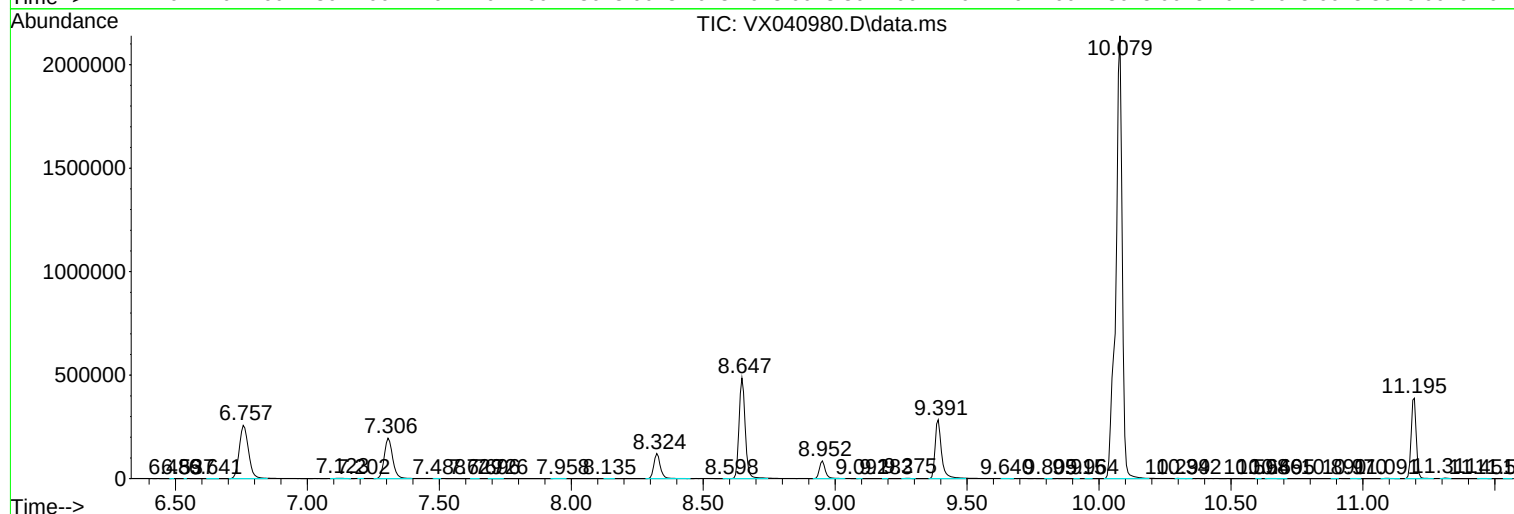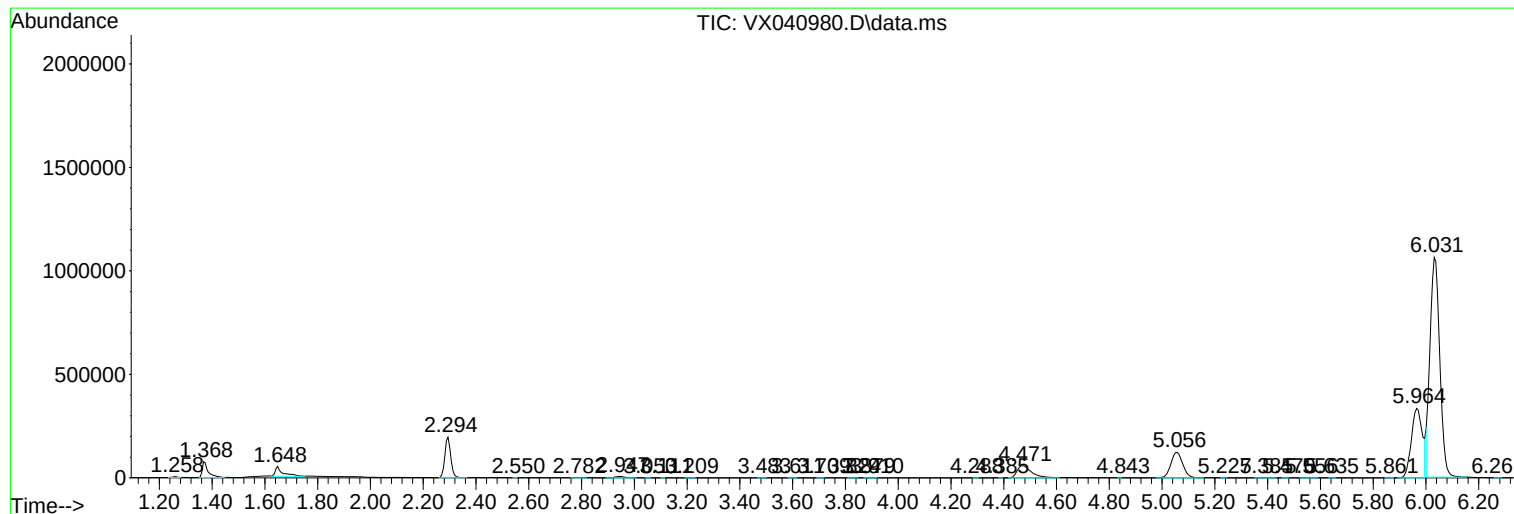

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040980.D
Acq On : 11 Apr 2024 17:02
Operator : JC/MD
Sample : P2048-06 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R54

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040980.D
Acq On : 11 Apr 2024 17:02
Operator : JC/MD
Sample : P2048-06 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R54

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------