

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040982.D
 Acq On : 11 Apr 2024 17:48
 Operator : JC/MD
 Sample : P2048-08 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M

Title : VOC Analysis

Signal : TIC: VX040982.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	24	28	36	rBV4	4571	8147	0.82%	0.111%
2	1.368	43	46	59	rVB	81033	114534	11.57%	1.557%
3	1.648	88	92	104	rBV	44701	80615	8.14%	1.096%
4	2.294	191	198	210	rVB	184240	293007	29.59%	3.982%
5	2.611	238	250	252	rBV3	1351	3866	0.39%	0.053%
6	2.788	273	279	285	rVB4	1418	2649	0.27%	0.036%
7	2.947	297	305	314	rBV2	6151	15128	1.53%	0.206%
8	3.105	328	331	333	rBV2	179	228	0.02%	0.003%
9	3.123	333	334	336	rVB	215	120	0.01%	0.002%
10	3.190	342	345	346	rBV2	91	105	0.01%	0.001%
11	3.367	371	374	377	rVB2	102	124	0.01%	0.002%
12	3.471	389	391	394	rBV2	141	151	0.02%	0.002%
13	3.605	411	413	415	rBV	172	124	0.01%	0.002%
14	3.812	443	447	448	rBV2	153	182	0.02%	0.002%
15	3.904	460	462	463	rBV2	117	104	0.01%	0.001%
16	3.971	472	473	476	rBV	130	97	0.01%	0.001%
17	4.288	523	525	526	rBV	168	100	0.01%	0.001%
18	4.330	529	532	534	rBV	128	140	0.01%	0.002%
19	4.349	534	535	538	rVB	172	149	0.02%	0.002%
20	4.471	545	555	578	rBV2	58489	216842	21.90%	2.947%
21	4.910	625	627	630	rBV2	320	326	0.03%	0.004%
22	5.056	639	651	666	rBV3	123843	381462	38.53%	5.184%
23	5.257	682	684	689	rVB2	216	322	0.03%	0.004%
24	5.391	702	706	712	rVB3	482	1006	0.10%	0.014%
25	5.434	712	713	715	rVB	189	104	0.01%	0.001%
26	5.556	727	733	734	rBV3	523	783	0.08%	0.011%
27	5.708	756	758	763	rBV2	96	162	0.02%	0.002%
28	5.763	766	767	770	rVB	138	106	0.01%	0.001%
29	5.794	770	772	774	rBV	166	99	0.01%	0.001%
30	5.830	774	778	781	rVB2	102	128	0.01%	0.002%
31	5.964	788	800	826	rBV2	333375	990092	100.00%	13.455%
32	6.361	861	865	868	rBV3	442	919	0.09%	0.012%
33	6.757	921	930	951	rBV	241254	591462	59.74%	8.038%
34	7.056	977	979	981	rBV	167	120	0.01%	0.002%
35	7.123	984	990	997	rVB7	1846	4350	0.44%	0.059%
36	7.208	997	1004	1007	rBV4	975	1885	0.19%	0.026%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040982.D
 Acq On : 11 Apr 2024 17:48
 Operator : JC/MD
 Sample : P2048-08 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	7.306	1012	1020	1041	rBV	195024	426713	43.10%	5.799%
38	7.446	1041	1043	1044	rVB	415	233	0.02%	0.003%
39	7.476	1044	1048	1049	rBV3	357	507	0.05%	0.007%
40	7.568	1061	1063	1064	rVB	331	160	0.02%	0.002%
41	7.592	1064	1067	1068	rBV	265	234	0.02%	0.003%
42	7.757	1091	1094	1095	rBV	199	180	0.02%	0.002%
43	7.927	1119	1122	1123	rBV	152	168	0.02%	0.002%
44	7.958	1123	1127	1129	rBV3	639	851	0.09%	0.012%
45	8.086	1146	1148	1149	rVB2	187	116	0.01%	0.002%
46	8.220	1169	1170	1172	rBV2	122	100	0.01%	0.001%
47	8.238	1172	1173	1175	rVB	199	99	0.01%	0.001%
48	8.324	1181	1187	1200	rBV	118779	197998	20.00%	2.691%
49	8.647	1234	1240	1255	rBV	490927	762505	77.01%	10.363%
50	8.952	1284	1290	1305	rBV	82635	128414	12.97%	1.745%
51	9.183	1325	1328	1329	rBV	202	161	0.02%	0.002%
52	9.256	1338	1340	1341	rBV	218	147	0.01%	0.002%
53	9.281	1342	1344	1346	rVB	390	266	0.03%	0.004%
54	9.391	1356	1362	1385	rBV	283343	474125	47.89%	6.443%
55	9.671	1406	1408	1410	rBV	183	196	0.02%	0.003%
56	9.805	1429	1430	1431	rBV	182	98	0.01%	0.001%
57	9.884	1441	1443	1445	rBV	163	134	0.01%	0.002%
58	10.012	1462	1464	1465	rBV	187	107	0.01%	0.001%
59	10.055	1465	1471	1489	rVV	483424	727549	73.48%	9.887%
60	10.311	1508	1513	1518	rBV3	654	1045	0.11%	0.014%
61	10.403	1526	1528	1529	rBV2	119	121	0.01%	0.002%
62	10.585	1557	1558	1561	rBV2	216	138	0.01%	0.002%
63	10.653	1564	1569	1572	rVV3	297	511	0.05%	0.007%
64	10.884	1606	1607	1610	rVB2	192	163	0.02%	0.002%
65	10.921	1610	1613	1614	rBV2	209	202	0.02%	0.003%
66	10.945	1614	1617	1618	rVV	133	123	0.01%	0.002%
67	10.963	1618	1620	1624	rVB3	306	462	0.05%	0.006%
68	11.098	1637	1642	1646	rBV5	760	1275	0.13%	0.017%
69	11.195	1652	1658	1670	rBV	401418	521077	52.63%	7.081%
70	11.311	1673	1677	1684	rVB	1551	2390	0.24%	0.032%
71	11.378	1687	1688	1689	rBV	225	132	0.01%	0.002%
72	11.451	1698	1700	1703	rBV2	310	299	0.03%	0.004%
73	11.701	1739	1741	1747	rBV2	233	289	0.03%	0.004%
74	11.762	1747	1751	1754	rBV3	385	485	0.05%	0.007%
75	11.975	1782	1786	1788	rBV3	842	1131	0.11%	0.015%
76	12.024	1788	1794	1809	rVV	492533	656029	66.26%	8.915%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040982.D
 Acq On : 11 Apr 2024 17:48
 Operator : JC/MD
 Sample : P2048-08 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041024WMA.M
 Title : VOC Analysis

77	12.232	1827	1828	1829	rBV	182	119	0.01%	0.002%
78	12.280	1834	1836	1837	rBV2	134	98	0.01%	0.001%
79	12.323	1837	1843	1862	rBV	541284	719661	72.69%	9.780%
80	12.573	1882	1884	1886	rBV	201	179	0.02%	0.002%
81	12.646	1894	1896	1900	rVB	163	177	0.02%	0.002%
82	12.762	1909	1915	1920	rVB2	3211	4626	0.47%	0.063%
83	12.872	1930	1933	1935	rBV	159	188	0.02%	0.003%
84	12.939	1943	1944	1946	rBV	138	116	0.01%	0.002%
85	13.042	1960	1961	1963	rBV2	132	97	0.01%	0.001%
86	13.091	1967	1969	1972	rBV2	170	136	0.01%	0.002%
87	13.115	1972	1973	1977	rVB2	190	163	0.02%	0.002%
88	13.280	1999	2000	2003	rVB2	172	127	0.01%	0.002%
89	13.311	2003	2005	2006	rBV	116	99	0.01%	0.001%
90	13.359	2011	2013	2017	rVV2	180	225	0.02%	0.003%
91	13.451	2026	2028	2030	rBV2	166	164	0.02%	0.002%
92	13.597	2049	2052	2056	rVV5	594	771	0.08%	0.010%
93	13.676	2063	2065	2068	rBV2	119	142	0.01%	0.002%
94	13.780	2080	2082	2083	rBV2	378	292	0.03%	0.004%
95	13.932	2105	2107	2108	rBV	197	132	0.01%	0.002%
96	13.975	2111	2114	2118	rVB4	408	600	0.06%	0.008%
97	14.128	2135	2139	2143	rBV	4395	5943	0.60%	0.081%
98	14.316	2169	2170	2171	rBV	305	150	0.02%	0.002%
99	15.389	2342	2346	2355	rVB2	4242	7172	0.72%	0.097%
100	16.438	2516	2518	2519	rBV2	468	258	0.03%	0.004%


Sum of corrected areas: 7358306

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040982.D
Acq On : 11 Apr 2024 17:48
Operator : JC/MD
Sample : P2048-08 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

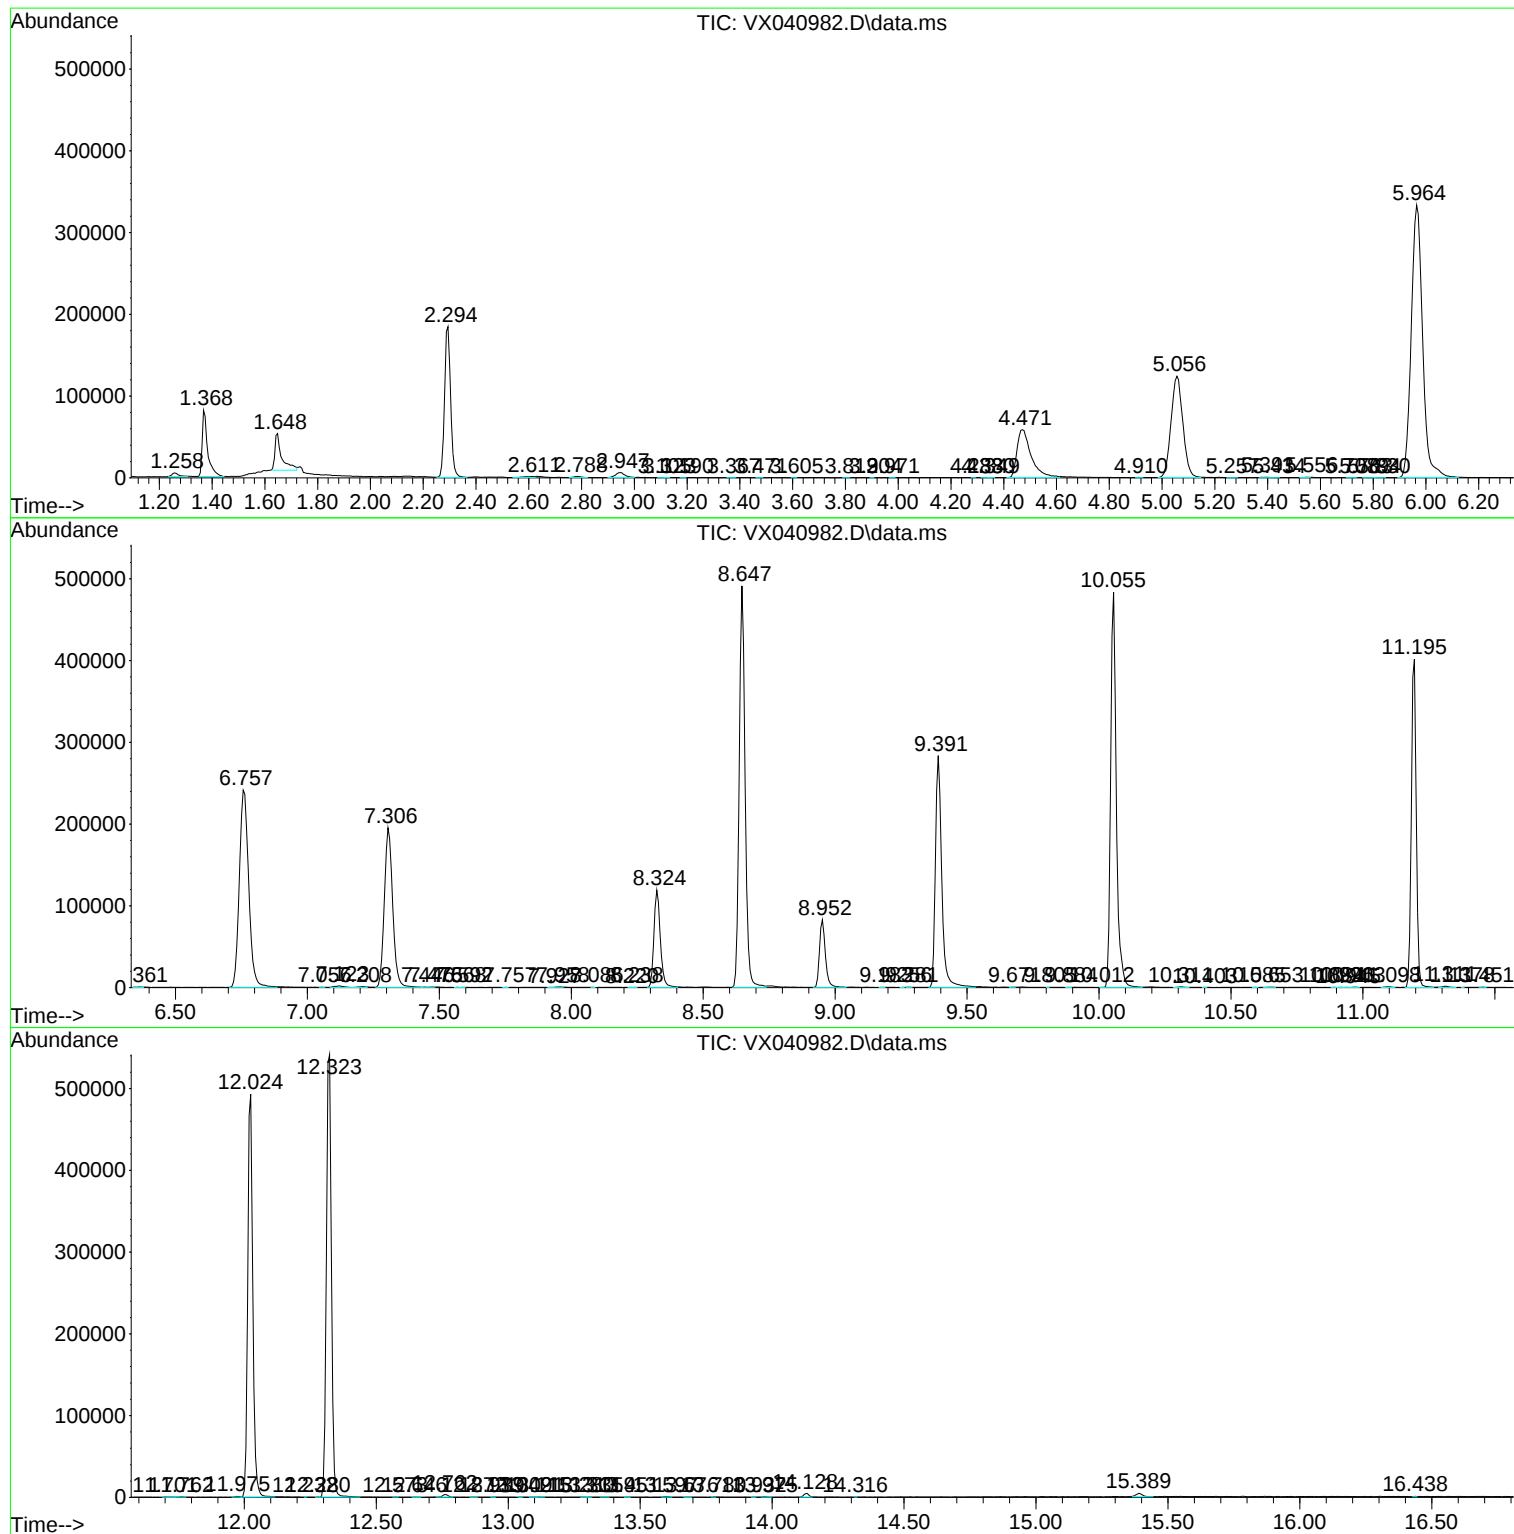

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040982.D
Acq On : 11 Apr 2024 17:48
Operator : JC/MD
Sample : P2048-08 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040982.D
Acq On : 11 Apr 2024 17:48
Operator : JC/MD
Sample : P2048-08 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc