

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040983.D
 Acq On : 11 Apr 2024 18:11
 Operator : JC/MD
 Sample : P2048-09 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M

Title : VOC Analysis

Signal : TIC: VX040983.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.257	25	28	32	rVB3	3460	4137	0.42%	0.055%
2	1.367	43	46	59	rVB	78495	114738	11.65%	1.534%
3	1.648	88	92	103	rBV	45451	77590	7.88%	1.038%
4	2.294	191	198	212	rVB	185964	292848	29.74%	3.916%
5	2.708	264	266	272	rVB2	432	637	0.06%	0.009%
6	2.782	272	278	286	rBV2	1573	2927	0.30%	0.039%
7	2.946	296	305	317	rVV	7937	20308	2.06%	0.272%
8	3.080	325	327	330	rVB2	184	140	0.01%	0.002%
9	3.117	330	333	337	rBV3	315	431	0.04%	0.006%
10	3.288	359	361	363	rBV2	210	187	0.02%	0.003%
11	3.446	385	387	389	rVB	185	126	0.01%	0.002%
12	3.507	393	397	398	rBV2	194	192	0.02%	0.003%
13	3.574	406	408	409	rBV2	148	120	0.01%	0.002%
14	3.672	422	424	425	rBV	166	123	0.01%	0.002%
15	3.696	425	428	431	rVV2	211	298	0.03%	0.004%
16	3.727	431	433	436	rVV2	109	130	0.01%	0.002%
17	3.812	445	447	450	rVV2	145	123	0.01%	0.002%
18	3.897	457	461	462	rBV2	97	144	0.01%	0.002%
19	3.964	470	472	475	rBV	125	122	0.01%	0.002%
20	3.995	475	477	480	rVV2	224	228	0.02%	0.003%
21	4.068	484	489	491	rBV	198	274	0.03%	0.004%
22	4.373	537	539	541	rVB	192	144	0.01%	0.002%
23	4.470	546	555	579	rBV	59122	212386	21.57%	2.840%
24	4.873	619	621	625	rVB2	179	169	0.02%	0.002%
25	5.056	639	651	670	rVV	125409	385639	39.16%	5.157%
26	5.202	673	675	679	rVB2	430	562	0.06%	0.008%
27	5.373	700	703	704	rBV	370	438	0.04%	0.006%
28	5.470	716	719	720	rBV3	186	206	0.02%	0.003%
29	5.543	728	731	732	rBV2	303	278	0.03%	0.004%
30	5.769	764	768	769	rBV2	147	137	0.01%	0.002%
31	5.964	789	800	824	rBV2	332780	984805	100.00%	13.169%
32	6.189	835	837	841	rVB3	286	299	0.03%	0.004%
33	6.354	862	864	865	rBV2	309	315	0.03%	0.004%
34	6.433	875	877	878	rBV2	163	122	0.01%	0.002%
35	6.464	880	882	884	rVB2	223	202	0.02%	0.003%
36	6.513	887	890	893	rBV	220	347	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040983.D
 Acq On : 11 Apr 2024 18:11
 Operator : JC/MD
 Sample : P2048-09 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	6.537	893	894	898	rBV2	167	183	0.02%	0.002%
38	6.756	921	930	956	rBV	260688	634656	64.44%	8.486%
39	7.128	982	991	998	rBV7	1816	4639	0.47%	0.062%
40	7.208	1001	1004	1006	rBV2	700	902	0.09%	0.012%
41	7.305	1012	1020	1035	rBV	190124	427352	43.39%	5.714%
42	7.482	1047	1049	1050	rBV	459	363	0.04%	0.005%
43	7.683	1080	1082	1085	rVB	228	168	0.02%	0.002%
44	7.768	1093	1096	1097	rBV2	115	123	0.01%	0.002%
45	7.884	1114	1115	1118	rVV2	118	124	0.01%	0.002%
46	7.957	1122	1127	1133	rBV5	758	1710	0.17%	0.023%
47	8.323	1181	1187	1200	rBV	118466	197120	20.02%	2.636%
48	8.439	1205	1206	1213	rVB	392	449	0.05%	0.006%
49	8.494	1213	1215	1216	rBV	299	304	0.03%	0.004%
50	8.585	1228	1230	1231	rVB	282	167	0.02%	0.002%
51	8.646	1234	1240	1256	rBV	477093	764313	77.61%	10.220%
52	8.951	1284	1290	1307	rBV	83252	128800	13.08%	1.722%
53	9.158	1323	1324	1326	rVB2	268	136	0.01%	0.002%
54	9.177	1326	1327	1330	rBV2	150	157	0.02%	0.002%
55	9.280	1341	1344	1350	rVB3	371	518	0.05%	0.007%
56	9.390	1356	1362	1381	rBV	279350	458286	46.54%	6.128%
57	9.792	1424	1428	1429	rBV3	188	262	0.03%	0.004%
58	9.835	1433	1435	1441	rBV3	171	267	0.03%	0.004%
59	10.055	1465	1471	1490	rBV	529266	773965	78.59%	10.349%
60	10.286	1507	1509	1510	rBV	218	203	0.02%	0.003%
61	10.305	1510	1512	1519	rVB4	822	1264	0.13%	0.017%
62	10.378	1522	1524	1526	rBV	189	130	0.01%	0.002%
63	10.408	1526	1529	1531	rVB	185	168	0.02%	0.002%
64	10.433	1531	1533	1537	rBV	160	158	0.02%	0.002%
65	10.591	1557	1559	1564	rBV	153	254	0.03%	0.003%
66	10.652	1564	1569	1570	rBV2	369	443	0.04%	0.006%
67	10.884	1604	1607	1610	rVB2	174	243	0.02%	0.003%
68	11.018	1624	1629	1631	rBV2	93	136	0.01%	0.002%
69	11.097	1638	1642	1646	rVB3	741	1173	0.12%	0.016%
70	11.134	1646	1648	1652	rBV2	137	181	0.02%	0.002%
71	11.195	1652	1658	1669	rBV	395632	517694	52.57%	6.923%
72	11.317	1674	1678	1682	rVB	1334	1793	0.18%	0.024%
73	11.463	1697	1702	1704	rBV4	479	643	0.07%	0.009%
74	11.567	1717	1719	1723	rVB2	205	299	0.03%	0.004%
75	11.603	1723	1725	1726	rBV	172	153	0.02%	0.002%
76	11.713	1739	1743	1745	rBV3	417	446	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040983.D
 Acq On : 11 Apr 2024 18:11
 Operator : JC/MD
 Sample : P2048-09 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041024WMA.M
 Title : VOC Analysis

77	11.762	1745	1751	1755	rVV3	403	622	0.06%	0.008%
78	11.975	1781	1786	1788	rBV	1000	1154	0.12%	0.015%
79	12.024	1788	1794	1806	rVV	552907	707294	71.82%	9.458%
80	12.158	1814	1816	1819	rBV2	453	372	0.04%	0.005%
81	12.323	1837	1843	1859	rBV	539433	731101	74.24%	9.776%
82	12.512	1873	1874	1876	rBV	318	188	0.02%	0.003%
83	12.566	1880	1883	1886	rBV2	101	160	0.02%	0.002%
84	12.761	1911	1915	1920	rVB2	3124	4220	0.43%	0.056%
85	12.926	1940	1942	1944	rBV2	114	136	0.01%	0.002%
86	12.963	1947	1948	1953	rBV2	158	253	0.03%	0.003%
87	13.066	1964	1965	1968	rBV	250	217	0.02%	0.003%
88	13.115	1972	1973	1977	rVV3	246	278	0.03%	0.004%
89	13.524	2038	2040	2042	rVB	175	125	0.01%	0.002%
90	13.597	2049	2052	2055	rBV3	657	901	0.09%	0.012%
91	13.670	2061	2064	2066	rBV2	123	155	0.02%	0.002%
92	13.786	2078	2083	2085	rBV3	389	600	0.06%	0.008%
93	13.841	2090	2092	2094	rVV	205	165	0.02%	0.002%
94	13.883	2097	2099	2103	rBV2	230	328	0.03%	0.004%
95	13.969	2110	2113	2117	rVV3	382	496	0.05%	0.007%
96	14.054	2125	2127	2130	rVB	246	189	0.02%	0.003%
97	14.133	2133	2140	2144	rBV2	2300	3345	0.34%	0.045%
98	14.212	2152	2153	2156	rBV2	204	195	0.02%	0.003%
99	14.395	2181	2183	2188	rVB2	282	305	0.03%	0.004%
100	15.389	2343	2346	2354	rVB4	2159	3405	0.35%	0.046%




Sum of corrected areas: 7478421

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040983.D
Acq On : 11 Apr 2024 18:11
Operator : JC/MD
Sample : P2048-09 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

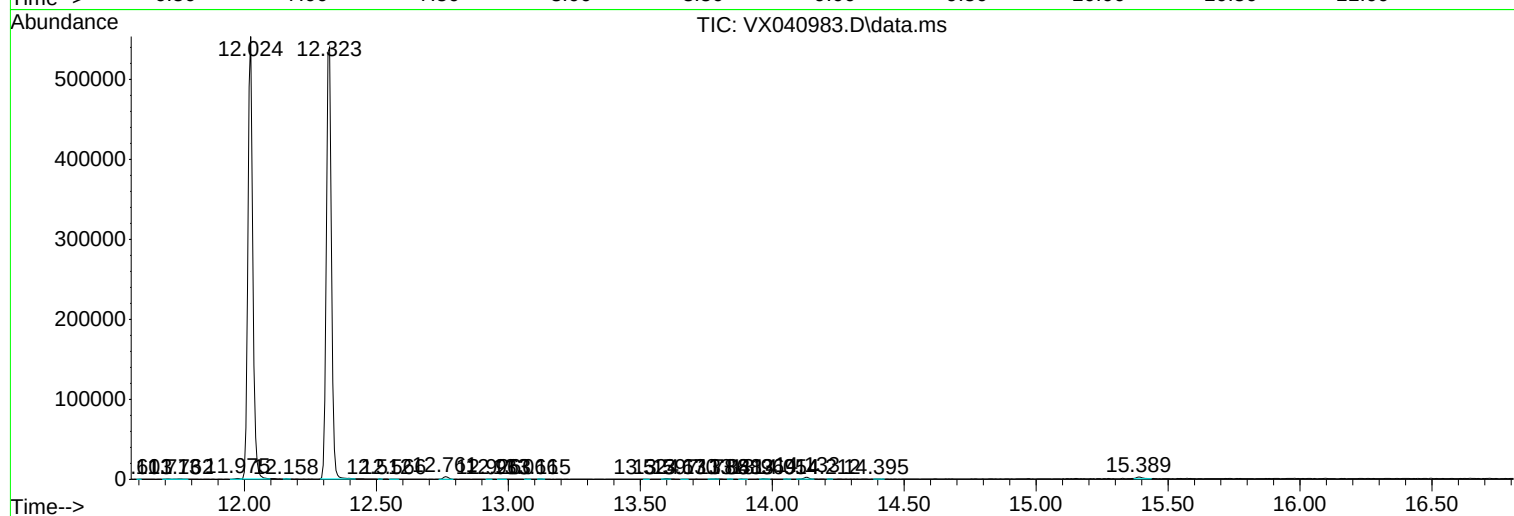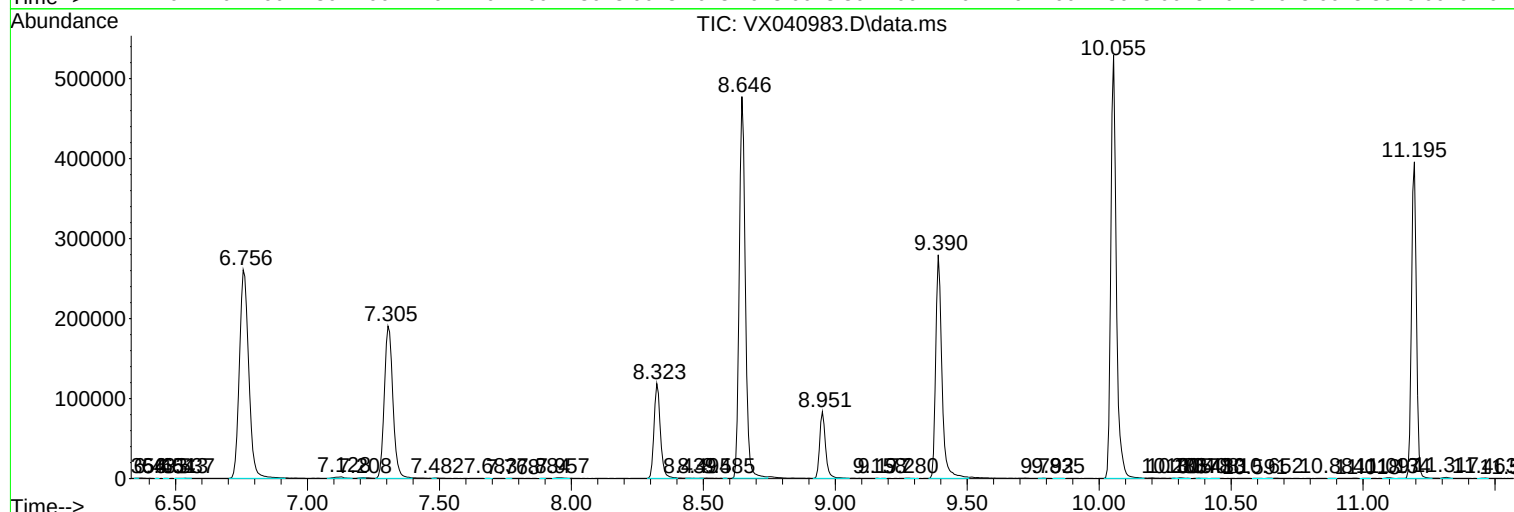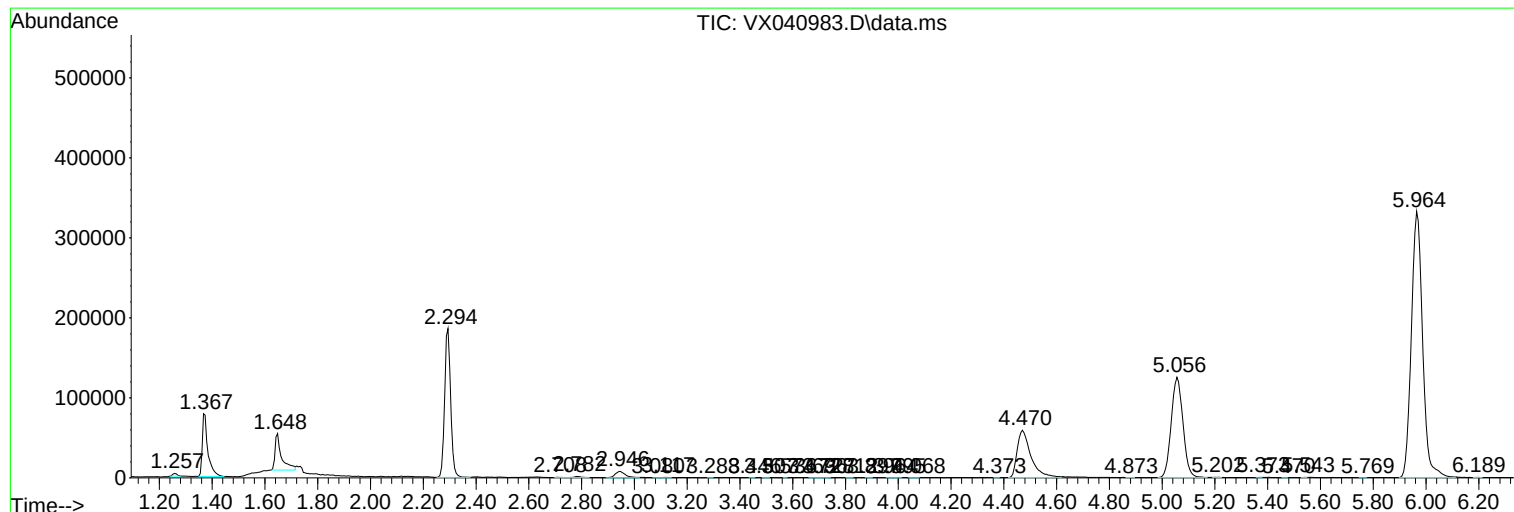

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040983.D
Acq On : 11 Apr 2024 18:11
Operator : JC/MD
Sample : P2048-09 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040983.D
Acq On : 11 Apr 2024 18:11
Operator : JC/MD
Sample : P2048-09 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc