

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040985.D
 Acq On : 11 Apr 2024 18:56
 Operator : JC/MD
 Sample : P2048-15 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R95

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M

Title : VOC Analysis

Signal : TIC: VX040985.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	63	rBV	78861	120388	12.15%	1.591%
2	1.648	88	92	98	rBV	46088	67881	6.85%	0.897%
3	2.294	191	198	211	rBV	190377	299631	30.25%	3.959%
4	2.788	273	279	285	rVB4	1246	2223	0.22%	0.029%
5	2.947	297	305	316	rVB	5845	13744	1.39%	0.182%
6	3.075	323	326	327	rBV	305	208	0.02%	0.003%
7	3.495	391	395	397	rBV2	160	201	0.02%	0.003%
8	3.599	409	412	414	rBV2	141	149	0.02%	0.002%
9	3.745	435	436	441	rVB2	148	140	0.01%	0.002%
10	3.788	441	443	447	rVB	167	176	0.02%	0.002%
11	3.818	447	448	451	rBV2	131	140	0.01%	0.002%
12	3.953	468	470	473	rBV2	117	165	0.02%	0.002%
13	3.983	473	475	477	rVV	101	107	0.01%	0.001%
14	4.001	477	478	482	rVB2	209	179	0.02%	0.002%
15	4.050	482	486	487	rBV	152	168	0.02%	0.002%
16	4.148	500	502	506	rBV2	100	104	0.01%	0.001%
17	4.257	518	520	521	rBV	147	144	0.01%	0.002%
18	4.465	545	554	583	rBV	59248	218269	22.04%	2.884%
19	5.056	638	651	667	rBV	123530	385666	38.94%	5.095%
20	5.385	701	705	708	rBV3	325	591	0.06%	0.008%
21	5.550	730	732	733	rBV	278	252	0.03%	0.003%
22	5.641	745	747	748	rBV	167	106	0.01%	0.001%
23	5.781	769	770	774	rVB2	164	136	0.01%	0.002%
24	5.964	788	800	832	rBV2	333787	990513	100.00%	13.087%
25	6.269	849	850	851	rBV	153	105	0.01%	0.001%
26	6.348	860	863	864	rBV2	531	579	0.06%	0.008%
27	6.489	884	886	889	rBV2	166	220	0.02%	0.003%
28	6.531	891	893	894	rVV2	227	178	0.02%	0.002%
29	6.580	899	901	904	rVB	106	124	0.01%	0.002%
30	6.757	920	930	947	rBV	265531	647113	65.33%	8.550%
31	7.123	983	990	999	rVB7	1930	4908	0.50%	0.065%
32	7.208	1000	1004	1011	rVB5	918	2180	0.22%	0.029%
33	7.306	1011	1020	1042	rBV	199121	434103	43.83%	5.735%
34	7.495	1049	1051	1052	rVB2	404	209	0.02%	0.003%
35	7.604	1068	1069	1071	rBV2	206	176	0.02%	0.002%
36	7.653	1076	1077	1080	rBV2	158	179	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040985.D
 Acq On : 11 Apr 2024 18:56
 Operator : JC/MD
 Sample : P2048-15 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R95

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	7.793	1098	1100	1105	rVB	163	204	0.02%	0.003%
38	7.958	1122	1127	1134	rVB4	772	1536	0.16%	0.020%
39	8.049	1137	1142	1144	rBV	115	175	0.02%	0.002%
40	8.104	1149	1151	1154	rBV2	151	166	0.02%	0.002%
41	8.324	1181	1187	1197	rBV	117527	196917	19.88%	2.602%
42	8.464	1208	1210	1211	rBV	286	192	0.02%	0.003%
43	8.513	1214	1218	1219	rVV	291	365	0.04%	0.005%
44	8.647	1234	1240	1255	rBV	487047	781075	78.86%	10.320%
45	8.891	1279	1280	1282	rBV	206	145	0.01%	0.002%
46	8.909	1282	1283	1284	rVV2	233	114	0.01%	0.002%
47	8.952	1284	1290	1308	rVV	81972	128269	12.95%	1.695%
48	9.110	1315	1316	1319	rBV2	211	199	0.02%	0.003%
49	9.165	1322	1325	1326	rBV2	229	178	0.02%	0.002%
50	9.269	1341	1342	1345	rVB2	299	279	0.03%	0.004%
51	9.342	1352	1354	1356	rBV	200	159	0.02%	0.002%
52	9.391	1356	1362	1378	rBV	292481	466873	47.13%	6.168%
53	9.708	1410	1414	1419	rBV4	364	778	0.08%	0.010%
54	9.799	1427	1429	1433	rVB	176	195	0.02%	0.003%
55	9.842	1433	1436	1438	rBV2	159	223	0.02%	0.003%
56	10.006	1458	1463	1465	rBV2	291	377	0.04%	0.005%
57	10.055	1465	1471	1488	rBV	539323	783013	79.05%	10.345%
58	10.195	1492	1494	1498	rVB3	747	892	0.09%	0.012%
59	10.311	1509	1513	1518	rBV3	548	924	0.09%	0.012%
60	10.354	1518	1520	1521	rVB	259	166	0.02%	0.002%
61	10.561	1553	1554	1557	rBV	158	116	0.01%	0.002%
62	10.585	1557	1558	1560	rBV	154	119	0.01%	0.002%
63	10.646	1565	1568	1571	rBV3	398	607	0.06%	0.008%
64	10.793	1590	1592	1595	rBV	151	164	0.02%	0.002%
65	10.970	1616	1621	1625	rBV2	322	495	0.05%	0.007%
66	11.000	1625	1626	1630	rVB	157	122	0.01%	0.002%
67	11.091	1638	1641	1645	rBV3	591	1049	0.11%	0.014%
68	11.189	1652	1657	1670	rVV	391530	521871	52.69%	6.895%
69	11.317	1674	1678	1682	rVB	1535	2052	0.21%	0.027%
70	11.506	1708	1709	1711	rBV	137	125	0.01%	0.002%
71	11.585	1719	1722	1723	rBV	137	134	0.01%	0.002%
72	11.707	1740	1742	1746	rVB2	227	288	0.03%	0.004%
73	11.762	1746	1751	1754	rBV3	315	424	0.04%	0.006%
74	11.975	1783	1786	1788	rBV3	981	976	0.10%	0.013%
75	12.024	1788	1794	1807	rBV	554637	723707	73.06%	9.562%
76	12.317	1837	1842	1859	rBV	570701	740399	74.75%	9.782%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040985.D
 Acq On : 11 Apr 2024 18:56
 Operator : JC/MD
 Sample : P2048-15 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R95

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M

Title : VOC Analysis

77	12.494	1869	1871	1873	rVB3	246	213	0.02%	0.003%
78	12.701	1904	1905	1907	rBV	223	118	0.01%	0.002%
79	12.731	1907	1910	1911	rVV2	141	157	0.02%	0.002%
80	12.762	1911	1915	1920	rVV2	3709	4648	0.47%	0.061%
81	12.902	1936	1938	1939	rVB	205	113	0.01%	0.001%
82	12.920	1939	1941	1944	rBV	182	183	0.02%	0.002%
83	12.975	1948	1950	1952	rBV2	131	159	0.02%	0.002%
84	13.128	1972	1975	1978	rVB	235	285	0.03%	0.004%
85	13.164	1978	1981	1985	rBV2	167	240	0.02%	0.003%
86	13.390	2017	2018	2020	rVB	235	136	0.01%	0.002%
87	13.414	2020	2022	2024	rBV2	185	187	0.02%	0.002%
88	13.439	2024	2026	2031	rBV	147	157	0.02%	0.002%
89	13.603	2048	2053	2055	rBV2	517	805	0.08%	0.011%
90	13.689	2065	2067	2068	rBV2	174	105	0.01%	0.001%
91	13.731	2073	2074	2076	rBV2	221	133	0.01%	0.002%
92	13.780	2080	2082	2084	rVV	308	340	0.03%	0.004%
93	13.823	2087	2089	2092	rBV2	383	301	0.03%	0.004%
94	13.871	2094	2097	2099	rBV2	245	229	0.02%	0.003%
95	13.975	2110	2114	2115	rBV	365	378	0.04%	0.005%
96	14.079	2129	2131	2133	rBB2	185	129	0.01%	0.002%
97	14.128	2135	2139	2144	rVB2	4373	5846	0.59%	0.077%
98	14.536	2204	2206	2208	rBV2	237	197	0.02%	0.003%
99	14.932	2269	2271	2272	rBV2	375	244	0.02%	0.003%
100	15.396	2342	2347	2353	rVB2	3729	6078	0.61%	0.080%




Sum of corrected areas: 7568798

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040985.D
Acq On : 11 Apr 2024 18:56
Operator : JC/MD
Sample : P2048-15 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R95

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

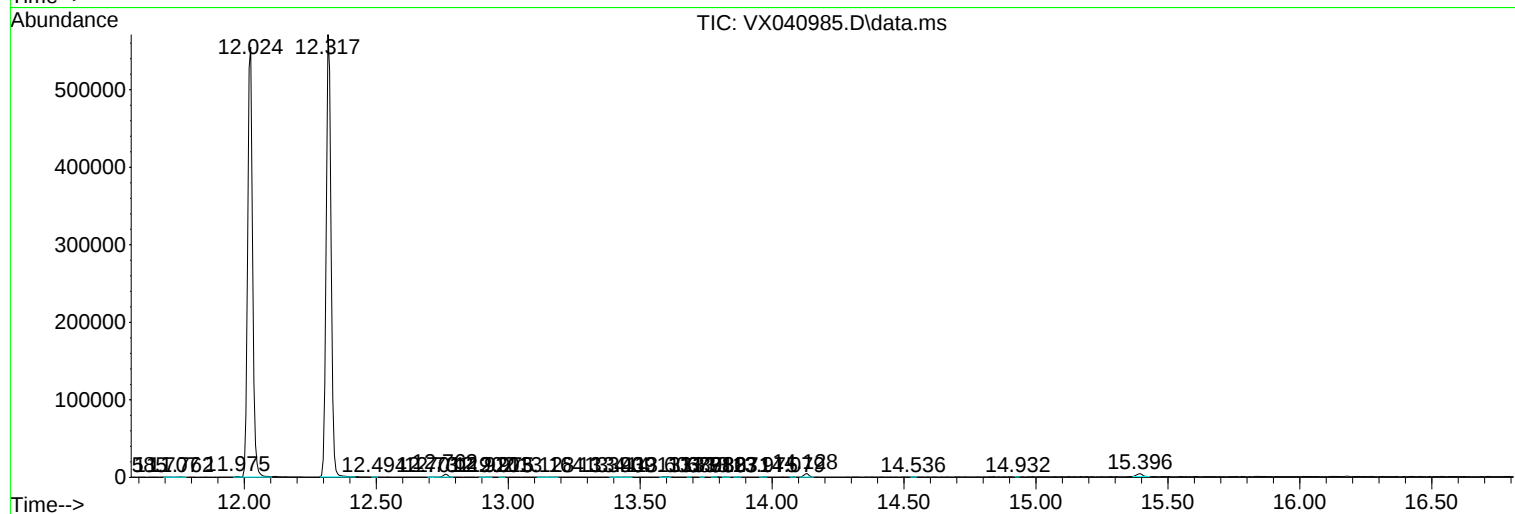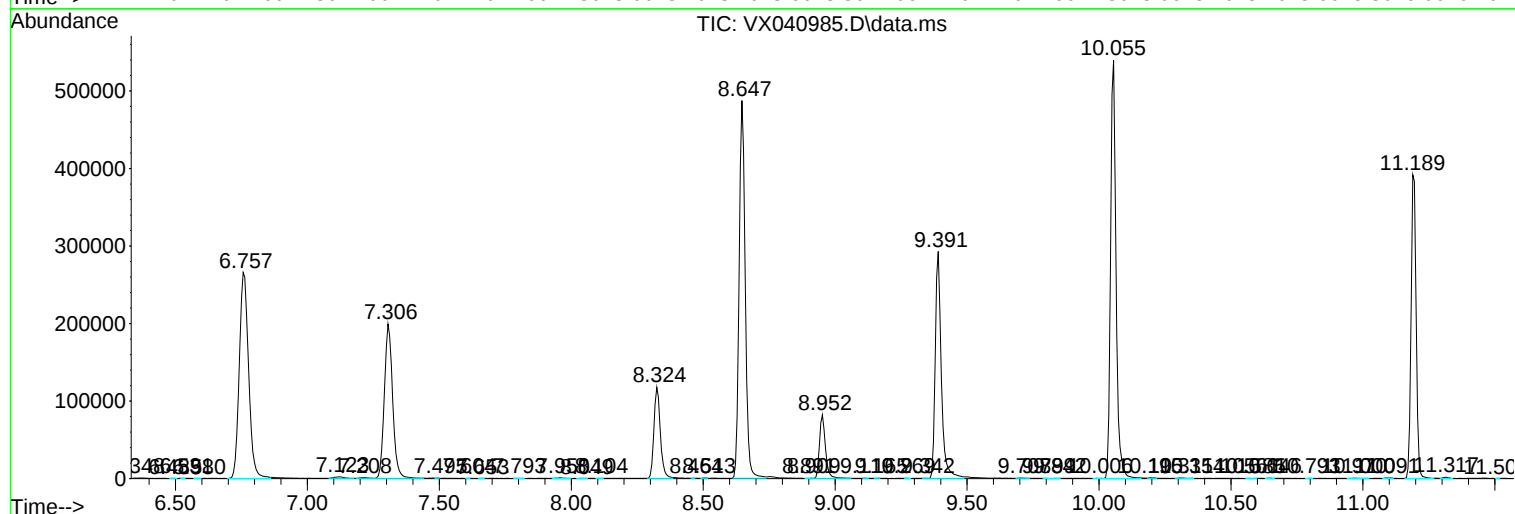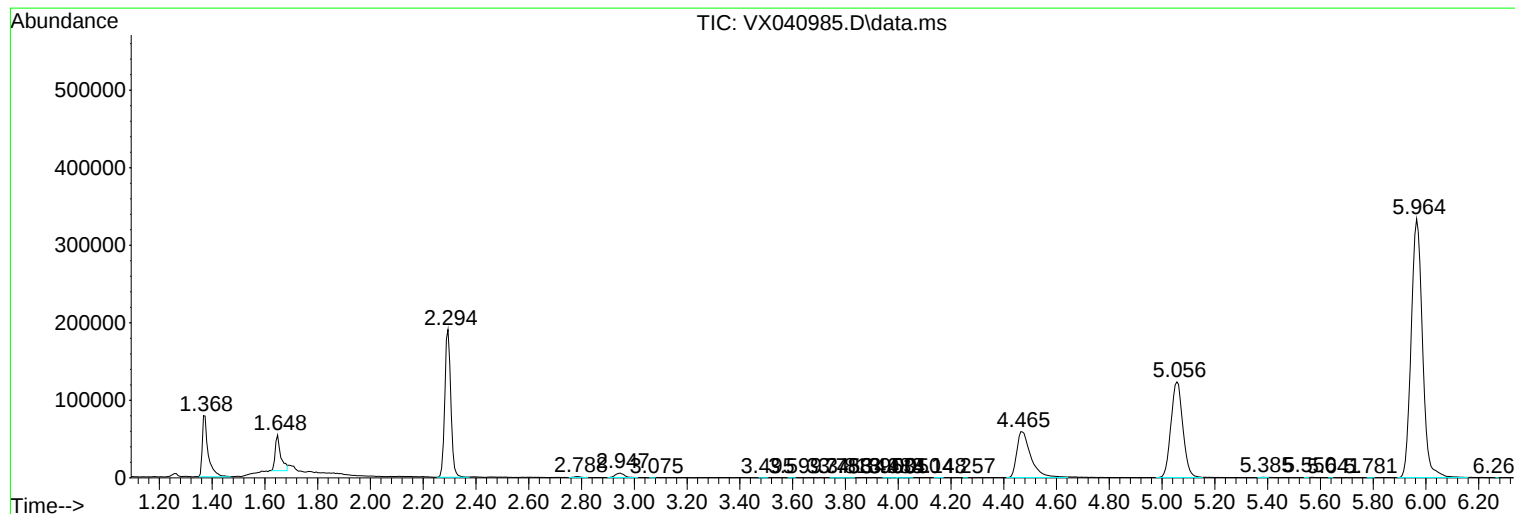

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040985.D
Acq On : 11 Apr 2024 18:56
Operator : JC/MD
Sample : P2048-15 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R95

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040985.D
Acq On : 11 Apr 2024 18:56
Operator : JC/MD
Sample : P2048-15 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R95

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc