

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040986.D
 Acq On : 11 Apr 2024 19:19
 Operator : JC/MD
 Sample : P2048-16 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R96

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX040986.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	24	28	36	rBV4	4155	6522	0.67%	0.090%
2	1.368	43	46	61	rBV	75848	114943	11.79%	1.586%
3	1.648	89	92	111	rVB	47087	97211	9.97%	1.342%
4	2.294	192	198	211	rVB	187975	292756	30.02%	4.040%
5	2.709	264	266	267	rBV2	302	234	0.02%	0.003%
6	2.788	274	279	282	rBV2	1486	2419	0.25%	0.033%
7	2.941	296	304	316	rBV	6517	15874	1.63%	0.219%
8	3.117	330	333	337	rVB3	269	411	0.04%	0.006%
9	3.148	337	338	341	rBV2	207	210	0.02%	0.003%
10	3.282	356	360	362	rBV2	117	209	0.02%	0.003%
11	3.886	455	459	463	rBV	106	158	0.02%	0.002%
12	3.989	473	476	477	rBV2	139	133	0.01%	0.002%
13	4.471	545	555	576	rBV	59386	218847	22.44%	3.020%
14	4.818	610	612	613	rBV2	188	135	0.01%	0.002%
15	4.904	624	626	629	rBV	222	206	0.02%	0.003%
16	4.934	629	631	634	rVB	223	178	0.02%	0.002%
17	5.056	634	651	672	rBV	124468	381853	39.16%	5.270%
18	5.379	701	704	706	rBV2	323	401	0.04%	0.006%
19	5.544	728	731	732	rBV	250	265	0.03%	0.004%
20	5.849	779	781	784	rVB	221	162	0.02%	0.002%
21	5.964	788	800	826	rBV2	327148	975058	100.00%	13.456%
22	6.245	844	846	848	rVB	216	161	0.02%	0.002%
23	6.294	853	854	857	rVB	185	167	0.02%	0.002%
24	6.367	862	866	872	rVB4	658	1361	0.14%	0.019%
25	6.550	893	896	900	rBV3	153	249	0.03%	0.003%
26	6.757	920	930	945	rBV	234972	577091	59.19%	7.964%
27	7.117	984	989	997	rVB7	1751	4397	0.45%	0.061%
28	7.214	1000	1005	1006	rBV2	763	1302	0.13%	0.018%
29	7.306	1012	1020	1037	rBV	191819	428199	43.92%	5.909%
30	7.476	1046	1048	1049	rBV2	273	216	0.02%	0.003%
31	7.757	1092	1094	1097	rBV2	127	159	0.02%	0.002%
32	7.958	1121	1127	1135	rBV5	684	1565	0.16%	0.022%
33	8.068	1142	1145	1149	rVB2	220	343	0.04%	0.005%
34	8.110	1149	1152	1153	rBV2	217	194	0.02%	0.003%
35	8.171	1160	1162	1165	rBV2	132	131	0.01%	0.002%
36	8.214	1167	1169	1172	rBV2	154	163	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040986.D
 Acq On : 11 Apr 2024 19:19
 Operator : JC/MD
 Sample : P2048-16 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R96

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	8.263	1175	1177	1181	rBV2	120	197	0.02%	0.003%
38	8.324	1181	1187	1203	rBV	112668	192979	19.79%	2.663%
39	8.452	1206	1208	1211	rVB3	374	350	0.04%	0.005%
40	8.494	1211	1215	1216	rBV3	271	263	0.03%	0.004%
41	8.537	1220	1222	1224	rVB2	283	141	0.01%	0.002%
42	8.574	1227	1228	1233	rBV3	163	206	0.02%	0.003%
43	8.647	1234	1240	1255	rBV	484786	761822	78.13%	10.514%
44	8.903	1280	1282	1284	rVB	270	177	0.02%	0.002%
45	8.952	1284	1290	1299	rBV	80411	124722	12.79%	1.721%
46	9.202	1329	1331	1334	rVB	225	170	0.02%	0.002%
47	9.281	1340	1344	1350	rBV3	476	721	0.07%	0.010%
48	9.391	1356	1362	1379	rBV	287482	468683	48.07%	6.468%
49	9.714	1410	1415	1419	rBV3	555	967	0.10%	0.013%
50	9.866	1438	1440	1443	rVB2	164	160	0.02%	0.002%
51	9.933	1448	1451	1452	rBV2	157	171	0.02%	0.002%
52	10.055	1465	1471	1490	rBV	479760	690938	70.86%	9.535%
53	10.201	1492	1495	1497	rVV3	500	688	0.07%	0.009%
54	10.250	1501	1503	1505	rBV2	189	139	0.01%	0.002%
55	10.311	1509	1513	1516	rBV3	581	857	0.09%	0.012%
56	10.555	1552	1553	1556	rBV2	169	173	0.02%	0.002%
57	10.646	1564	1568	1572	rBV3	330	428	0.04%	0.006%
58	10.683	1572	1574	1576	rVV2	164	168	0.02%	0.002%
59	10.976	1615	1622	1624	rBV3	320	510	0.05%	0.007%
60	11.098	1639	1642	1647	rBV3	787	1214	0.12%	0.017%
61	11.146	1647	1650	1652	rBV	144	191	0.02%	0.003%
62	11.195	1652	1658	1669	rVV	387693	518474	53.17%	7.155%
63	11.311	1673	1677	1683	rVB	1428	2113	0.22%	0.029%
64	11.463	1697	1702	1706	rBV3	399	529	0.05%	0.007%
65	11.640	1730	1731	1735	rVB	190	142	0.01%	0.002%
66	11.713	1741	1743	1745	rBV	393	313	0.03%	0.004%
67	11.756	1748	1750	1755	rVB3	379	435	0.04%	0.006%
68	11.799	1755	1757	1759	rBV2	183	154	0.02%	0.002%
69	11.976	1783	1786	1788	rBV2	521	641	0.07%	0.009%
70	12.024	1788	1794	1809	rVV	472040	622416	63.83%	8.590%
71	12.268	1832	1834	1835	rBV2	151	134	0.01%	0.002%
72	12.317	1837	1842	1852	rBV	528629	706998	72.51%	9.757%
73	12.536	1876	1878	1880	rVB	305	174	0.02%	0.002%
74	12.561	1880	1882	1887	rVB3	245	389	0.04%	0.005%
75	12.603	1887	1889	1890	rBV	150	148	0.02%	0.002%
76	12.719	1906	1908	1910	rBV	152	141	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040986.D
 Acq On : 11 Apr 2024 19:19
 Operator : JC/MD
 Sample : P2048-16 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R96

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	12.762	1910	1915	1920	rBV2	3379	4928	0.51%	0.068%
78	12.963	1946	1948	1953	rVB	221	282	0.03%	0.004%
79	13.000	1953	1954	1956	rBV	198	163	0.02%	0.002%
80	13.128	1973	1975	1977	rBV2	304	204	0.02%	0.003%
81	13.225	1990	1991	1993	rBV2	175	160	0.02%	0.002%
82	13.542	2040	2043	2045	rBV	234	243	0.02%	0.003%
83	13.603	2048	2053	2057	rVB4	619	1064	0.11%	0.015%
84	13.634	2057	2058	2061	rBV2	169	209	0.02%	0.003%
85	13.676	2064	2065	2067	rBV2	174	139	0.01%	0.002%
86	13.713	2067	2071	2075	rVB2	210	285	0.03%	0.004%
87	13.756	2077	2078	2081	rBV	218	255	0.03%	0.004%
88	13.792	2081	2084	2086	rVV2	309	323	0.03%	0.004%
89	13.829	2088	2090	2093	rVB	222	239	0.02%	0.003%
90	13.853	2093	2094	2098	rBV2	261	371	0.04%	0.005%
91	13.884	2098	2099	2101	rBV	219	140	0.01%	0.002%
92	13.963	2110	2112	2116	rBV2	354	425	0.04%	0.006%
93	14.067	2127	2129	2130	rBV2	201	176	0.02%	0.002%
94	14.079	2130	2131	2132	rVV	398	189	0.02%	0.003%
95	14.128	2135	2139	2146	rVV	3817	5247	0.54%	0.072%
96	14.256	2158	2160	2162	rBV	195	197	0.02%	0.003%
97	14.353	2174	2176	2178	rBV2	180	152	0.02%	0.002%
98	14.390	2180	2182	2188	rVB3	300	385	0.04%	0.005%
99	14.896	2264	2265	2266	rBV	337	156	0.02%	0.002%
100	15.390	2341	2346	2354	rVB	3609	6063	0.62%	0.084%


Sum of corrected areas: 7246114

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040986.D
Acq On : 11 Apr 2024 19:19
Operator : JC/MD
Sample : P2048-16 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R96

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

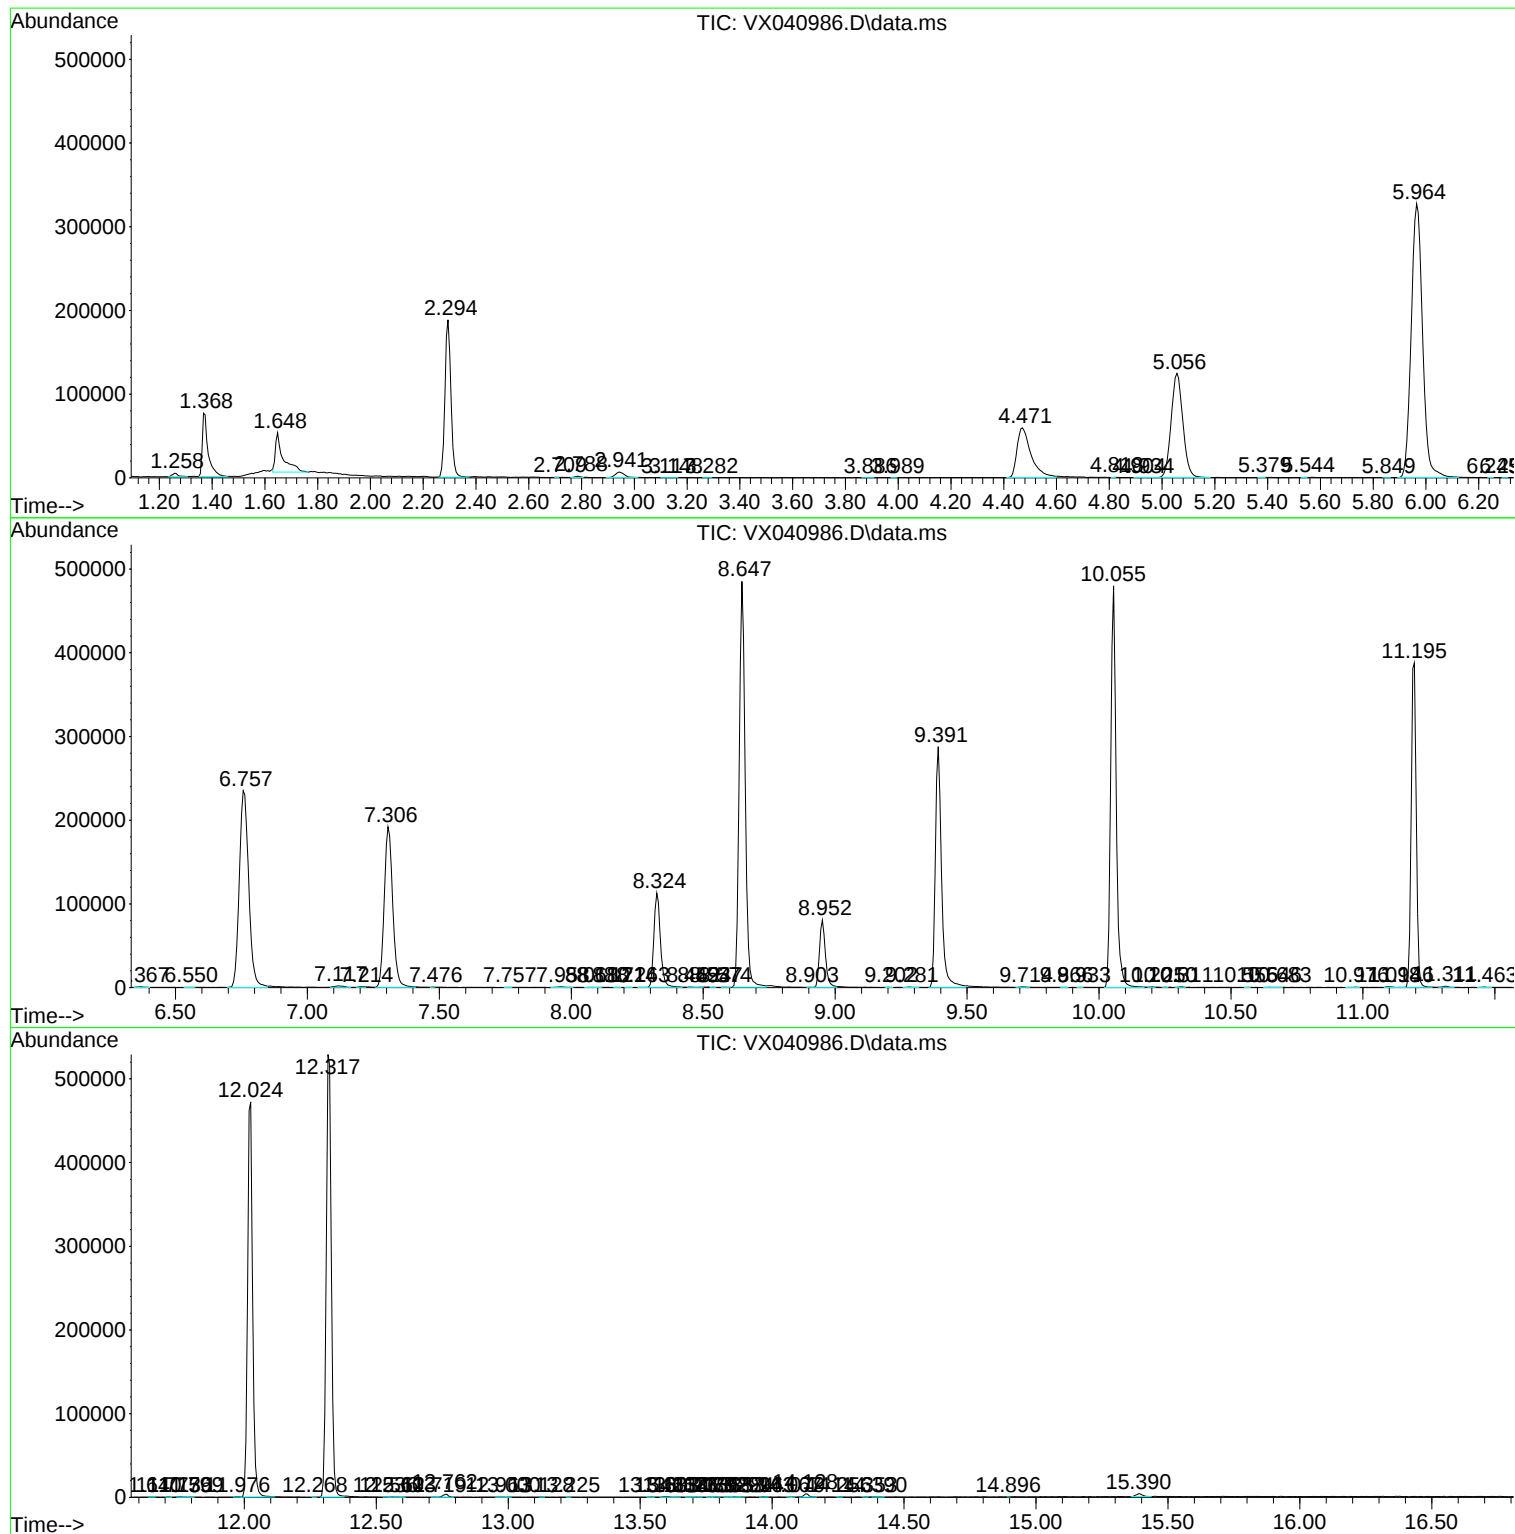

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040986.D
Acq On : 11 Apr 2024 19:19
Operator : JC/MD
Sample : P2048-16 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R96

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040986.D
Acq On : 11 Apr 2024 19:19
Operator : JC/MD
Sample : P2048-16 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R96

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc