

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040993.D
 Acq On : 11 Apr 2024 22:25
 Operator : JC/MD
 Sample : P2048-03DL 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R47DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M

Title : VOC Analysis

Signal : TIC: VX040993.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.306	197	200	207	rVB2	2321	3966	0.07%	0.027%
2	2.379	208	212	219	rVB2	811	1201	0.02%	0.008%
3	2.532	231	237	243	rBV5	1691	3482	0.06%	0.023%
4	2.654	255	257	261	rVB2	168	153	0.00%	0.001%
5	2.709	264	266	269	rVB	225	258	0.00%	0.002%
6	2.739	269	271	273	rBV2	119	111	0.00%	0.001%
7	2.794	275	280	283	rVB3	631	1005	0.02%	0.007%
8	2.824	283	285	288	rVB2	114	109	0.00%	0.001%
9	2.861	288	291	292	rBV2	139	148	0.00%	0.001%
10	2.946	298	305	313	rVB2	3850	8867	0.15%	0.060%
11	3.001	313	314	316	rVB	286	116	0.00%	0.001%
12	3.026	316	318	319	rBV2	176	150	0.00%	0.001%
13	3.081	323	327	328	rBV	210	179	0.00%	0.001%
14	3.123	333	334	336	rVB2	254	149	0.00%	0.001%
15	3.178	341	343	346	rVB2	113	137	0.00%	0.001%
16	3.318	365	366	369	rVB	195	127	0.00%	0.001%
17	3.416	380	382	383	rBV2	156	125	0.00%	0.001%
18	3.483	392	393	396	rBV2	176	152	0.00%	0.001%
19	3.605	411	413	417	rBV	240	323	0.01%	0.002%
20	3.641	417	419	420	rVB	193	110	0.00%	0.001%
21	3.745	433	436	438	rBV	132	119	0.00%	0.001%
22	3.806	443	446	449	rVB2	134	157	0.00%	0.001%
23	3.891	458	460	461	rVB	219	107	0.00%	0.001%
24	3.910	461	463	466	rBV	189	195	0.00%	0.001%
25	4.239	515	517	520	rVB2	159	168	0.00%	0.001%
26	4.269	520	522	524	rBV	185	227	0.00%	0.002%
27	4.306	524	528	532	rVB3	483	544	0.01%	0.004%
28	4.495	557	559	560	rBV	303	172	0.00%	0.001%
29	4.562	564	570	583	rVB2	3489	10914	0.18%	0.074%
30	4.751	600	601	606	rVB	248	150	0.00%	0.001%
31	4.855	616	618	621	rVB3	159	124	0.00%	0.001%
32	4.995	638	641	643	rBV2	141	173	0.00%	0.001%
33	5.068	646	653	657	rVV3	786	2213	0.04%	0.015%
34	5.123	661	662	666	rBV2	117	159	0.00%	0.001%
35	5.226	676	679	682	rBV2	176	201	0.00%	0.001%
36	5.336	694	697	698	rBV2	111	110	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040993.D
 Acq On : 11 Apr 2024 22:25
 Operator : JC/MD
 Sample : P2048-03DL 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R47DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	5.379	702	704	706	rVV	314	227	0.00%	0.002%
38	5.403	706	708	712	rVB2	309	309	0.01%	0.002%
39	5.458	714	717	718	rBV	214	143	0.00%	0.001%
40	5.513	724	726	728	rBV	134	113	0.00%	0.001%
41	5.617	741	743	746	rBV2	150	170	0.00%	0.001%
42	5.806	770	774	775	rBV2	111	134	0.00%	0.001%
43	5.860	781	783	785	rBV	145	127	0.00%	0.001%
44	6.037	794	812	830	rBV	2291345	6059761	100.00%	40.824%
45	6.610	904	906	908	rVB2	187	130	0.00%	0.001%
46	6.763	919	931	951	rBV	264161	638601	10.54%	4.302%
47	7.135	989	992	997	rVB5	484	738	0.01%	0.005%
48	7.318	1016	1022	1027	rVV3	945	1772	0.03%	0.012%
49	7.385	1031	1033	1038	rVB3	235	276	0.00%	0.002%
50	7.470	1044	1047	1049	rBV	246	236	0.00%	0.002%
51	7.878	1112	1114	1116	rBV	197	181	0.00%	0.001%
52	8.336	1185	1189	1194	rBV2	838	1390	0.02%	0.009%
53	8.464	1208	1210	1213	rVB2	155	151	0.00%	0.001%
54	8.586	1226	1230	1232	rBV2	228	281	0.00%	0.002%
55	8.653	1237	1241	1250	rBV2	5130	9009	0.15%	0.061%
56	8.726	1250	1253	1257	rVB2	524	727	0.01%	0.005%
57	8.848	1270	1273	1274	rBV2	143	171	0.00%	0.001%
58	8.964	1288	1292	1295	rBV3	709	1005	0.02%	0.007%
59	8.994	1295	1297	1300	rVB3	266	262	0.00%	0.002%
60	9.110	1312	1316	1317	rBV2	142	198	0.00%	0.001%
61	9.256	1337	1340	1341	rBV2	140	161	0.00%	0.001%
62	9.274	1341	1343	1348	rVB3	516	489	0.01%	0.003%
63	9.403	1361	1364	1366	rBV3	556	737	0.01%	0.005%
64	9.506	1377	1381	1383	rBV	203	220	0.00%	0.001%
65	9.811	1428	1431	1432	rBV	187	201	0.00%	0.001%
66	9.927	1448	1450	1452	rBV2	84	108	0.00%	0.001%
67	10.079	1465	1475	1492	rBV2	3521114	5492866	90.64%	37.005%
68	10.427	1531	1532	1534	rVB	377	166	0.00%	0.001%
69	10.616	1560	1563	1564	rBV	166	190	0.00%	0.001%
70	10.646	1566	1568	1570	rVV	505	317	0.01%	0.002%
71	10.713	1577	1579	1582	rVB	258	170	0.00%	0.001%
72	10.963	1613	1620	1626	rBV3	521	886	0.01%	0.006%
73	11.085	1639	1640	1645	rVB3	494	636	0.01%	0.004%
74	11.140	1647	1649	1652	rVB	199	172	0.00%	0.001%
75	11.195	1652	1658	1666	rBV	3059	4484	0.07%	0.030%
76	11.311	1674	1677	1681	rVB3	357	613	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040993.D
 Acq On : 11 Apr 2024 22:25
 Operator : JC/MD
 Sample : P2048-03DL 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R47DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	11.372	1684	1687	1688	rBV	156	198	0.00%	0.001%
78	11.457	1697	1701	1706	rVB3	456	837	0.01%	0.006%
79	11.500	1706	1708	1712	rBV2	145	211	0.00%	0.001%
80	11.561	1715	1718	1719	rBV	139	120	0.00%	0.001%
81	11.756	1747	1750	1753	rBV3	442	480	0.01%	0.003%
82	11.872	1767	1769	1770	rVB	202	116	0.00%	0.001%
83	11.969	1780	1785	1789	rBV	50106	61387	1.01%	0.414%
84	12.036	1789	1796	1815	rVB2	927473	1842751	30.41%	12.414%
85	12.335	1837	1845	1864	rBV	490050	648728	10.71%	4.370%
86	12.597	1886	1888	1892	rBV2	154	221	0.00%	0.001%
87	12.762	1911	1915	1920	rVB2	2332	3048	0.05%	0.021%
88	13.121	1971	1974	1979	rVB3	316	556	0.01%	0.004%
89	13.414	2020	2022	2024	rBV2	189	196	0.00%	0.001%
90	13.591	2046	2051	2058	rBV	14893	19789	0.33%	0.133%
91	13.664	2061	2063	2065	rVV	212	157	0.00%	0.001%
92	13.682	2065	2066	2069	rVB	196	197	0.00%	0.001%
93	13.786	2080	2083	2086	rBV	674	680	0.01%	0.005%
94	13.877	2097	2098	2100	rBV2	164	137	0.00%	0.001%
95	13.969	2110	2113	2117	rVV3	700	964	0.02%	0.006%
96	13.999	2117	2118	2120	rVB	250	158	0.00%	0.001%
97	14.024	2120	2122	2126	rBV2	223	347	0.01%	0.002%
98	14.127	2135	2139	2146	rVB	5084	6913	0.11%	0.047%
99	14.639	2222	2223	2224	rBV	280	138	0.00%	0.001%
100	14.725	2236	2237	2238	rBV	349	148	0.00%	0.001%

Sum of corrected areas: 14843606




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040993.D
Acq On : 11 Apr 2024 22:25
Operator : JC/MD
Sample : P2048-03DL 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R47DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

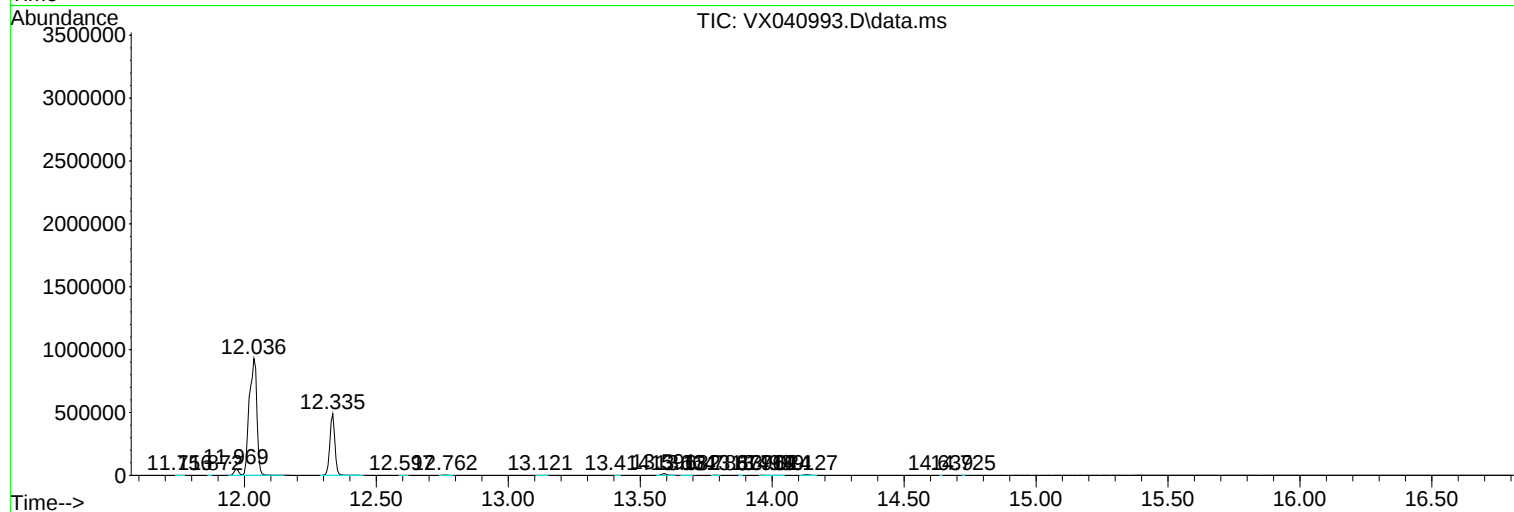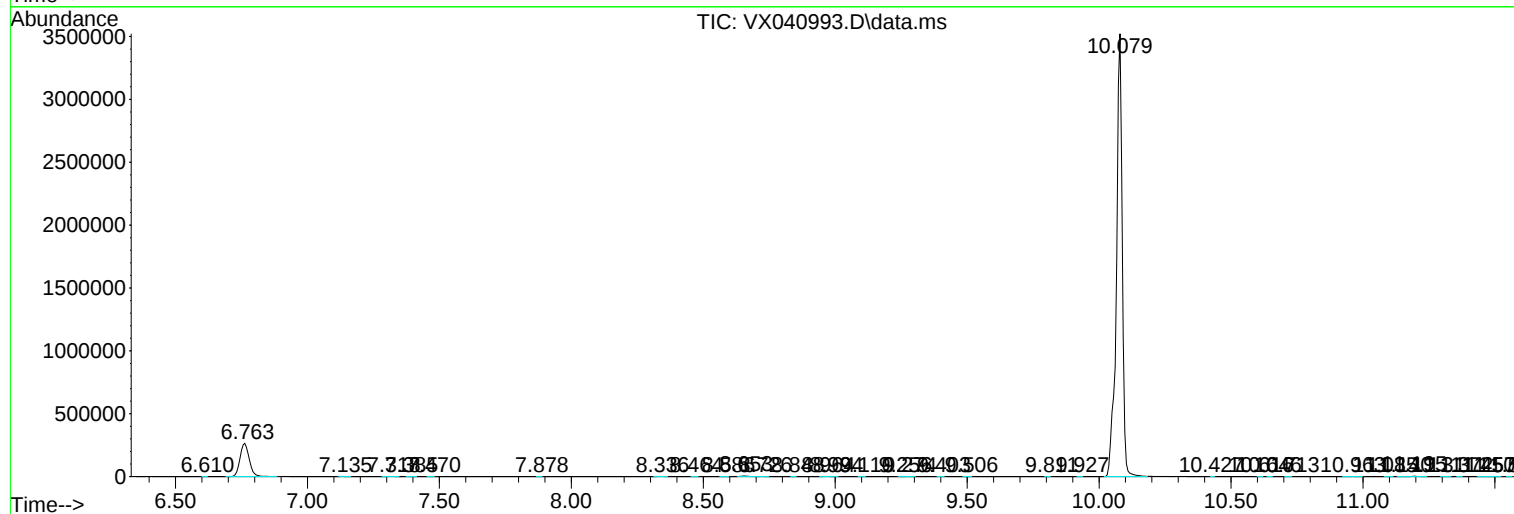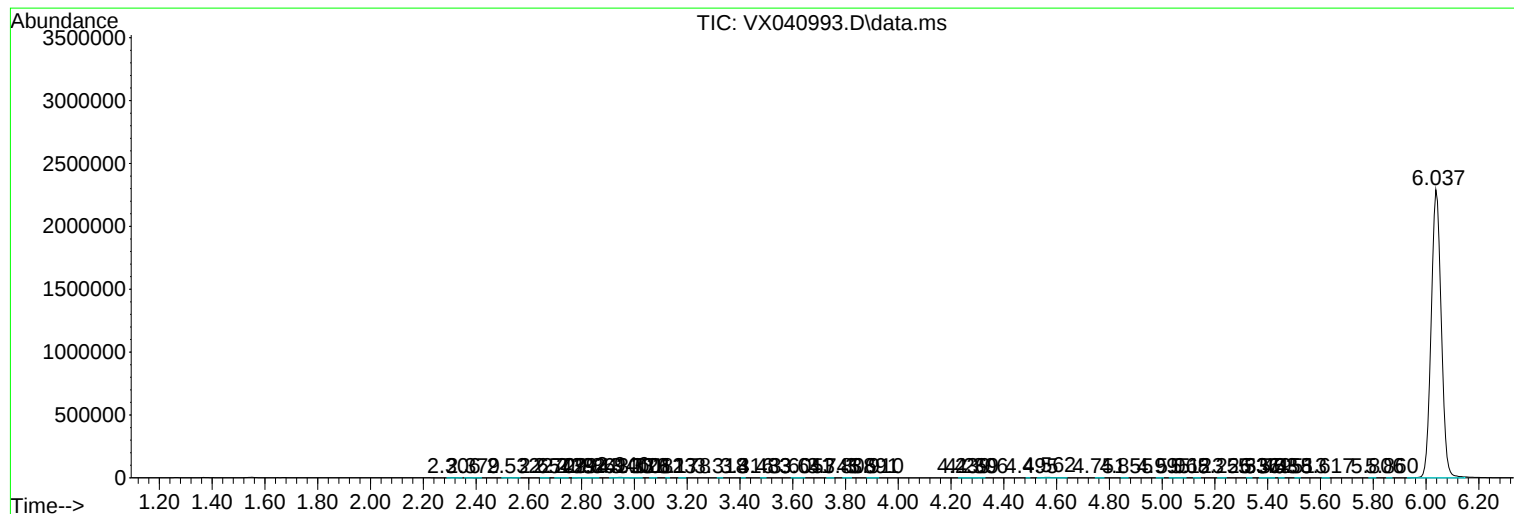

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040993.D
Acq On : 11 Apr 2024 22:25
Operator : JC/MD
Sample : P2048-03DL 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R47DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040993.D
Acq On : 11 Apr 2024 22:25
Operator : JC/MD
Sample : P2048-03DL 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R47DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc