

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040994.D
 Acq On : 11 Apr 2024 22:48
 Operator : JC/MD
 Sample : P2048-04DL 400X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R51DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M

Title : VOC Analysis

Signal : TIC: VX040994.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	59	rVB	110462	125330	3.21%	0.808%
2	1.672	91	96	115	rVB	84102	131620	3.38%	0.849%
3	2.306	194	200	209	rBV	194034	304906	7.82%	1.967%
4	2.532	231	237	244	rVB3	1890	3929	0.10%	0.025%
5	2.788	274	279	285	rBV4	1012	1895	0.05%	0.012%
6	2.941	297	304	315	rVB2	5775	13161	0.34%	0.085%
7	3.099	328	330	333	rBV2	286	386	0.01%	0.002%
8	3.507	396	397	400	rVB2	154	131	0.00%	0.001%
9	3.587	408	410	412	rBV2	122	115	0.00%	0.001%
10	3.812	445	447	448	rBV	171	117	0.00%	0.001%
11	3.940	467	468	471	rBV2	141	146	0.00%	0.001%
12	3.977	473	474	477	rVV	140	128	0.00%	0.001%
13	4.050	483	486	490	rBV2	139	206	0.01%	0.001%
14	4.166	503	505	508	rVV	161	120	0.00%	0.001%
15	4.324	529	531	535	rVB	180	159	0.00%	0.001%
16	4.459	544	553	569	rBV2	73583	240187	6.16%	1.549%
17	4.800	608	609	611	rBV2	280	220	0.01%	0.001%
18	4.855	615	618	619	rBV2	165	162	0.00%	0.001%
19	4.904	624	626	627	rBV2	210	140	0.00%	0.001%
20	4.940	630	632	634	rBV2	137	112	0.00%	0.001%
21	5.056	638	651	675	rBV	131126	406938	10.44%	2.625%
22	5.385	701	705	706	rBV4	382	421	0.01%	0.003%
23	5.434	712	713	715	rBV2	127	112	0.00%	0.001%
24	5.464	716	718	722	rVB2	274	289	0.01%	0.002%
25	5.513	722	726	727	rBV	205	158	0.00%	0.001%
26	5.544	727	731	732	rBV2	386	402	0.01%	0.003%
27	5.684	752	754	756	rVB	246	189	0.00%	0.001%
28	5.708	756	758	763	rBV2	79	128	0.00%	0.001%
29	5.842	778	780	783	rBV	127	141	0.00%	0.001%
30	5.970	789	801	805	rBV2	333625	943436	24.20%	6.085%
31	6.038	806	812	842	rVB	1273870	3347761	85.88%	21.592%
32	6.470	882	883	886	rVB2	283	181	0.00%	0.001%
33	6.537	891	894	895	rBV3	185	218	0.01%	0.001%
34	6.586	901	902	904	rBV2	175	149	0.00%	0.001%
35	6.763	919	931	947	rBV	279056	674041	17.29%	4.347%
36	7.117	983	989	1000	rVB8	2182	5933	0.15%	0.038%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040994.D
 Acq On : 11 Apr 2024 22:48
 Operator : JC/MD
 Sample : P2048-04DL 400X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R51DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	7.306	1012	1020	1039	rBV	195251	441183	11.32%	2.845%
38	7.470	1045	1047	1048	rBV2	308	246	0.01%	0.002%
39	7.531	1055	1057	1060	rVB3	313	269	0.01%	0.002%
40	7.677	1080	1081	1085	rVV2	135	132	0.00%	0.001%
41	7.763	1091	1095	1096	rVB2	141	168	0.00%	0.001%
42	7.830	1104	1106	1109	rBV	163	206	0.01%	0.001%
43	7.958	1122	1127	1131	rVV3	712	1191	0.03%	0.008%
44	8.013	1135	1136	1137	rVV	248	112	0.00%	0.001%
45	8.324	1181	1187	1204	rBV	124987	210048	5.39%	1.355%
46	8.580	1226	1229	1234	rBV2	369	628	0.02%	0.004%
47	8.647	1234	1240	1252	rBV	506824	796845	20.44%	5.139%
48	8.952	1284	1290	1304	rBV	88803	136858	3.51%	0.883%
49	9.195	1328	1330	1335	rVB2	160	227	0.01%	0.001%
50	9.275	1339	1343	1347	rVB3	613	854	0.02%	0.006%
51	9.384	1356	1361	1386	rBV	326829	508907	13.05%	3.282%
52	9.762	1421	1423	1425	rVB	172	120	0.00%	0.001%
53	9.909	1445	1447	1451	rVB2	171	187	0.00%	0.001%
54	9.945	1451	1453	1455	rBV	118	122	0.00%	0.001%
55	10.079	1465	1475	1493	rBV2	2299604	3898333	100.00%	25.143%
56	10.305	1509	1512	1515	rBV3	762	952	0.02%	0.006%
57	10.457	1534	1537	1540	rBV2	227	273	0.01%	0.002%
58	10.537	1547	1550	1551	rBV2	147	123	0.00%	0.001%
59	10.604	1560	1561	1564	rBV	155	141	0.00%	0.001%
60	10.653	1565	1569	1572	rBV4	345	626	0.02%	0.004%
61	10.799	1589	1593	1596	rBV2	176	190	0.00%	0.001%
62	10.896	1608	1609	1612	rVB2	210	193	0.00%	0.001%
63	10.970	1616	1621	1626	rVV2	418	620	0.02%	0.004%
64	11.049	1631	1634	1636	rBV2	116	157	0.00%	0.001%
65	11.098	1636	1642	1646	rVB2	574	800	0.02%	0.005%
66	11.128	1646	1647	1652	rBV	111	125	0.00%	0.001%
67	11.189	1652	1657	1669	rBV	411214	526020	13.49%	3.393%
68	11.311	1674	1677	1682	rVB2	1391	2018	0.05%	0.013%
69	11.457	1697	1701	1704	rBV3	366	566	0.01%	0.004%
70	11.506	1707	1709	1711	rVB2	138	121	0.00%	0.001%
71	11.549	1711	1716	1717	rBV2	80	125	0.00%	0.001%
72	11.567	1717	1719	1720	rVB	179	118	0.00%	0.001%
73	11.591	1720	1723	1727	rBV2	218	281	0.01%	0.002%
74	11.671	1733	1736	1739	rVB2	134	135	0.00%	0.001%
75	11.707	1739	1742	1746	rVB2	214	309	0.01%	0.002%
76	11.756	1746	1750	1755	rVB3	485	747	0.02%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040994.D
 Acq On : 11 Apr 2024 22:48
 Operator : JC/MD
 Sample : P2048-04DL 400X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R51DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	11.799	1755	1757	1759	rBV	191	178	0.00%	0.001%
78	11.969	1781	1785	1789	rBV	17947	23948	0.61%	0.154%
79	12.024	1789	1794	1811	rVB2	708578	1497720	38.42%	9.660%
80	12.213	1822	1825	1829	rVB2	322	431	0.01%	0.003%
81	12.323	1837	1843	1858	rBV2	687108	1217359	31.23%	7.851%
82	12.512	1873	1874	1880	rBV2	328	387	0.01%	0.002%
83	12.567	1880	1883	1885	rBV2	183	198	0.01%	0.001%
84	12.658	1896	1898	1899	rBV	133	139	0.00%	0.001%
85	12.762	1911	1915	1920	rBV2	3101	4233	0.11%	0.027%
86	12.823	1923	1925	1929	rVB2	186	233	0.01%	0.002%
87	12.872	1931	1933	1934	rBV	193	138	0.00%	0.001%
88	13.048	1959	1962	1964	rBV	112	153	0.00%	0.001%
89	13.109	1968	1972	1980	rVB2	1981	2929	0.08%	0.019%
90	13.500	2034	2036	2039	rBV	164	249	0.01%	0.002%
91	13.591	2045	2051	2059	rBV3	7162	10709	0.27%	0.069%
92	13.664	2062	2063	2065	rVB	270	112	0.00%	0.001%
93	13.762	2077	2079	2080	rBV2	185	184	0.00%	0.001%
94	13.786	2080	2083	2089	rVB3	795	1162	0.03%	0.007%
95	13.926	2104	2106	2108	rBV2	145	170	0.00%	0.001%
96	13.963	2108	2112	2117	rVV4	970	1506	0.04%	0.010%
97	14.128	2135	2139	2147	rVB	3223	4465	0.11%	0.029%
98	15.390	2342	2346	2350	rVB3	1497	2304	0.06%	0.015%
99	16.139	2467	2469	2470	rBV2	536	345	0.01%	0.002%
100	16.377	2506	2508	2513	rVB2	591	603	0.02%	0.004%




Sum of corrected areas: 15504798

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040994.D
Acq On : 11 Apr 2024 22:48
Operator : JC/MD
Sample : P2048-04DL 400X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R51DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

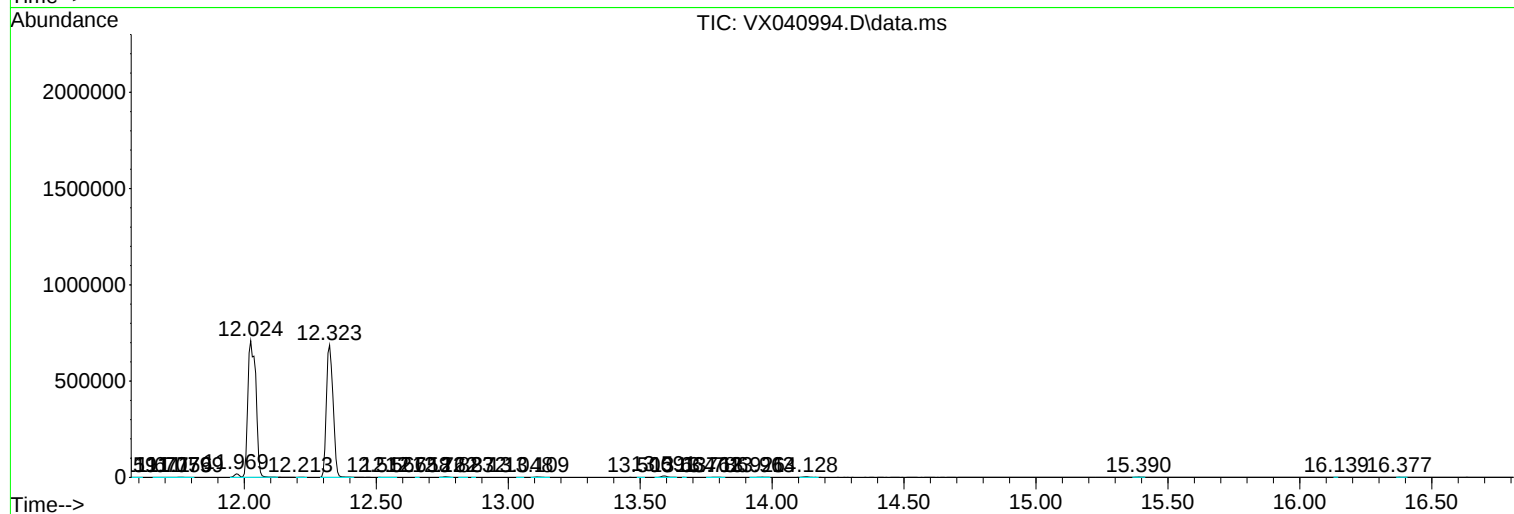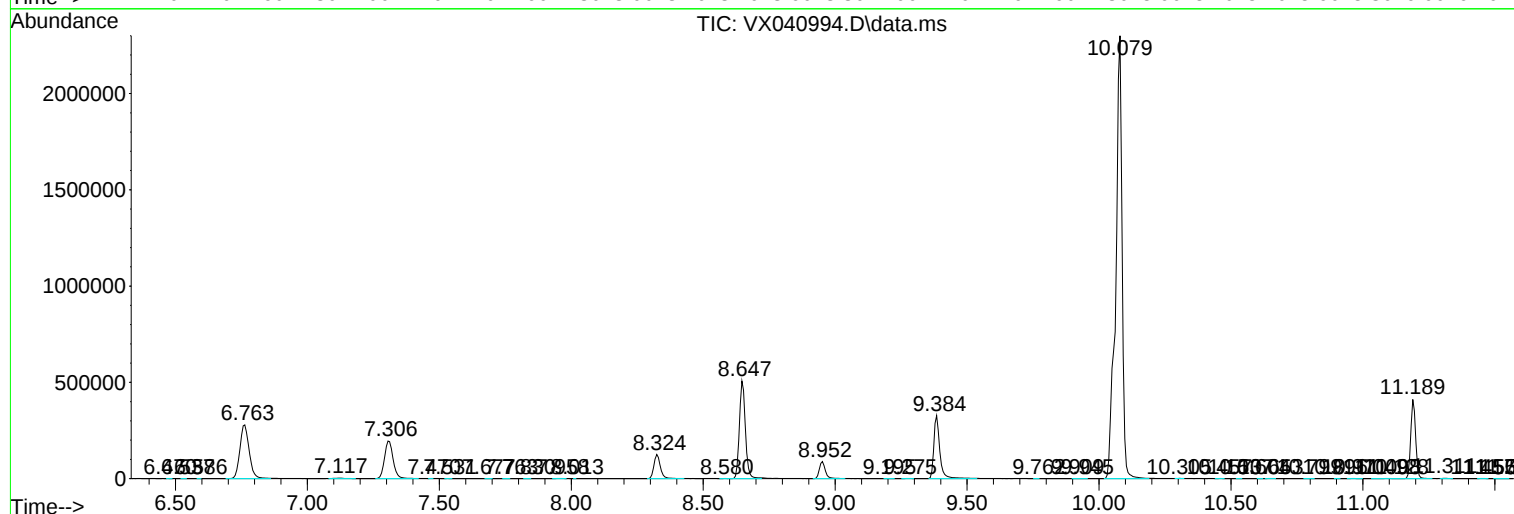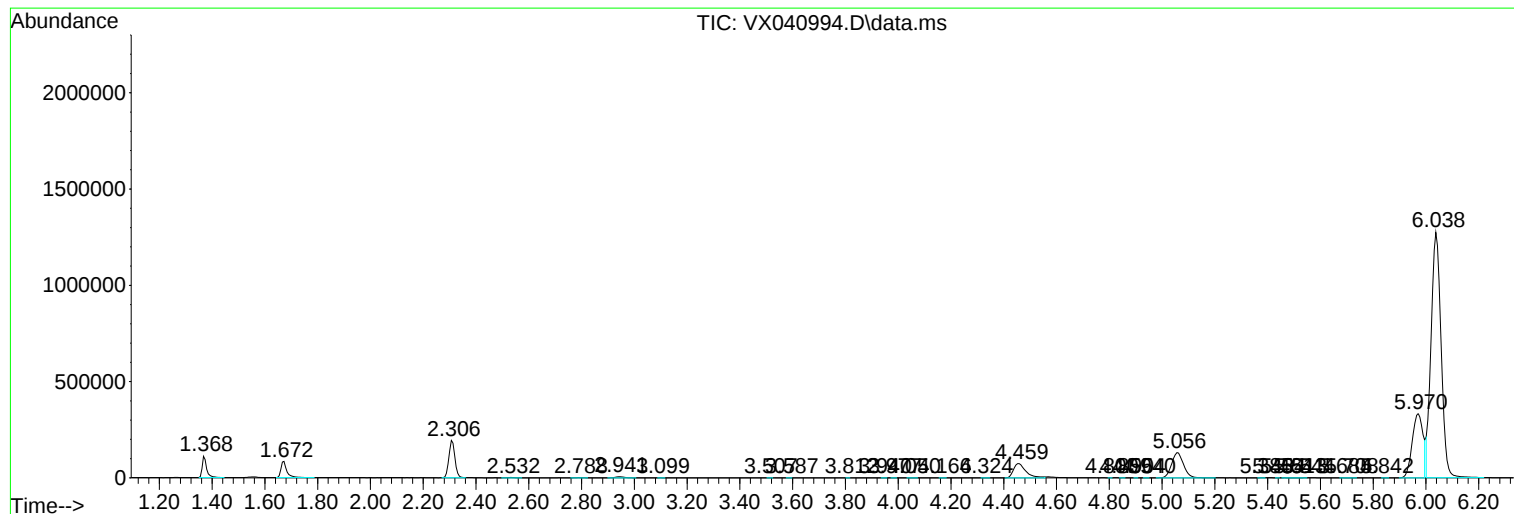

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040994.D
Acq On : 11 Apr 2024 22:48
Operator : JC/MD
Sample : P2048-04DL 400X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R51DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040994.D
Acq On : 11 Apr 2024 22:48
Operator : JC/MD
Sample : P2048-04DL 400X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R51DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
