

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040996.D
 Acq On : 11 Apr 2024 23:34
 Operator : JC/MD
 Sample : P2049-01 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0RB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M

Title : VOC Analysis

Signal : TIC: VX040996.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	63	rVB	116846	130099	12.53%	1.591%
2	1.666	91	95	112	rVB	84677	127962	12.33%	1.565%
3	2.306	194	200	208	rBV	201592	313576	30.21%	3.834%
4	2.459	224	225	230	rVB3	362	457	0.04%	0.006%
5	2.508	230	233	234	rBV2	516	481	0.05%	0.006%
6	2.672	258	260	262	rBV	146	170	0.02%	0.002%
7	2.697	262	264	271	rVB4	279	454	0.04%	0.006%
8	2.751	271	273	275	rBV2	105	115	0.01%	0.001%
9	2.794	275	280	285	rVV3	1059	2023	0.19%	0.025%
10	2.855	288	290	293	rVB2	120	103	0.01%	0.001%
11	2.947	298	305	313	rBV	4264	9708	0.94%	0.119%
12	3.099	326	330	332	rVV2	181	260	0.03%	0.003%
13	3.434	382	385	387	rBV2	119	134	0.01%	0.002%
14	3.556	403	405	407	rBV	170	124	0.01%	0.002%
15	3.861	454	455	457	rVB	160	95	0.01%	0.001%
16	3.934	465	467	469	rBV	115	122	0.01%	0.001%
17	4.038	483	484	487	rBV	180	149	0.01%	0.002%
18	4.068	487	489	492	rVB2	145	141	0.01%	0.002%
19	4.239	515	517	520	rBV	136	112	0.01%	0.001%
20	4.367	534	538	540	rBV2	127	157	0.02%	0.002%
21	4.452	544	552	581	rBV	80353	256805	24.74%	3.140%
22	4.788	606	607	608	rBV	240	98	0.01%	0.001%
23	4.910	624	627	629	rBV	172	266	0.03%	0.003%
24	5.056	639	651	673	rBV2	134160	420668	40.53%	5.143%
25	5.403	702	708	711	rVB4	287	701	0.07%	0.009%
26	5.501	723	724	727	rVB2	101	98	0.01%	0.001%
27	5.550	729	732	733	rBV2	355	421	0.04%	0.005%
28	5.678	752	753	755	rVB	213	101	0.01%	0.001%
29	5.842	778	780	783	rVB2	168	133	0.01%	0.002%
30	5.873	783	785	787	rBV2	102	99	0.01%	0.001%
31	5.970	789	801	829	rBV2	343202	1037921	100.00%	12.691%
32	6.245	844	846	848	rVB	210	142	0.01%	0.002%
33	6.336	859	861	863	rBV	144	102	0.01%	0.001%
34	6.397	868	871	872	rBV2	128	120	0.01%	0.001%
35	6.415	872	874	877	rBV2	123	121	0.01%	0.001%
36	6.550	893	896	900	rBV3	160	278	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040996.D
 Acq On : 11 Apr 2024 23:34
 Operator : JC/MD
 Sample : P2049-01 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0RB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	6.763	922	931	948	rBV	280392	681744	65.68%	8.336%
38	7.043	975	977	978	rBV	183	101	0.01%	0.001%
39	7.117	983	989	998	rVB5	1892	5020	0.48%	0.061%
40	7.238	1008	1009	1012	rBV2	105	96	0.01%	0.001%
41	7.306	1012	1020	1039	rBV	207702	462460	44.56%	5.654%
42	7.659	1076	1078	1081	rVB	156	129	0.01%	0.002%
43	7.690	1081	1083	1084	rBV	121	95	0.01%	0.001%
44	7.763	1094	1095	1098	rBV	175	163	0.02%	0.002%
45	7.946	1120	1125	1127	rBV2	641	953	0.09%	0.012%
46	8.135	1155	1156	1158	rBV	151	122	0.01%	0.001%
47	8.190	1163	1165	1167	rVV2	120	129	0.01%	0.002%
48	8.324	1181	1187	1203	rVV	132071	217223	20.93%	2.656%
49	8.580	1225	1229	1231	rBV3	395	528	0.05%	0.006%
50	8.647	1234	1240	1253	rBV	521149	818322	78.84%	10.006%
51	8.952	1284	1290	1304	rBV	90810	141279	13.61%	1.727%
52	9.195	1329	1330	1333	rBV2	157	109	0.01%	0.001%
53	9.275	1336	1343	1348	rBV	6053	9473	0.91%	0.116%
54	9.384	1356	1361	1385	rBV	342551	525297	50.61%	6.423%
55	9.695	1410	1412	1413	rBV2	524	500	0.05%	0.006%
56	9.836	1433	1435	1436	rBV	144	99	0.01%	0.001%
57	9.909	1444	1447	1450	rBV	259	351	0.03%	0.004%
58	9.951	1453	1454	1456	rBV	208	123	0.01%	0.002%
59	9.988	1458	1460	1461	rVB	209	134	0.01%	0.002%
60	10.055	1465	1471	1489	rBV	571925	836010	80.55%	10.222%
61	10.396	1526	1527	1531	rVB	118	95	0.01%	0.001%
62	10.482	1539	1541	1544	rVB2	236	213	0.02%	0.003%
63	10.598	1558	1560	1561	rVB	167	96	0.01%	0.001%
64	10.646	1564	1568	1569	rVV3	303	321	0.03%	0.004%
65	10.677	1569	1573	1579	rVB3	252	541	0.05%	0.007%
66	10.963	1617	1620	1624	rVB3	440	600	0.06%	0.007%
67	10.994	1624	1625	1626	rBV	167	95	0.01%	0.001%
68	11.085	1639	1640	1645	rBV3	373	524	0.05%	0.006%
69	11.189	1652	1657	1666	rBV	409683	538376	51.87%	6.583%
70	11.311	1672	1677	1682	rVB	10819	15196	1.46%	0.186%
71	11.372	1686	1687	1690	rVB	266	149	0.01%	0.002%
72	11.451	1697	1700	1705	rBV4	428	767	0.07%	0.009%
73	11.537	1711	1714	1717	rVB2	163	157	0.02%	0.002%
74	11.567	1717	1719	1720	rBV	180	105	0.01%	0.001%
75	11.707	1740	1742	1744	rBV	474	354	0.03%	0.004%
76	11.756	1748	1750	1754	rVV2	404	481	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040996.D
 Acq On : 11 Apr 2024 23:34
 Operator : JC/MD
 Sample : P2049-01 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0RB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	11.969	1781	1785	1788	rBV	1250	1506	0.15%	0.018%
78	12.018	1788	1793	1811	rVV	617880	810479	78.09%	9.910%
79	12.317	1837	1842	1856	rBV	611903	782282	75.37%	9.565%
80	12.762	1911	1915	1923	rVV2	5426	7127	0.69%	0.087%
81	13.055	1961	1963	1964	rVV2	146	102	0.01%	0.001%
82	13.122	1970	1974	1977	rBV2	348	519	0.05%	0.006%
83	13.493	2034	2035	2037	rVB	191	99	0.01%	0.001%
84	13.518	2037	2039	2040	rBV	174	117	0.01%	0.001%
85	13.567	2045	2047	2048	rBV	123	103	0.01%	0.001%
86	13.597	2048	2052	2058	rVV3	1151	1748	0.17%	0.021%
87	13.695	2066	2068	2069	rVV	190	106	0.01%	0.001%
88	13.719	2071	2072	2077	rVB2	349	311	0.03%	0.004%
89	13.786	2080	2083	2088	rBV3	511	986	0.09%	0.012%
90	13.932	2105	2107	2110	rBV2	161	135	0.01%	0.002%
91	13.975	2110	2114	2116	rBV3	425	656	0.06%	0.008%
92	14.030	2121	2123	2124	rVV	216	144	0.01%	0.002%
93	14.060	2127	2128	2130	rBV	291	209	0.02%	0.003%
94	14.128	2135	2139	2144	rBV	3829	5559	0.54%	0.068%
95	14.262	2159	2161	2162	rBV	249	132	0.01%	0.002%
96	14.304	2166	2168	2171	rBV	176	199	0.02%	0.002%
97	14.347	2174	2175	2178	rVV3	173	142	0.01%	0.002%
98	14.396	2182	2183	2186	rVB	257	159	0.02%	0.002%
99	14.762	2241	2243	2246	rBV3	371	544	0.05%	0.007%
100	15.389	2343	2346	2351	rVB5	1501	2246	0.22%	0.027%




Sum of corrected areas: 8178656

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040996.D
Acq On : 11 Apr 2024 23:34
Operator : JC/MD
Sample : P2049-01 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

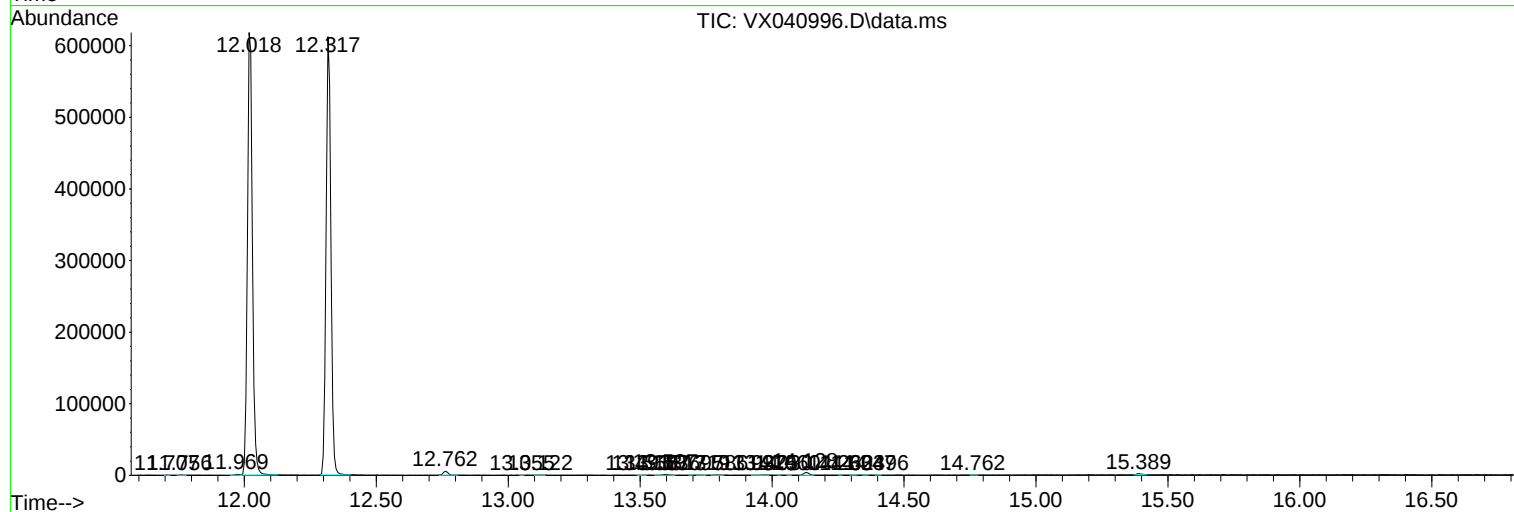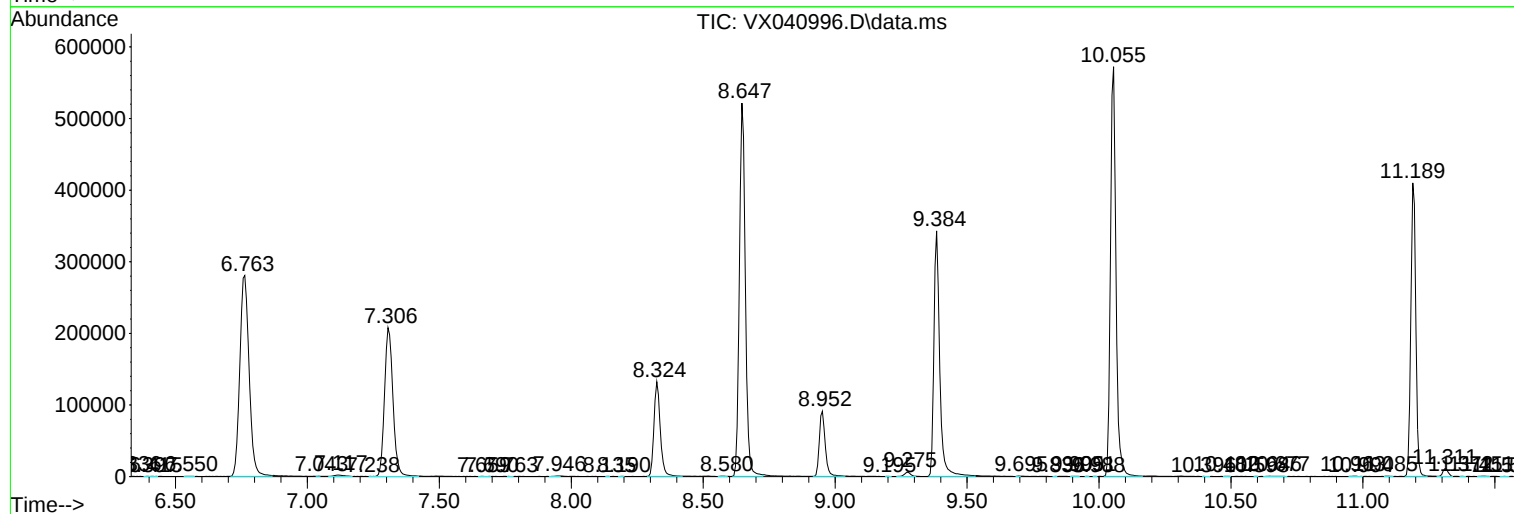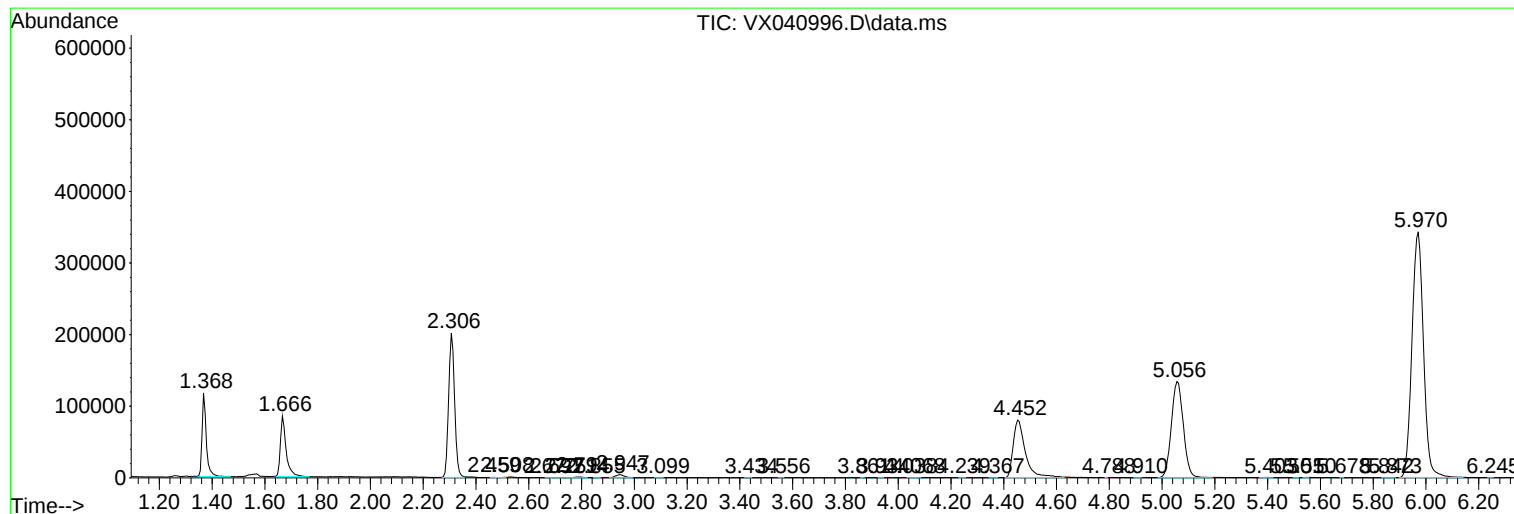

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040996.D
Acq On : 11 Apr 2024 23:34
Operator : JC/MD
Sample : P2049-01 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040996.D
Acq On : 11 Apr 2024 23:34
Operator : JC/MD
Sample : P2049-01 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc