

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040997.D
 Acq On : 11 Apr 2024 23:57
 Operator : JC/MD
 Sample : P2049-02 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0RB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX040997.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	60	rBV	115962	131146	12.72%	1.585%
2	1.666	91	95	114	rVB	89062	134925	13.09%	1.630%
3	2.306	194	200	211	rBV	204794	317155	30.76%	3.833%
4	2.434	219	221	222	rVB	278	148	0.01%	0.002%
5	2.507	230	233	234	rBV	621	530	0.05%	0.006%
6	2.642	254	255	257	rBV2	228	197	0.02%	0.002%
7	2.684	260	262	263	rVV2	237	161	0.02%	0.002%
8	2.715	263	267	271	rVV3	289	431	0.04%	0.005%
9	2.745	271	272	274	rVB	163	113	0.01%	0.001%
10	2.788	274	279	289	rBV4	1007	2154	0.21%	0.026%
11	2.940	297	304	315	rVB2	4001	9206	0.89%	0.111%
12	3.117	326	333	339	rBV3	2215	4895	0.47%	0.059%
13	3.196	345	346	350	rVB	122	106	0.01%	0.001%
14	3.239	352	353	355	rVV2	163	97	0.01%	0.001%
15	3.294	359	362	365	rVB2	132	175	0.02%	0.002%
16	3.318	365	366	370	rBV2	124	147	0.01%	0.002%
17	3.477	390	392	394	rVV	158	177	0.02%	0.002%
18	3.605	410	413	414	rBV2	208	211	0.02%	0.003%
19	3.660	418	422	426	rBB2	110	216	0.02%	0.003%
20	3.800	442	445	448	rBB2	124	139	0.01%	0.002%
21	3.873	453	457	458	rBV	119	178	0.02%	0.002%
22	3.989	473	476	481	rBV2	226	351	0.03%	0.004%
23	4.312	526	529	530	rBV	173	172	0.02%	0.002%
24	4.452	544	552	568	rBV	83126	254576	24.69%	3.076%
25	5.056	635	651	666	rBV	133903	413675	40.12%	4.999%
26	5.281	686	688	693	rVB3	238	292	0.03%	0.004%
27	5.476	718	720	722	rVV	138	103	0.01%	0.001%
28	5.501	722	724	726	rVB	211	193	0.02%	0.002%
29	5.531	726	729	730	rBV	192	211	0.02%	0.003%
30	5.678	750	753	757	rBV2	208	294	0.03%	0.004%
31	5.745	763	764	767	rBV2	193	157	0.02%	0.002%
32	5.970	789	801	831	rBV2	339719	1031062	100.00%	12.459%
33	6.251	845	847	848	rVB	264	114	0.01%	0.001%
34	6.312	854	857	859	rBV3	292	377	0.04%	0.005%
35	6.409	870	873	874	rVV2	176	140	0.01%	0.002%
36	6.427	874	876	879	rVB	217	215	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040997.D
 Acq On : 11 Apr 2024 23:57
 Operator : JC/MD
 Sample : P2049-02 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0RB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	6.525	889	892	893	rBV2	148	181	0.02%	0.002%
38	6.763	921	931	947	rBV	282891	686458	66.58%	8.295%
39	7.110	982	988	990	rBV5	1591	2527	0.25%	0.031%
40	7.202	1001	1003	1006	rVB	196	165	0.02%	0.002%
41	7.305	1009	1020	1033	rBV	207475	456841	44.31%	5.520%
42	7.946	1120	1125	1127	rBV4	644	949	0.09%	0.011%
43	8.080	1145	1147	1150	rBV2	109	153	0.01%	0.002%
44	8.134	1154	1156	1157	rBV	181	121	0.01%	0.001%
45	8.202	1166	1167	1170	rVB2	129	119	0.01%	0.001%
46	8.244	1170	1174	1175	rBV	121	153	0.01%	0.002%
47	8.323	1181	1187	1208	rVV	130243	218813	21.22%	2.644%
48	8.580	1227	1229	1232	rVB	394	330	0.03%	0.004%
49	8.647	1234	1240	1258	rBV	524519	830651	80.56%	10.038%
50	8.951	1284	1290	1299	rBV	94251	143274	13.90%	1.731%
51	9.159	1322	1324	1326	rBV	186	147	0.01%	0.002%
52	9.275	1338	1343	1348	rBV2	1816	2965	0.29%	0.036%
53	9.384	1356	1361	1386	rBV	351427	541873	52.55%	6.548%
54	9.567	1389	1391	1394	rVB3	375	233	0.02%	0.003%
55	9.793	1427	1428	1431	rBV	152	106	0.01%	0.001%
56	9.817	1431	1432	1434	rBV	254	159	0.02%	0.002%
57	10.055	1465	1471	1490	rBV	604024	852409	82.67%	10.301%
58	10.317	1509	1514	1518	rVB4	703	1102	0.11%	0.013%
59	10.433	1532	1533	1537	rBV2	290	203	0.02%	0.002%
60	10.646	1563	1568	1571	rBV2	483	687	0.07%	0.008%
61	10.719	1576	1580	1582	rBV	276	356	0.03%	0.004%
62	10.902	1607	1610	1614	rBV2	96	148	0.01%	0.002%
63	10.963	1618	1620	1627	rVB2	441	674	0.07%	0.008%
64	11.018	1627	1629	1631	rVB2	158	121	0.01%	0.001%
65	11.091	1639	1641	1647	rVB2	452	600	0.06%	0.007%
66	11.189	1652	1657	1671	rVV	440986	559032	54.22%	6.755%
67	11.311	1673	1677	1682	rVB	3663	5491	0.53%	0.066%
68	11.366	1684	1686	1688	rBV	155	101	0.01%	0.001%
69	11.457	1698	1701	1704	rVV2	437	599	0.06%	0.007%
70	11.536	1712	1714	1716	rVB	134	98	0.01%	0.001%
71	11.573	1716	1720	1721	rBV2	147	192	0.02%	0.002%
72	11.585	1721	1722	1727	rVV2	165	148	0.01%	0.002%
73	11.707	1740	1742	1744	rBV2	321	281	0.03%	0.003%
74	11.756	1747	1750	1753	rBV3	418	648	0.06%	0.008%
75	11.975	1782	1786	1788	rBV2	1047	1297	0.13%	0.016%
76	12.024	1788	1794	1804	rVV	620639	832612	80.75%	10.061%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040997.D
 Acq On : 11 Apr 2024 23:57
 Operator : JC/MD
 Sample : P2049-02 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0RB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	12.317	1837	1842	1862	rVB	628838	805547	78.13%	9.734%
78	12.731	1909	1910	1911	rBV	204	101	0.01%	0.001%
79	12.768	1911	1916	1919	rVV2	4039	5425	0.53%	0.066%
80	12.908	1938	1939	1941	rVB	205	134	0.01%	0.002%
81	12.939	1941	1944	1945	rBV	156	143	0.01%	0.002%
82	13.030	1956	1959	1960	rBV	186	159	0.02%	0.002%
83	13.115	1970	1973	1977	rBV	461	537	0.05%	0.006%
84	13.207	1986	1988	1990	rBV	91	102	0.01%	0.001%
85	13.310	2003	2005	2008	rBV2	139	141	0.01%	0.002%
86	13.341	2008	2010	2012	rBV	200	127	0.01%	0.002%
87	13.597	2049	2052	2057	rVB4	664	1089	0.11%	0.013%
88	13.688	2066	2067	2069	rBV	167	108	0.01%	0.001%
89	13.792	2077	2084	2088	rBV3	520	979	0.09%	0.012%
90	13.902	2100	2102	2104	rVB	169	129	0.01%	0.002%
91	13.963	2110	2112	2117	rBV4	455	622	0.06%	0.008%
92	14.036	2122	2124	2126	rVB2	210	154	0.01%	0.002%
93	14.054	2126	2127	2130	rBV2	191	217	0.02%	0.003%
94	14.127	2135	2139	2145	rVB	4868	6873	0.67%	0.083%
95	14.316	2168	2170	2171	rBV2	184	128	0.01%	0.002%
96	14.341	2171	2174	2180	rVV3	273	410	0.04%	0.005%
97	14.432	2186	2189	2191	rBV3	190	278	0.03%	0.003%
98	14.481	2196	2197	2200	rBV2	294	250	0.02%	0.003%
99	15.389	2342	2346	2351	rVB2	2591	4044	0.39%	0.049%
100	16.182	2475	2476	2477	rBV	426	205	0.02%	0.002%



Sum of corrected areas: 8275358

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040997.D
Acq On : 11 Apr 2024 23:57
Operator : JC/MD
Sample : P2049-02 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RB5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

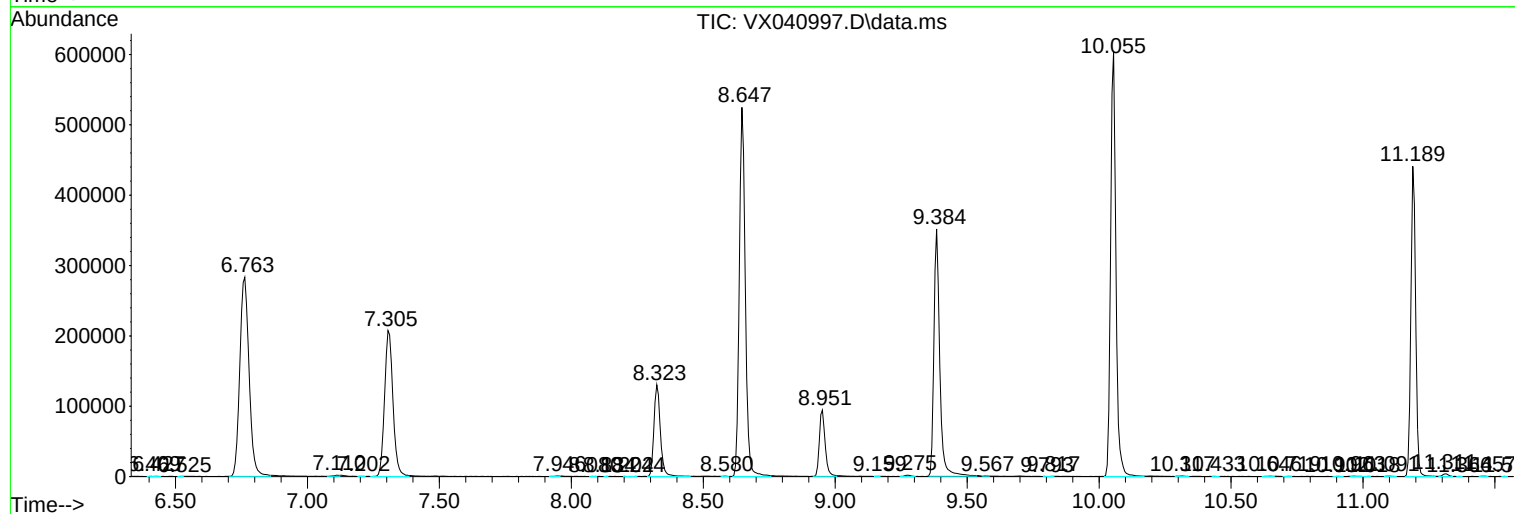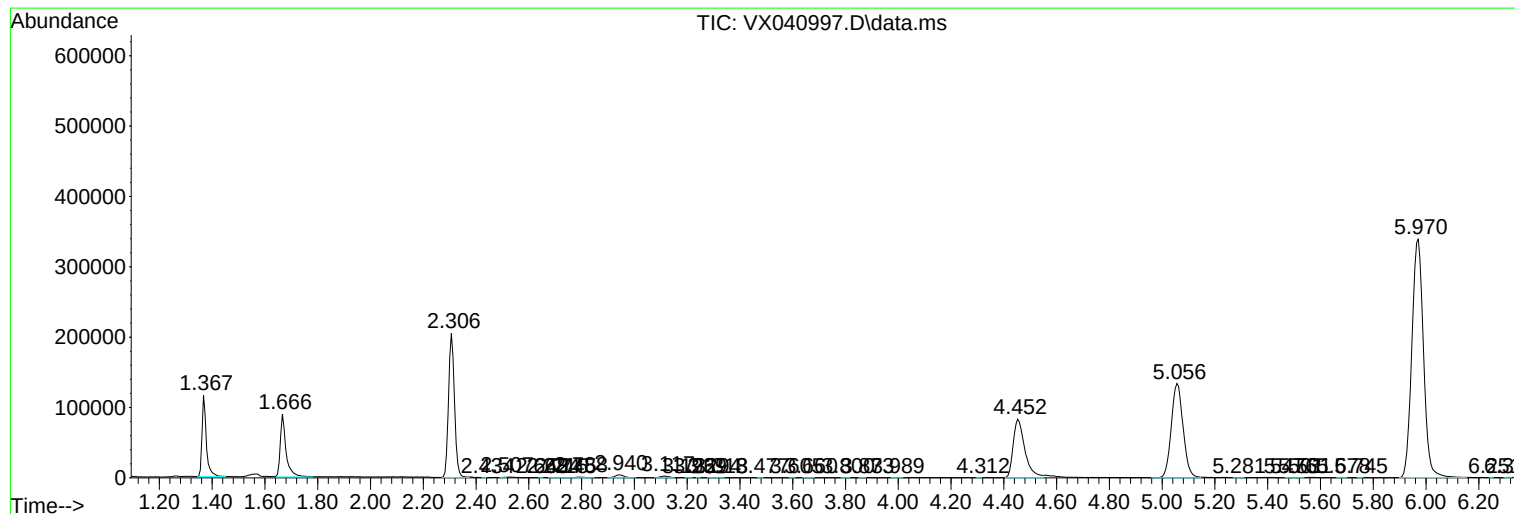

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040997.D
Acq On : 11 Apr 2024 23:57
Operator : JC/MD
Sample : P2049-02 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RB5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040997.D
Acq On : 11 Apr 2024 23:57
Operator : JC/MD
Sample : P2049-02 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RB5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc