

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040999.D
 Acq On : 12 Apr 2024 00:43
 Operator : JC/MD
 Sample : P2049-04 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0RC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX040999.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	61	rVB	102482	120092	8.63%	1.385%
2	1.666	91	95	107	rBV	78507	119672	8.60%	1.380%
3	2.306	194	200	211	rBV	183858	288256	20.71%	3.324%
4	2.623	250	252	255	rVB2	160	126	0.01%	0.001%
5	2.708	262	266	269	rBV	336	361	0.03%	0.004%
6	2.794	275	280	286	rBV4	935	1755	0.13%	0.020%
7	2.940	298	304	314	rVB2	4337	9896	0.71%	0.114%
8	3.013	314	316	319	rBV	158	120	0.01%	0.001%
9	3.068	323	325	326	rBV2	125	116	0.01%	0.001%
10	3.099	328	330	332	rBV2	203	172	0.01%	0.002%
11	3.452	387	388	391	rVB2	157	106	0.01%	0.001%
12	3.617	411	415	418	rBV2	163	259	0.02%	0.003%
13	3.806	443	446	447	rVB2	136	113	0.01%	0.001%
14	3.867	453	456	459	rBV2	136	200	0.01%	0.002%
15	3.916	462	464	467	rVB2	133	149	0.01%	0.002%
16	4.141	499	501	502	rBV	145	121	0.01%	0.001%
17	4.178	506	507	510	rVV	161	123	0.01%	0.001%
18	4.342	532	534	535	rBV2	149	115	0.01%	0.001%
19	4.458	544	553	568	rBV	74833	233040	16.74%	2.687%
20	4.793	607	608	609	rVB	297	109	0.01%	0.001%
21	5.056	639	651	669	rBV	125680	386801	27.79%	4.460%
22	5.287	687	689	690	rBV	208	139	0.01%	0.002%
23	5.379	701	704	705	rBV2	330	315	0.02%	0.004%
24	5.549	730	732	733	rBV	274	187	0.01%	0.002%
25	5.732	759	762	763	rBV2	235	238	0.02%	0.003%
26	5.970	789	801	821	rBV2	313899	948804	68.16%	10.940%
27	6.318	854	858	862	rBV	196	271	0.02%	0.003%
28	6.641	909	911	915	rBV2	131	233	0.02%	0.003%
29	6.763	921	931	947	rBV	260104	630422	45.29%	7.269%
30	7.116	983	989	1000	rBV4	1921	4848	0.35%	0.056%
31	7.226	1005	1007	1009	rVB2	194	168	0.01%	0.002%
32	7.305	1011	1020	1041	rBV	189994	424783	30.52%	4.898%
33	7.537	1056	1058	1061	rBB	121	101	0.01%	0.001%
34	7.610	1068	1070	1072	rBV2	154	116	0.01%	0.001%
35	7.793	1098	1100	1104	rVB2	153	194	0.01%	0.002%
36	7.836	1104	1107	1108	rBV2	150	163	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040999.D
 Acq On : 12 Apr 2024 00:43
 Operator : JC/MD
 Sample : P2049-04 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0RC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	7.897	1114	1117	1118	rBV2	132	110	0.01%	0.001%
38	7.951	1122	1126	1131	rBV3	536	1007	0.07%	0.012%
39	8.067	1144	1145	1146	rBV	184	100	0.01%	0.001%
40	8.146	1153	1158	1161	rBV2	132	266	0.02%	0.003%
41	8.183	1161	1164	1166	rBV2	174	161	0.01%	0.002%
42	8.323	1181	1187	1202	rBV	120936	201792	14.50%	2.327%
43	8.506	1214	1217	1224	rBV4	558	1030	0.07%	0.012%
44	8.573	1227	1228	1234	rBV3	321	283	0.02%	0.003%
45	8.646	1234	1240	1258	rBV	482860	768371	55.20%	8.860%
46	8.951	1284	1290	1300	rBV	85292	130263	9.36%	1.502%
47	9.091	1311	1313	1315	rBV3	176	189	0.01%	0.002%
48	9.213	1331	1333	1337	rBV3	141	170	0.01%	0.002%
49	9.274	1339	1343	1347	rVB2	771	1178	0.08%	0.014%
50	9.335	1351	1353	1355	rBV2	173	133	0.01%	0.002%
51	9.384	1356	1361	1382	rBV	328937	499458	35.88%	5.759%
52	9.610	1396	1398	1399	rVB2	408	208	0.01%	0.002%
53	9.628	1399	1401	1405	rVB3	373	408	0.03%	0.005%
54	9.671	1405	1408	1409	rBV2	201	183	0.01%	0.002%
55	9.701	1411	1413	1419	rVB4	724	960	0.07%	0.011%
56	9.854	1437	1438	1441	rVB	177	123	0.01%	0.001%
57	9.914	1444	1448	1451	rBV2	145	258	0.02%	0.003%
58	10.055	1465	1471	1492	rBV2	559216	992952	71.33%	11.449%
59	10.305	1510	1512	1519	rVB3	618	799	0.06%	0.009%
60	10.378	1522	1524	1526	rVB	261	226	0.02%	0.003%
61	10.439	1532	1534	1537	rBV	172	189	0.01%	0.002%
62	10.616	1561	1563	1566	rBV2	92	113	0.01%	0.001%
63	10.652	1566	1569	1570	rBV2	431	411	0.03%	0.005%
64	10.719	1579	1580	1582	rBV	141	104	0.01%	0.001%
65	10.805	1591	1594	1596	rBV2	156	153	0.01%	0.002%
66	10.847	1599	1601	1602	rBV	204	117	0.01%	0.001%
67	10.866	1602	1604	1606	rBV2	124	119	0.01%	0.001%
68	11.036	1628	1632	1633	rBV2	113	153	0.01%	0.002%
69	11.097	1639	1642	1647	rBV2	718	814	0.06%	0.009%
70	11.189	1652	1657	1673	rVV	389564	517470	37.18%	5.967%
71	11.317	1673	1678	1681	rVB	1700	2495	0.18%	0.029%
72	11.457	1697	1701	1705	rBV3	451	736	0.05%	0.008%
73	11.628	1727	1729	1730	rVV2	126	133	0.01%	0.002%
74	11.670	1734	1736	1738	rVB	160	121	0.01%	0.001%
75	11.701	1738	1741	1746	rBV2	226	465	0.03%	0.005%
76	11.756	1747	1750	1754	rVB2	476	622	0.04%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040999.D
 Acq On : 12 Apr 2024 00:43
 Operator : JC/MD
 Sample : P2049-04 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0RC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	11.810	1756	1759	1763	rBV2	125	175	0.01%	0.002%
78	11.908	1772	1775	1777	rBV2	88	105	0.01%	0.001%
79	11.969	1781	1785	1789	rVV	12783	16543	1.19%	0.191%
80	12.018	1789	1793	1811	rVB	615973	855393	61.45%	9.863%
81	12.256	1831	1832	1835	rBV3	160	206	0.01%	0.002%
82	12.323	1837	1843	1853	rBV2	754818	1391969	100.00%	16.050%
83	12.554	1879	1881	1884	rVB2	283	255	0.02%	0.003%
84	12.682	1900	1902	1904	rBV	119	115	0.01%	0.001%
85	12.762	1911	1915	1920	rVB2	3407	4906	0.35%	0.057%
86	12.932	1941	1943	1947	rBV	253	238	0.02%	0.003%
87	13.005	1953	1955	1957	rBV	140	102	0.01%	0.001%
88	13.054	1961	1963	1964	rBV2	162	114	0.01%	0.001%
89	13.115	1970	1973	1978	rBV2	284	423	0.03%	0.005%
90	13.188	1983	1985	1986	rVB	216	110	0.01%	0.001%
91	13.255	1995	1996	2001	rBV2	160	176	0.01%	0.002%
92	13.438	2022	2026	2028	rBV2	140	164	0.01%	0.002%
93	13.487	2031	2034	2037	rBV2	148	193	0.01%	0.002%
94	13.591	2045	2051	2068	rVB	59208	80664	5.79%	0.930%
95	13.786	2080	2083	2088	rVV3	409	682	0.05%	0.008%
96	13.895	2100	2101	2104	rVB2	173	107	0.01%	0.001%
97	13.963	2104	2112	2119	rBV	10584	13715	0.99%	0.158%
98	14.042	2122	2125	2129	rBV2	195	308	0.02%	0.004%
99	14.127	2134	2139	2143	rBV	3966	5286	0.38%	0.061%
100	15.389	2343	2346	2353	rVB3	2026	3224	0.23%	0.037%




Sum of corrected areas: 8672700

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040999.D
Acq On : 12 Apr 2024 00:43
Operator : JC/MD
Sample : P2049-04 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

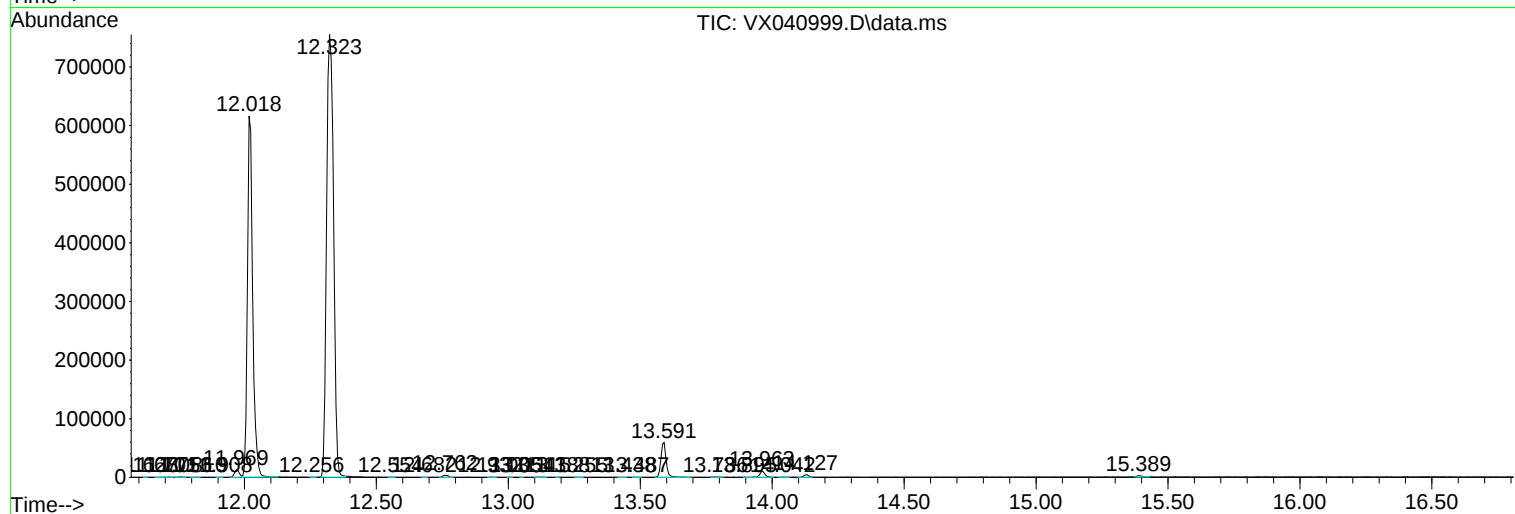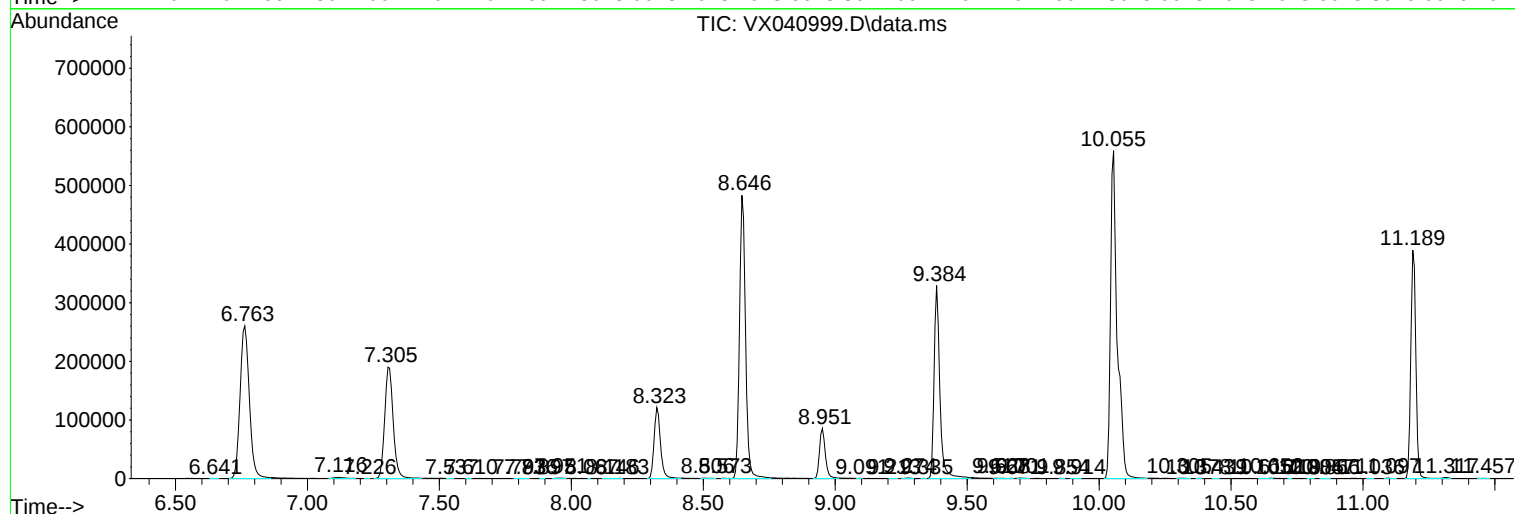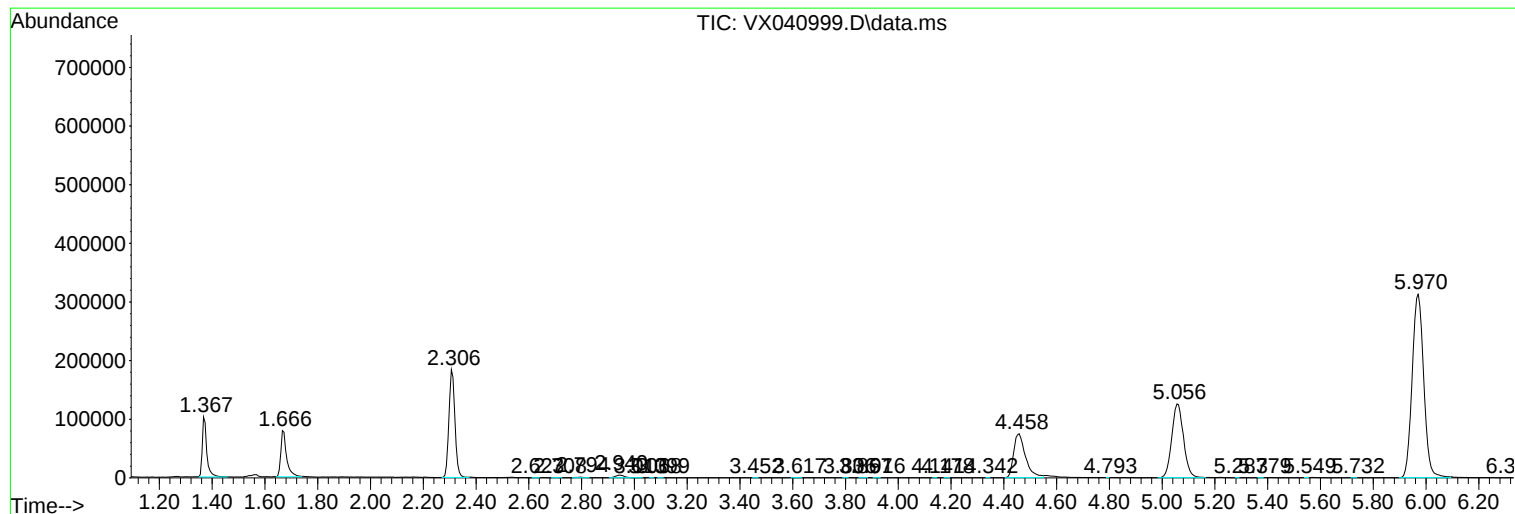

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040999.D
Acq On : 12 Apr 2024 00:43
Operator : JC/MD
Sample : P2049-04 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040999.D
Acq On : 12 Apr 2024 00:43
Operator : JC/MD
Sample : P2049-04 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc