

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX041000.D
 Acq On : 12 Apr 2024 01:06
 Operator : JC/MD
 Sample : P2049-05 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0RC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M

Title : VOC Analysis

Signal : TIC: VX041000.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	59	rVB	108182	119690	12.48%	1.508%
2	1.666	91	95	113	rVB	80428	122253	12.75%	1.540%
3	2.306	194	200	209	rBV	188844	293219	30.58%	3.693%
4	2.532	230	237	245	rVB4	886	2054	0.21%	0.026%
5	2.703	263	265	266	rVV2	231	153	0.02%	0.002%
6	2.721	266	268	272	rVB3	290	276	0.03%	0.003%
7	2.788	274	279	284	rVV3	848	1632	0.17%	0.021%
8	2.849	287	289	293	rVB2	141	109	0.01%	0.001%
9	2.947	298	305	315	rVB2	4290	9744	1.02%	0.123%
10	3.154	337	339	340	rBV	176	104	0.01%	0.001%
11	3.166	340	341	345	rVB2	284	295	0.03%	0.004%
12	3.197	345	346	348	rBV2	181	143	0.01%	0.002%
13	3.270	355	358	360	rBV	166	174	0.02%	0.002%
14	3.331	366	368	371	rVV2	141	158	0.02%	0.002%
15	3.440	385	386	388	rVV2	135	103	0.01%	0.001%
16	3.562	403	406	409	rVB2	102	109	0.01%	0.001%
17	3.623	414	416	418	rBV2	119	112	0.01%	0.001%
18	3.654	418	421	422	rBV2	101	118	0.01%	0.001%
19	3.715	428	431	434	rVB2	134	131	0.01%	0.002%
20	3.763	434	439	440	rBV2	205	251	0.03%	0.003%
21	3.800	443	445	448	rVV2	144	123	0.01%	0.002%
22	3.928	464	466	469	rBV2	113	109	0.01%	0.001%
23	4.050	485	486	487	rBV	151	99	0.01%	0.001%
24	4.093	491	493	494	rBV2	207	162	0.02%	0.002%
25	4.233	514	516	518	rBV	175	115	0.01%	0.001%
26	4.276	521	523	526	rVV2	133	148	0.02%	0.002%
27	4.361	533	537	538	rBV2	153	190	0.02%	0.002%
28	4.452	544	552	567	rBV	77649	231652	24.16%	2.918%
29	4.788	605	607	608	rBV2	211	105	0.01%	0.001%
30	4.855	616	618	622	rBV	171	152	0.02%	0.002%
31	4.910	626	627	630	rBV2	195	198	0.02%	0.002%
32	5.056	639	651	668	rBV	126957	388304	40.49%	4.891%
33	5.458	716	717	720	rBV	163	194	0.02%	0.002%
34	5.556	729	733	738	rBV2	325	627	0.07%	0.008%
35	5.775	767	769	770	rBV	126	103	0.01%	0.001%
36	5.970	785	801	823	rBV2	318269	958956	100.00%	12.079%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX041000.D
 Acq On : 12 Apr 2024 01:06
 Operator : JC/MD
 Sample : P2049-05 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0RC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	6.330	858	860	863	rBV2	110	122	0.01%	0.002%
38	6.556	894	897	901	rVB2	246	380	0.04%	0.005%
39	6.592	901	903	905	rBV2	138	119	0.01%	0.001%
40	6.641	909	911	912	rBV2	105	99	0.01%	0.001%
41	6.763	920	931	950	rBV	259176	623890	65.06%	7.858%
42	7.117	983	989	996	rVB4	1977	4947	0.52%	0.062%
43	7.306	1011	1020	1038	rBV	193752	428028	44.63%	5.391%
44	7.476	1046	1048	1049	rBV2	278	251	0.03%	0.003%
45	7.659	1076	1078	1079	rBV	112	111	0.01%	0.001%
46	7.879	1112	1114	1117	rVB2	150	149	0.02%	0.002%
47	7.946	1122	1125	1132	rBV2	584	1182	0.12%	0.015%
48	8.055	1140	1143	1146	rBV2	161	238	0.02%	0.003%
49	8.177	1161	1163	1165	rBV2	191	181	0.02%	0.002%
50	8.324	1181	1187	1201	rBV	121930	202914	21.16%	2.556%
51	8.647	1234	1240	1265	rBV	484715	771878	80.49%	9.722%
52	8.952	1284	1290	1307	rVV	87059	132784	13.85%	1.673%
53	9.275	1337	1343	1347	rBV4	827	1158	0.12%	0.015%
54	9.384	1356	1361	1391	rVV	320022	498976	52.03%	6.285%
55	9.695	1410	1412	1420	rVB3	774	1365	0.14%	0.017%
56	9.756	1420	1422	1423	rVB	228	166	0.02%	0.002%
57	9.775	1423	1425	1427	rBV	259	233	0.02%	0.003%
58	9.848	1434	1437	1439	rVB2	234	263	0.03%	0.003%
59	10.000	1461	1462	1465	rBV	230	226	0.02%	0.003%
60	10.055	1465	1471	1488	rBV	545586	822492	85.77%	10.360%
61	10.238	1500	1501	1504	rVB	182	102	0.01%	0.001%
62	10.396	1524	1527	1528	rBV2	142	122	0.01%	0.002%
63	10.561	1553	1554	1557	rVB2	187	124	0.01%	0.002%
64	10.585	1557	1558	1561	rBV2	105	103	0.01%	0.001%
65	10.652	1565	1569	1571	rVV2	328	479	0.05%	0.006%
66	10.683	1572	1574	1579	rVB2	232	217	0.02%	0.003%
67	10.817	1595	1596	1599	rBV2	112	118	0.01%	0.001%
68	10.860	1601	1603	1606	rVB	175	158	0.02%	0.002%
69	10.970	1617	1621	1625	rBV3	427	602	0.06%	0.008%
70	11.037	1627	1632	1635	rBV2	171	245	0.03%	0.003%
71	11.091	1639	1641	1648	rVB3	472	559	0.06%	0.007%
72	11.189	1652	1657	1667	rBV	406633	516143	53.82%	6.501%
73	11.311	1674	1677	1682	rVB	1536	2011	0.21%	0.025%
74	11.360	1683	1685	1687	rVV	196	104	0.01%	0.001%
75	11.457	1697	1701	1705	rVB2	484	472	0.05%	0.006%
76	11.524	1711	1712	1715	rBV	143	139	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX041000.D
 Acq On : 12 Apr 2024 01:06
 Operator : JC/MD
 Sample : P2049-05 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0RC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	11.713	1739	1743	1744	rVV	261	293	0.03%	0.004%
78	11.756	1747	1750	1755	rVB3	358	497	0.05%	0.006%
79	11.835	1761	1763	1766	rBV2	111	139	0.01%	0.002%
80	11.975	1780	1786	1788	rBV	4258	5908	0.62%	0.074%
81	12.024	1788	1794	1805	rVB	576720	785846	81.95%	9.898%
82	12.317	1837	1842	1853	rBV2	608652	949633	99.03%	11.961%
83	12.548	1878	1880	1881	rVB2	198	128	0.01%	0.002%
84	12.628	1892	1893	1894	rBV	226	112	0.01%	0.001%
85	12.762	1911	1915	1920	rBV2	3151	4421	0.46%	0.056%
86	12.835	1925	1927	1931	rBV2	136	105	0.01%	0.001%
87	13.067	1963	1965	1966	rBV	159	131	0.01%	0.002%
88	13.103	1969	1971	1972	rBV2	196	158	0.02%	0.002%
89	13.122	1972	1974	1976	rVB2	356	318	0.03%	0.004%
90	13.341	2008	2010	2011	rBV	143	129	0.01%	0.002%
91	13.500	2033	2036	2038	rVB	173	187	0.02%	0.002%
92	13.591	2046	2051	2060	rBV	22021	31172	3.25%	0.393%
93	13.780	2080	2082	2086	rVV2	482	596	0.06%	0.008%
94	13.963	2109	2112	2116	rBV2	3495	4704	0.49%	0.059%
95	14.134	2135	2140	2144	rVB	4135	5063	0.53%	0.064%
96	14.219	2153	2154	2156	rVB	162	106	0.01%	0.001%
97	14.243	2156	2158	2161	rBV2	177	135	0.01%	0.002%
98	14.591	2213	2215	2219	rBV2	191	234	0.02%	0.003%
99	15.292	2329	2330	2332	rBV2	375	202	0.02%	0.003%
100	15.389	2343	2346	2351	rVB4	1951	3004	0.31%	0.038%


Sum of corrected areas: 7939136

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX041000.D
Acq On : 12 Apr 2024 01:06
Operator : JC/MD
Sample : P2049-05 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

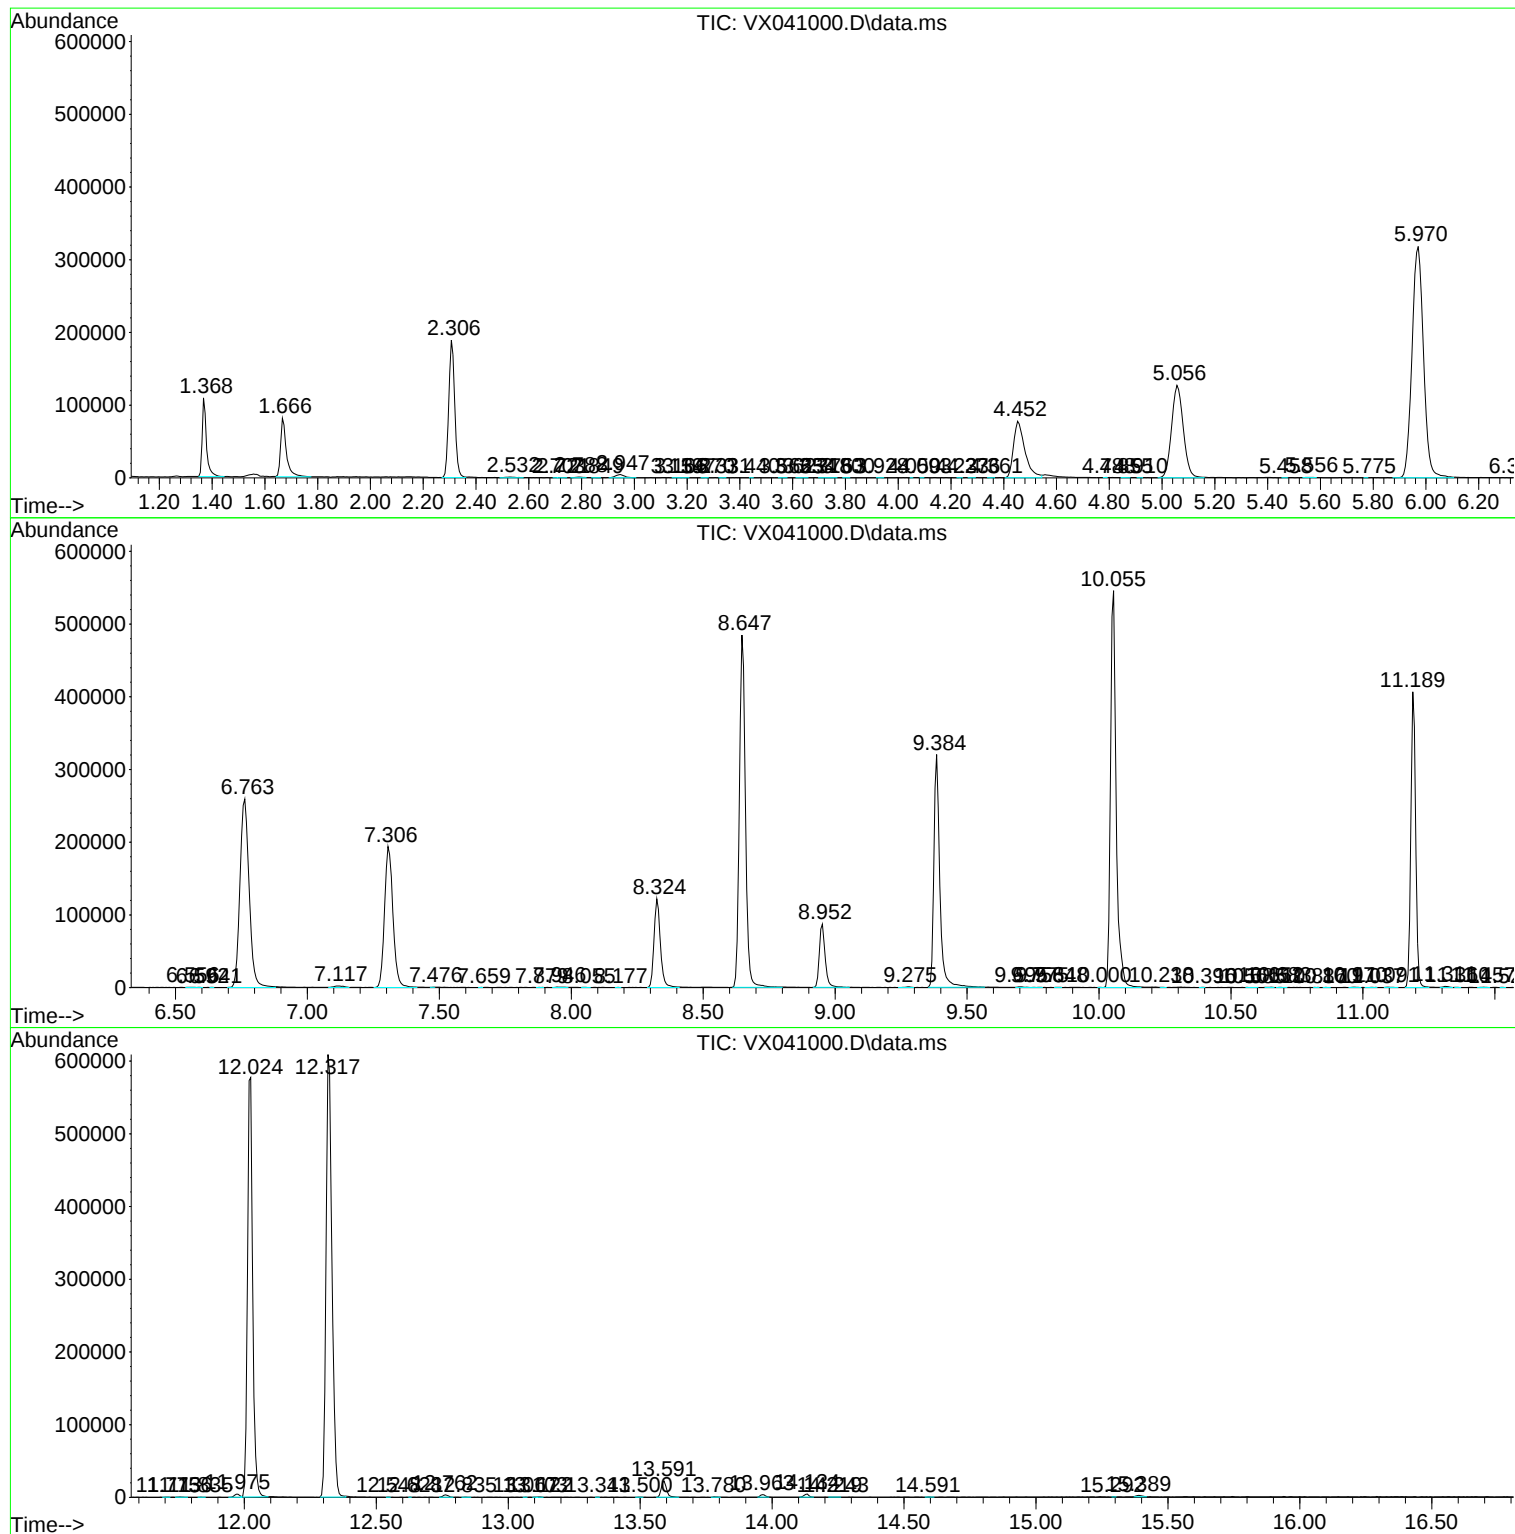

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX041000.D
Acq On : 12 Apr 2024 01:06
Operator : JC/MD
Sample : P2049-05 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX041000.D
Acq On : 12 Apr 2024 01:06
Operator : JC/MD
Sample : P2049-05 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
