

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX041002.D
 Acq On : 12 Apr 2024 01:52
 Operator : JC/MD
 Sample : P2049-09 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CORH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M

Title : VOC Analysis

Signal : TIC: VX041002.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	59	rBV	105491	118206	12.17%	1.550%
2	1.666	91	95	109	rBV	83357	118542	12.21%	1.555%
3	2.306	194	200	210	rBV	184276	282314	29.07%	3.703%
4	2.471	225	227	228	rBV	296	224	0.02%	0.003%
5	2.532	231	237	241	rVV3	796	1717	0.18%	0.023%
6	2.697	261	264	265	rBV	175	161	0.02%	0.002%
7	2.794	274	280	285	rVB4	1001	1729	0.18%	0.023%
8	2.880	292	294	297	rVB	196	137	0.01%	0.002%
9	2.947	297	305	313	rBV	4581	10907	1.12%	0.143%
10	3.099	326	330	332	rBV2	266	253	0.03%	0.003%
11	3.264	355	357	361	rVB2	122	154	0.02%	0.002%
12	3.367	371	374	377	rVV2	131	157	0.02%	0.002%
13	3.562	402	406	407	rBV	131	198	0.02%	0.003%
14	3.611	411	414	417	rVB2	115	154	0.02%	0.002%
15	3.648	417	420	421	rBV	205	146	0.02%	0.002%
16	3.739	432	435	436	rBV2	120	155	0.02%	0.002%
17	3.837	446	451	452	rBV	107	122	0.01%	0.002%
18	4.026	480	482	484	rVB2	142	121	0.01%	0.002%
19	4.129	497	499	504	rBB2	91	127	0.01%	0.002%
20	4.318	525	530	533	rBV2	162	261	0.03%	0.003%
21	4.452	542	552	569	rBV	81629	252278	25.98%	3.309%
22	4.800	606	609	611	rBV3	149	183	0.02%	0.002%
23	5.056	638	651	673	rBV	130540	400330	41.22%	5.251%
24	5.282	687	688	691	rVB	278	174	0.02%	0.002%
25	5.312	691	693	695	rBV2	203	186	0.02%	0.002%
26	5.562	729	734	739	rBV3	451	902	0.09%	0.012%
27	5.617	741	743	746	rBV2	198	220	0.02%	0.003%
28	5.666	749	751	752	rBV2	140	139	0.01%	0.002%
29	5.800	771	773	776	rVB2	220	236	0.02%	0.003%
30	5.830	776	778	779	rBV	164	136	0.01%	0.002%
31	5.970	788	801	820	rBV2	318547	971187	100.00%	12.739%
32	6.257	847	848	852	rBV3	145	184	0.02%	0.002%
33	6.306	854	856	858	rVV	323	226	0.02%	0.003%
34	6.373	862	867	871	rBV2	204	327	0.03%	0.004%
35	6.501	886	888	891	rVB	206	158	0.02%	0.002%
36	6.562	891	898	901	rBV3	242	469	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX041002.D
 Acq On : 12 Apr 2024 01:52
 Operator : JC/MD
 Sample : P2049-09 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CORH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	6.757	921	930	953	rBV	266247	654296	67.37%	8.582%
38	7.117	983	989	996	rBV3	1890	4523	0.47%	0.059%
39	7.208	1002	1004	1007	rVB2	154	131	0.01%	0.002%
40	7.306	1012	1020	1039	rBV	197186	438156	45.12%	5.747%
41	7.543	1057	1059	1061	rBV2	292	198	0.02%	0.003%
42	7.641	1073	1075	1077	rBV2	125	133	0.01%	0.002%
43	7.738	1089	1091	1093	rVB2	143	120	0.01%	0.002%
44	7.836	1104	1107	1111	rBV3	191	264	0.03%	0.003%
45	7.952	1122	1126	1128	rBV3	560	878	0.09%	0.012%
46	8.123	1150	1154	1157	rBV2	120	199	0.02%	0.003%
47	8.159	1159	1160	1162	rVB	234	154	0.02%	0.002%
48	8.183	1162	1164	1166	rBV	166	152	0.02%	0.002%
49	8.324	1181	1187	1199	rBV	122688	203322	20.94%	2.667%
50	8.574	1226	1228	1229	rBV2	201	211	0.02%	0.003%
51	8.647	1234	1240	1258	rBV	470596	743776	76.58%	9.756%
52	8.952	1284	1290	1302	rBV	89915	135781	13.98%	1.781%
53	9.135	1318	1320	1321	rBV2	233	180	0.02%	0.002%
54	9.275	1340	1343	1351	rVB3	771	925	0.10%	0.012%
55	9.384	1356	1361	1377	rBV	342740	521579	53.71%	6.841%
56	9.708	1409	1414	1419	rVB4	692	1291	0.13%	0.017%
57	9.811	1429	1431	1433	rVV	192	136	0.01%	0.002%
58	10.055	1465	1471	1485	rBV	532356	782624	80.58%	10.266%
59	10.275	1505	1507	1509	rVB2	181	121	0.01%	0.002%
60	10.311	1509	1513	1518	rVB3	513	801	0.08%	0.011%
61	10.360	1518	1521	1522	rBV	175	163	0.02%	0.002%
62	10.409	1526	1529	1531	rVB	182	145	0.01%	0.002%
63	10.433	1531	1533	1536	rVB2	203	183	0.02%	0.002%
64	10.457	1536	1537	1539	rBV	152	126	0.01%	0.002%
65	10.567	1554	1555	1559	rBV2	135	150	0.02%	0.002%
66	10.646	1566	1568	1572	rBV	365	397	0.04%	0.005%
67	10.726	1580	1581	1583	rBV	150	120	0.01%	0.002%
68	10.762	1585	1587	1591	rVV2	129	203	0.02%	0.003%
69	10.963	1618	1620	1625	rVB	445	479	0.05%	0.006%
70	11.091	1639	1641	1646	rBV3	429	644	0.07%	0.008%
71	11.189	1652	1657	1666	rBV	402438	520835	53.63%	6.832%
72	11.311	1673	1677	1681	rVB2	1670	2290	0.24%	0.030%
73	11.451	1695	1700	1706	rBV3	444	687	0.07%	0.009%
74	11.640	1730	1731	1734	rBV2	110	131	0.01%	0.002%
75	11.756	1749	1750	1753	rVB	361	284	0.03%	0.004%
76	11.890	1770	1772	1775	rBV2	131	122	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX041002.D
 Acq On : 12 Apr 2024 01:52
 Operator : JC/MD
 Sample : P2049-09 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0RH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	11.975	1783	1786	1788	rBV3	828	1025	0.11%	0.013%
78	12.018	1788	1793	1806	rBV	544979	730644	75.23%	9.584%
79	12.317	1837	1842	1853	rBV	538721	695904	71.65%	9.128%
80	12.695	1902	1904	1906	rBV	213	120	0.01%	0.002%
81	12.762	1911	1915	1921	rVB2	3175	3927	0.40%	0.052%
82	13.122	1970	1974	1979	rVB2	383	535	0.06%	0.007%
83	13.164	1979	1981	1984	rBV2	195	225	0.02%	0.003%
84	13.237	1988	1993	1996	rBV2	92	163	0.02%	0.002%
85	13.323	2005	2007	2010	rBV2	149	180	0.02%	0.002%
86	13.396	2018	2019	2023	rBV2	122	179	0.02%	0.002%
87	13.597	2047	2052	2056	rBV2	973	1243	0.13%	0.016%
88	13.786	2080	2083	2085	rBV2	325	399	0.04%	0.005%
89	13.847	2091	2093	2095	rBV2	192	209	0.02%	0.003%
90	13.902	2098	2102	2103	rBV	204	188	0.02%	0.002%
91	13.963	2110	2112	2113	rBV	270	225	0.02%	0.003%
92	14.128	2135	2139	2144	rVB	2774	3868	0.40%	0.051%
93	14.219	2151	2154	2155	rBV2	247	268	0.03%	0.004%
94	14.256	2158	2160	2163	rVV2	246	218	0.02%	0.003%
95	14.451	2190	2192	2195	rBV2	263	295	0.03%	0.004%
96	14.536	2204	2206	2209	rVB3	219	167	0.02%	0.002%
97	14.640	2221	2223	2226	rBV3	289	318	0.03%	0.004%
98	14.713	2234	2235	2238	rBV2	301	336	0.03%	0.004%
99	15.389	2342	2346	2351	rBV3	1794	2710	0.28%	0.036%
100	16.475	2522	2524	2526	rBV	505	432	0.04%	0.006%




Sum of corrected areas: 7623808

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX041002.D
Acq On : 12 Apr 2024 01:52
Operator : JC/MD
Sample : P2049-09 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0RH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

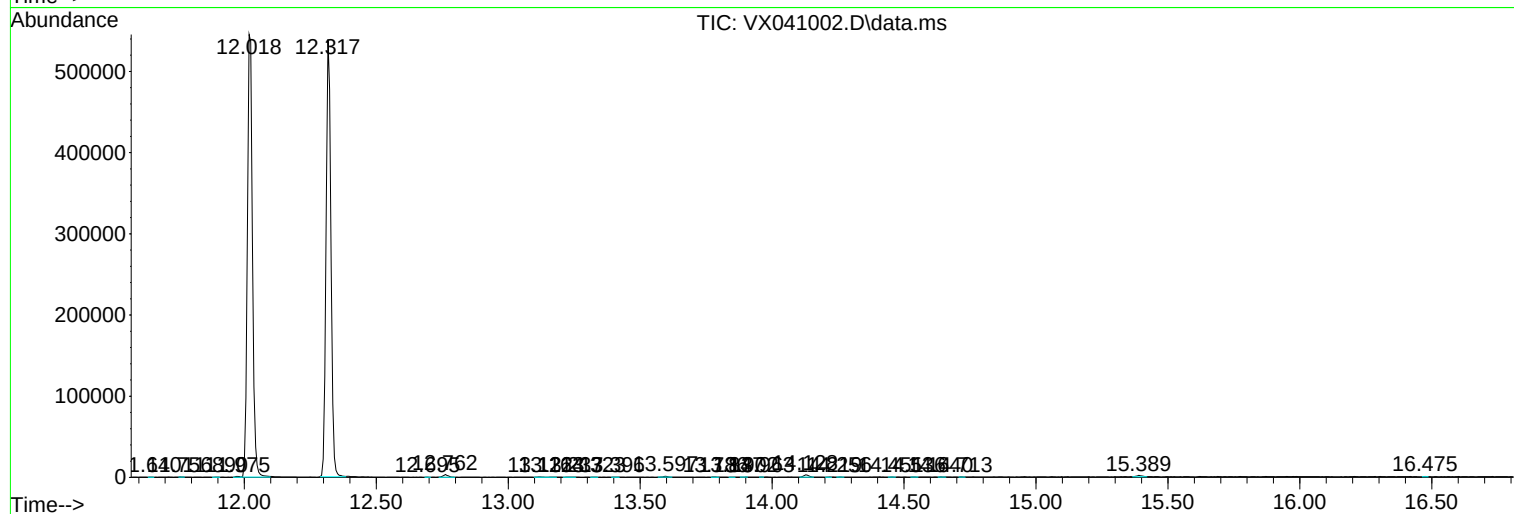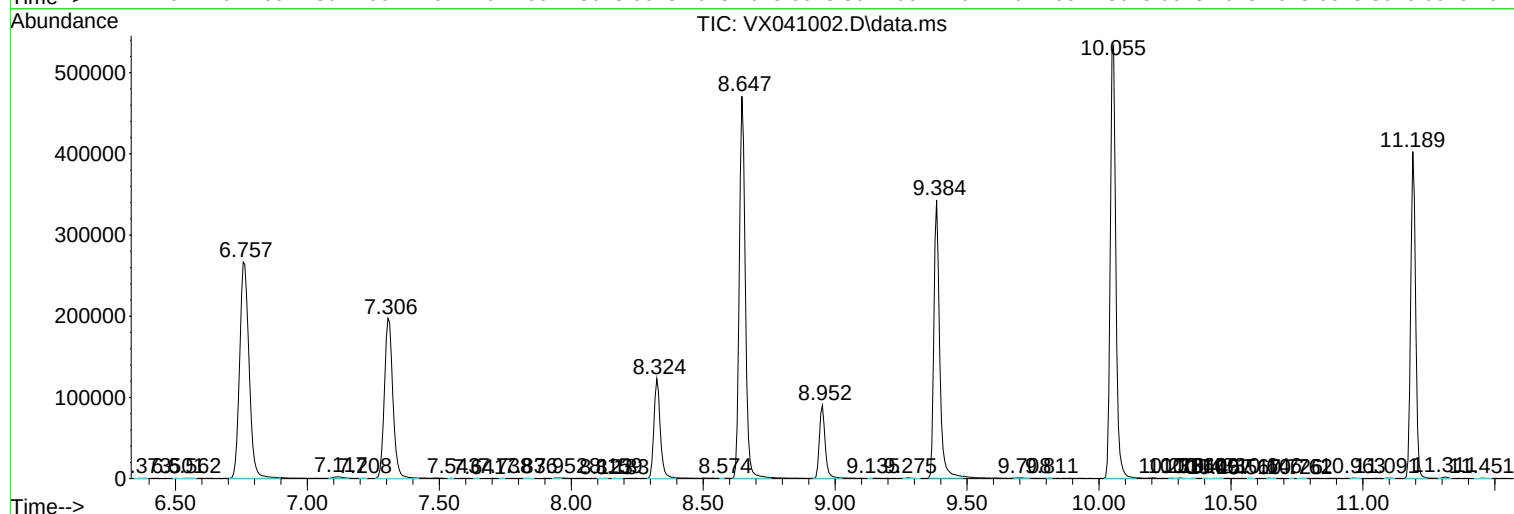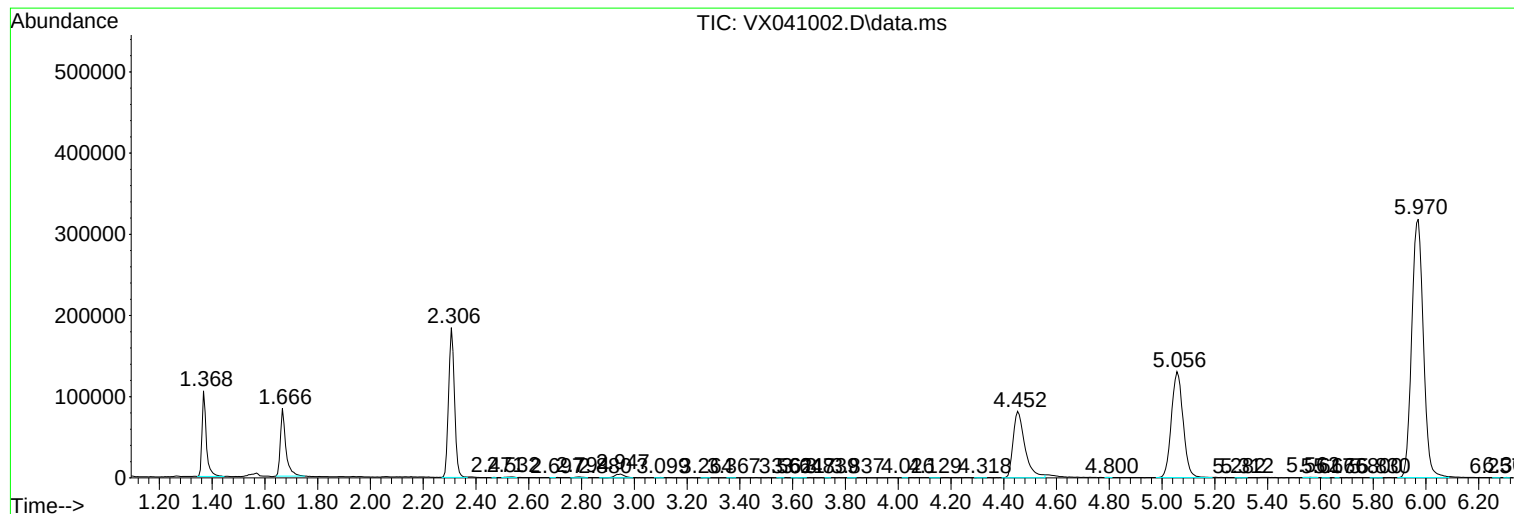

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX041002.D
Acq On : 12 Apr 2024 01:52
Operator : JC/MD
Sample : P2049-09 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0RH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX041002.D
Acq On : 12 Apr 2024 01:52
Operator : JC/MD
Sample : P2049-09 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0RH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc