

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX041003.D
 Acq On : 12 Apr 2024 02:14
 Operator : JC/MD
 Sample : P2049-10 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CORH7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX041003.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	57	rBV	103787	117421	12.55%	1.559%
2	1.666	91	95	114	rVB	79319	118951	12.72%	1.580%
3	2.306	194	200	210	rBV	184072	285674	30.54%	3.794%
4	2.477	227	228	231	rBV	254	182	0.02%	0.002%
5	2.532	233	237	242	rVB4	605	1269	0.14%	0.017%
6	2.794	275	280	288	rVB2	1093	1817	0.19%	0.024%
7	2.880	292	294	296	rVB	211	132	0.01%	0.002%
8	2.947	296	305	314	rVB	4080	9653	1.03%	0.128%
9	3.081	324	327	328	rBV2	155	143	0.02%	0.002%
10	3.178	342	343	346	rBV2	142	141	0.02%	0.002%
11	3.349	367	371	372	rVV	231	153	0.02%	0.002%
12	3.507	395	397	400	rBV2	213	149	0.02%	0.002%
13	3.843	450	452	455	rVB2	138	131	0.01%	0.002%
14	4.026	479	482	484	rVB2	122	120	0.01%	0.002%
15	4.141	497	501	503	rBV2	124	175	0.02%	0.002%
16	4.209	509	512	513	rVV	158	147	0.02%	0.002%
17	4.245	515	518	519	rBV	147	177	0.02%	0.002%
18	4.324	529	531	533	rBV2	156	152	0.02%	0.002%
19	4.452	544	552	569	rBV	74655	234873	25.11%	3.119%
20	5.056	639	651	666	rBV	122188	381252	40.76%	5.063%
21	5.227	677	679	681	rVB	265	164	0.02%	0.002%
22	5.263	683	685	687	rBV2	183	182	0.02%	0.002%
23	5.282	687	688	694	rVB3	280	376	0.04%	0.005%
24	5.373	700	703	704	rBV	248	240	0.03%	0.003%
25	5.672	748	752	754	rVV2	154	179	0.02%	0.002%
26	5.970	789	801	821	rBV2	312128	935285	100.00%	12.421%
27	6.306	853	856	859	rVB3	221	290	0.03%	0.004%
28	6.379	866	868	869	rBV	184	153	0.02%	0.002%
29	6.409	872	873	877	rBV	182	177	0.02%	0.002%
30	6.446	877	879	882	rVV2	133	154	0.02%	0.002%
31	6.763	921	931	948	rBV	261308	634390	67.83%	8.425%
32	7.117	983	989	999	rVB5	1971	5100	0.55%	0.068%
33	7.214	1001	1005	1007	rBV	143	210	0.02%	0.003%
34	7.306	1011	1020	1035	rBV	190718	418463	44.74%	5.557%
35	7.604	1065	1069	1073	rVB2	135	173	0.02%	0.002%
36	7.696	1082	1084	1087	rBV2	170	189	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX041003.D
 Acq On : 12 Apr 2024 02:14
 Operator : JC/MD
 Sample : P2049-10 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CORH7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	7.726	1087	1089	1091	rBV	147	120	0.01%	0.002%
38	7.836	1104	1107	1109	rBV2	162	181	0.02%	0.002%
39	7.879	1111	1114	1116	rVB2	193	185	0.02%	0.002%
40	7.921	1116	1121	1122	rBV2	120	168	0.02%	0.002%
41	7.952	1122	1126	1133	rBV4	475	1020	0.11%	0.014%
42	8.031	1138	1139	1142	rVB	290	212	0.02%	0.003%
43	8.074	1142	1146	1148	rBV2	142	217	0.02%	0.003%
44	8.135	1152	1156	1161	rBV2	207	340	0.04%	0.005%
45	8.196	1161	1166	1168	rBV2	164	217	0.02%	0.003%
46	8.324	1180	1187	1204	rBV	118510	197100	21.07%	2.618%
47	8.494	1213	1215	1216	rBV	334	183	0.02%	0.002%
48	8.507	1216	1217	1219	rBV2	472	388	0.04%	0.005%
49	8.647	1234	1240	1257	rBV	469622	744196	79.57%	9.883%
50	8.952	1285	1290	1304	rBV	84845	130087	13.91%	1.728%
51	9.275	1339	1343	1347	rVB2	605	742	0.08%	0.010%
52	9.384	1356	1361	1385	rBV	317330	493957	52.81%	6.560%
53	9.695	1410	1412	1417	rVB	784	969	0.10%	0.013%
54	9.799	1427	1429	1430	rBV2	244	166	0.02%	0.002%
55	9.854	1435	1438	1441	rVB2	220	291	0.03%	0.004%
56	9.884	1441	1443	1446	rBV2	298	341	0.04%	0.005%
57	9.988	1459	1460	1463	rBV	189	179	0.02%	0.002%
58	10.055	1465	1471	1491	rBV	542546	773920	82.75%	10.278%
59	10.232	1498	1500	1505	rVB2	347	268	0.03%	0.004%
60	10.305	1510	1512	1520	rVB4	533	920	0.10%	0.012%
61	10.403	1526	1528	1530	rBV2	139	120	0.01%	0.002%
62	10.464	1536	1538	1540	rVB	169	124	0.01%	0.002%
63	10.592	1557	1559	1562	rBV2	162	173	0.02%	0.002%
64	10.653	1565	1569	1570	rBV3	452	464	0.05%	0.006%
65	10.872	1603	1605	1606	rBV2	138	135	0.01%	0.002%
66	10.970	1618	1621	1627	rVB	330	420	0.04%	0.006%
67	11.049	1632	1634	1637	rBV	105	148	0.02%	0.002%
68	11.098	1639	1642	1645	rVB3	442	484	0.05%	0.006%
69	11.189	1652	1657	1670	rBV	393926	509632	54.49%	6.768%
70	11.311	1674	1677	1683	rVB2	1489	2034	0.22%	0.027%
71	11.408	1690	1693	1696	rBV2	124	193	0.02%	0.003%
72	11.451	1698	1700	1705	rBV3	425	610	0.07%	0.008%
73	11.665	1734	1735	1738	rBV2	104	131	0.01%	0.002%
74	11.707	1740	1742	1745	rVB2	287	340	0.04%	0.005%
75	11.762	1745	1751	1754	rBV3	493	737	0.08%	0.010%
76	11.969	1782	1785	1788	rBV4	783	939	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX041003.D
 Acq On : 12 Apr 2024 02:14
 Operator : JC/MD
 Sample : P2049-10 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0RH7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	12.018	1788	1793	1806	rBV	583706	768962	82.22%	10.212%
78	12.238	1827	1829	1831	rBV	238	244	0.03%	0.003%
79	12.317	1837	1842	1855	rBV	564003	734425	78.52%	9.753%
80	12.585	1884	1886	1889	rVB2	178	177	0.02%	0.002%
81	12.762	1911	1915	1919	rVV	3198	4255	0.45%	0.057%
82	12.908	1935	1939	1941	rVB2	222	177	0.02%	0.002%
83	13.061	1962	1964	1966	rVB2	222	158	0.02%	0.002%
84	13.085	1966	1968	1969	rBV2	125	124	0.01%	0.002%
85	13.115	1971	1973	1978	rVB3	379	353	0.04%	0.005%
86	13.201	1985	1987	1989	rBV	158	144	0.02%	0.002%
87	13.256	1993	1996	1998	rVV2	111	122	0.01%	0.002%
88	13.311	2002	2005	2008	rBV	202	258	0.03%	0.003%
89	13.378	2014	2016	2020	rBV2	198	265	0.03%	0.004%
90	13.487	2033	2034	2038	rBV2	234	233	0.02%	0.003%
91	13.597	2049	2052	2056	rVB	872	1027	0.11%	0.014%
92	13.713	2066	2071	2073	rVB2	197	293	0.03%	0.004%
93	13.969	2109	2113	2116	rBV5	480	680	0.07%	0.009%
94	14.067	2126	2129	2130	rVB	280	230	0.02%	0.003%
95	14.085	2130	2132	2133	rBV	190	162	0.02%	0.002%
96	14.128	2135	2139	2144	rVV	4115	5005	0.54%	0.066%
97	14.316	2168	2170	2173	rBV2	221	216	0.02%	0.003%
98	14.438	2188	2190	2191	rBV2	202	148	0.02%	0.002%
99	14.920	2268	2269	2272	rBV2	385	371	0.04%	0.005%
100	14.969	2275	2277	2280	rBV	382	353	0.04%	0.005%




Sum of corrected areas: 7529870

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX041003.D
Acq On : 12 Apr 2024 02:14
Operator : JC/MD
Sample : P2049-10 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CORH7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

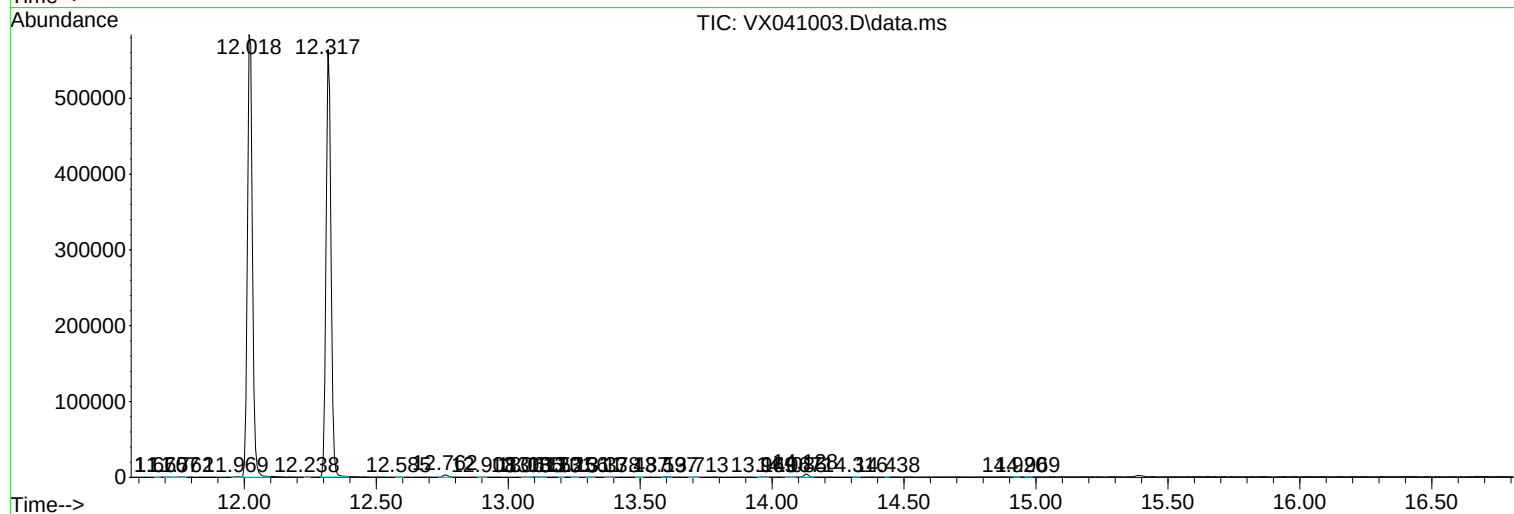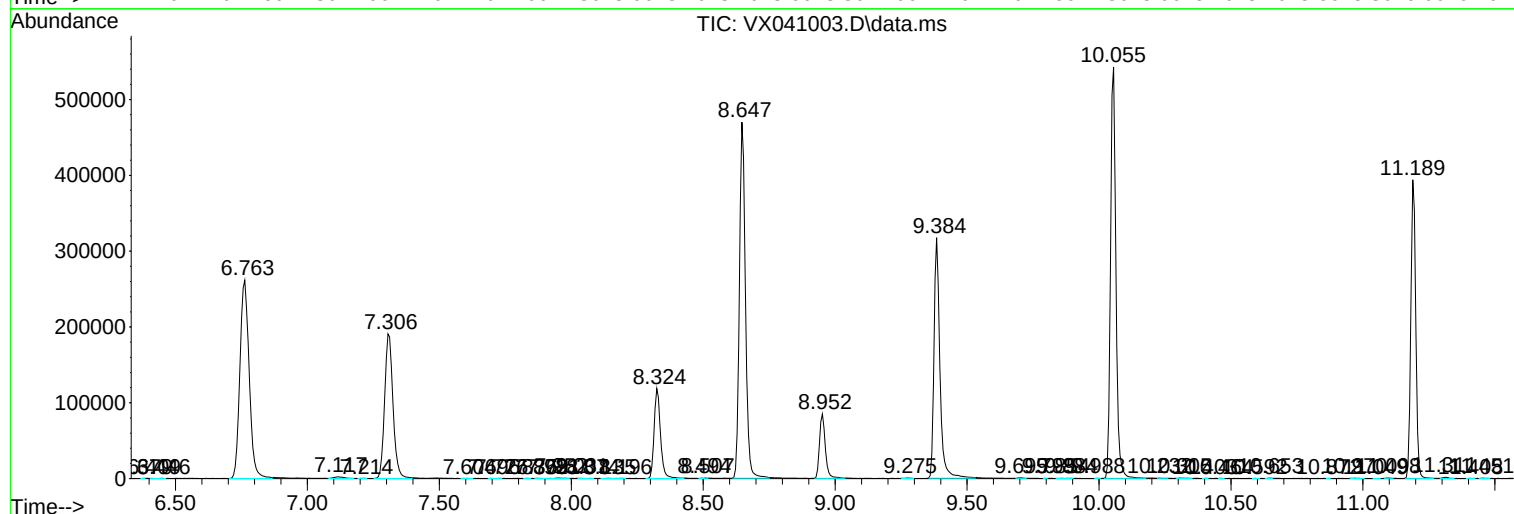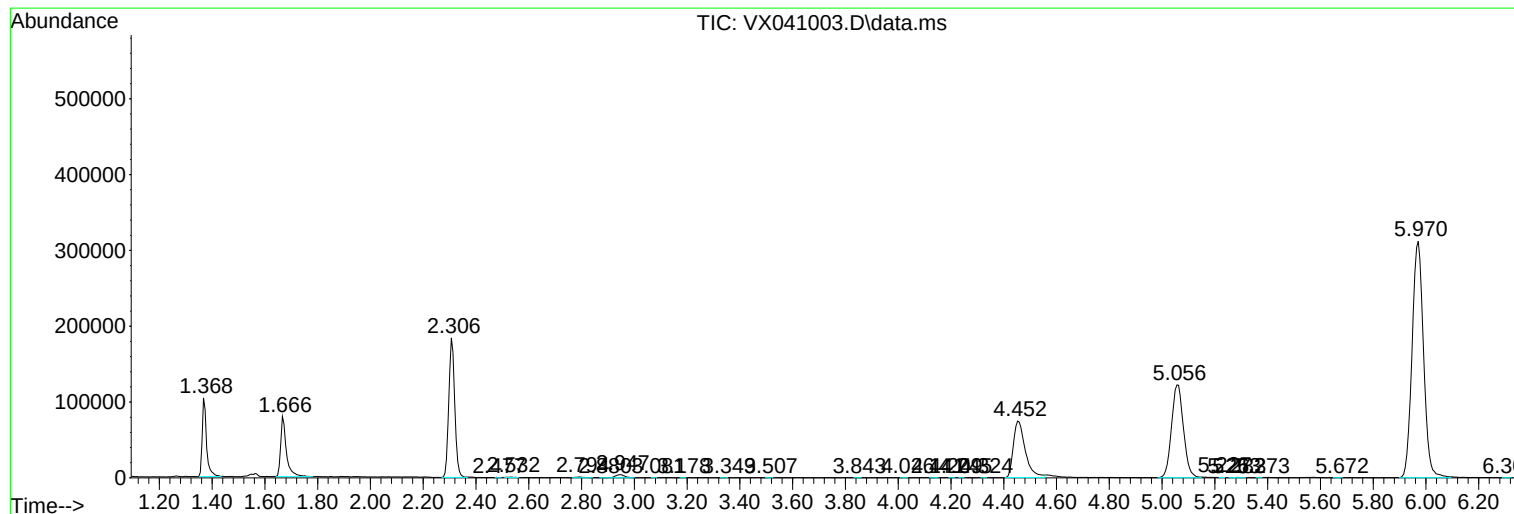

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX041003.D
Acq On : 12 Apr 2024 02:14
Operator : JC/MD
Sample : P2049-10 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0RH7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX041003.D
Acq On : 12 Apr 2024 02:14
Operator : JC/MD
Sample : P2049-10 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0RH7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------