

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX041005.D
 Acq On : 12 Apr 2024 03:00
 Operator : JC/MD
 Sample : P2049-12 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CORH9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX041005.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	58	rVB	98064	111095	3.23%	0.710%
2	1.666	91	95	112	rVB	75818	115706	3.37%	0.739%
3	2.306	193	200	210	rBV	167799	264156	7.69%	1.687%
4	2.465	224	226	228	rVB	281	247	0.01%	0.002%
5	2.532	232	237	244	rVB3	1217	2271	0.07%	0.015%
6	2.703	263	265	267	rVB2	207	155	0.00%	0.001%
7	2.727	267	269	273	rVB2	146	153	0.00%	0.001%
8	2.794	273	280	287	rBV5	1079	2193	0.06%	0.014%
9	2.849	287	289	292	rVB2	242	216	0.01%	0.001%
10	2.885	292	295	296	rBV	167	139	0.00%	0.001%
11	2.946	296	305	314	rVV	4138	8973	0.26%	0.057%
12	3.020	316	317	320	rBV	165	189	0.01%	0.001%
13	3.105	328	331	332	rBV2	152	141	0.00%	0.001%
14	3.263	356	357	361	rBV2	126	135	0.00%	0.001%
15	3.355	370	372	376	rVB2	191	248	0.01%	0.002%
16	3.398	376	379	381	rBV2	132	188	0.01%	0.001%
17	3.526	398	400	403	rBV	168	132	0.00%	0.001%
18	3.739	433	435	438	rBV	156	209	0.01%	0.001%
19	3.806	443	446	449	rBV2	100	158	0.00%	0.001%
20	3.837	449	451	453	rVB	201	140	0.00%	0.001%
21	3.928	463	466	467	rBV2	122	135	0.00%	0.001%
22	4.019	479	481	484	rBV	156	170	0.00%	0.001%
23	4.263	519	521	524	rVB2	129	139	0.00%	0.001%
24	4.452	543	552	568	rBV	72389	228098	6.64%	1.457%
25	4.897	623	625	628	rVB	195	159	0.00%	0.001%
26	4.964	633	636	638	rBV2	151	149	0.00%	0.001%
27	5.056	639	651	670	rVV	123611	397002	11.55%	2.536%
28	5.355	699	700	701	rBV	170	115	0.00%	0.001%
29	5.391	701	706	708	rVV3	527	956	0.03%	0.006%
30	5.476	717	720	721	rBV	168	167	0.00%	0.001%
31	5.556	731	733	745	rVB4	821	1826	0.05%	0.012%
32	5.769	767	768	770	rBV	195	132	0.00%	0.001%
33	5.824	776	777	782	rVB	163	159	0.00%	0.001%
34	5.970	789	801	806	rBV2	301151	891868	25.96%	5.696%
35	6.434	875	877	880	rBV2	125	127	0.00%	0.001%
36	6.531	892	893	894	rBV	198	105	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX041005.D
 Acq On : 12 Apr 2024 03:00
 Operator : JC/MD
 Sample : P2049-12 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CORH9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	6.549	894	896	899	rVV2	188	203	0.01%	0.001%
38	6.610	903	906	908	rBV2	166	190	0.01%	0.001%
39	6.641	910	911	912	rBV	211	126	0.00%	0.001%
40	6.684	917	918	921	rBV	265	206	0.01%	0.001%
41	6.763	922	931	951	rBV	231096	561165	16.33%	3.584%
42	7.116	984	989	996	rVB4	1735	4066	0.12%	0.026%
43	7.305	1011	1020	1040	rBV	185569	412770	12.01%	2.636%
44	7.866	1110	1112	1114	rBV2	155	133	0.00%	0.001%
45	7.958	1122	1127	1128	rBV3	429	524	0.02%	0.003%
46	8.324	1181	1187	1200	rBV	114014	192320	5.60%	1.228%
47	8.500	1214	1216	1219	rBV3	229	255	0.01%	0.002%
48	8.647	1234	1240	1265	rBV	440399	696490	20.27%	4.448%
49	8.951	1284	1290	1309	rBV	83915	126619	3.68%	0.809%
50	9.281	1339	1344	1348	rVB4	707	1198	0.03%	0.008%
51	9.311	1348	1349	1351	rBV2	196	148	0.00%	0.001%
52	9.384	1356	1361	1377	rBV2	308833	479861	13.97%	3.065%
53	9.695	1410	1412	1420	rVB2	817	1476	0.04%	0.009%
54	9.896	1443	1445	1446	rBV	200	134	0.00%	0.001%
55	9.963	1454	1456	1457	rBV	108	105	0.00%	0.001%
56	10.079	1465	1475	1494	rBV2	1522148	2777794	80.84%	17.742%
57	10.305	1511	1512	1516	rVB2	509	408	0.01%	0.003%
58	10.341	1516	1518	1522	rVB	355	250	0.01%	0.002%
59	10.543	1550	1551	1554	rBV	122	133	0.00%	0.001%
60	10.652	1564	1569	1571	rBV2	339	458	0.01%	0.003%
61	10.677	1571	1573	1574	rVB	263	130	0.00%	0.001%
62	10.805	1591	1594	1597	rVB2	266	290	0.01%	0.002%
63	10.872	1603	1605	1608	rVB2	150	130	0.00%	0.001%
64	10.933	1613	1615	1617	rBV2	138	124	0.00%	0.001%
65	10.963	1617	1620	1625	rVB2	263	431	0.01%	0.003%
66	11.097	1637	1642	1646	rVB3	605	926	0.03%	0.006%
67	11.189	1652	1657	1668	rBV	393353	507190	14.76%	3.239%
68	11.317	1673	1678	1682	rVB2	1437	2099	0.06%	0.013%
69	11.463	1697	1702	1707	rVB4	412	732	0.02%	0.005%
70	11.549	1714	1716	1719	rVB	168	139	0.00%	0.001%
71	11.713	1740	1743	1745	rBV2	351	388	0.01%	0.002%
72	11.762	1748	1751	1755	rVV3	344	554	0.02%	0.004%
73	11.792	1755	1756	1758	rVB2	170	114	0.00%	0.001%
74	11.914	1770	1776	1777	rVB2	123	180	0.01%	0.001%
75	11.969	1780	1785	1789	rBV	371660	452722	13.18%	2.892%
76	12.036	1789	1796	1810	rVB2	1903493	3096506	90.12%	19.777%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX041005.D
 Acq On : 12 Apr 2024 03:00
 Operator : JC/MD
 Sample : P2049-12 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0RH9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041024WMA.M
 Title : VOC Analysis

77	12.335	1837	1845	1861	rBV2	2251033	3436114	100.00%	21.947%
78	12.597	1885	1888	1891	rBV3	153	248	0.01%	0.002%
79	12.762	1910	1915	1921	rBV	3178	4348	0.13%	0.028%
80	12.859	1930	1931	1933	rBV2	186	165	0.00%	0.001%
81	12.932	1939	1943	1947	rVB2	1958	2788	0.08%	0.018%
82	13.067	1961	1965	1966	rBV2	507	517	0.02%	0.003%
83	13.103	1967	1971	1978	rVV3	7390	11150	0.32%	0.071%
84	13.201	1981	1987	1991	rBV3	1655	2244	0.07%	0.014%
85	13.298	2001	2003	2004	rVB2	223	125	0.00%	0.001%
86	13.347	2010	2011	2013	rVB	195	136	0.00%	0.001%
87	13.371	2013	2015	2017	rBV2	205	178	0.01%	0.001%
88	13.451	2026	2028	2029	rBV2	234	133	0.00%	0.001%
89	13.499	2034	2036	2038	rBV2	187	168	0.00%	0.001%
90	13.585	2045	2050	2064	rBV	479412	591726	17.22%	3.779%
91	13.786	2079	2083	2089	rVB3	643	926	0.03%	0.006%
92	13.896	2099	2101	2103	rBV	209	203	0.01%	0.001%
93	13.963	2106	2112	2120	rBV	179835	236053	6.87%	1.508%
94	14.054	2126	2127	2130	rVB2	233	184	0.01%	0.001%
95	14.133	2134	2140	2144	rBV2	4080	5233	0.15%	0.033%
96	14.268	2158	2162	2170	rBV5	991	1795	0.05%	0.011%
97	14.469	2193	2195	2197	rBV2	229	202	0.01%	0.001%
98	14.518	2199	2203	2205	rBV2	274	288	0.01%	0.002%
99	14.786	2243	2247	2252	rVB2	3172	4333	0.13%	0.028%
100	15.249	2319	2323	2330	rVB2	6851	9679	0.28%	0.062%




Sum of corrected areas: 15656774

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX041005.D
Acq On : 12 Apr 2024 03:00
Operator : JC/MD
Sample : P2049-12 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0RH9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

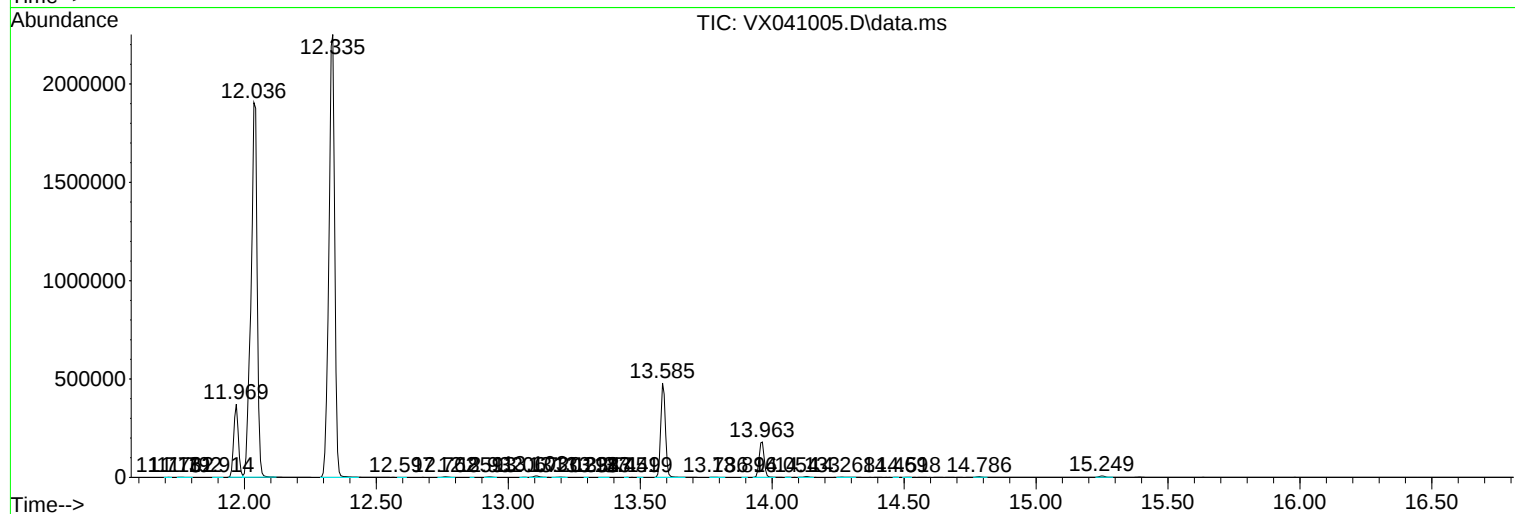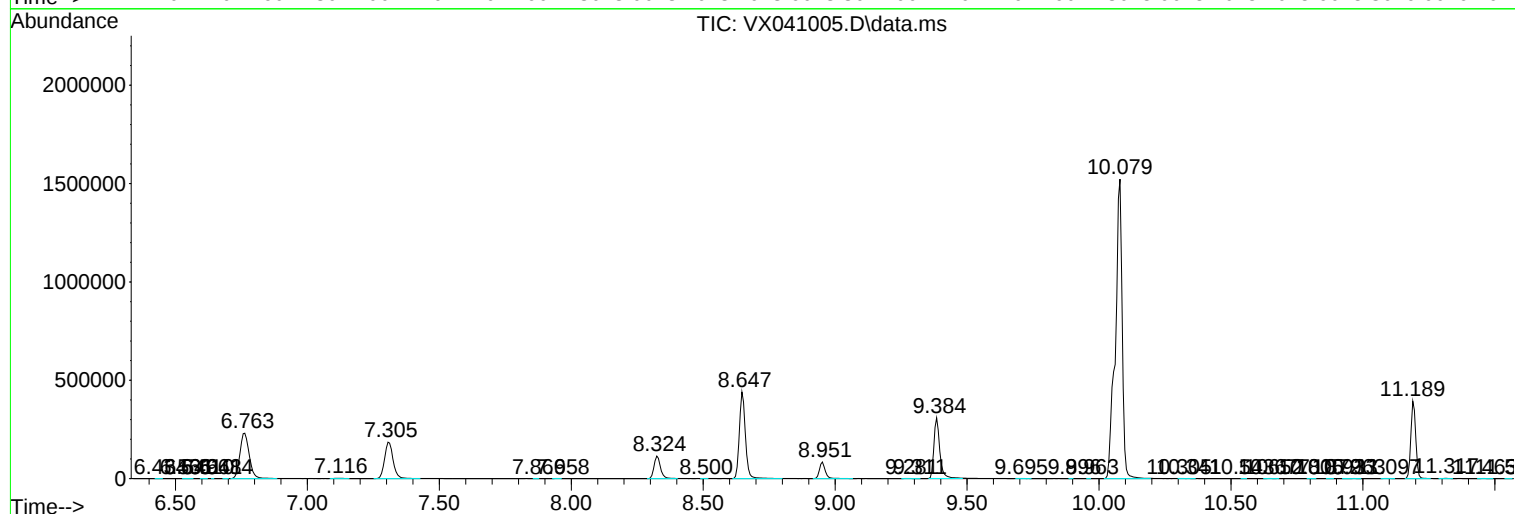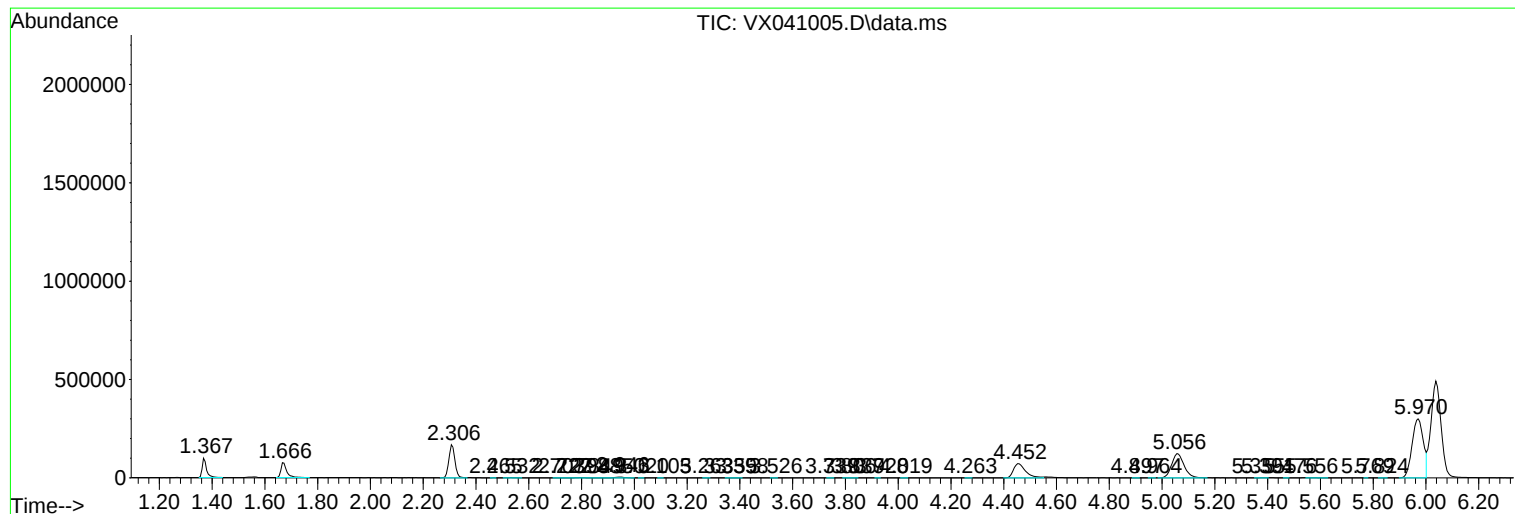

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX041005.D
Acq On : 12 Apr 2024 03:00
Operator : JC/MD
Sample : P2049-12 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0RH9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX041005.D
Acq On : 12 Apr 2024 03:00
Operator : JC/MD
Sample : P2049-12 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0RH9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc