

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX041007.D
 Acq On : 12 Apr 2024 03:46
 Operator : JC/MD
 Sample : P2049-14 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX041007.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	59	rVB	100187	115358	12.35%	1.548%
2	1.672	91	96	109	rBV	75941	117133	12.54%	1.571%
3	2.306	194	200	211	rBV	178136	278502	29.81%	3.736%
4	2.452	223	224	225	rVB	334	122	0.01%	0.002%
5	2.538	232	238	243	rVB5	1402	2963	0.32%	0.040%
6	2.794	274	280	285	rBV3	943	1592	0.17%	0.021%
7	2.837	285	287	292	rVB2	252	324	0.03%	0.004%
8	2.946	297	305	314	rVV2	3957	8322	0.89%	0.112%
9	3.123	332	334	335	rBV	252	142	0.02%	0.002%
10	3.617	412	415	416	rVB2	157	147	0.02%	0.002%
11	3.635	416	418	421	rVB	204	140	0.01%	0.002%
12	3.672	421	424	427	rBV	144	201	0.02%	0.003%
13	3.763	437	439	442	rVB2	151	137	0.01%	0.002%
14	3.788	442	443	446	rBV	164	147	0.02%	0.002%
15	3.928	464	466	468	rBV2	115	135	0.01%	0.002%
16	3.983	472	475	478	rVV	119	152	0.02%	0.002%
17	4.025	481	482	486	rBV2	200	266	0.03%	0.004%
18	4.141	497	501	502	rVB2	221	228	0.02%	0.003%
19	4.208	510	512	514	rVV	186	133	0.01%	0.002%
20	4.263	517	521	522	rBV2	209	206	0.02%	0.003%
21	4.452	544	552	566	rBV	74808	227679	24.37%	3.055%
22	4.836	614	615	617	rBV	245	148	0.02%	0.002%
23	5.056	639	651	669	rBV	124375	380951	40.77%	5.111%
24	5.202	673	675	677	rVV2	223	142	0.02%	0.002%
25	5.306	690	692	694	rBV	256	217	0.02%	0.003%
26	5.379	702	704	705	rBV	295	212	0.02%	0.003%
27	5.470	717	719	722	rVB2	169	138	0.01%	0.002%
28	5.543	727	731	732	rBV2	420	547	0.06%	0.007%
29	5.610	740	742	744	rVB	195	172	0.02%	0.002%
30	5.732	756	762	766	rVB2	177	308	0.03%	0.004%
31	5.812	772	775	776	rBV	195	136	0.01%	0.002%
32	5.970	789	801	828	rBV2	310224	934401	100.00%	12.536%
33	6.373	865	867	869	rBV	131	148	0.02%	0.002%
34	6.507	886	889	892	rBV2	113	147	0.02%	0.002%
35	6.555	895	897	898	rVV	180	177	0.02%	0.002%
36	6.592	901	903	906	rVB2	138	143	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX041007.D
 Acq On : 12 Apr 2024 03:46
 Operator : JC/MD
 Sample : P2049-14 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	6.622	906	908	911	rBV2	93	134	0.01%	0.002%
38	6.763	922	931	947	rBV	250729	604553	64.70%	8.111%
39	7.116	983	989	998	rVB5	1725	4453	0.48%	0.060%
40	7.305	1012	1020	1044	rBV	188478	421756	45.14%	5.658%
41	7.604	1066	1069	1070	rBV	167	158	0.02%	0.002%
42	7.860	1109	1111	1115	rVB	287	326	0.03%	0.004%
43	7.921	1115	1121	1122	rBV2	134	233	0.02%	0.003%
44	7.945	1122	1125	1127	rBV3	461	659	0.07%	0.009%
45	8.055	1140	1143	1145	rBV	301	264	0.03%	0.004%
46	8.147	1156	1158	1159	rBV	219	157	0.02%	0.002%
47	8.323	1181	1187	1206	rBV	117333	195464	20.92%	2.622%
48	8.592	1225	1231	1233	rBV2	283	395	0.04%	0.005%
49	8.646	1234	1240	1258	rBV	454636	738640	79.05%	9.910%
50	8.951	1285	1290	1304	rBV	83615	128178	13.72%	1.720%
51	9.061	1306	1308	1310	rVV	206	162	0.02%	0.002%
52	9.104	1313	1315	1317	rVB2	253	200	0.02%	0.003%
53	9.128	1317	1319	1320	rBV	232	143	0.02%	0.002%
54	9.274	1340	1343	1349	rVB3	461	770	0.08%	0.010%
55	9.384	1356	1361	1391	rBV	322438	490092	52.45%	6.575%
56	9.695	1410	1412	1415	rVB	562	526	0.06%	0.007%
57	9.744	1419	1420	1425	rVB2	206	198	0.02%	0.003%
58	9.799	1425	1429	1432	rBV2	227	373	0.04%	0.005%
59	9.896	1442	1445	1449	rBV3	239	353	0.04%	0.005%
60	10.055	1465	1471	1490	rBV	535553	755007	80.80%	10.129%
61	10.311	1511	1513	1520	rVB5	463	567	0.06%	0.008%
62	10.414	1529	1530	1534	rBV	175	163	0.02%	0.002%
63	10.646	1566	1568	1570	rBV	294	238	0.03%	0.003%
64	10.719	1578	1580	1583	rBV	158	135	0.01%	0.002%
65	10.744	1583	1584	1587	rVV2	203	166	0.02%	0.002%
66	10.866	1602	1604	1606	rBV2	153	127	0.01%	0.002%
67	10.969	1618	1621	1625	rVB2	297	360	0.04%	0.005%
68	11.067	1633	1637	1638	rBV	138	211	0.02%	0.003%
69	11.091	1638	1641	1642	rBV3	306	290	0.03%	0.004%
70	11.189	1652	1657	1666	rBV	388147	507484	54.31%	6.808%
71	11.317	1674	1678	1682	rVB2	1217	1506	0.16%	0.020%
72	11.347	1682	1683	1686	rVB	281	146	0.02%	0.002%
73	11.384	1686	1689	1690	rBV2	127	144	0.02%	0.002%
74	11.457	1697	1701	1705	rVB2	387	584	0.06%	0.008%
75	11.542	1711	1715	1718	rBV2	216	257	0.03%	0.003%
76	11.701	1740	1741	1743	rVV2	234	128	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX041007.D
 Acq On : 12 Apr 2024 03:46
 Operator : JC/MD
 Sample : P2049-14 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	11.756	1747	1750	1756	rVB3	404	644	0.07%	0.009%
78	11.975	1781	1786	1788	rBV3	2148	2653	0.28%	0.036%
79	12.024	1788	1794	1806	rVV	577710	755206	80.82%	10.132%
80	12.317	1837	1842	1853	rBV	559932	744967	79.73%	9.995%
81	12.768	1910	1916	1922	rVB2	2749	3910	0.42%	0.052%
82	12.816	1922	1924	1927	rBV	121	128	0.01%	0.002%
83	12.932	1940	1943	1944	rBV2	195	144	0.02%	0.002%
84	13.042	1960	1961	1968	rBV	230	271	0.03%	0.004%
85	13.121	1970	1974	1975	rBV	426	373	0.04%	0.005%
86	13.335	2007	2009	2014	rVB2	158	215	0.02%	0.003%
87	13.396	2014	2019	2020	rBV2	130	154	0.02%	0.002%
88	13.457	2027	2029	2032	rBV2	213	201	0.02%	0.003%
89	13.542	2039	2043	2045	rBV2	207	330	0.04%	0.004%
90	13.591	2048	2051	2056	rBV2	3662	5087	0.54%	0.068%
91	13.889	2098	2100	2103	rBV2	276	343	0.04%	0.005%
92	13.963	2109	2112	2117	rBV3	1119	1658	0.18%	0.022%
93	14.127	2135	2139	2146	rVB	3606	4918	0.53%	0.066%
94	14.511	2200	2202	2203	rBV	290	162	0.02%	0.002%
95	14.664	2224	2227	2231	rBV2	272	370	0.04%	0.005%
96	14.865	2259	2260	2262	rBV	383	190	0.02%	0.003%
97	14.969	2275	2277	2278	rBV	391	273	0.03%	0.004%
98	15.145	2303	2306	2308	rBV3	398	534	0.06%	0.007%
99	15.389	2344	2346	2352	rVB4	2050	2824	0.30%	0.038%
100	16.730	2564	2566	2570	rBV	530	473	0.05%	0.006%




Sum of corrected areas: 7453744

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX041007.D
Acq On : 12 Apr 2024 03:46
Operator : JC/MD
Sample : P2049-14 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

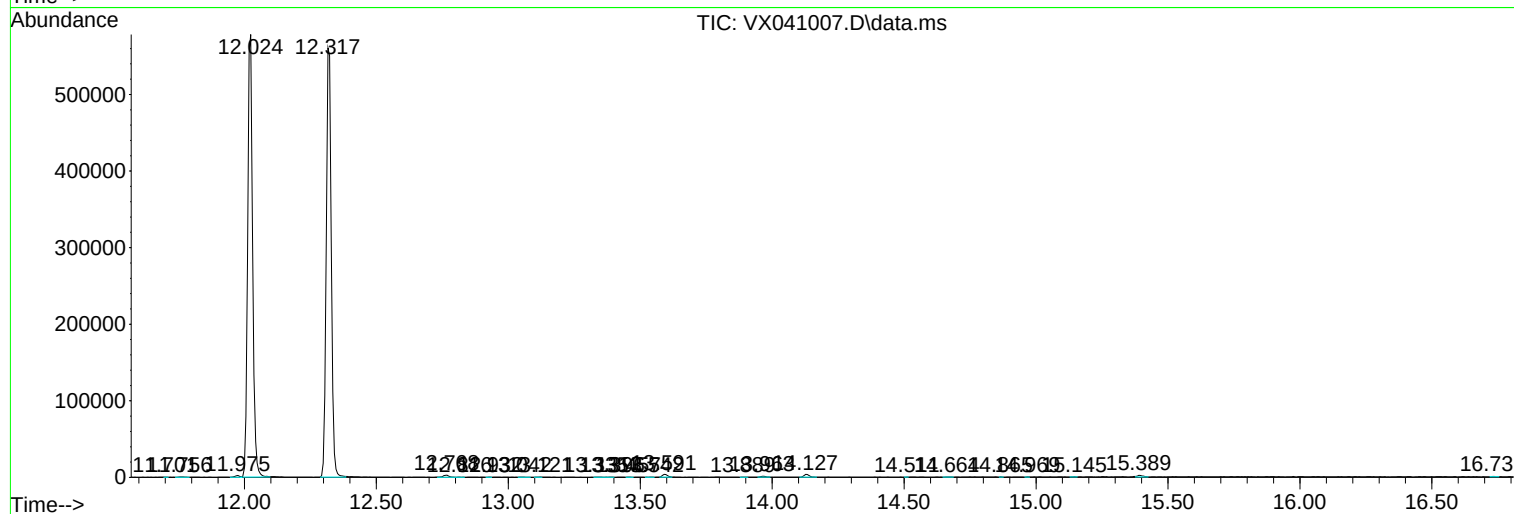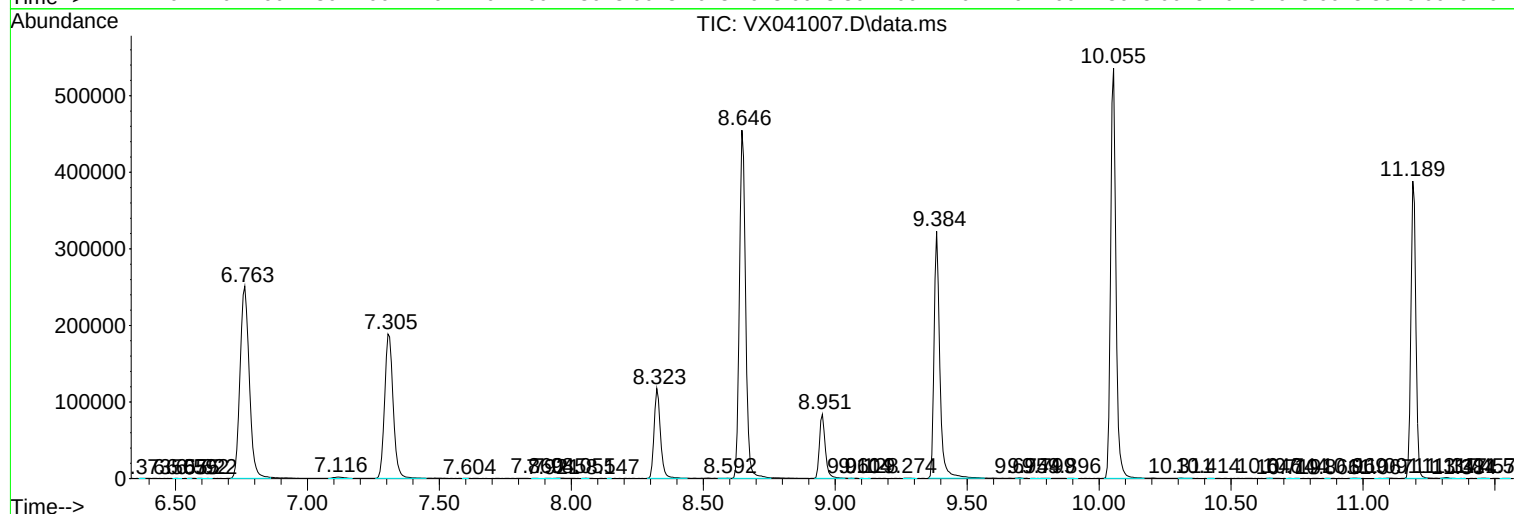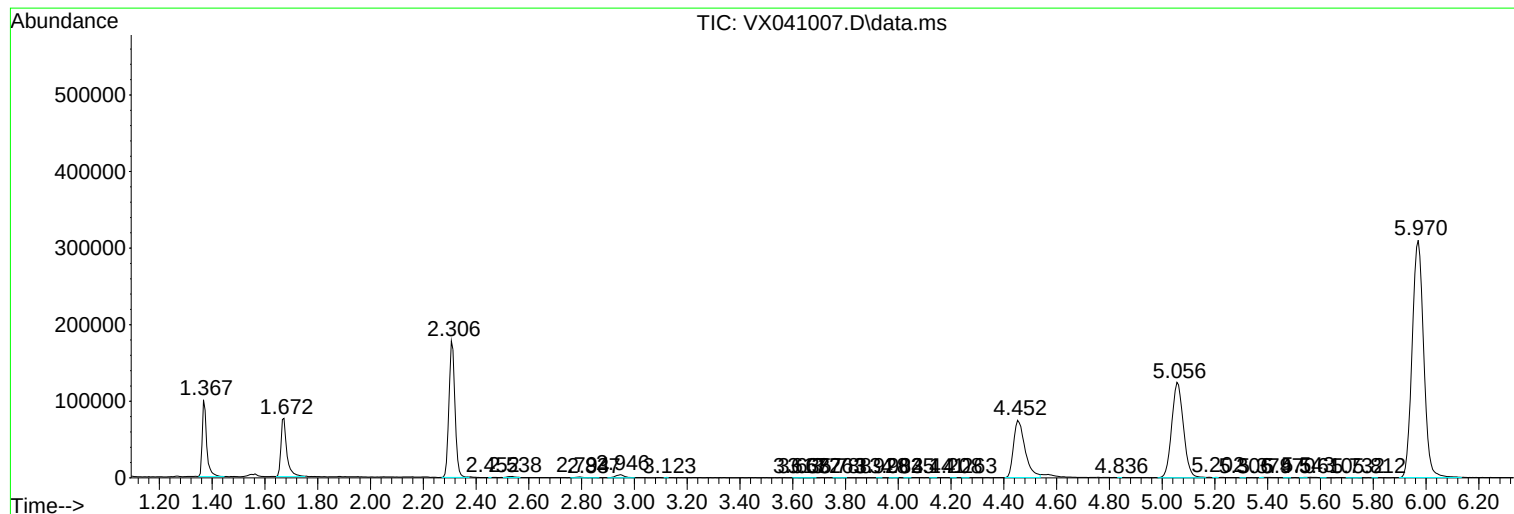

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX041007.D
Acq On : 12 Apr 2024 03:46
Operator : JC/MD
Sample : P2049-14 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX041007.D
Acq On : 12 Apr 2024 03:46
Operator : JC/MD
Sample : P2049-14 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------