

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041125\
 Data File : VX045735.D
 Acq On : 11 Apr 2025 12:45
 Operator : JC/MD
 Sample : Q1773-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TT190D2-GW-20250407

Quant Time: Apr 11 23:04:23 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 02 03:11:43 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	64518	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	124304	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	112481	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	44175	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	62219	52.734	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 105.460%			
35) Dibromofluoromethane	5.379	113	44969	50.989	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 101.980%			
50) Toluene-d8	8.647	98	155879	50.638	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 101.280%			
62) 4-Bromofluorobenzene	11.079	95	55472	49.472	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 98.940%			
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.166	85	404	0.419	ug/l	90
3) Chloromethane	1.300	50	243	0.245	ug/l #	42
5) Bromomethane	1.599	94	98	0.228	ug/l #	73
7) Trichlorofluoromethane	1.880	101	442	0.327	ug/l	91
9) 1,1,2-Trichlorotrifluo...	2.325	101	15502	19.557	ug/l	100
11) Tert butyl alcohol	2.946	59	278	1.753	ug/l #	72
12) 1,1-Dichloroethene	2.312	96	2976	3.842	ug/l	94
16) Acetone	2.379	43	575	1.187	ug/l #	88
17) Carbon Disulfide	2.508	76	654	0.342	ug/l #	76
18) Methyl Acetate	2.709	43	452	0.405	ug/l #	64
24) 1,1-Dichloroethane	3.605	63	913	0.558	ug/l #	83
27) cis-1,2-Dichloroethene	4.489	96	1620	1.680	ug/l	99
30) Chloroform	5.092	83	744	0.442	ug/l	97
31) Cyclohexane	5.550	56	1945	1.344	ug/l #	1
32) 1,1,1-Trichloroethane	5.385	97	611	0.429	ug/l #	46
36) 1,1-Dichloropropene	5.550	75	6532	5.485	ug/l #	50
38) Carbon Tetrachloride	5.665	117	1233	0.958	ug/l	85
42) 1,2-Dichloroethane	6.098	62	557	0.371	ug/l #	78
44) Trichloroethene	7.123	130	112715	130.395	ug/l	92
49) 1,4-Dioxane	7.683	88	85	4.001	ug/l #	1
51) 4-Methyl-2-Pentanone	8.641	43	979	0.649	ug/l #	1
52) Toluene	8.720	92	445	0.202	ug/l	77
55) 1,1,2-Trichloroethane	9.165	97	341	0.389	ug/l #	67
60) Dibromochloromethane	9.275	129	245	0.256	ug/l #	10
64) Tetrachloroethene	9.281	164	211	0.266	ug/l #	59
76) 1,2,3-Trichloropropane	11.079	75	32537	30.196	ug/l #	37
81) trans-1,4-Dichloro-2-b...	11.079	75	32537	102.481	ug/l #	1
93) 1,2,4-Trichlorobenzene	13.603	180	284	0.345	ug/l #	74
95) Naphthalene	13.780	128	1588	0.518	ug/l #	79
96) 1,2,3-Trichlorobenzene	13.969	180	330	0.383	ug/l	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041125\
Data File : VX045735.D
Acq On : 11 Apr 2025 12:45
Operator : JC/MD
Sample : Q1773-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TT190D2-GW-20250407


Quant Time: Apr 11 23:04:23 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 02 03:11:43 2025
Response via : Initial Calibration

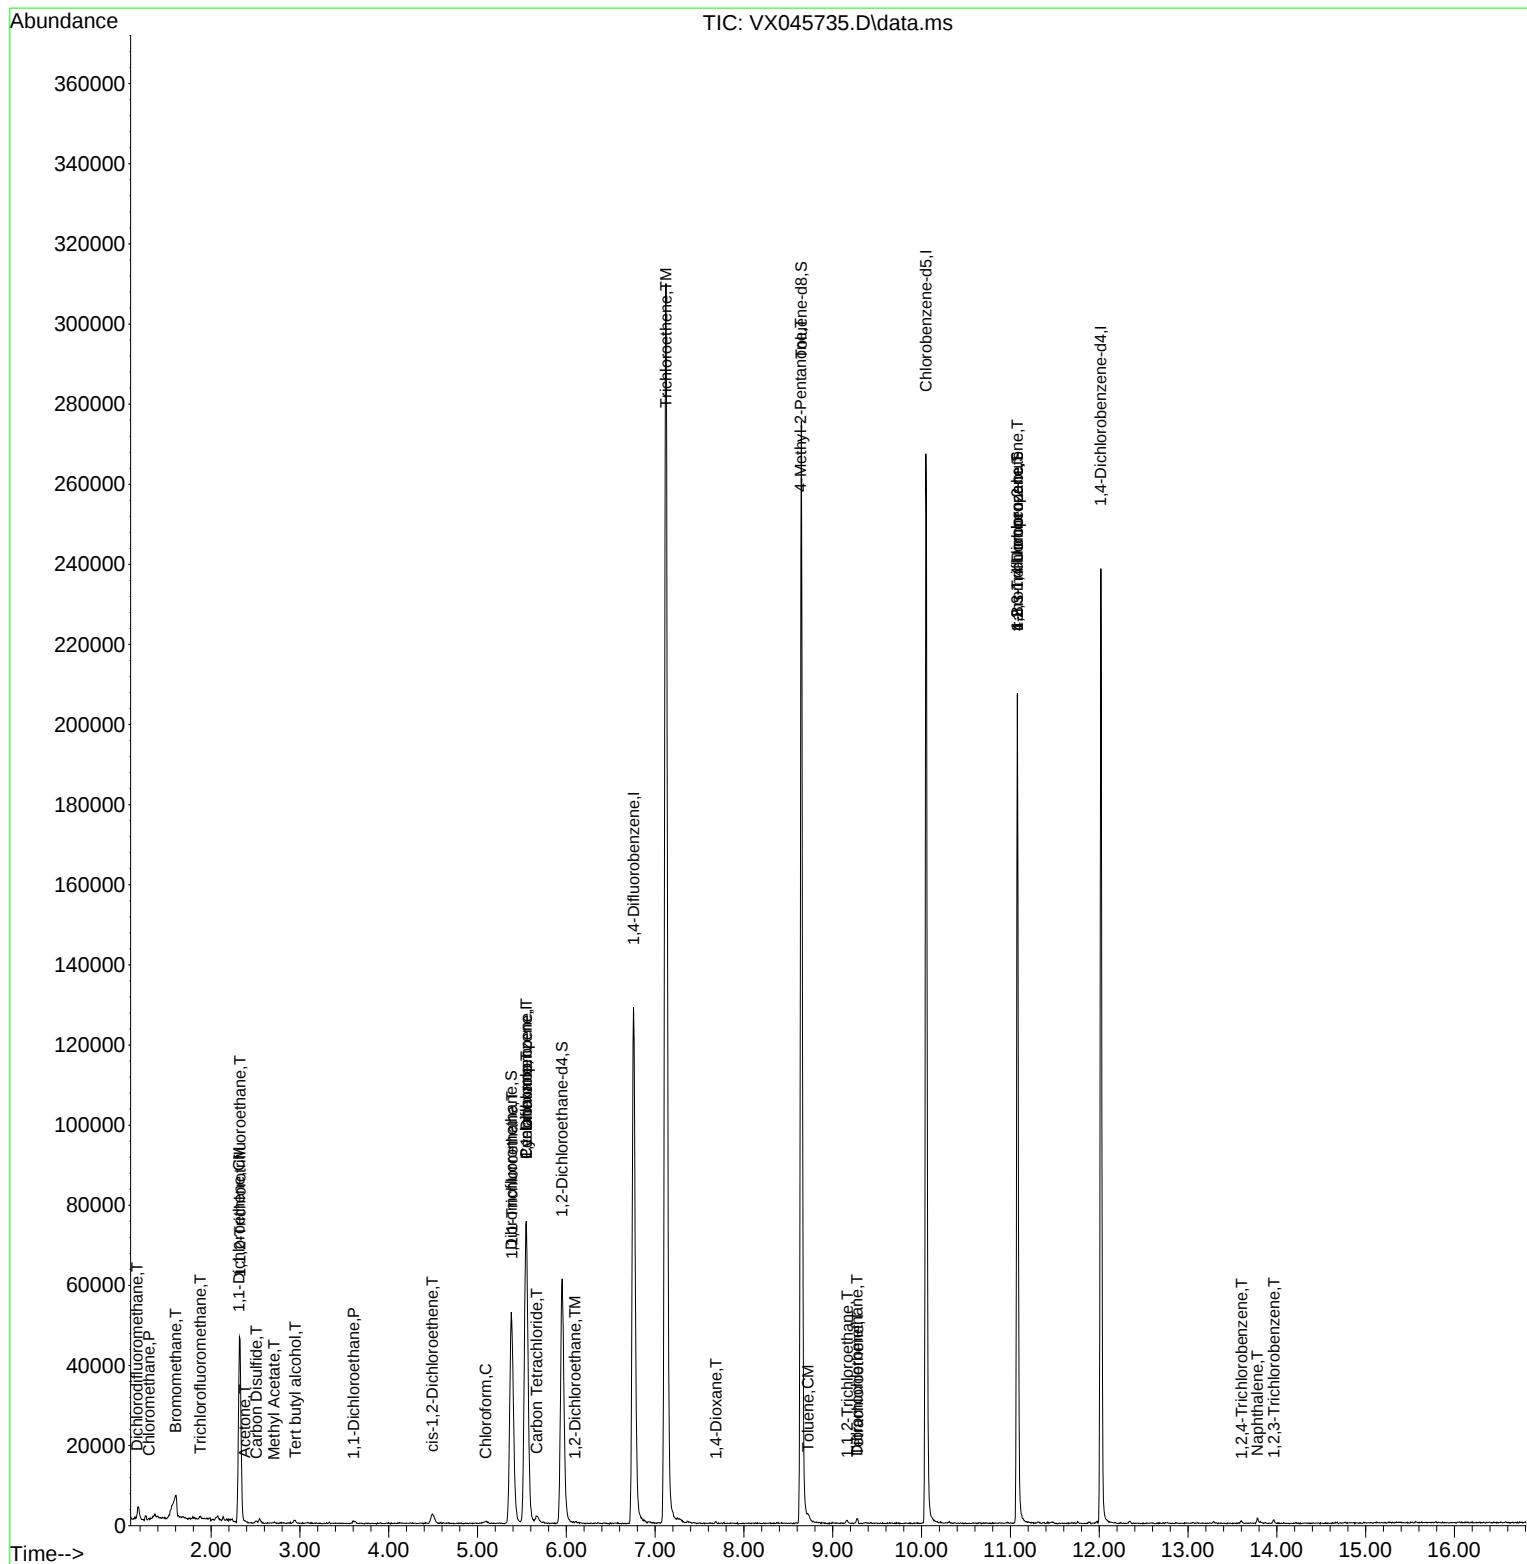






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX045735.D
Acq: 11 Apr 2025 12:45

Instrument :
MSVOA_X
ClientSampleId :
BP-TT190D2-GW-20250407







Tgt Ion:168 Resp: 64518
Ion Ratio Lower Upper
168 100
99 66.1 52.3 78.5



#2
Dichlorodifluoromethane
Concen: 0.419 ug/l
RT: 1.166 min Scan# 13
Delta R.T. -0.000 min
Lab File: VX045735.D
Acq: 11 Apr 2025 12:45

Tgt Ion: 85 Resp: 404
Ion Ratio Lower Upper
85 100
87 37.8 16.1 48.2







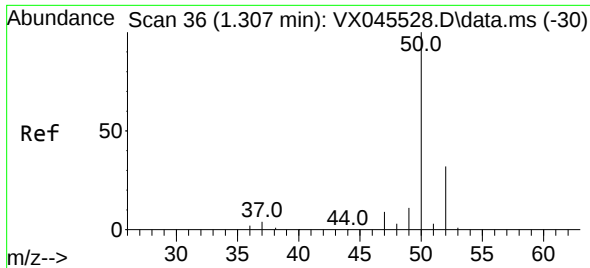

#3
Chloromethane
Concen: 0.245 ug/l
RT: 1.300 min Scan# 31
Delta R.T. -0.006 min
Lab File: VX045735.D
Acq: 11 Apr 2025 12:45




Instrument :
MSVOA_X
ClientSampleId :
BP-TT190D2-GW-20250407


Tgt Ion: 50 Resp: 243
Ion Ratio Lower Upper
50 100
52 0.0 25.9 38.9#

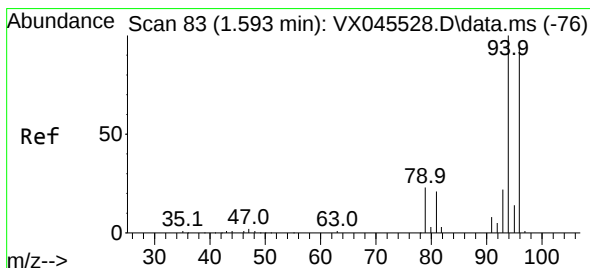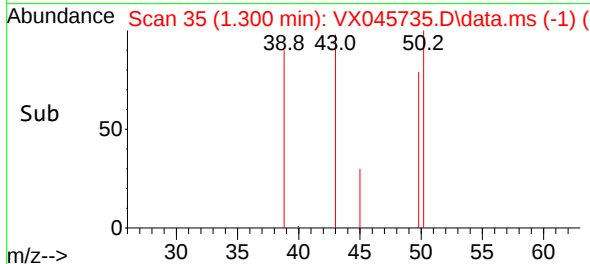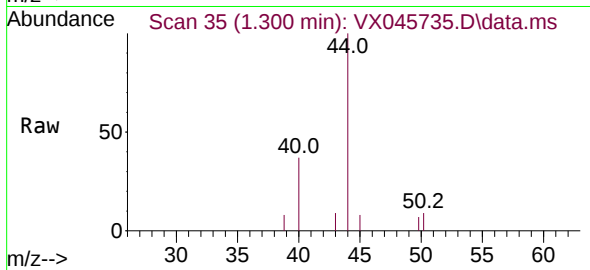

#5
Bromomethane
Concen: 0.228 ug/l
RT: 1.599 min Scan# 84
Delta R.T. 0.006 min
Lab File: VX045735.D
Acq: 11 Apr 2025 12:45

Tgt Ion: 94 Resp: 98
Ion Ratio Lower Upper
94 100
96 67.2 74.8 112.2#


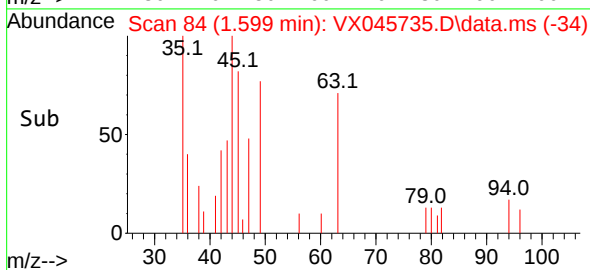

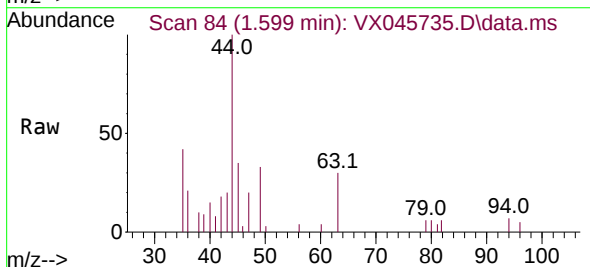




#7
 Trichlorofluoromethane
 Concen: 0.327 ug/l
 RT: 1.880 min Scan# 11
 Delta R.T. 0.006 min
 Lab File: VX045735.D
 Acq: 11 Apr 2025 12:45




Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TT190D2-GW-20250407


Tgt Ion:101 Resp: 442
 Ion Ratio Lower Upper
 101 100
 103 57.1 51.1 76.7



#9
 1,1,2-Trichlorotrifluoroethane
 Concen: 19.557 ug/l
 RT: 2.325 min Scan# 203
 Delta R.T. -0.000 min
 Lab File: VX045735.D
 Acq: 11 Apr 2025 12:45

Tgt Ion:101 Resp: 15502
 Ion Ratio Lower Upper
 101 100
 85 49.2 38.9 58.3
 151 71.9 57.5 86.3









#11
Tert butyl alcohol
Concen: 1.753 ug/l
RT: 2.946 min Scan# 305
Delta R.T. -0.031 min
Lab File: VX045735.D
Acq: 11 Apr 2025 12:45




Instrument : MSVOA_X
ClientSampleId : BP-TT190D2-GW-20250407


Tgt Ion: 59 Resp: 278
Ion Ratio Lower Upper
59 100
57 0.0 8.6 12.8#



#12
1,1-Dichloroethene
Concen: 3.842 ug/l
RT: 2.312 min Scan# 201
Delta R.T. -0.000 min
Lab File: VX045735.D
Acq: 11 Apr 2025 12:45

Tgt Ion: 96 Resp: 2976
Ion Ratio Lower Upper
96 100
61 188.0 145.7 218.5
98 72.5 51.6 77.4









#16
Acetone
Concen: 1.187 ug/l
RT: 2.379 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX045735.D
Acq: 11 Apr 2025 12:45




Instrument : MSVOA_X
ClientSampleId : BP-TT190D2-GW-20250407


Tgt Ion: 43 Resp: 575
Ion Ratio Lower Upper
43 100
58 21.6 22.3 33.5#



#17
Carbon Disulfide
Concen: 0.342 ug/l
RT: 2.508 min Scan# 233
Delta R.T. -0.000 min
Lab File: VX045735.D
Acq: 11 Apr 2025 12:45

Tgt Ion: 76 Resp: 654
Ion Ratio Lower Upper
76 100
78 0.0 7.0 10.6#









#18
Methyl Acetate
Concen: 0.405 ug/l
RT: 2.709 min Scan# 20
Delta R.T. 0.006 min
Lab File: VX045735.D
Acq: 11 Apr 2025 12:45




Instrument :
MSVOA_X
ClientSampleId :
BP-TT190D2-GW-20250407


Tgt Ion: 43 Resp: 452
Ion Ratio Lower Upper
43 100
74 4.6 17.5 26.3#



#24
1,1-Dichloroethane
Concen: 0.558 ug/l
RT: 3.605 min Scan# 413
Delta R.T. -0.000 min
Lab File: VX045735.D
Acq: 11 Apr 2025 12:45

Tgt Ion: 63 Resp: 913
Ion Ratio Lower Upper
63 100
98 0.0 3.4 10.1#
100 0.0 2.2 6.6#





#27

cis-1,2-Dichloroethene

Concen: 1.680 ug/l

RT: 4.489 min Scan# 51

Delta R.T. 0.006 min

Lab File: VX045735.D

Acq: 11 Apr 2025 12:45

Instrument :

MSVOA_X

ClientSampleId :

BP-TT190D2-GW-20250407





Tgt Ion: 96 Resp: 1620

Ion Ratio Lower Upper

96 100

61 156.9 0.0 313.2

98 60.4 0.0 126.4

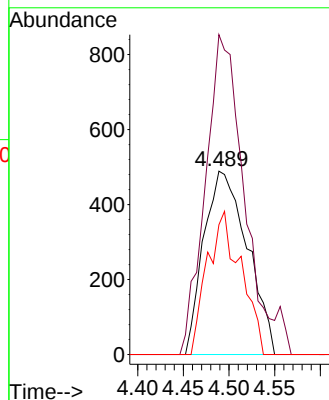

#30

Chloroform

Concen: 0.442 ug/l

RT: 5.092 min Scan# 657

Delta R.T. 0.006 min

Lab File: VX045735.D




Acq: 11 Apr 2025 12:45


Tgt Ion: 83 Resp: 744

Ion Ratio Lower Upper

83 100

85 68.7 52.8 79.2



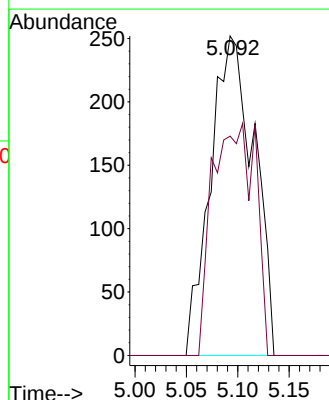





#31
Cyclohexane
Concen: 1.344 ug/l
RT: 5.550 min Scan# 718
Delta R.T. 0.085 min
Lab File: VX045735.D
Acq: 11 Apr 2025 12:45




Instrument :
MSVOA_X
ClientSampleId :
BP-TT190D2-GW-20250407


Tgt Ion: 56 Resp: 1945
Ion Ratio Lower Upper
56 100
69 167.3 23.6 35.4#
84 125.4 67.7 101.5#



#32
1,1,1-Trichloroethane
Concen: 0.429 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.006 min
Lab File: VX045735.D
Acq: 11 Apr 2025 12:45

Tgt Ion: 97 Resp: 611
Ion Ratio Lower Upper
97 100
99 0.0 51.7 77.5#
61 38.1 41.0 61.4#





#33

1,2-Dichloroethane-d4

Concen: 52.734 ug/l

RT: 5.952 min Scan# 798

Delta R.T. -0.000 min

Lab File: VX045735.D

Acq: 11 Apr 2025 12:45

Instrument :

MSVOA_X

ClientSampleId :





BP-TT190D2-GW-20250407

Tgt Ion: 65 Resp: 62219

Ion Ratio Lower Upper

65 100

67 49.3 0.0 99.0

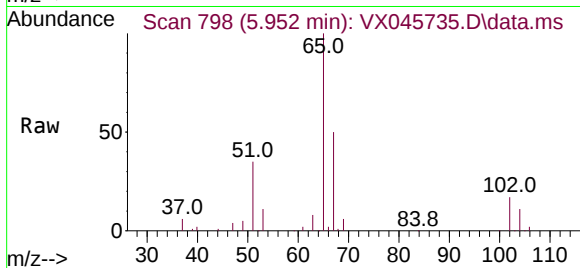

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. -0.000 min

Lab File: VX045735.D

Acq: 11 Apr 2025 12:45




Tgt Ion: 114 Resp: 124304


Ion Ratio Lower Upper

114 100

63 26.0 0.0 46.8

88 17.5 0.0 35.4




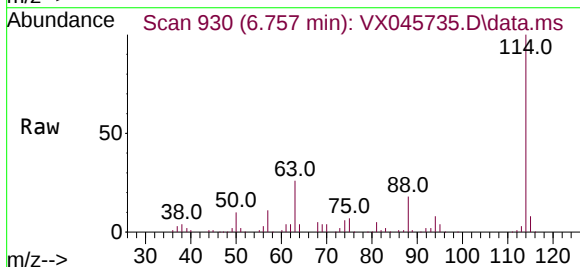




#35
Dibromofluoromethane
Concen: 50.989 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.000 min
Lab File: VX045735.D
Acq: 11 Apr 2025 12:45




Instrument :
MSVOA_X
ClientSampleId :
BP-TT190D2-GW-20250407


Tgt Ion:	113	Resp:	44969
Ion	Ratio	Lower	Upper
113	100		
111	104.1	81.8	122.6
192	16.5	13.8	20.6



#36
1,1-Dichloropropene
Concen: 5.485 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.134 min
Lab File: VX045735.D
Acq: 11 Apr 2025 12:45


Tgt Ion:	75	Resp:	6532
Ion	Ratio	Lower	Upper
75	100		
110	8.3	16.9	50.6#
77	0.0	25.0	37.4#

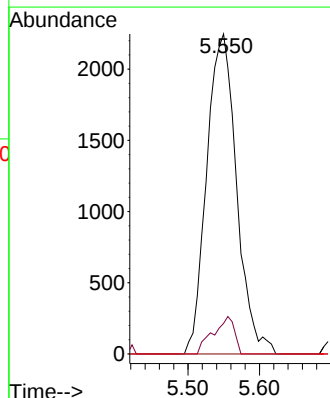






#38
Carbon Tetrachloride
Concen: 0.958 ug/l
RT: 5.665 min Scan# 751
Delta R.T. -0.006 min
Lab File: VX045735.D
Acq: 11 Apr 2025 12:45

Instrument :
MSVOA_X
ClientSampleId :
BP-TT190D2-GW-20250407







Tgt Ion:117 Resp: 1233
Ion Ratio Lower Upper
117 100
119 78.4 76.9 115.3
121 32.8 24.2 36.2

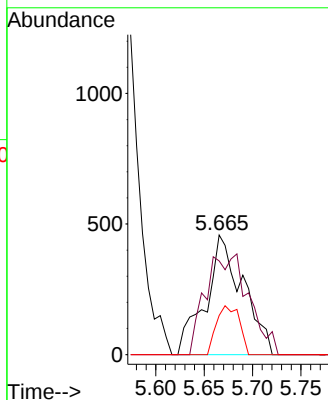

#42
1,2-Dichloroethane
Concen: 0.371 ug/l
RT: 6.098 min Scan# 822
Delta R.T. 0.018 min
Lab File: VX045735.D
Acq: 11 Apr 2025 12:45

Tgt Ion: 62 Resp: 557
Ion Ratio Lower Upper
62 100
98 0.0 0.0 15.2


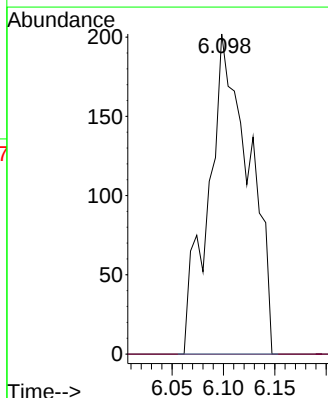
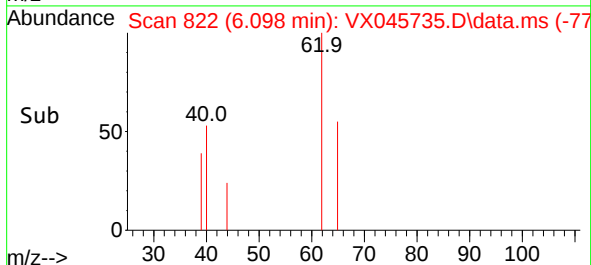
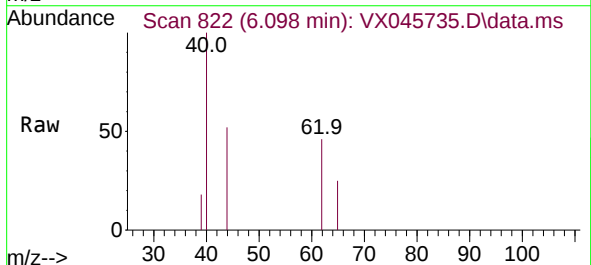




#44
Trichloroethene
Concen: 130.395 ug/l
RT: 7.123 min Scan# 990
Delta R.T. -0.000 min
Lab File: VX045735.D
Acq: 11 Apr 2025 12:45




Instrument :
MSVOA_X
ClientSampleId :
BP-TT190D2-GW-20250407


Tgt Ion:130 Resp: 112715
Ion Ratio Lower Upper
130 100
95 108.6 0.0 202.0



#49
1,4-Dioxane
Concen: 4.001 ug/l
RT: 7.683 min Scan# 1082
Delta R.T. 0.024 min
Lab File: VX045735.D
Acq: 11 Apr 2025 12:45

Tgt Ion: 88 Resp: 85
Ion Ratio Lower Upper
88 100
43 149.4 32.2 48.4#
58 200.0 58.6 88.0#









#50
Toluene-d8
Concen: 50.638 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX045735.D
Acq: 11 Apr 2025 12:45




Instrument :
MSVOA_X
ClientSampleId :
BP-TT190D2-GW-20250407


Tgt Ion: 98 Resp: 155879
Ion Ratio Lower Upper
98 100
100 64.8 52.2 78.4



#51
4-Methyl-2-Pentanone
Concen: 0.649 ug/l
RT: 8.641 min Scan# 1239
Delta R.T. 0.067 min
Lab File: VX045735.D
Acq: 11 Apr 2025 12:45

Tgt Ion: 43 Resp: 979
Ion Ratio Lower Upper
43 100
58 160.9 28.5 42.7#









#52
Toluene
Concen: 0.202 ug/l
RT: 8.720 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX045735.D
Acq: 11 Apr 2025 12:45




Instrument :
MSVOA_X
ClientSampleId :
BP-TT190D2-GW-20250407


Tgt Ion: 92 Resp: 445
Ion Ratio Lower Upper
92 100
91 205.4 138.7 208.1



#55
1,1,2-Trichloroethane
Concen: 0.389 ug/l
RT: 9.165 min Scan# 1325
Delta R.T. 0.018 min
Lab File: VX045735.D
Acq: 11 Apr 2025 12:45

Tgt Ion: 97 Resp: 341
Ion Ratio Lower Upper
97 100
83 57.3 71.8 107.8#
85 25.0 47.0 70.6#
99 75.4 48.6 73.0#









#60
Dibromochloromethane
Concen: 0.256 ug/l
RT: 9.275 min Scan# 1343
Delta R.T. -0.244 min
Lab File: VX045735.D
Acq: 11 Apr 2025 12:45




Instrument :
MSVOA_X
ClientSampleId :
BP-TT190D2-GW-20250407


Tgt Ion:129 Resp: 245
Ion Ratio Lower Upper
129 100
127 0.0 39.4 118.2#



#62
4-Bromofluorobenzene
Concen: 49.472 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX045735.D
Acq: 11 Apr 2025 12:45

Tgt Ion: 95 Resp: 55472
Ion Ratio Lower Upper
95 100
174 66.4 0.0 135.8
176 63.4 0.0 131.4





#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.049 min Scan# 1470

Delta R.T. -0.000 min

Lab File: VX045735.D

Acq: 11 Apr 2025 12:45

Instrument :

MSVOA_X

ClientSampleId :

BP-TT190D2-GW-20250407





Tgt Ion:117 Resp: 112481

Ion Ratio Lower Upper

117 100

82 61.1 49.2 73.8

119 30.9 25.1 37.7

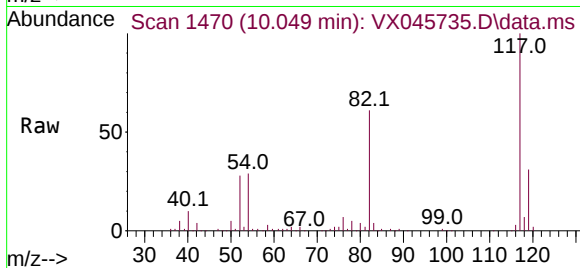

#64

Tetrachloroethene

Concen: 0.266 ug/l

RT: 9.281 min Scan# 1344

Delta R.T. 0.012 min

Lab File: VX045735.D

Acq: 11 Apr 2025 12:45

Tgt Ion:164 Resp: 211




Ion Ratio Lower Upper


164 100

166 93.8 103.8 155.8#

129 73.2 84.3 126.5#

131 37.5 80.9 121.3#



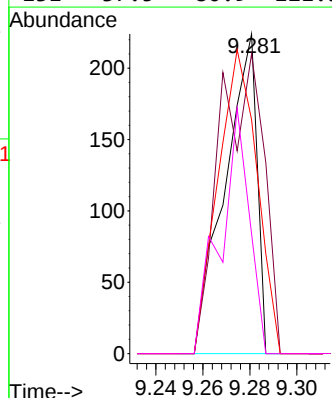
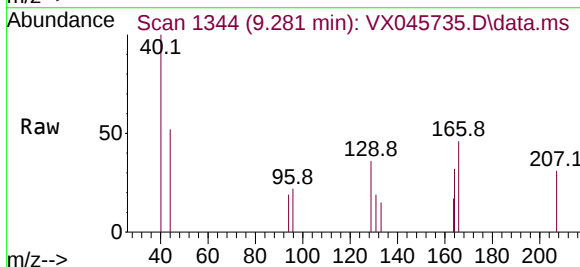




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.018 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: VX045735.D
 Acq: 11 Apr 2025 12:45




Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TT190D2-GW-20250407


Tgt Ion:152 Resp: 44175
 Ion Ratio Lower Upper
 152 100
 115 64.5 46.9 140.7
 150 156.5 0.0 349.4

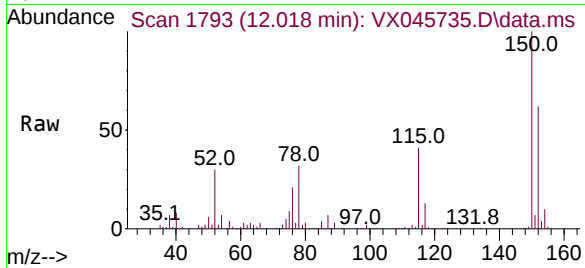

#76
 1,2,3-Trichloropropane
 Concen: 30.196 ug/l
 RT: 11.079 min Scan# 1639
 Delta R.T. -0.159 min
 Lab File: VX045735.D
 Acq: 11 Apr 2025 12:45

Tgt Ion: 75 Resp: 32537
 Ion Ratio Lower Upper
 75 100
 77 1.2 20.0 59.9#




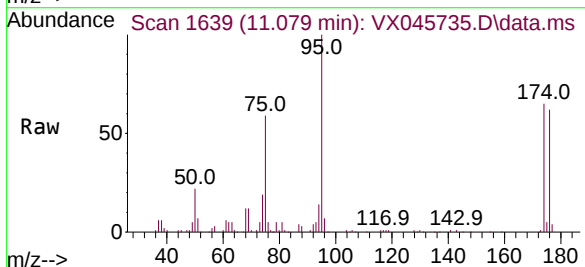




#81
trans-1,4-Dichloro-2-butene
Concen: 102.481 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX045735.D
Acq: 11 Apr 2025 12:45




Instrument :
MSVOA_X
ClientSampleId :
BP-TT190D2-GW-20250407


Tgt Ion: 75 Resp: 32537
Ion Ratio Lower Upper
75 100
53 0.0 101.8 152.6#
89 0.0 37.2 55.8#

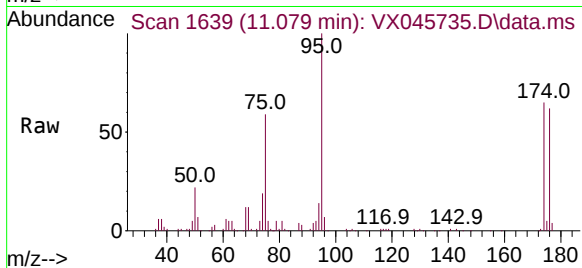

#93
1,2,4-Trichlorobenzene
Concen: 0.345 ug/l
RT: 13.603 min Scan# 2053
Delta R.T. 0.018 min
Lab File: VX045735.D
Acq: 11 Apr 2025 12:45

Tgt Ion:180 Resp: 284
Ion Ratio Lower Upper
180 100
182 83.5 47.9 143.6
145 0.0 17.9 53.8#

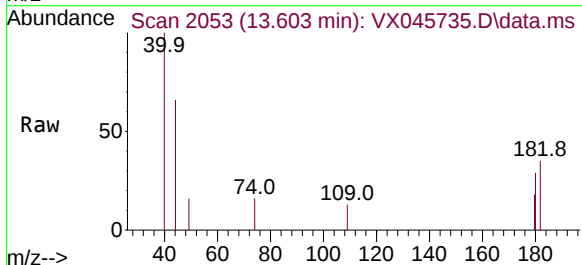



#95

Naphthalene

Concen: 0.518 ug/l

RT: 13.780 min Scan# 2081

Delta R.T. 0.006 min

Lab File: VX045735.D

Acq: 11 Apr 2025 12:45

Instrument :

MSVOA_X

ClientSampleId :

BP-TT190D2-GW-20250407





Tgt Ion:128 Resp: 1588

Ion Ratio Lower Upper

128 100

127 1.4 10.3 15.5#

129 6.1 8.6 12.8#

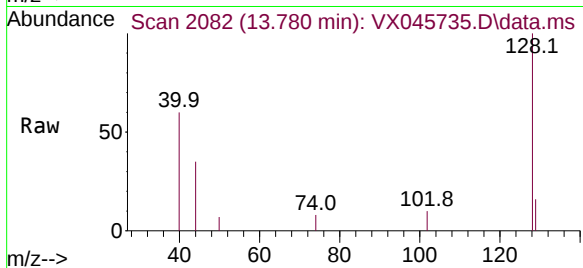

#96

1,2,3-Trichlorobenzene

Concen: 0.383 ug/l

RT: 13.969 min Scan# 2113

Delta R.T. 0.012 min

Lab File: VX045735.D

Acq: 11 Apr 2025 12:45

Tgt Ion:180 Resp: 330

Ion Ratio Lower Upper

180 100

182 85.8 47.3 141.8

145 29.1 18.2 54.6

