

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041125\
 Data File : VX045749.D
 Acq On : 11 Apr 2025 18:10
 Operator : JC/MD
 Sample : Q1790-04 20X
 Misc : 6.84g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S-871-G1-SO-23.0-23.5-041025

Quant Time: Apr 12 00:21:58 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 02 03:11:43 2025
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.544	168	62547	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	122428	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	114378	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	47831	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	61995	54.200	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 108.400%	
35) Dibromofluoromethane	5.385	113	43714	50.325	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 100.660%	
50) Toluene-d8	8.647	98	151283	49.898	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 99.800%	
62) 4-Bromofluorobenzene	11.079	95	57868	52.400	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 104.800%	
Target Compounds						Qvalue
20) Methylene Chloride	2.788	84	247	0.281	ug/l #	66
44) Trichloroethene	7.129	130	2315	2.719	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041125\
Data File : VX045749.D
Acq On : 11 Apr 2025 18:10
Operator : JC/MD
Sample : Q1790-04 20X
Misc : 6.84g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S-871-G1-SO-23.0-23.5-041025

Quant Time: Apr 12 00:21:58 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 02 03:11:43 2025
Response via : Initial Calibration




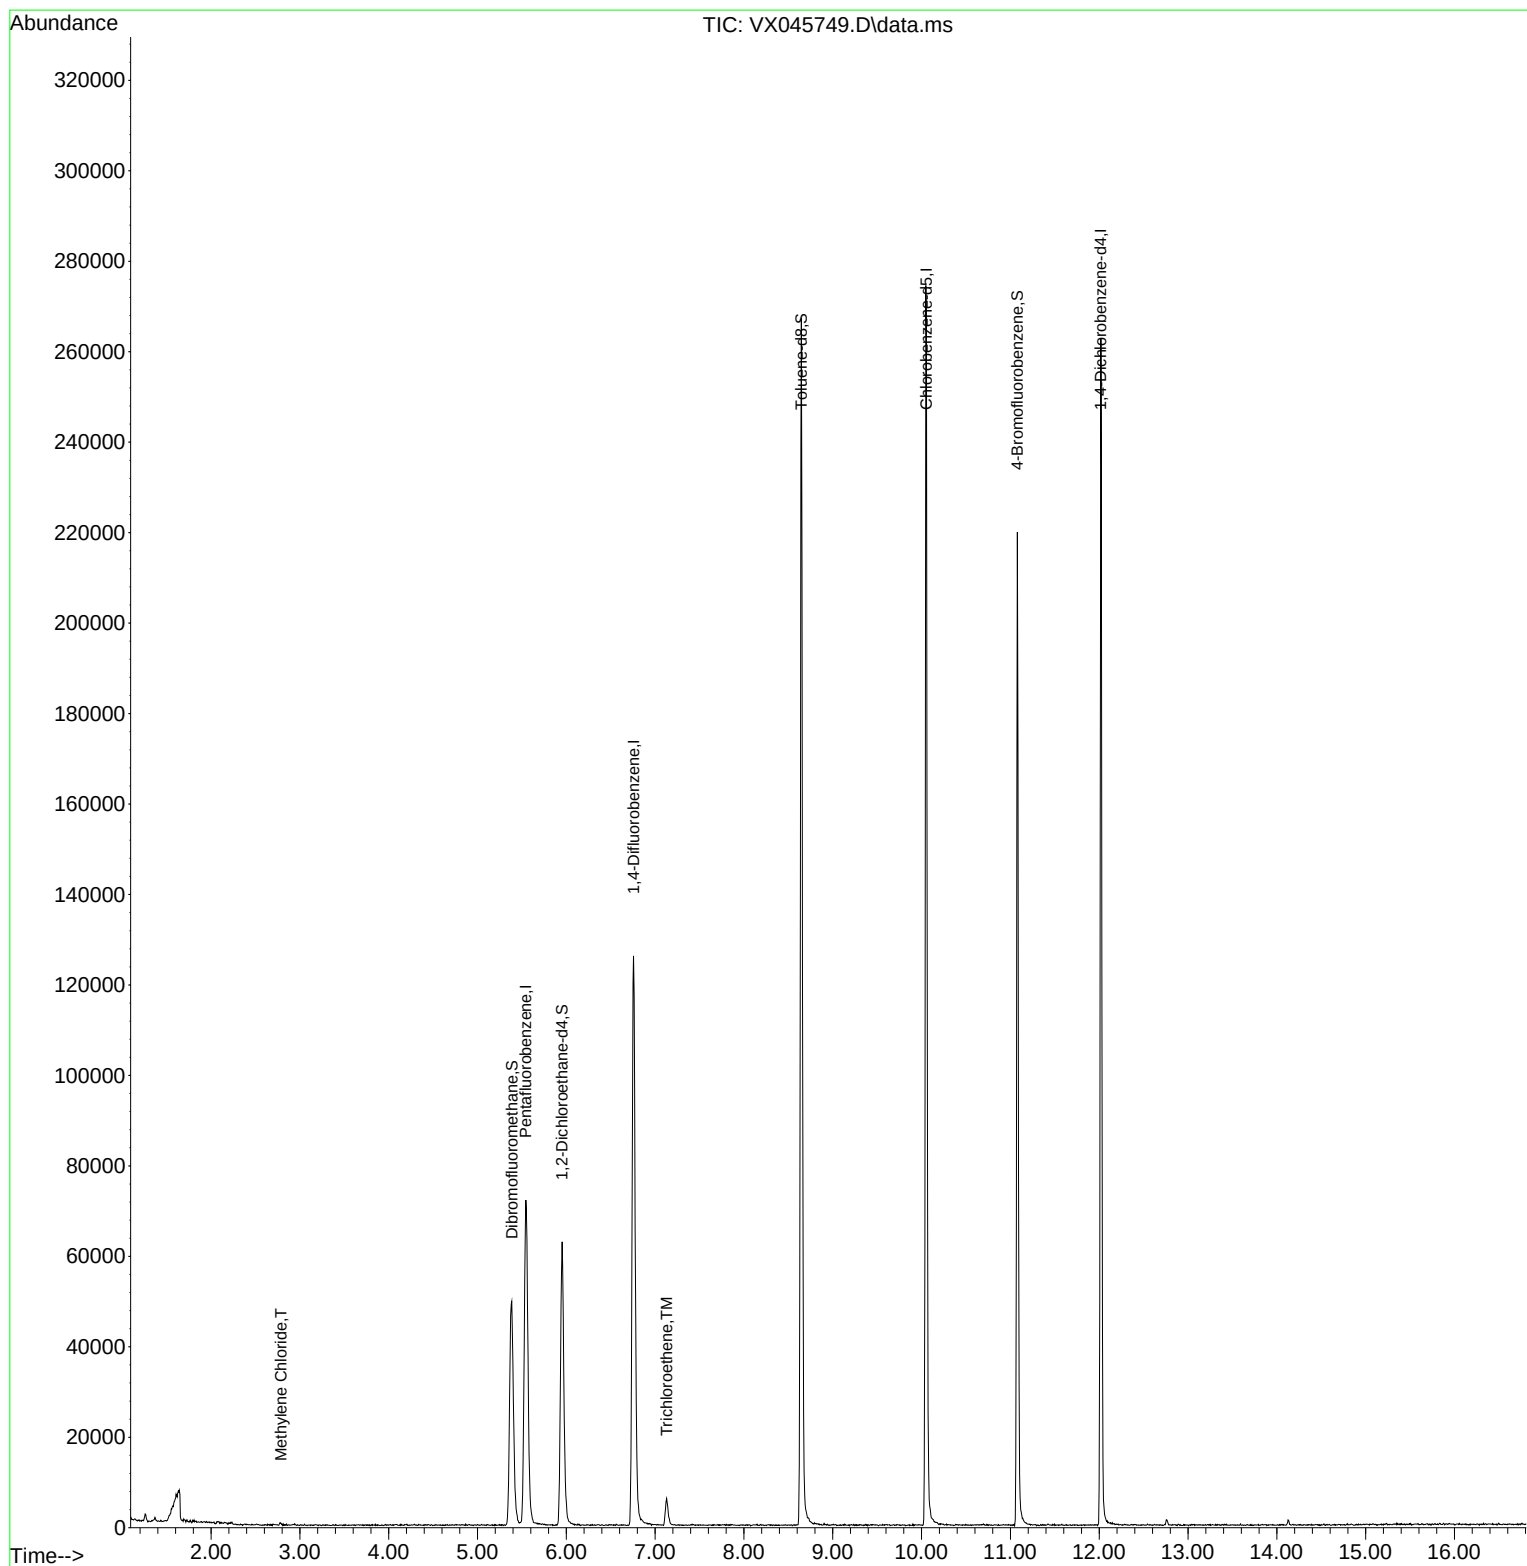


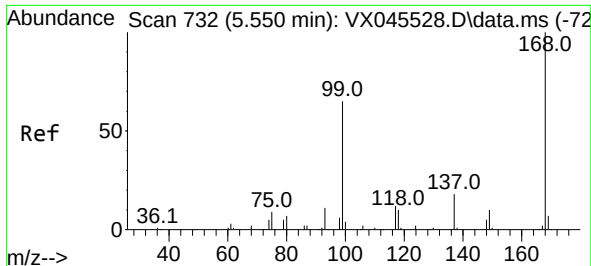

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.006 min
Lab File: VX045749.D
Acq: 11 Apr 2025 18:10




Instrument :
MSVOA_X
ClientSampleId :
S-871-G1-SO-23.0-23.5-041025


Tgt Ion:168 Resp: 62547
Ion Ratio Lower Upper
168 100
99 65.5 52.3 78.5

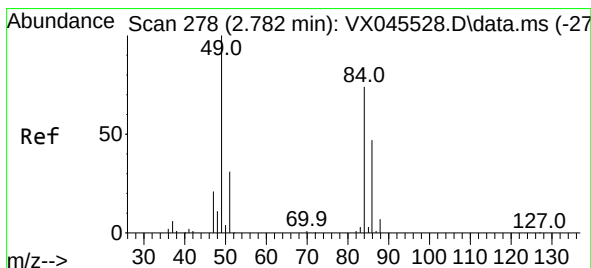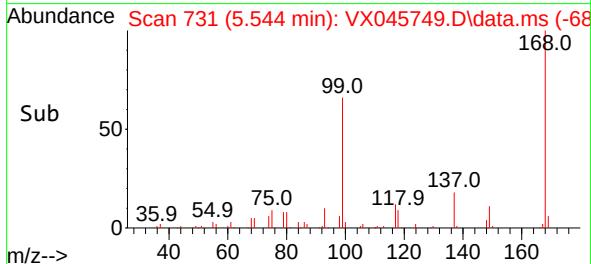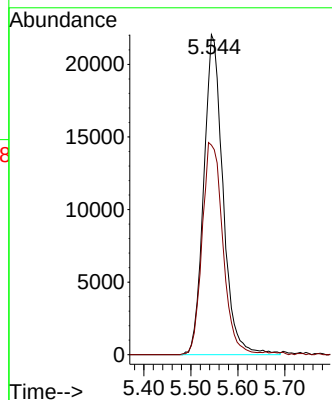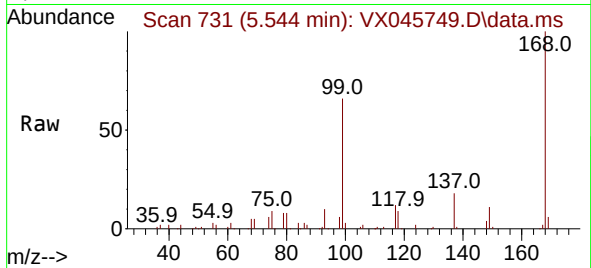

#20
Methylene Chloride
Concen: 0.281 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.006 min
Lab File: VX045749.D
Acq: 11 Apr 2025 18:10

Tgt Ion: 84 Resp: 247
Ion Ratio Lower Upper
84 100
49 97.1 107.5 161.3#
51 0.0 33.0 49.6#
86 47.1 50.1 75.1#


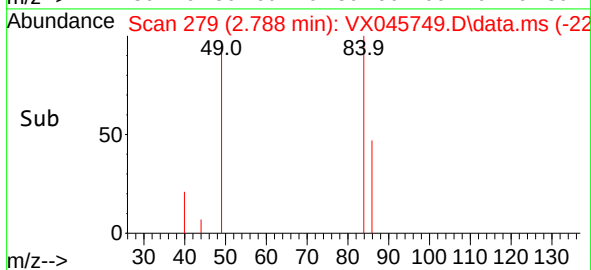
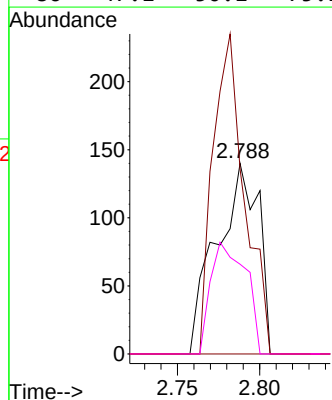
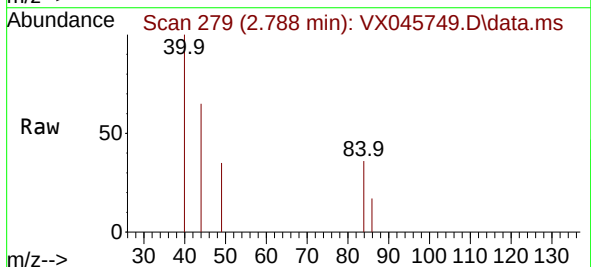


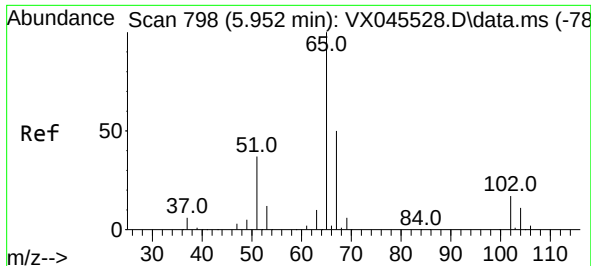

#33
 1,2-Dichloroethane-d4
 Concen: 54.200 ug/l
 RT: 5.952 min Scan# 798
 Delta R.T. -0.000 min
 Lab File: VX045749.D
 Acq: 11 Apr 2025 18:10




Instrument : MSVOA_X
 ClientSampleId : S-871-G1-SO-23.0-23.5-041025


Tgt Ion: 65 Resp: 61995
 Ion Ratio Lower Upper
 65 100
 67 49.6 0.0 99.0

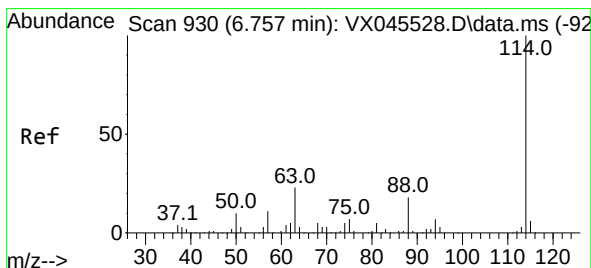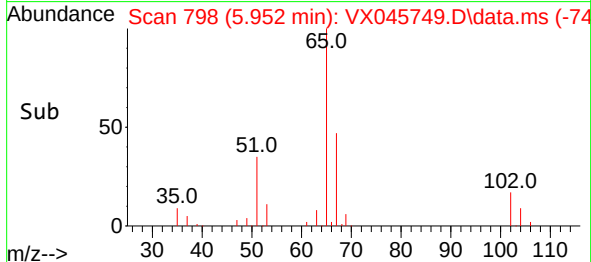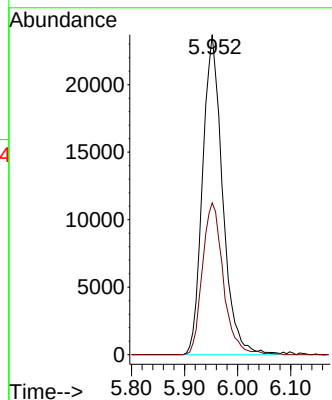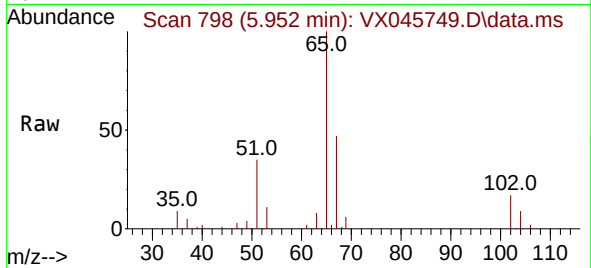

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.757 min Scan# 930
 Delta R.T. -0.000 min
 Lab File: VX045749.D
 Acq: 11 Apr 2025 18:10

Tgt Ion: 114 Resp: 122428
 Ion Ratio Lower Upper
 114 100
 63 24.5 0.0 46.8
 88 17.8 0.0 35.4


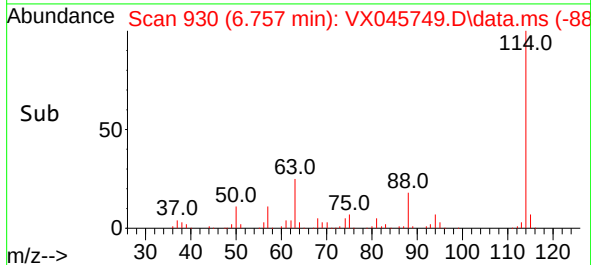
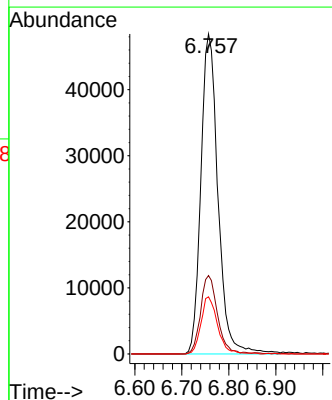
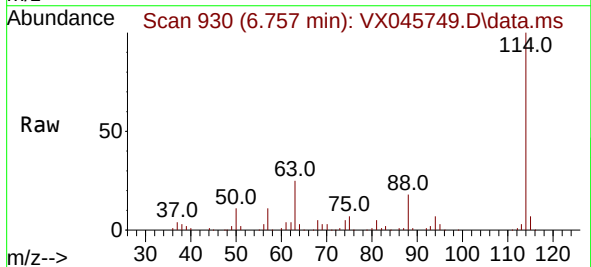


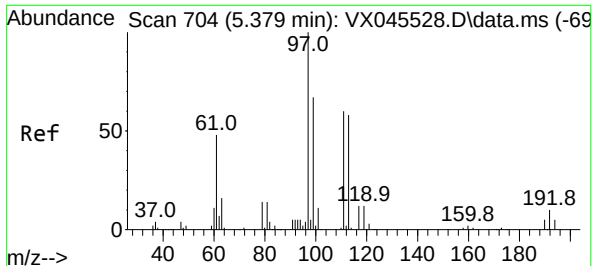

#35
Dibromofluoromethane
Concen: 50.325 ug/l
RT: 5.385 min Scan# 704
Delta R.T. 0.006 min
Lab File: VX045749.D
Acq: 11 Apr 2025 18:10




Instrument :
MSVOA_X
ClientSampleId :
S-871-G1-SO-23.0-23.5-041025


Tgt Ion:113 Resp: 43714
Ion Ratio Lower Upper
113 100
111 104.3 81.8 122.6
192 16.5 13.8 20.6

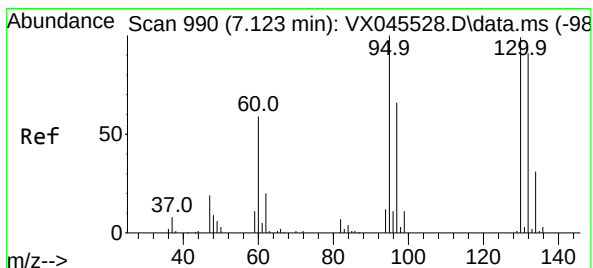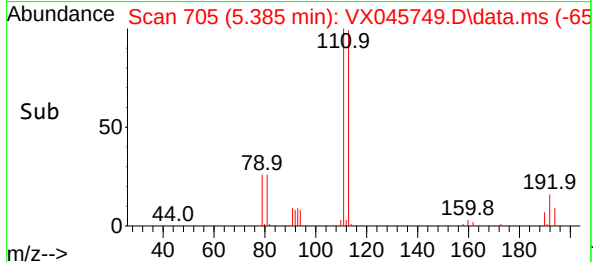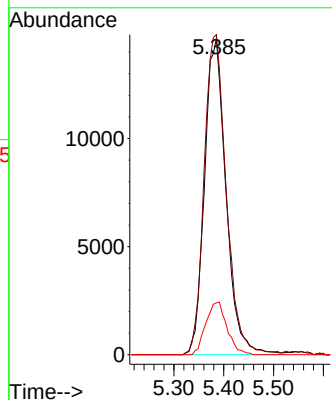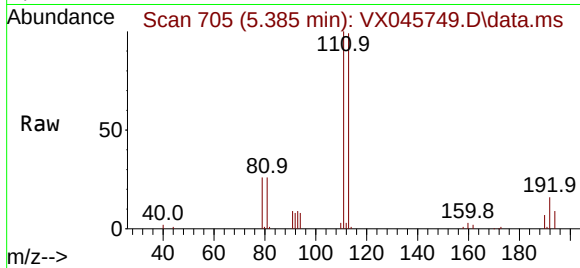

#44
Trichloroethene
Concen: 2.719 ug/l
RT: 7.129 min Scan# 991
Delta R.T. 0.006 min
Lab File: VX045749.D
Acq: 11 Apr 2025 18:10

Tgt Ion:130 Resp: 2315
Ion Ratio Lower Upper
130 100
95 98.2 0.0 202.0


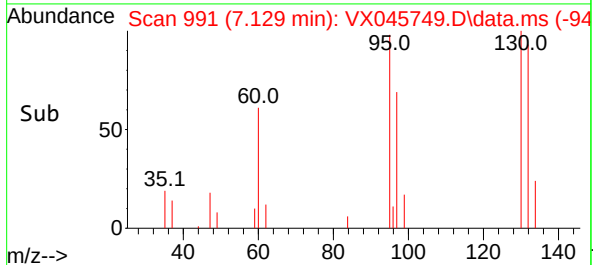
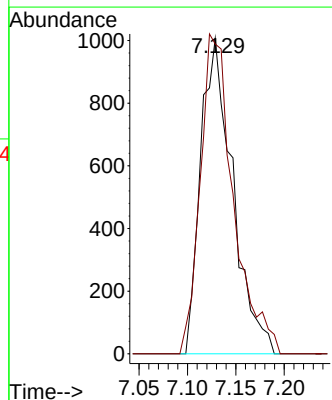
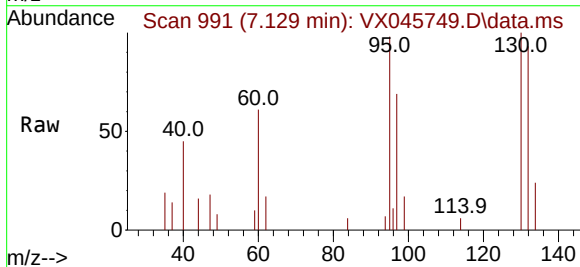


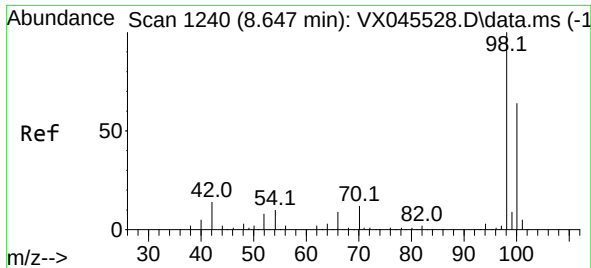

#50
Toluene-d8
Concen: 49.898 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX045749.D
Acq: 11 Apr 2025 18:10




Instrument :
MSVOA_X
ClientSampleId :
S-871-G1-SO-23.0-23.5-041025


Tgt Ion: 98 Resp: 151283
Ion Ratio Lower Upper
98 100
100 65.0 52.2 78.4

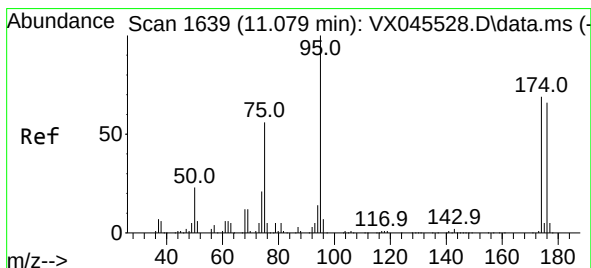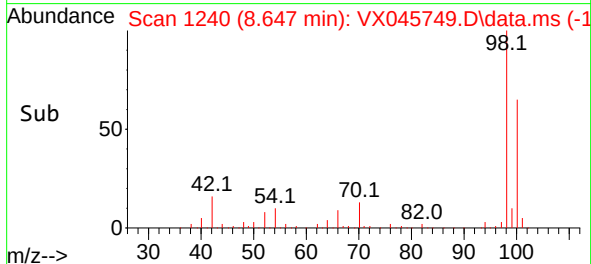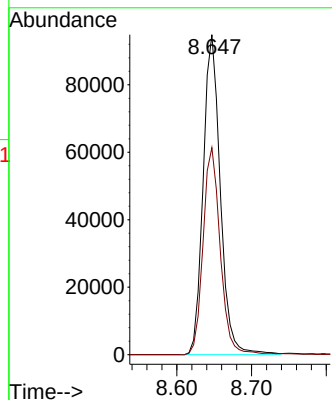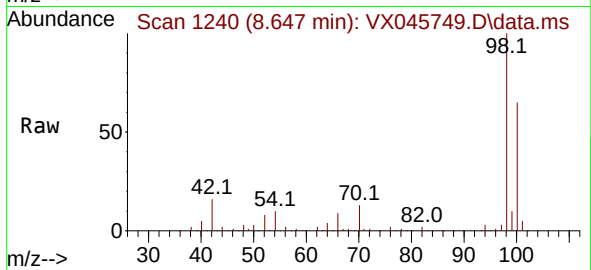

#62
4-Bromofluorobenzene
Concen: 52.400 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX045749.D
Acq: 11 Apr 2025 18:10

Tgt Ion: 95 Resp: 57868
Ion Ratio Lower Upper
95 100
174 66.2 0.0 135.8
176 65.1 0.0 131.4

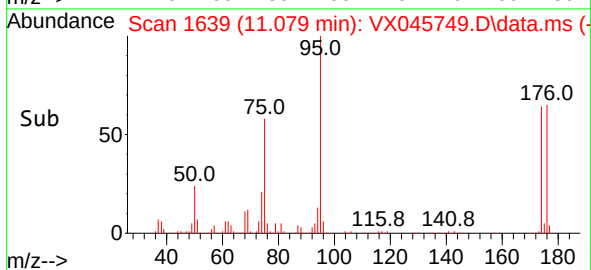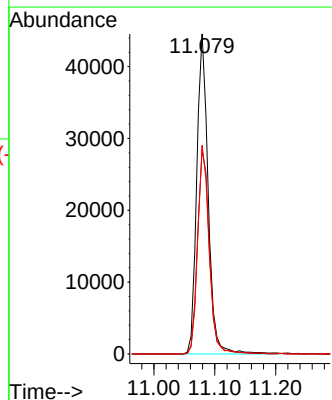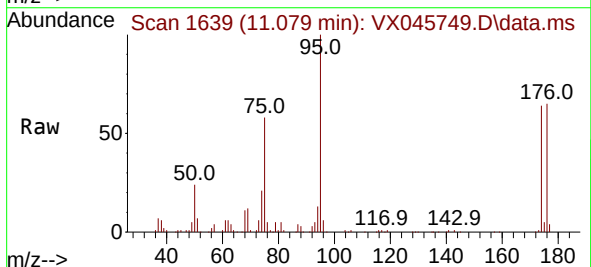

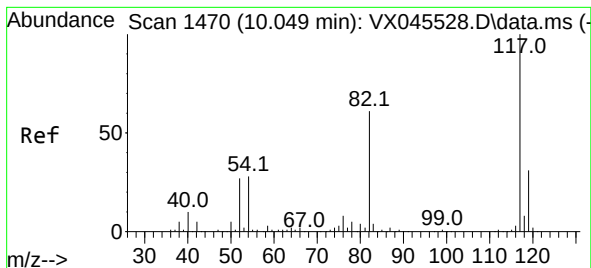

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1470

Delta R.T. 0.006 min

Lab File: VX045749.D

Acq: 11 Apr 2025 18:10

Instrument :

MSVOA_X

ClientSampleId :

S-871-G1-SO-23.0-23.5-041025





Tgt Ion:117 Resp: 114378

Ion Ratio Lower Upper

117 100

82 58.1 49.2 73.8

119 31.5 25.1 37.7

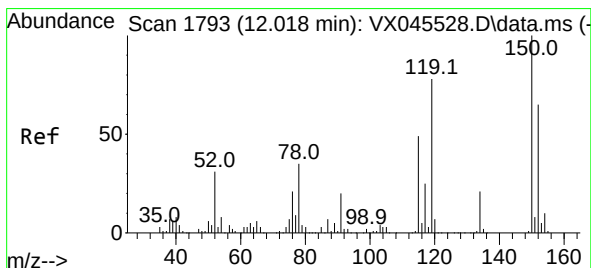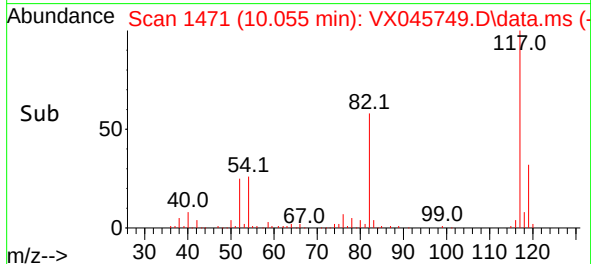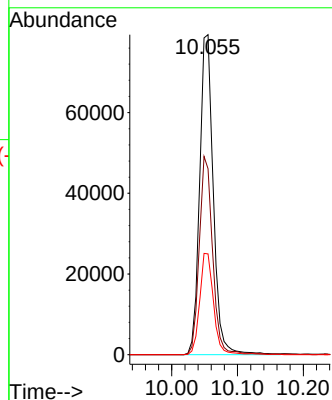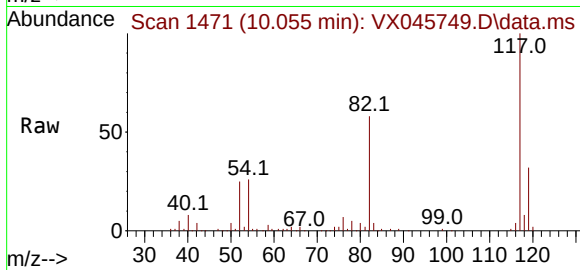

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. -0.000 min

Lab File: VX045749.D

Acq: 11 Apr 2025 18:10

Tgt Ion:152 Resp: 47831

Ion Ratio Lower Upper

152 100

115 66.0 46.9 140.7

150 159.3 0.0 349.4

