

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX041219\
 Data File : VX008883.D
 Acq On : 12 Apr 2019 13:57
 Operator : JC/SP
 Sample : K2366-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SA-PZ118S-20190409

Quant Time: Apr 13 05:28:51 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 04 04:47:41 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.66	168	195487	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	317040	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	277744	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	119800	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.06	65	129754	45.51	ug/l	0.00
Spiked Amount 50.000			Recovery	=	91.02%	
35) Dibromofluoromethane	5.50	113	93026	45.89	ug/l	0.00
Spiked Amount 50.000			Recovery	=	91.78%	
50) Toluene-d8	8.71	98	395509	49.00	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.00%	
62) 4-Bromofluorobenzene	11.13	95	134389	46.95	ug/l	0.00
Spiked Amount 50.000			Recovery	=	93.90%	
Target Compounds						
16) Acetone	2.44	43	4022	2.449	ug/l	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX041219\
Data File : VX008883.D
Acq On : 12 Apr 2019 13:57
Operator : JC/SP
Sample : K2366-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ118S-20190409

Quant Time: Apr 13 05:28:51 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
Quant Title : SW846 8260
QLast Update : Thu Apr 04 04:47:41 2019
Response via : Initial Calibration

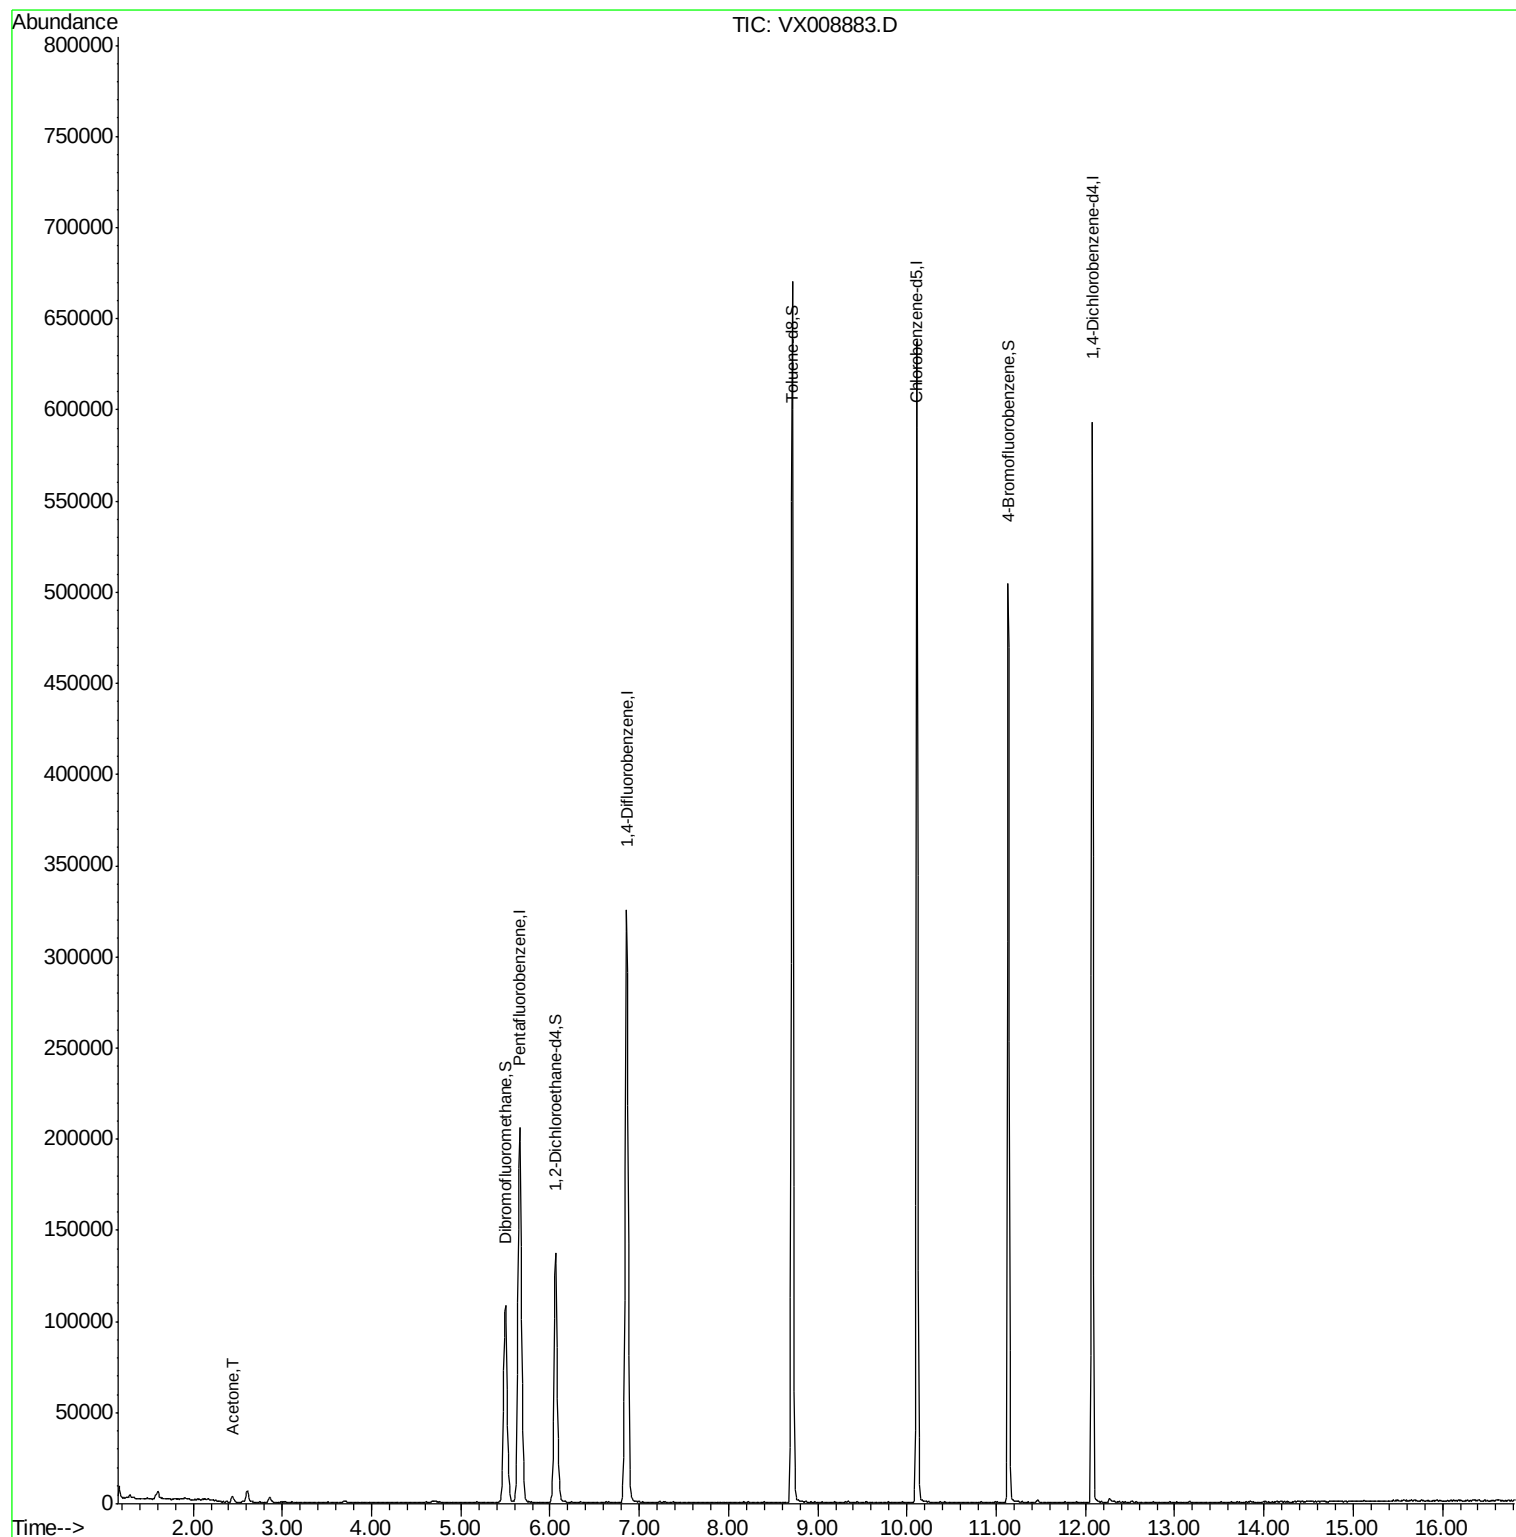

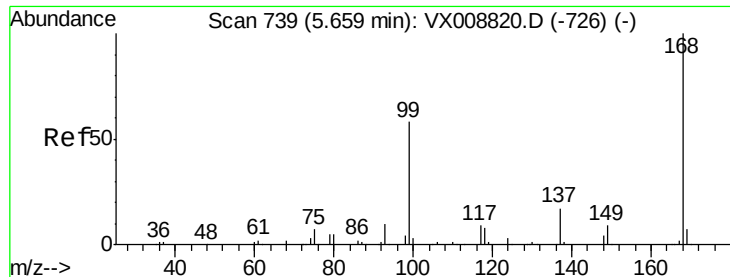

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.00 min

Lab File: VX008883.D

Acq: 12 Apr 2019 13:57

Instrument :

MSVOA_X

ClientSampleId :


SA-PZ118S-20190409

Tgt Ion:168 Resp: 195487

Ion Ratio Lower Upper

168 100

99 56.2 46.7 70.1

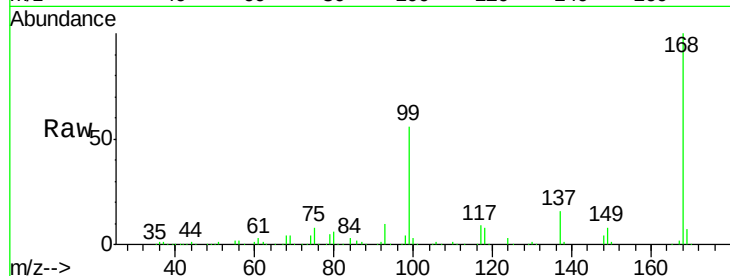

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.66

80000



60000

40000

20000

0

Time-->

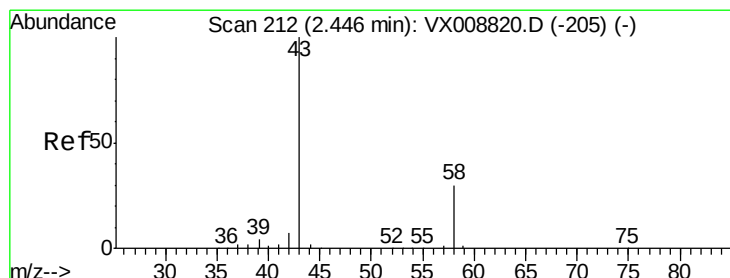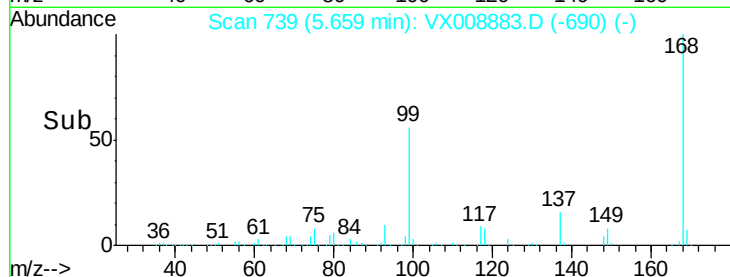

#16

Acetone

Concen: 2.449 ug/l

RT: 2.44 min Scan# 211

Delta R.T. -0.01 min

Lab File: VX008883.D


Acq: 12 Apr 2019 13:57

Tgt Ion: 43 Resp: 4022

Ion Ratio Lower Upper

43 100

58 27.0 24.8 37.2

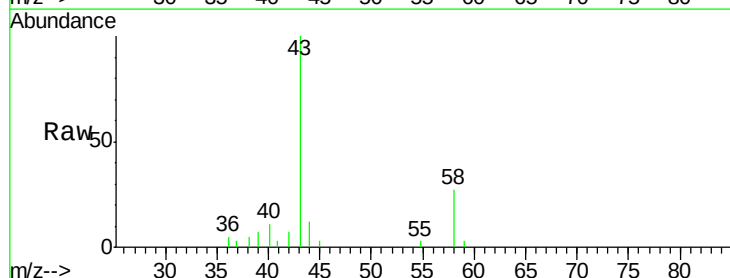

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

2.44

2500

2000


1500


1000

500

0

Time-->




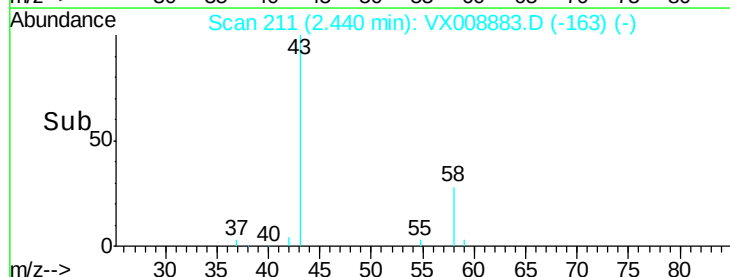


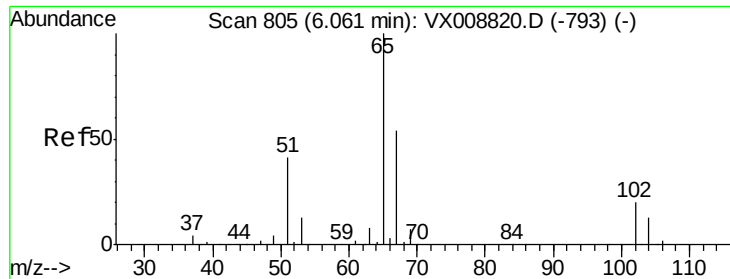

#33
 1,2-Dichloroethane-d4
 Concen: 45.507 ug/l
 RT: 6.06 min Scan# 805
 Delta R.T. -0.00 min
 Lab File: VX008883.D
 Acq: 12 Apr 2019 13:57




Instrument :
 MSVOA_X
 ClientSampleId :
 SA-PZ118S-20190409


Tgt Ion: 65 Resp: 129754
 Ion Ratio Lower Upper
 65 100
 67 53.7 0.0 107.2

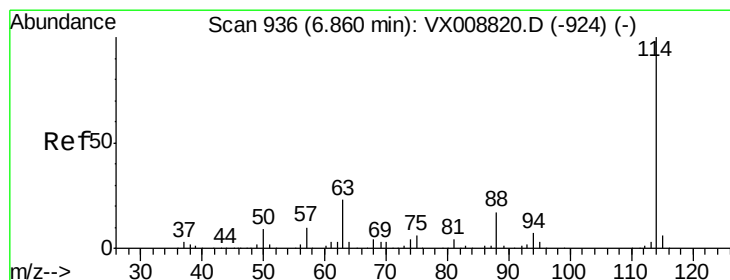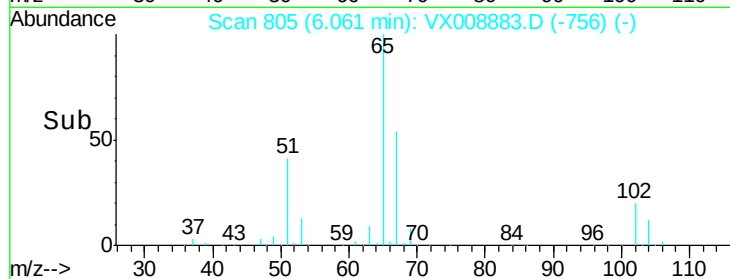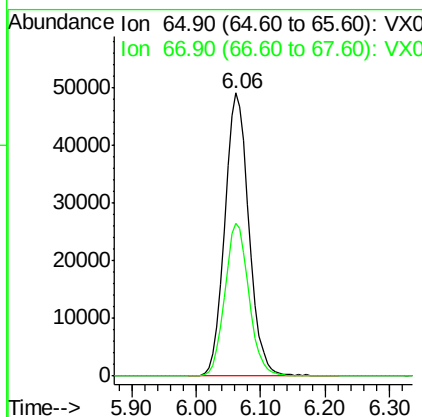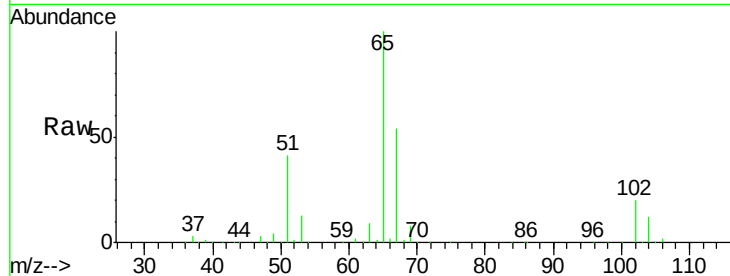

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.86 min Scan# 936
 Delta R.T. -0.00 min
 Lab File: VX008883.D
 Acq: 12 Apr 2019 13:57

Tgt Ion: 114 Resp: 317040
 Ion Ratio Lower Upper
 114 100
 63 22.1 0.0 47.2
 88 16.5 0.0 34.0


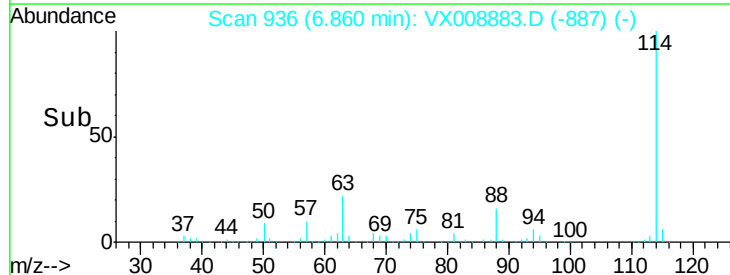
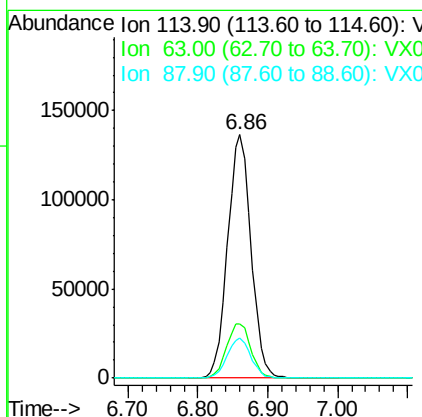
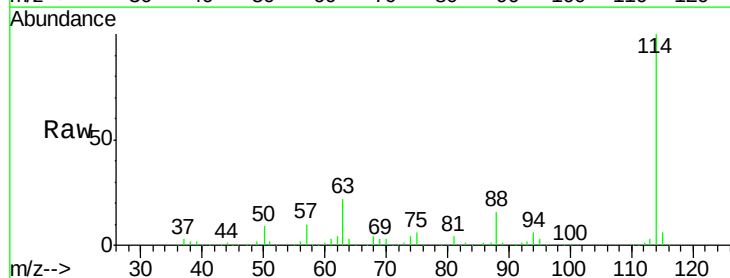


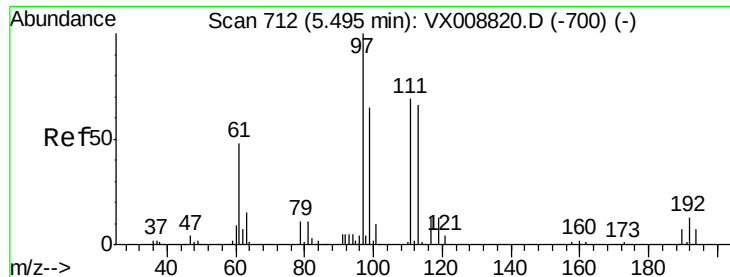

#35
 Dibromofluoromethane
 Concen: 45.893 ug/l
 RT: 5.50 min Scan# 713
 Delta R.T. -0.00 min
 Lab File: VX008883.D
 Acq: 12 Apr 2019 13:57




Instrument :
 MSVOA_X
 ClientSampleId :
 SA-PZ118S-20190409


Tgt Ion: 113 Resp: 93026
 Ion Ratio Lower Upper
 113 100
 111 102.1 83.4 125.2
 192 20.8 16.1 24.1

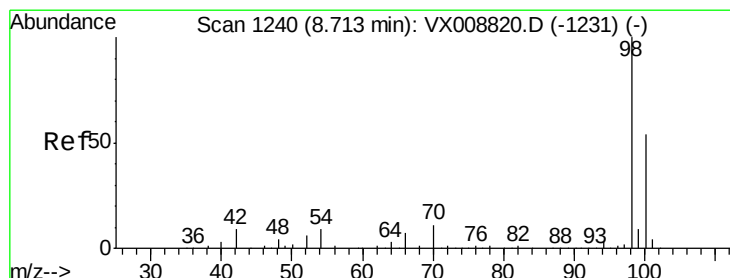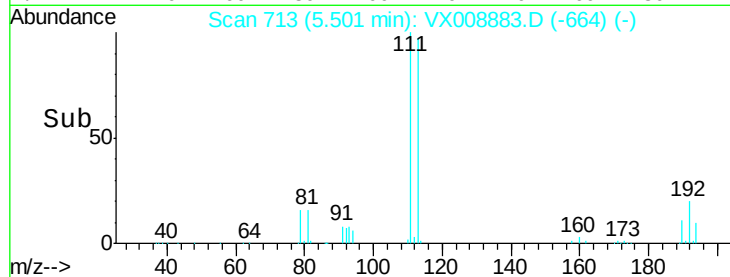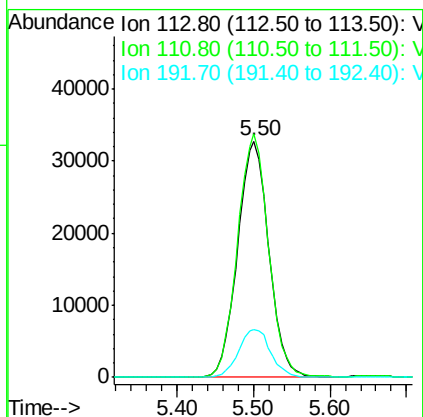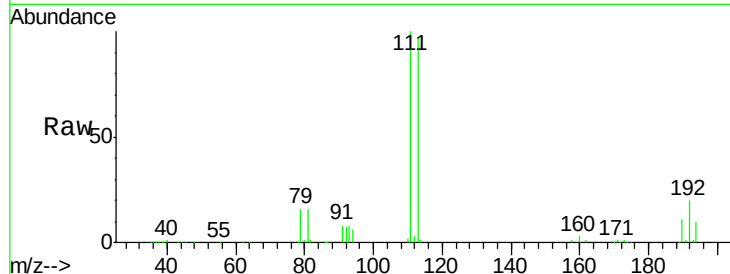

#50
 Toluene-d8
 Concen: 49.003 ug/l
 RT: 8.71 min Scan# 1240
 Delta R.T. -0.00 min
 Lab File: VX008883.D
 Acq: 12 Apr 2019 13:57

Tgt Ion: 98 Resp: 395509
 Ion Ratio Lower Upper
 98 100
 100 64.8 51.4 77.0

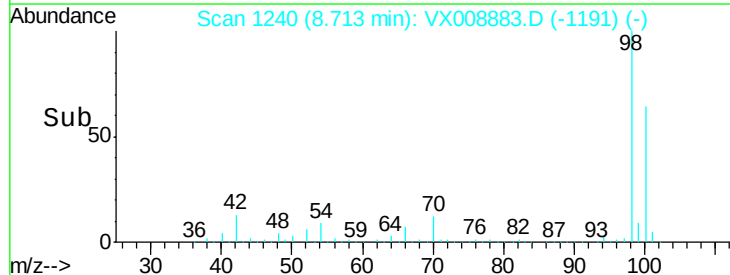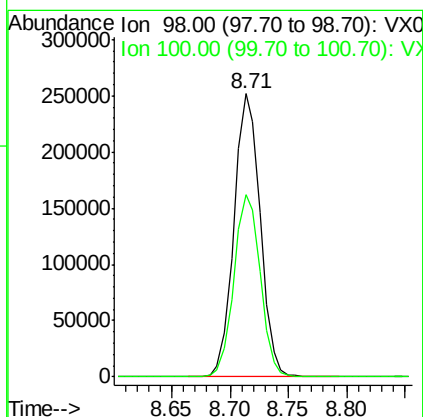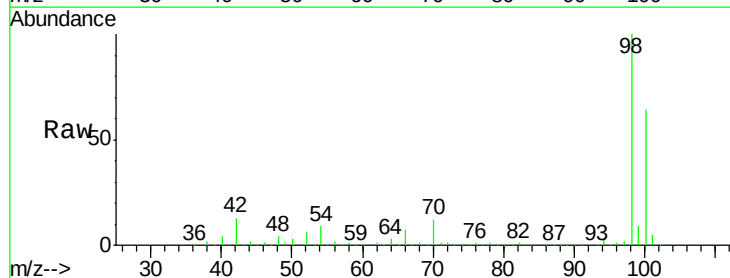

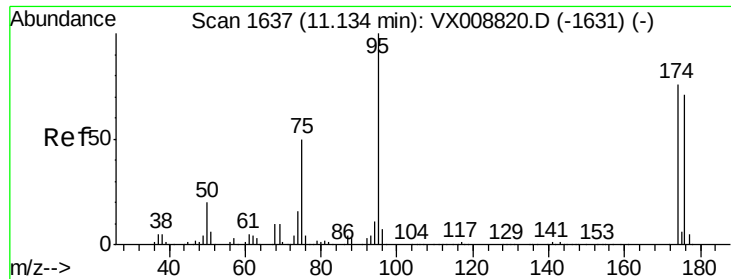

#62

4-Bromofluorobenzene

Concen: 46.954 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.00 min

Lab File: VX008883.D

Acq: 12 Apr 2019 13:57

Instrument :

MSVOA_X

ClientSampleId :

SA-PZ118S-20190409


Tgt Ion: 95 Resp: 134389

Ion Ratio Lower Upper

95 100

174 79.2 0.0 151.8




176 77.0 0.0 145.8

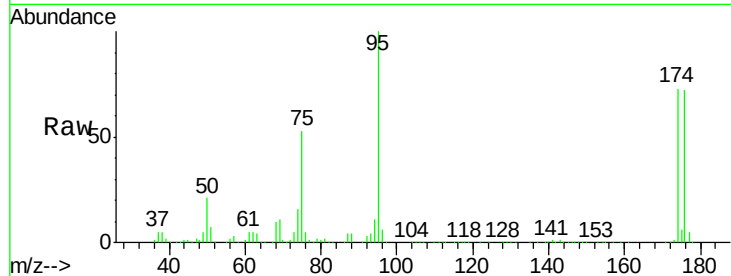

Abundance Ion 94.90 (94.60 to 95.60): VX008820.D (-1631) (-)

Ion 173.80 (173.50 to 174.50): VX008820.D (-1631) (-)

Ion 175.80 (175.50 to 176.50): VX008820.D (-1631) (-)

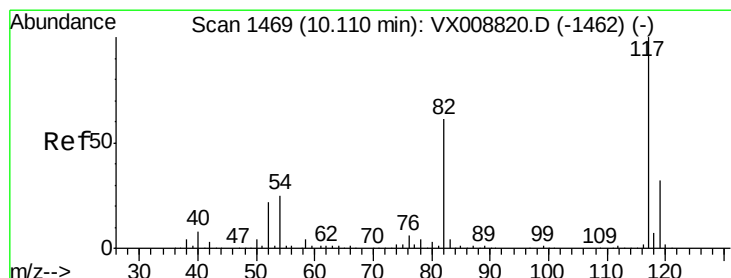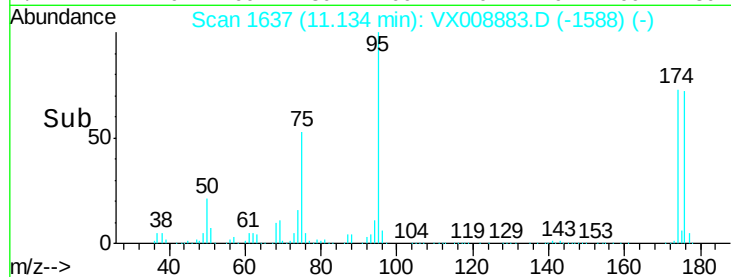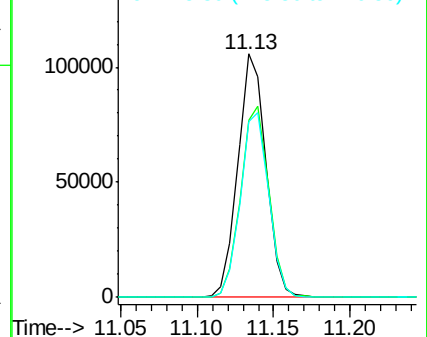

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.11 min Scan# 1469

Delta R.T. -0.00 min

Lab File: VX008883.D

Acq: 12 Apr 2019 13:57


Tgt Ion: 117 Resp: 277744

Ion Ratio Lower Upper

117 100

82 60.7 49.6 74.4



119 31.7 25.0 37.4

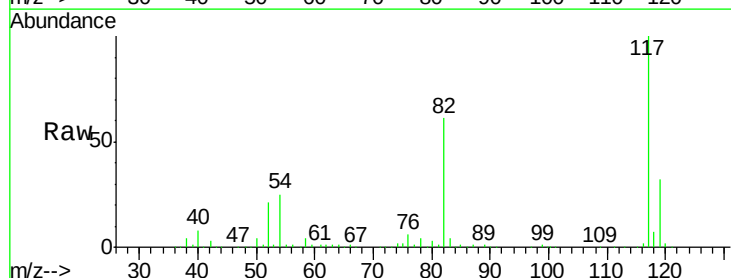


Abundance Ion 116.90 (116.60 to 117.60): VX008820.D (-1462) (-)

Ion 82.00 (81.70 to 82.70): VX008820.D (-1462) (-)

Ion 118.90 (118.60 to 119.60): VX008820.D (-1462) (-)

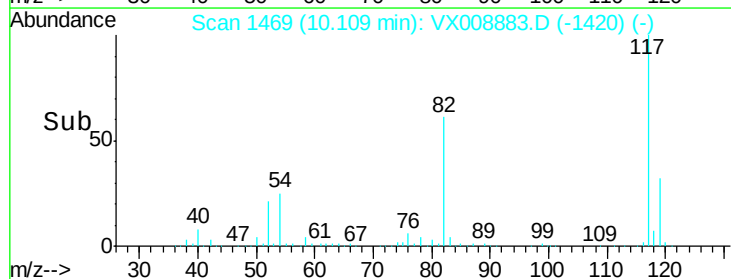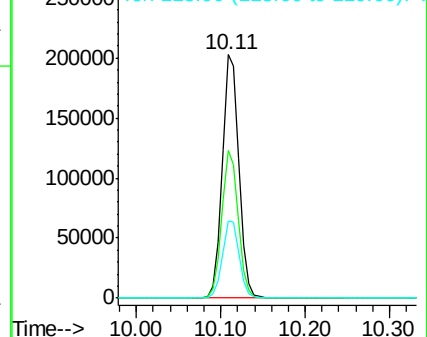


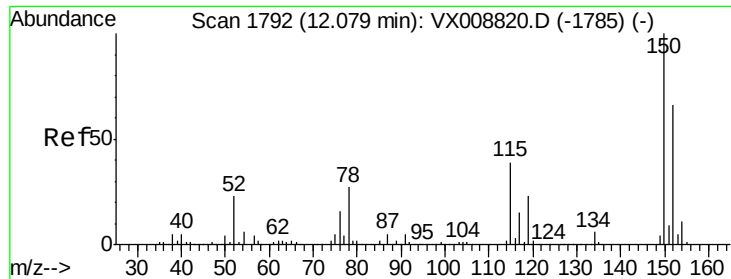

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.08 min Scan# 1792
 Delta R.T. -0.00 min
 Lab File: VX008883.D
 Acq: 12 Apr 2019 13:57

Instrument :
 MSVOA_X
 ClientSampleId :
 SA-PZ118S-20190409

Tgt Ion:152 Resp: 119800
 Ion Ratio Lower Upper
 152 100
 115 60.3 43.5 130.5
 150 156.3 0.0 348.8

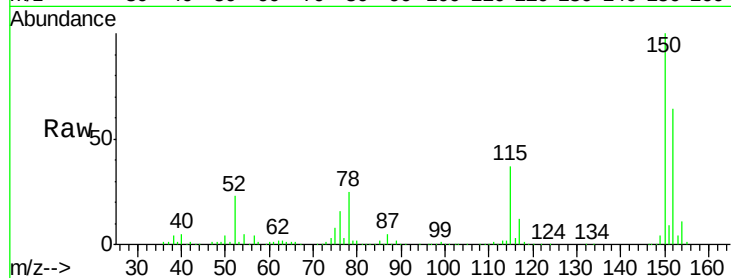

Abundance Ion 151.90 (151.60 to 152.60): V
 Ion 114.90 (114.60 to 115.60): V
 Ion 149.90 (149.60 to 150.60): V

