

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX041219\
 Data File : VX008893.D
 Acq On : 12 Apr 2019 17:51
 Operator : JC/SP
 Sample : K2366-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP01-20190409

Quant Time: Apr 13 05:53:24 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 04 04:47:41 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	193965	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	311251	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	267793	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	114153	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.06	65	128535	45.43	ug/l	0.00
Spiked Amount 50.000			Recovery	=	90.86%	
35) Dibromofluoromethane	5.50	113	93144	46.81	ug/l	0.00
Spiked Amount 50.000			Recovery	=	93.62%	
50) Toluene-d8	8.71	98	389033	49.10	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.20%	
62) 4-Bromofluorobenzene	11.13	95	128412	45.70	ug/l	0.00
Spiked Amount 50.000			Recovery	=	91.40%	
Target Compounds						
16) Acetone	2.44	43	4446	2.728	ug/l	Qvalue 92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX041219\
Data File : VX008893.D
Acq On : 12 Apr 2019 17:51
Operator : JC/SP
Sample : K2366-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP01-20190409

Quant Time: Apr 13 05:53:24 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
Quant Title : SW846 8260
QLast Update : Thu Apr 04 04:47:41 2019
Response via : Initial Calibration

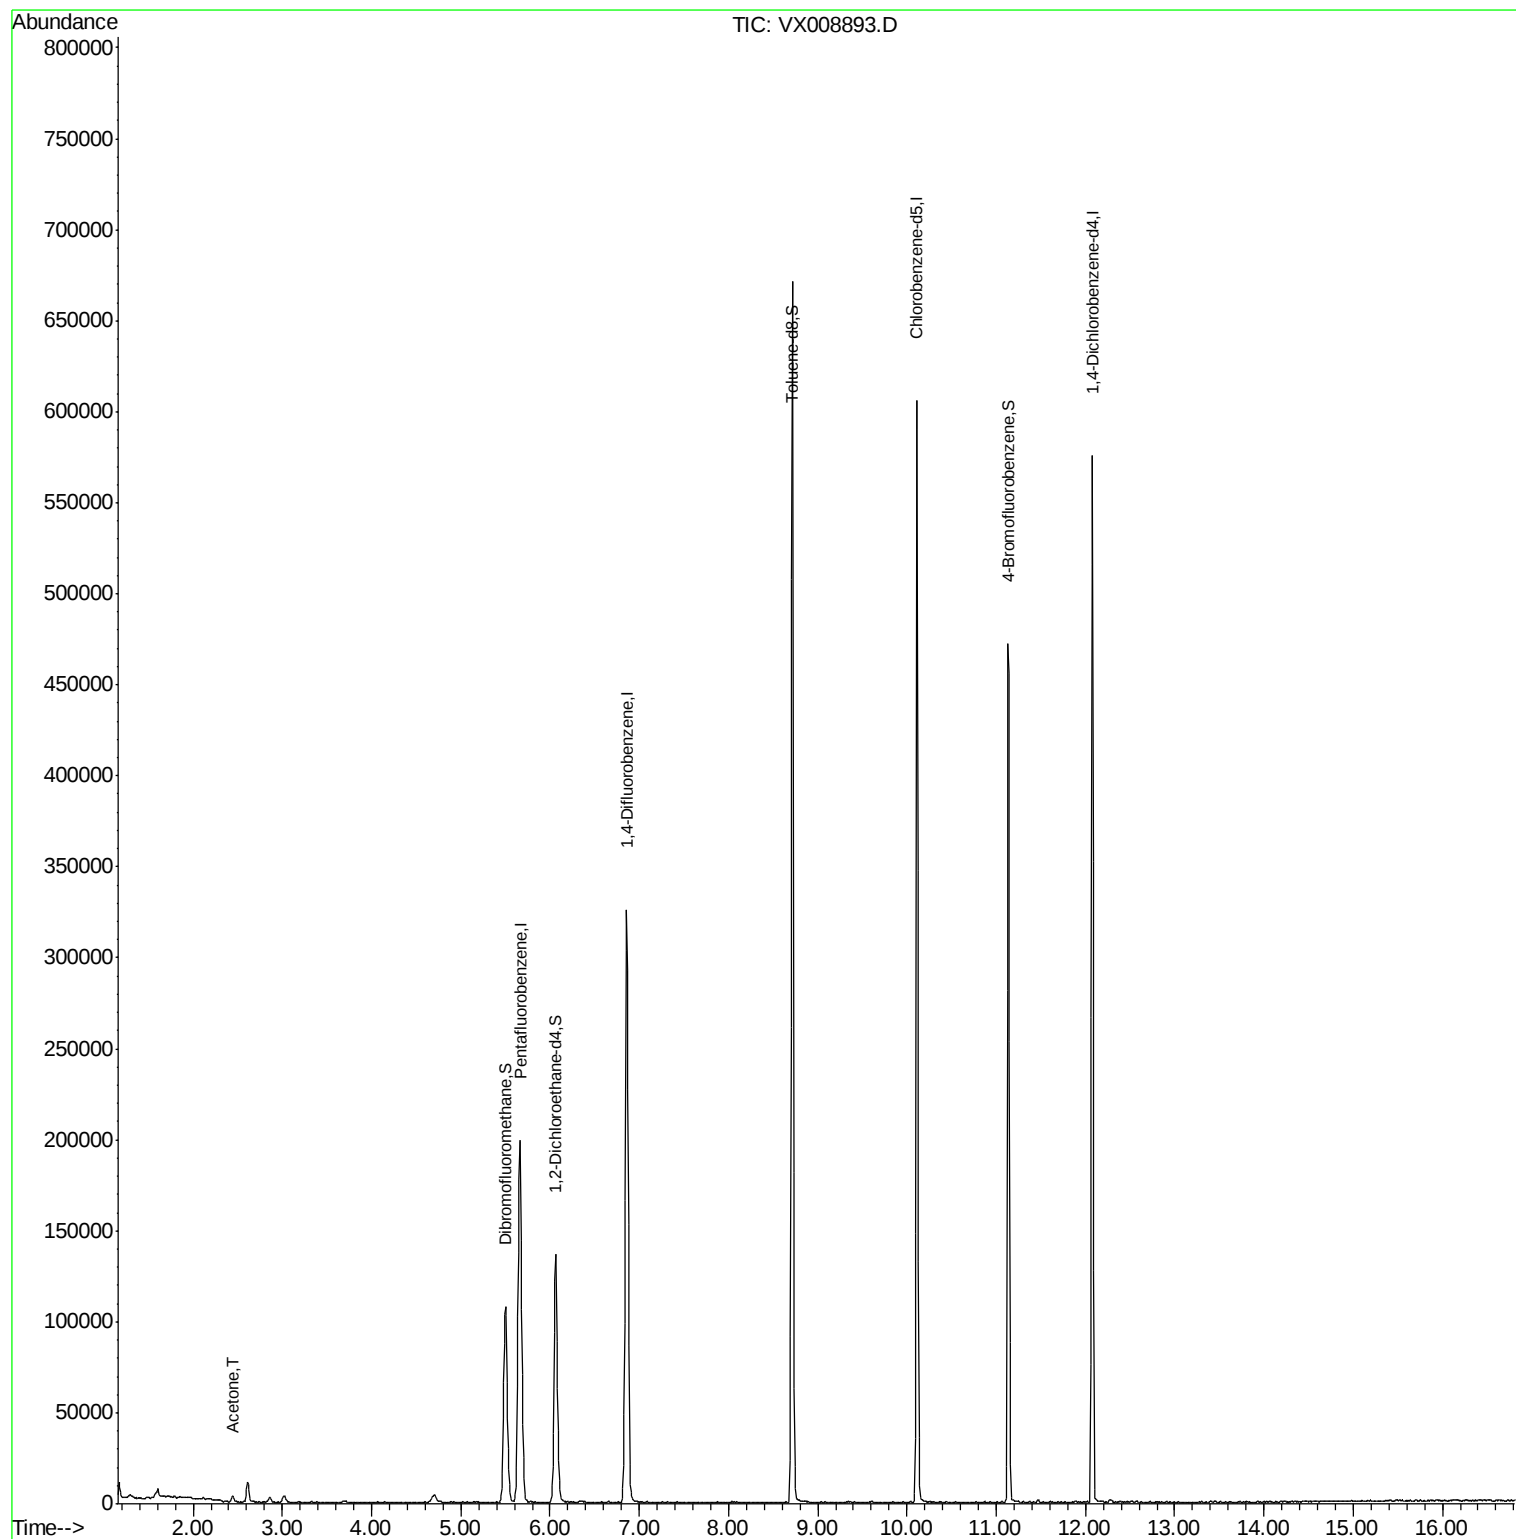



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.01 min

Lab File: VX008893.D

Acq: 12 Apr 2019 17:51

Instrument :

MSVOA_X

ClientSampleId :


DUP01-20190409

Tgt Ion:168 Resp: 193965

Ion Ratio Lower Upper

168 100

99 53.2 46.7 70.1

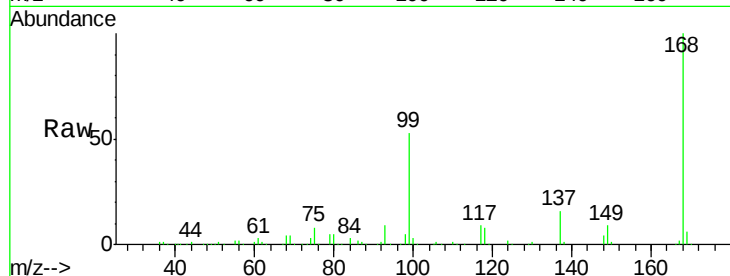

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

80000

60000



40000

20000

0

Time-->

5.50 5.60 5.70 5.80 5.90

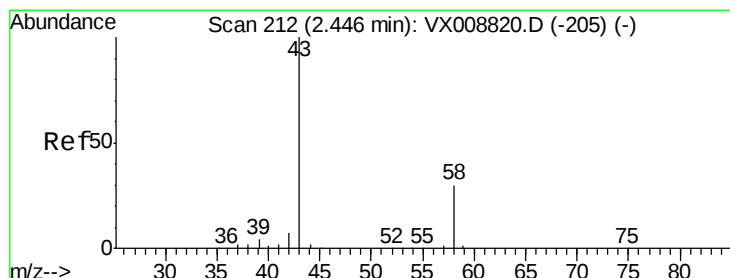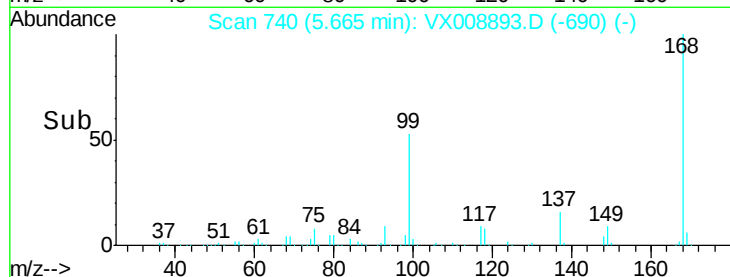

#16

Acetone

Concen: 2.728 ug/l

RT: 2.44 min Scan# 211

Delta R.T. -0.01 min

Lab File: VX008893.D


Acq: 12 Apr 2019 17:51

Tgt Ion: 43 Resp: 4446

Ion Ratio Lower Upper

43 100

58 26.8 24.8 37.2

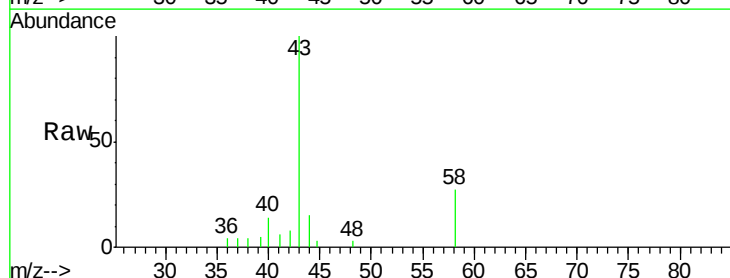

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

2.44

2500

2000

1500


1000


500

0

Time-->

2.35 2.40 2.45 2.50 2.55




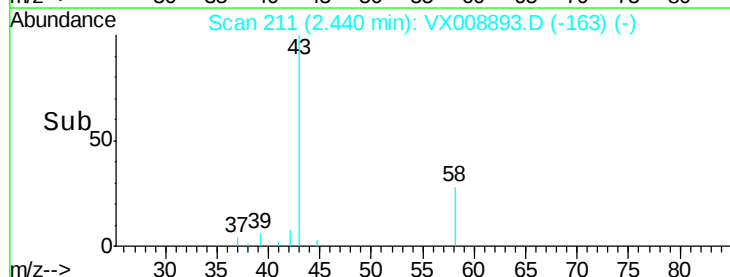


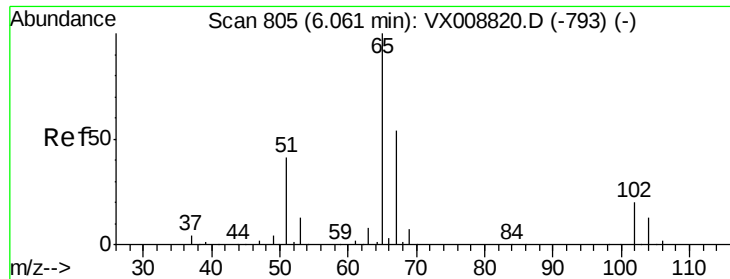

#33
 1,2-Dichloroethane-d4
 Concen: 45.433 ug/l
 RT: 6.06 min Scan# 805
 Delta R.T. -0.00 min
 Lab File: VX008893.D
 Acq: 12 Apr 2019 17:51




Instrument :
 MSVOA_X
 ClientSampleId :
 DUP01-20190409


Tgt Ion: 65 Resp: 128535
 Ion Ratio Lower Upper
 65 100
 67 53.8 0.0 107.2

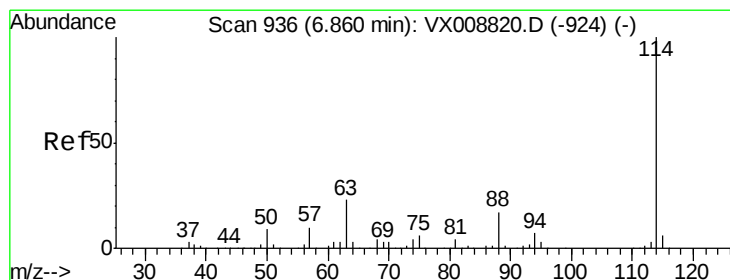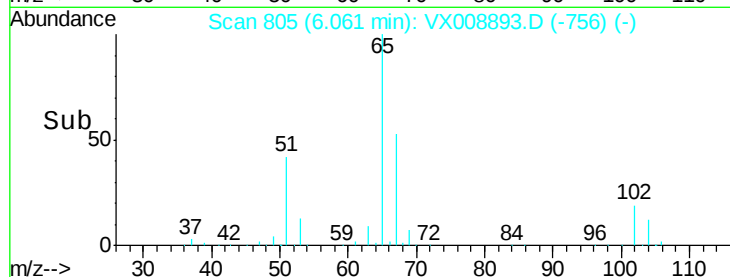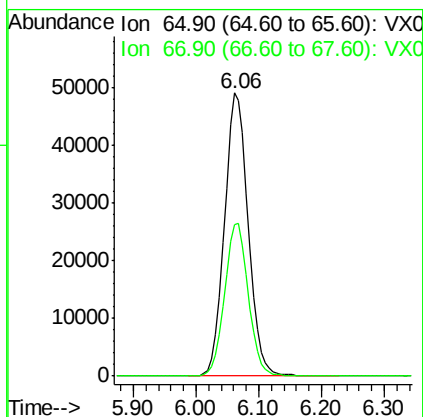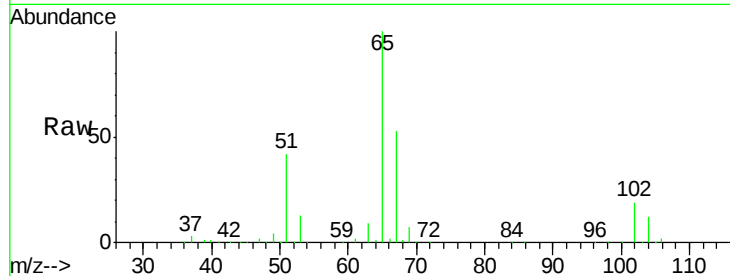

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.86 min Scan# 936
 Delta R.T. -0.00 min
 Lab File: VX008893.D
 Acq: 12 Apr 2019 17:51

Tgt Ion: 114 Resp: 311251
 Ion Ratio Lower Upper
 114 100
 63 23.3 0.0 47.2
 88 16.5 0.0 34.0


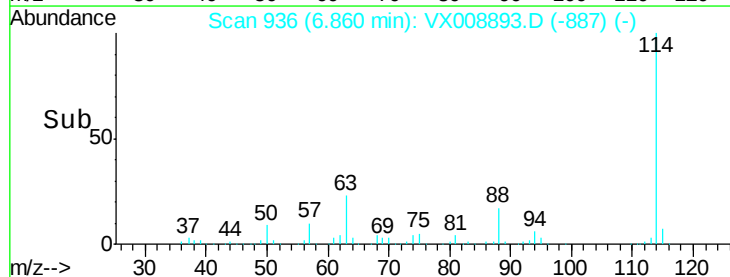
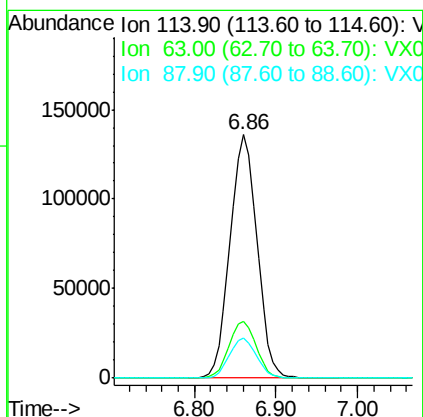
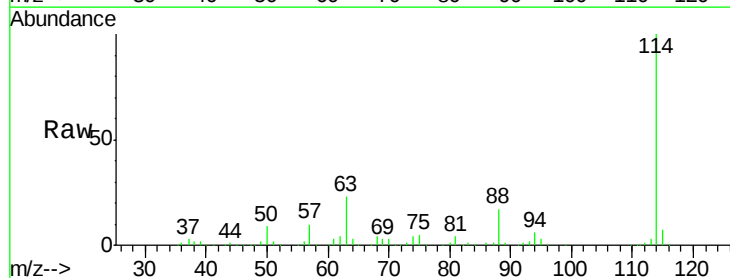


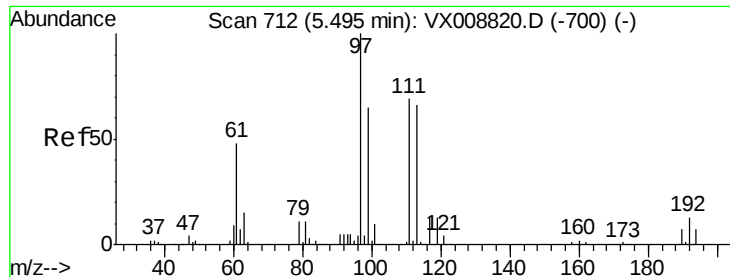

#35
 Dibromofluoromethane
 Concen: 46.806 ug/l
 RT: 5.50 min Scan# 713
 Delta R.T. -0.00 min
 Lab File: VX008893.D
 Acq: 12 Apr 2019 17:51




Instrument :
 MSVOA_X
 ClientSampleId :
 DUP01-20190409


Tgt Ion:113 Resp: 93144
 Ion Ratio Lower Upper
 113 100
 111 102.9 83.4 125.2
 192 20.9 16.1 24.1

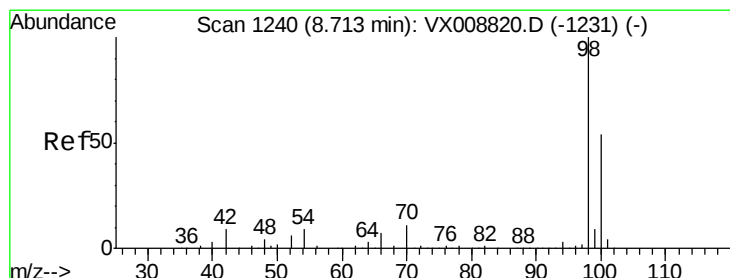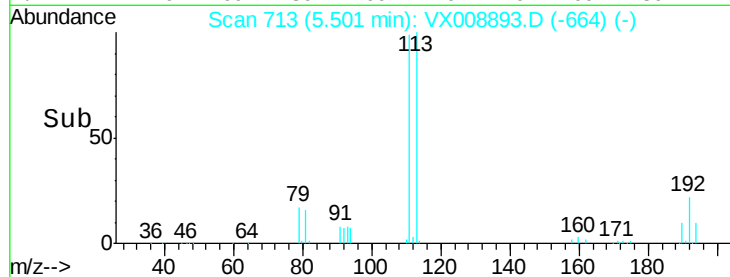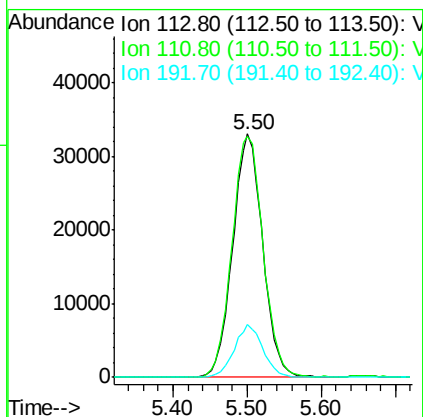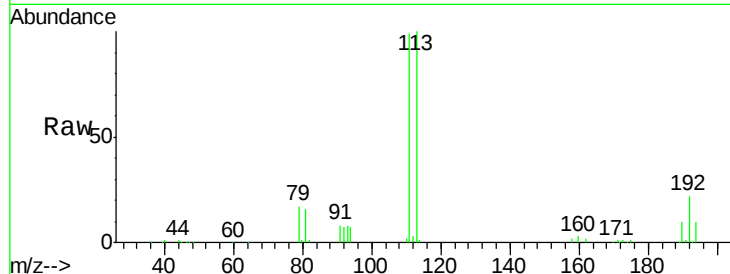

#50
 Toluene-d8
 Concen: 49.097 ug/l
 RT: 8.71 min Scan# 1240
 Delta R.T. -0.00 min
 Lab File: VX008893.D
 Acq: 12 Apr 2019 17:51

Tgt Ion: 98 Resp: 389033
 Ion Ratio Lower Upper
 98 100
 100 64.1 51.4 77.0


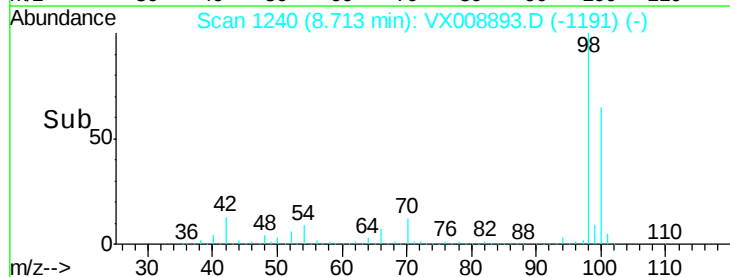
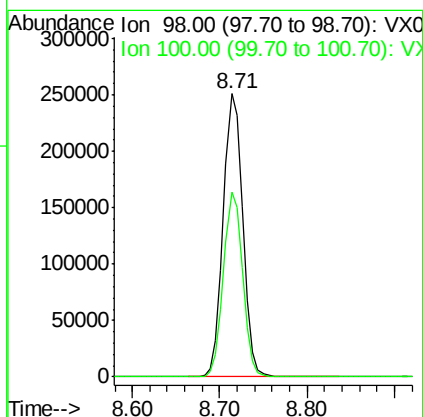
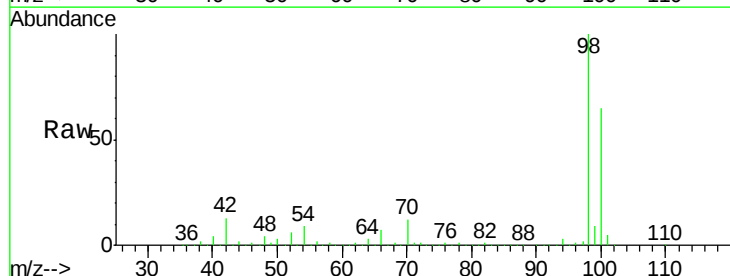


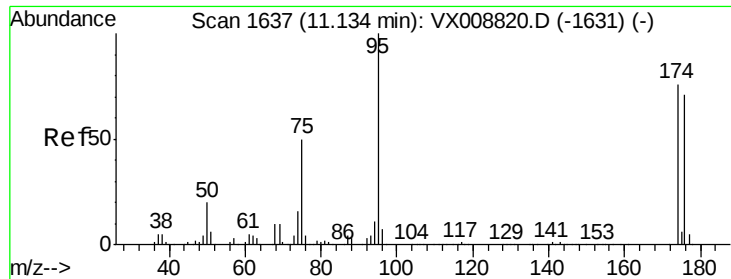

#62
 4-Bromofluorobenzene
 Concen: 45.700 ug/l
 RT: 11.13 min Scan# 1637
 Delta R.T. -0.00 min
 Lab File: VX008893.D
 Acq: 12 Apr 2019 17:51




Instrument :
 MSVOA_X
 ClientSampled :
 DUP01-20190409


Tgt Ion: 95 Resp: 128412
 Ion Ratio Lower Upper
 95 100
 174 79.2 0.0 151.8
 176 76.7 0.0 145.8

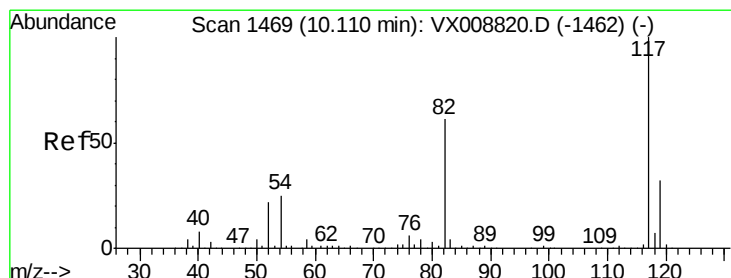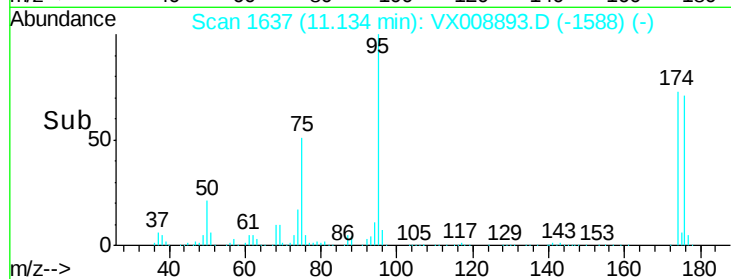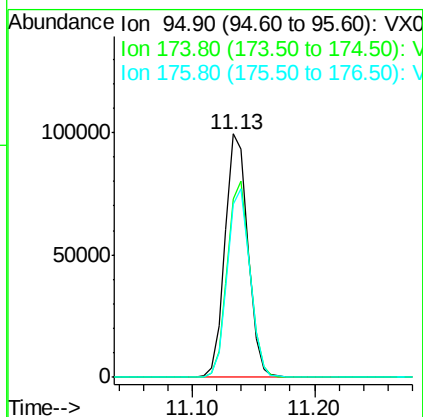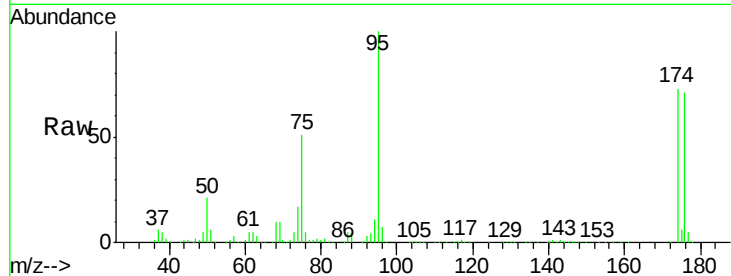

#63
 Chlorobenzene-d5
 Concen: 50.000 ug/l
 RT: 10.11 min Scan# 1469
 Delta R.T. -0.00 min
 Lab File: VX008893.D
 Acq: 12 Apr 2019 17:51

Tgt Ion: 117 Resp: 267793
 Ion Ratio Lower Upper
 117 100
 82 60.9 49.6 74.4
 119 31.6 25.0 37.4

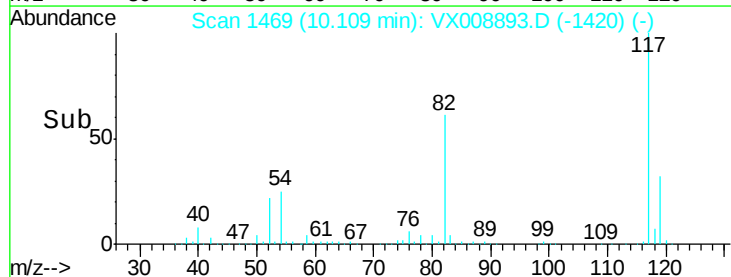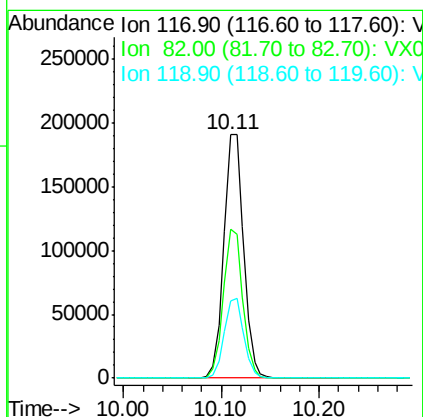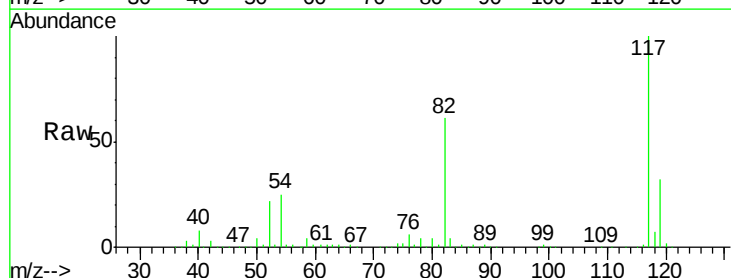

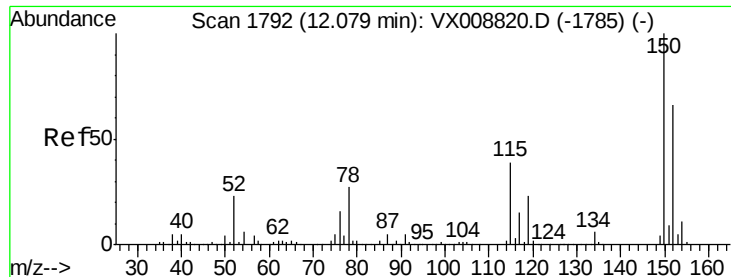

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. -0.00 min

Lab File: VX008893.D


Acq: 12 Apr 2019 17:51

Instrument :

MSVOA_X

ClientSampleId :

DUP01-20190409

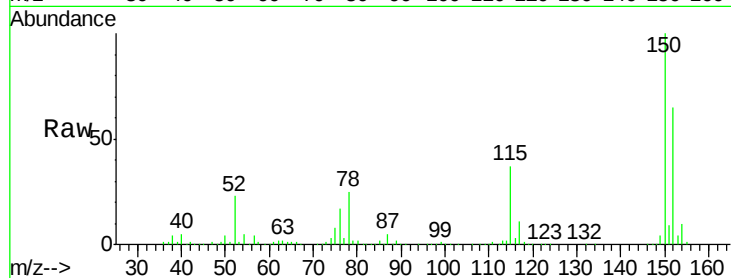


Tgt Ion:152 Resp: 114153

Ion Ratio Lower Upper

152 100

115 59.2 43.5 130.5

150 157.1 0.0 348.8

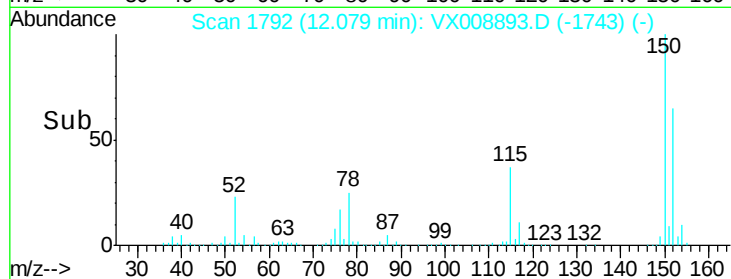

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

