

Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_X\DATA\VX041219\  
 Data File : VX008905.D  
 Acq On : 12 Apr 2019 23:18  
 Operator : JC/SP  
 Sample : K2311-11  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 35 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 0236-COMP-CS-1-ELTRT-DISS

## Integration Parameters: RTEINT.P

Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X040319W.M  
 Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.623       | 66            | 77          | 83           | rBV      | 5831           | 15557         | 1.54%           | 0.298%        |
| 2         | 2.446       | 205           | 212         | 226          | rVB      | 28640          | 52928         | 5.22%           | 1.015%        |
| 3         | 2.855       | 273           | 279         | 290          | rBV      | 24717          | 50695         | 5.00%           | 0.972%        |
| 4         | 4.702       | 573           | 582         | 591          | rBV3     | 3721           | 12867         | 1.27%           | 0.247%        |
| 5         | 5.501       | 699           | 713         | 725          | rBV2     | 102438         | 300565        | 29.66%          | 5.765%        |
| 6         | 5.665       | 728           | 740         | 754          | rVB      | 193437         | 547114        | 53.99%          | 10.493%       |
| 7         | 6.061       | 795           | 805         | 821          | rBV      | 135347         | 352122        | 34.75%          | 6.754%        |
| 8         | 6.860       | 924           | 936         | 948          | rBV      | 313172         | 731940        | 72.23%          | 14.038%       |
| 9         | 8.713       | 1233          | 1240        | 1249         | rBV      | 655872         | 1013407       | 100.00%         | 19.437%       |
| 10        | 10.110      | 1462          | 1469        | 1479         | rBV      | 592602         | 822815        | 81.19%          | 15.781%       |
| 11        | 10.713      | 1559          | 1568        | 1578         | rBV2     | 7141           | 12946         | 1.28%           | 0.248%        |
| 12        | 11.134      | 1631          | 1637        | 1650         | rBV      | 457153         | 604811        | 59.68%          | 11.600%       |
| 13        | 12.079      | 1786          | 1792        | 1799         | rBV      | 559489         | 696114        | 68.69%          | 13.351%       |


Sum of corrected areas: 5213881

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX041219\  
Data File : VX008905.D  
Acq On : 12 Apr 2019 23:18  
Operator : JC/SP  
Sample : K2311-11  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 35 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
0236-COMP-CS-1-ELTRT-DISS

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X040319W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

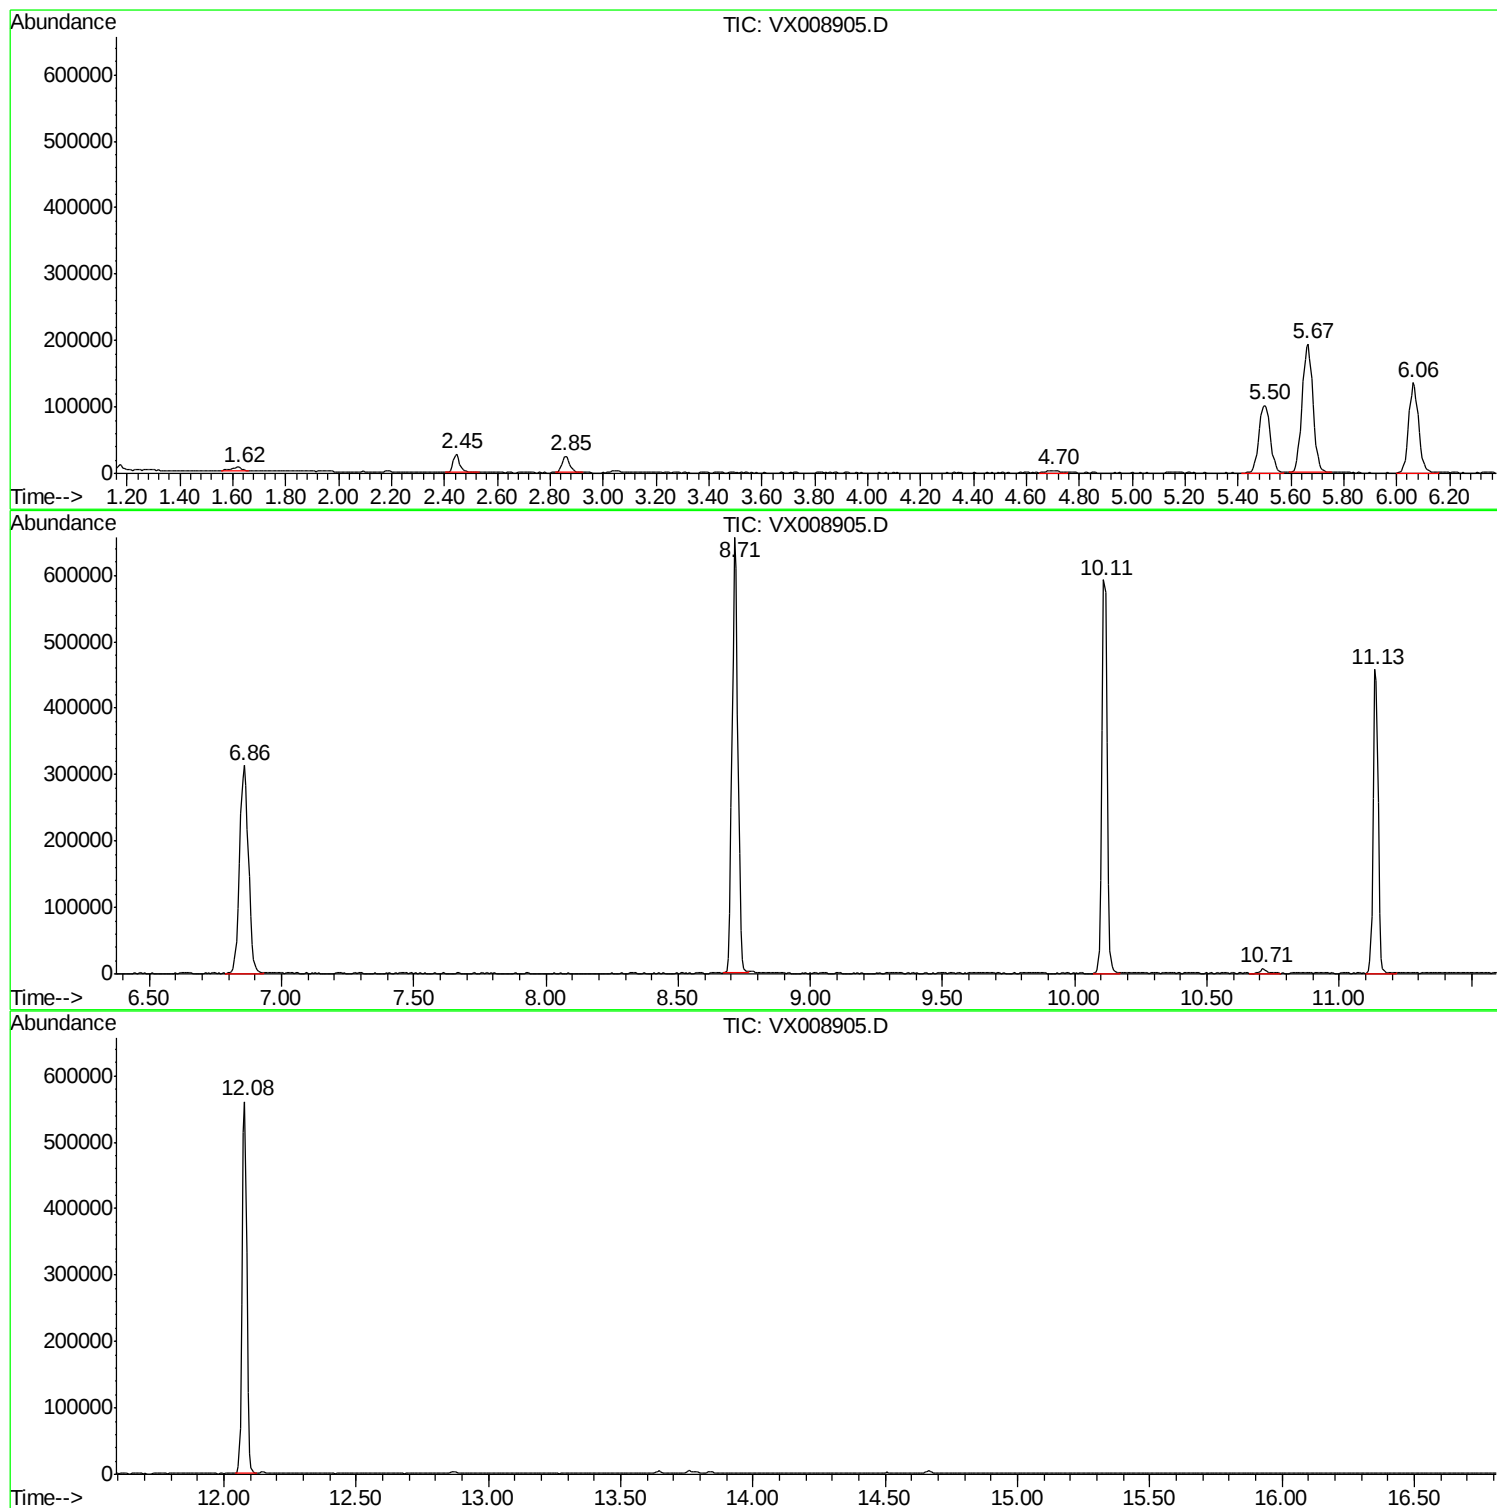

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX041219\  
Data File : VX008905.D  
Acq On : 12 Apr 2019 23:18  
Operator : JC/SP  
Sample : K2311-11  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 35 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
0236-COMP-CS-1-ELTRT-DISS

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X040319W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX041219\  
Data File : VX008905.D  
Acq On : 12 Apr 2019 23:18  
Operator : JC/SP  
Sample : K2311-11  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 35 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
0236-COMP-CS-1-ELTRT-DISS

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X040319W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | ---Internal Standard--- |
|------------------|----|---------|-------|----------|-------------------------|
|                  |    |         |       |          | # RT Resp Conc          |