

Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX041219\
 Data File : VX008920.D
 Acq On : 13 Apr 2019 05:08
 Operator : JC/SP
 Sample : K2367-07
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S8-0703

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.489	51	55	62	rBV	40785	49759	3.21%	0.205%
2	4.403	524	533	544	rVB2	26293	78205	5.05%	0.323%
3	4.598	554	565	574	rBV2	14271	42043	2.71%	0.174%
4	5.501	701	713	721	rBV	107248	310974	20.08%	1.284%
5	5.586	721	727	731	rVV2	26952	80501	5.20%	0.332%
6	5.659	731	739	759	rVB	201506	618250	39.91%	2.552%
7	5.933	773	784	795	rBV3	14925	50880	3.28%	0.210%
8	6.061	795	805	813	rVV	132809	354003	22.85%	1.461%
9	6.141	813	818	830	rVV	48284	134179	8.66%	0.554%
10	6.263	830	838	845	rVV4	12069	41692	2.69%	0.172%
11	6.360	846	854	862	rVV3	18055	55792	3.60%	0.230%
12	6.860	925	936	947	rBV	319687	753355	48.63%	3.110%
13	7.464	1024	1035	1044	rBV	86737	206802	13.35%	0.854%
14	7.726	1070	1078	1091	rVB2	23897	55308	3.57%	0.228%
15	8.713	1234	1240	1246	rVV	672530	1062646	68.60%	4.387%
16	8.774	1246	1250	1256	rVB2	72397	113446	7.32%	0.468%
17	9.037	1288	1293	1299	rVB	25483	41835	2.70%	0.173%
18	9.305	1332	1337	1342	rVV	37455	55212	3.56%	0.228%
19	9.366	1342	1347	1354	rVB	46725	67290	4.34%	0.278%
20	9.439	1354	1359	1364	rBV	33141	48224	3.11%	0.199%
21	9.518	1364	1372	1377	rBV	146581	217044	14.01%	0.896%
22	10.006	1447	1452	1457	rBV	36615	49278	3.18%	0.203%
23	10.110	1464	1469	1474	rBV	617050	825268	53.28%	3.407%
24	10.250	1486	1492	1500	rBV	549609	750295	48.44%	3.098%
25	10.360	1501	1510	1517	rVB	1128908	1549047	100.00%	6.395%
26	10.695	1561	1565	1570	rVB	67702	89514	5.78%	0.370%
27	10.945	1602	1606	1612	rVB	77371	121827	7.86%	0.503%
28	11.018	1612	1618	1622	rBV	56193	75769	4.89%	0.313%
29	11.134	1630	1637	1643	rBV2	592021	1085300	70.06%	4.481%
30	11.183	1643	1645	1649	rVB	55282	64674	4.18%	0.267%
31	11.237	1649	1654	1658	rBV	88329	115188	7.44%	0.476%
32	11.286	1658	1662	1665	rBV	73594	111175	7.18%	0.459%
33	11.323	1665	1668	1670	rBV	56661	59896	3.87%	0.247%
34	11.353	1670	1673	1680	rVB2	268869	344701	22.25%	1.423%

Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX041219\
 Data File : VX008920.D
 Acq On : 13 Apr 2019 05:08
 Operator : JC/SP
 Sample : K2367-07
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S8-0703

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
 Title : SW846 8260

35	11.432	1680	1686	1687	rBV2	85059	121498	7.84%	0.502%
36	11.451	1687	1689	1692	rVB	165603	171997	11.10%	0.710%
37	11.481	1692	1694	1697	rBV	49052	48739	3.15%	0.201%
38	11.664	1719	1724	1728	rVV2	265647	403359	26.04%	1.665%
39	11.695	1728	1729	1734	rVB	63109	51612	3.33%	0.213%
40	11.804	1742	1747	1752	rVB	726460	885967	57.19%	3.658%
41	12.079	1786	1792	1797	rBV	640138	858209	55.40%	3.543%
42	12.140	1797	1802	1806	rBV	327094	399187	25.77%	1.648%
43	12.201	1806	1812	1814	rBV4	28403	43387	2.80%	0.179%
44	12.298	1824	1828	1832	rBV	229199	314627	20.31%	1.299%
45	12.335	1832	1834	1837	rVV	128121	143633	9.27%	0.593%
46	12.365	1837	1839	1847	rVB3	104553	182795	11.80%	0.755%
47	12.469	1852	1856	1860	rBV4	33655	61804	3.99%	0.255%
48	12.518	1860	1864	1870	rVB	86061	118332	7.64%	0.489%
49	12.585	1870	1875	1877	rBV2	185922	256055	16.53%	1.057%
50	12.609	1877	1879	1883	rVB	140778	147097	9.50%	0.607%
51	12.664	1884	1888	1892	rVB	186109	214054	13.82%	0.884%
52	12.725	1895	1898	1901	rBV	83707	96310	6.22%	0.398%
53	12.762	1901	1904	1909	rVV5	49860	90835	5.86%	0.375%
54	12.804	1909	1911	1916	rVB4	73277	96925	6.26%	0.400%
55	12.902	1922	1927	1932	rVB2	112413	145048	9.36%	0.599%
56	12.975	1932	1939	1942	rBV2	205038	354731	22.90%	1.464%
57	13.018	1942	1946	1951	rVB	258151	323530	20.89%	1.336%
58	13.072	1951	1955	1961	rVB5	153544	235713	15.22%	0.973%
59	13.139	1961	1966	1971	rBV3	131147	217975	14.07%	0.900%
60	13.194	1971	1975	1978	rBV2	208759	283274	18.29%	1.169%
61	13.225	1978	1980	1983	rVB2	76520	73836	4.77%	0.305%
62	13.286	1988	1990	1993	rVV	89814	133811	8.64%	0.552%
63	13.347	1993	2000	2005	rVV2	411641	742482	47.93%	3.065%
64	13.389	2005	2007	2010	rVV	58045	61441	3.97%	0.254%
65	13.426	2010	2013	2017	rVV3	133654	176294	11.38%	0.728%
66	13.475	2017	2021	2025	rVV	200429	272268	17.58%	1.124%
67	13.530	2025	2030	2033	rVV	233864	273060	17.63%	1.127%
68	13.560	2033	2035	2038	rVB4	47429	49757	3.21%	0.205%
69	13.603	2038	2042	2045	rBV	209096	299247	19.32%	1.235%
70	13.633	2045	2047	2054	rVV3	94102	169103	10.92%	0.698%
71	13.719	2055	2061	2067	rVB3	367763	645090	41.64%	2.663%

Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX041219\
 Data File : VX008920.D
 Acq On : 13 Apr 2019 05:08
 Operator : JC/SP
 Sample : K2367-07
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S8-0703

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
 Title : SW846 8260

72	13.786	2067	2072	2074	rBV	101135	140244	9.05%	0.579%
73	13.834	2076	2080	2087	rVB	187078	311632	20.12%	1.287%
74	13.908	2087	2092	2094	rBV3	100080	138716	8.95%	0.573%
75	13.938	2094	2097	2100	rVV	151324	164108	10.59%	0.678%
76	13.981	2100	2104	2108	rVB4	75926	96270	6.21%	0.397%
77	14.036	2108	2113	2120	rVB6	83827	177131	11.43%	0.731%
78	14.109	2120	2125	2128	rBV5	55901	102141	6.59%	0.422%
79	14.152	2128	2132	2136	rVB3	123358	175937	11.36%	0.726%
80	14.261	2146	2150	2153	rBV2	135755	182345	11.77%	0.753%
81	14.365	2163	2167	2173	rVB4	113747	199811	12.90%	0.825%
82	14.426	2173	2177	2186	rVB2	182913	267379	17.26%	1.104%
83	14.536	2192	2195	2198	rVV2	80410	108183	6.98%	0.447%
84	14.566	2198	2200	2207	rVB2	106736	138962	8.97%	0.574%
85	14.633	2207	2211	2213	rBV4	48859	65861	4.25%	0.272%
86	14.664	2213	2216	2218	rVV3	50298	70795	4.57%	0.292%
87	14.694	2218	2221	2230	rVV3	296594	496449	32.05%	2.050%
88	14.767	2230	2233	2239	rVB5	51503	89370	5.77%	0.369%
89	14.834	2239	2244	2249	rVB	223126	317127	20.47%	1.309%
90	14.956	2258	2264	2272	rVB	299014	478626	30.90%	1.976%
91	15.029	2272	2276	2285	rVB5	61678	122056	7.88%	0.504%
92	15.115	2285	2290	2296	rBV3	90729	179231	11.57%	0.740%
93	15.231	2305	2309	2313	rBV2	66522	117092	7.56%	0.483%
94	15.389	2330	2335	2341	rVB	289558	414660	26.77%	1.712%
95	15.548	2356	2361	2365	rBV	63662	108198	6.98%	0.447%
96	15.621	2370	2373	2378	rVV3	27406	48077	3.10%	0.198%
97	15.688	2378	2384	2387	rVV	51821	94740	6.12%	0.391%
98	15.724	2387	2390	2396	rVB	47319	74375	4.80%	0.307%
99	15.913	2414	2421	2428	rVB5	18043	50420	3.25%	0.208%
100	16.047	2437	2443	2450	rBV	252562	449976	29.05%	1.858%


Sum of corrected areas: 24222366

Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX041219\
Data File : VX008920.D
Acq On : 13 Apr 2019 05:08
Operator : JC/SP
Sample : K2367-07
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S8-0703

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

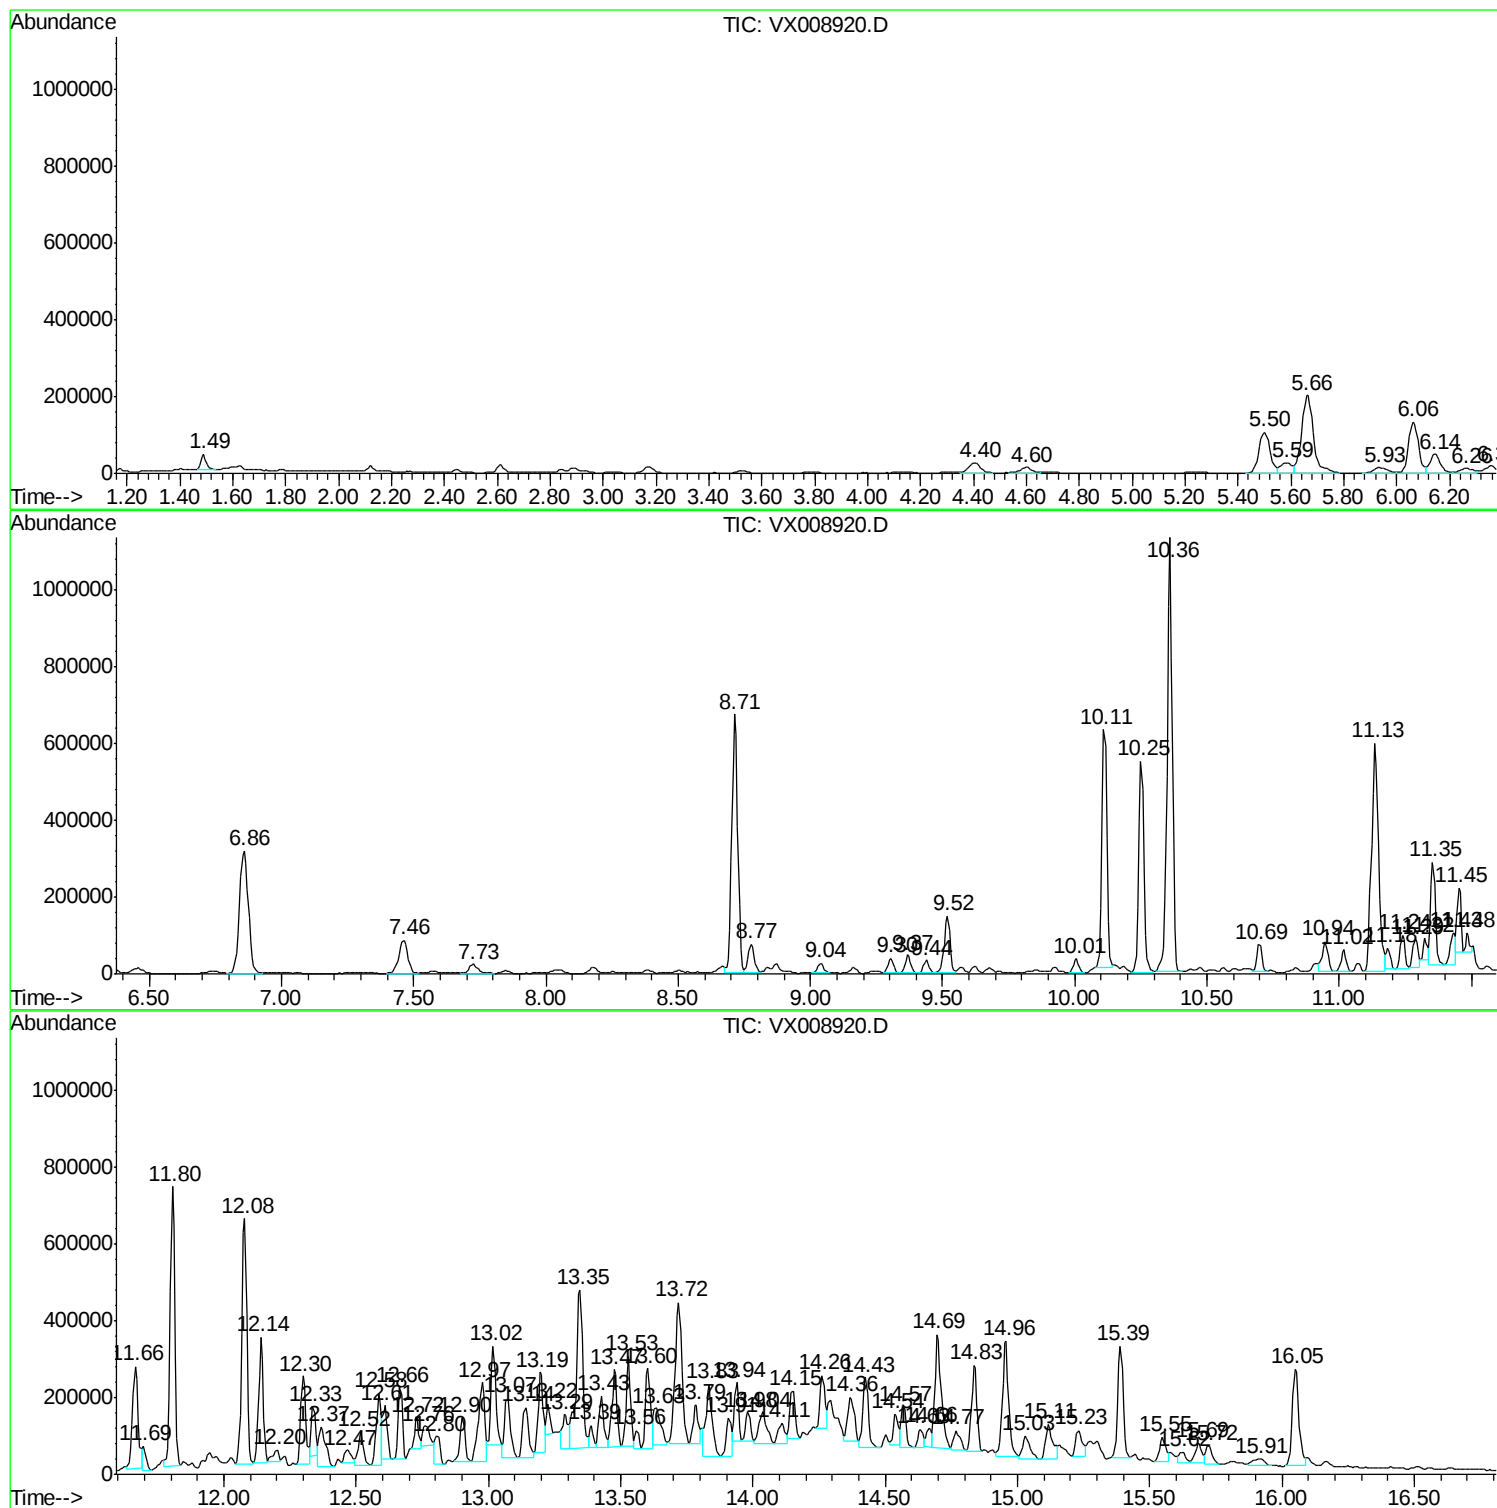

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041219\
Data File : VX008920.D
Acq On : 13 Apr 2019 05:08
Operator : JC/SP
Sample : K2367-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S8-0703

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041219\
Data File : VX008920.D
Acq On : 13 Apr 2019 05:08
Operator : JC/SP
Sample : K2367-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S8-0703

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc