


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX041219\
Data File : VX008873.D
Acq On : 12 Apr 2019 09:02
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
Title : SW846 8260
Last Update : Thu Apr 04 04:47:41 2019

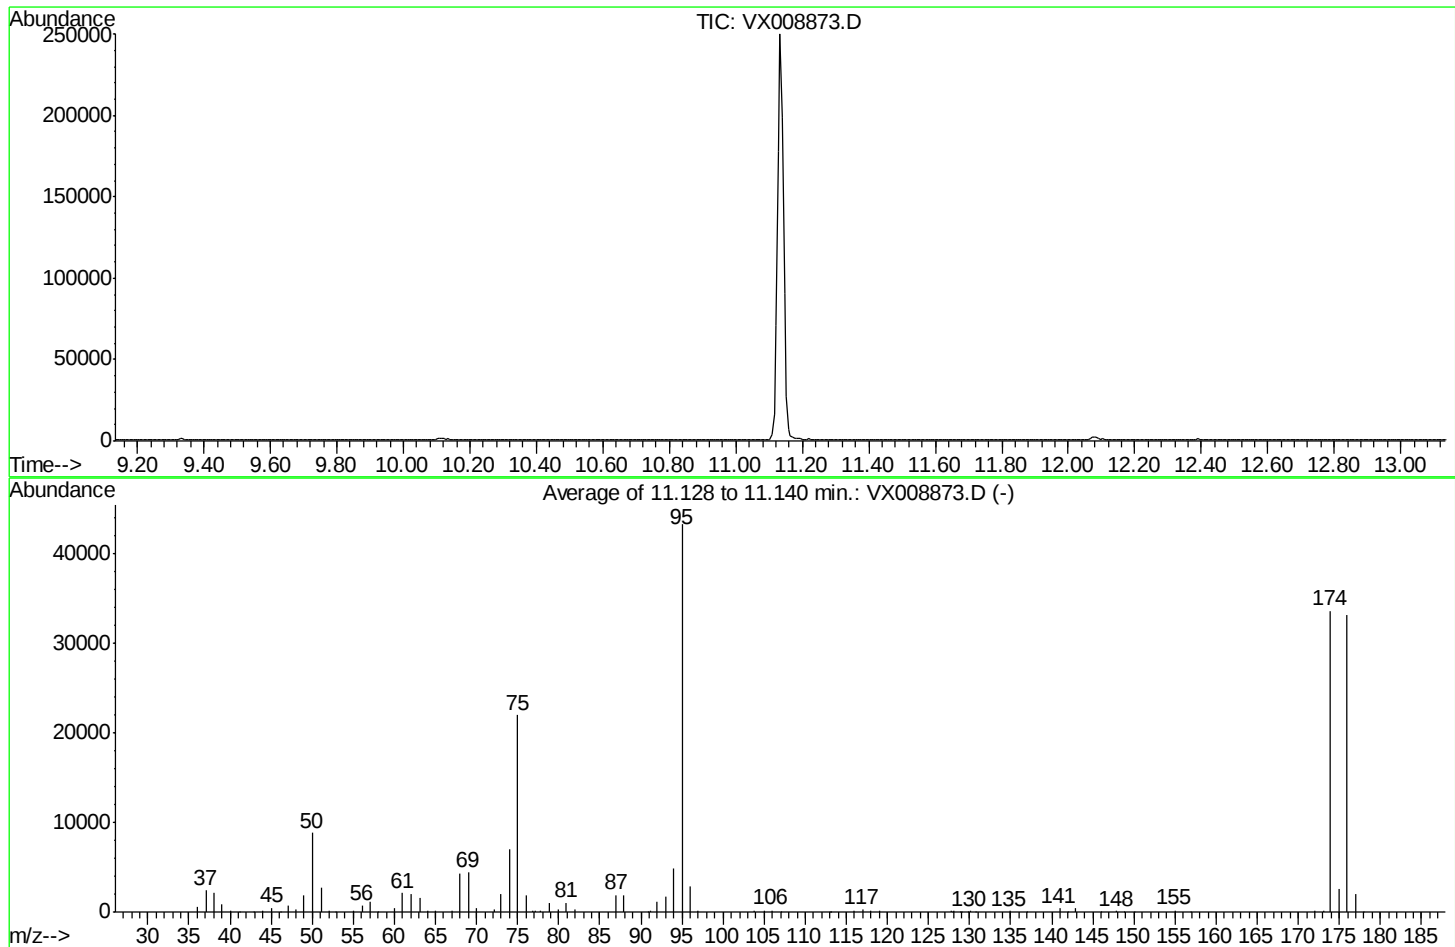

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	8829	PASS
75	95	30	60	50.7	21944	PASS
95	95	100	100	100.0	43256	PASS
96	95	5	9	6.7	2905	PASS
173	174	0.00	2	0.5	153	PASS
174	95	50	100	77.7	33629	PASS
175	174	5	9	7.4	2504	PASS
176	174	95	101	98.7	33205	PASS
177	176	5	9	6.2	2062	PASS