


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX041219\
Data File : VX008901.D
Acq On : 12 Apr 2019 21:21
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
Title : SW846 8260
Last Update : Thu Apr 04 04:47:41 2019

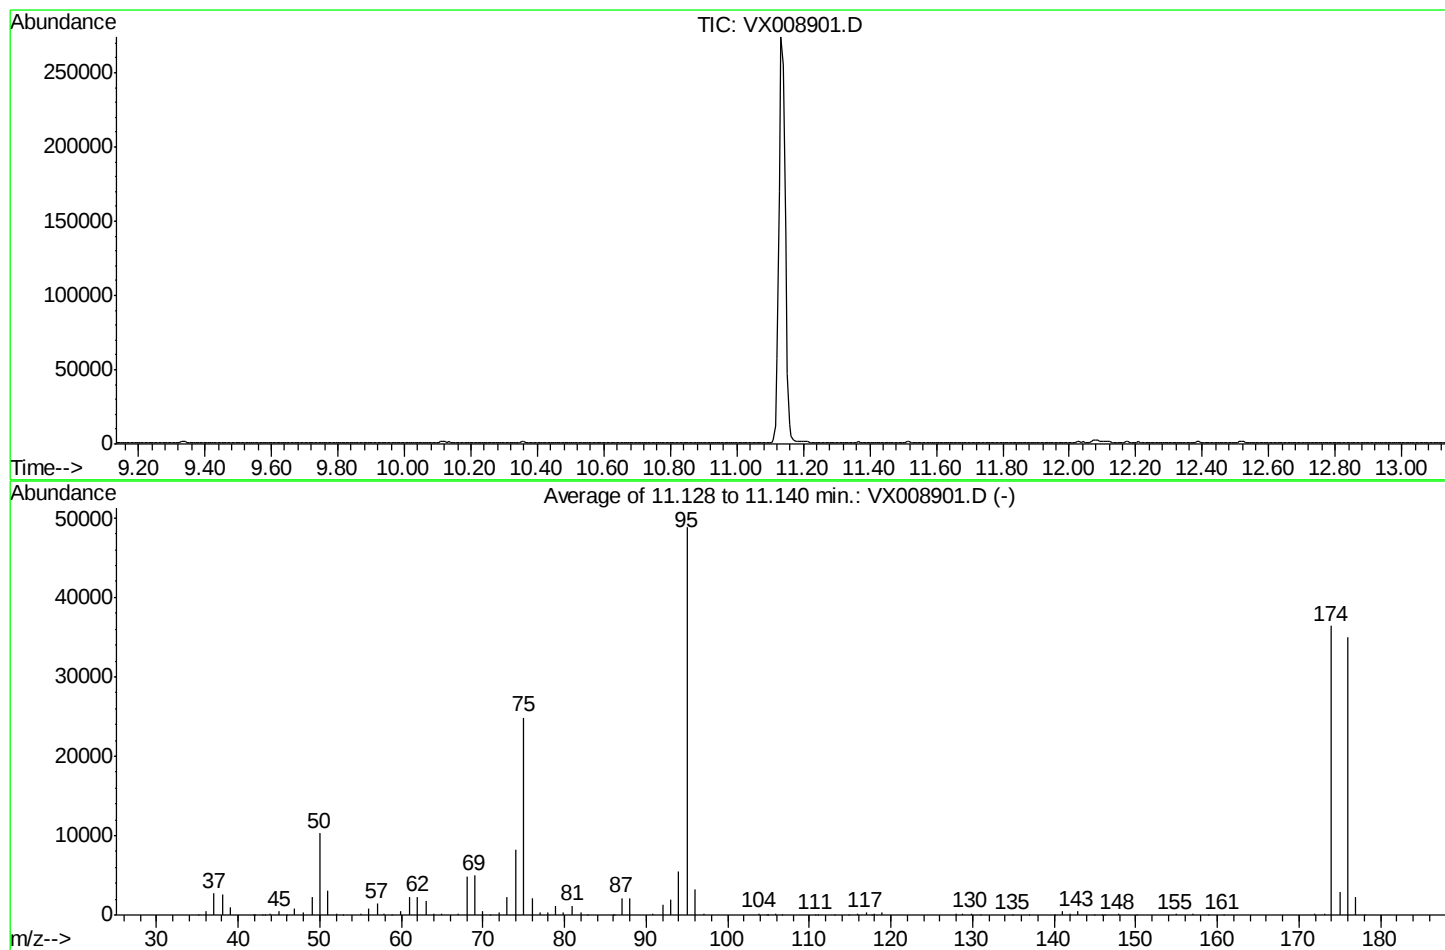

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	10314	PASS
75	95	30	60	50.9	24845	PASS
95	95	100	100	100.0	48821	PASS
96	95	5	9	6.7	3257	PASS
173	174	0.00	2	0.3	122	PASS
174	95	50	100	74.5	36376	PASS
175	174	5	9	8.1	2948	PASS
176	174	95	101	96.0	34914	PASS
177	176	5	9	6.6	2316	PASS