

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041222\
 Data File : VX028068.D
 Acq On : 12 Apr 2022 19:53
 Operator : JC/MD
 Sample : N2333-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-9

Quant Time: Apr 13 01:14:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 12 22:07:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	207510	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	361376	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	340863	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	186600	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	139033	49.386	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	98.780%		
35) Dibromofluoromethane	5.391	113	118216	49.922	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	99.840%		
50) Toluene-d8	8.653	98	442400	50.093	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	100.180%		
62) 4-Bromofluorobenzene	11.085	95	150271	45.571	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	91.140%		
Target Compounds						
					Qvalue	
5) Bromomethane	1.617	94	714	Below Cal	#	69
6) Chloroethane	1.684	64	46	2.622	ug/l #	69
11) Tert butyl alcohol	2.958	59	3423	5.238	ug/l	98
13) Acrolein	2.251	56	84	Below Cal	#	15
16) Acetone	2.379	43	4799	4.091	ug/l	92
20) Methylene Chloride	2.794	84	801	0.343	ug/l #	83
25) 2-Butanone	4.574	43	953	0.470	ug/l #	75
31) Cyclohexane	5.482	56	2005	0.518	ug/l	90
36) 1,1-Dichloropropene	5.556	75	16766	4.639	ug/l #	50
38) Carbon Tetrachloride	5.562	117	20525	5.320	ug/l #	15
39) Methylcyclohexane	7.384	83	4772	1.117	ug/l #	87
51) 4-Methyl-2-Pentanone	8.579	43	2516	0.563	ug/l #	84
55) 1,1,2-Trichloroethane	9.104	97	4714	1.659	ug/l #	20
56) Ethyl methacrylate	9.104	69	1295	0.290	ug/l #	1
59) 2-Hexanone	9.445	43	1076	0.307	ug/l	95
67) Ethyl Benzene	10.305	91	108303	8.269	ug/l #	66
68) m/p-Xylenes	10.305	106	52770	9.649	ug/l	97
69) o-Xylene	10.646	106	20561	3.868	ug/l	94
70) Styrene	10.646	104	1139	4.803	ug/l #	1
73) Isopropylbenzene	10.963	105	3764	0.284	ug/l	98
74) N-amyl acetate	10.866	43	1167	0.204	ug/l #	1
76) 1,2,3-Trichloropropane	11.384	75	11615	2.796	ug/l #	1
78) n-propylbenzene	11.305	91	8055	0.523	ug/l #	52
79) 2-Chlorotoluene	11.384	91	161555	17.292	ug/l #	40
80) 1,3,5-Trimethylbenzene	11.451	105	1086812	94.911	ug/l	98
81) trans-1,4-Dichloro-2-b...	11.079	75	84759	57.466	ug/l #	15
82) 4-Chlorotoluene	11.451	91	125511	11.412	ug/l #	45
83) tert-Butylbenzene	11.756	119	224866	20.296	ug/l #	50
84) 1,2,4-Trimethylbenzene	11.756	105	1803460	160.867	ug/l	98
85) sec-Butylbenzene	11.756	105	1803460	127.540	ug/l #	56
86) p-Isopropyltoluene	12.012	119	30636	2.557	ug/l	97
89) n-Butylbenzene	12.323	91	271330	26.457	ug/l #	1
90) Hexachloroethane	12.536	117	49083	24.381	ug/l #	10
92) 1,2-Dibromo-3-Chloropr...	12.920	75	7628	7.487	ug/l #	1
95) Naphthalene	13.780	128	293190	23.811	ug/l #	94

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041222\
Data File : VX028068.D
Acq On : 12 Apr 2022 19:53
Operator : JC/MD
Sample : N2333-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-9

Quant Time: Apr 13 01:14:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 12 22:07:23 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041222\
Data File : VX028068.D
Acq On : 12 Apr 2022 19:53
Operator : JC/MD
Sample : N2333-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-9

Quant Time: Apr 13 01:14:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 12 22:07:23 2022
Response via : Initial Calibration




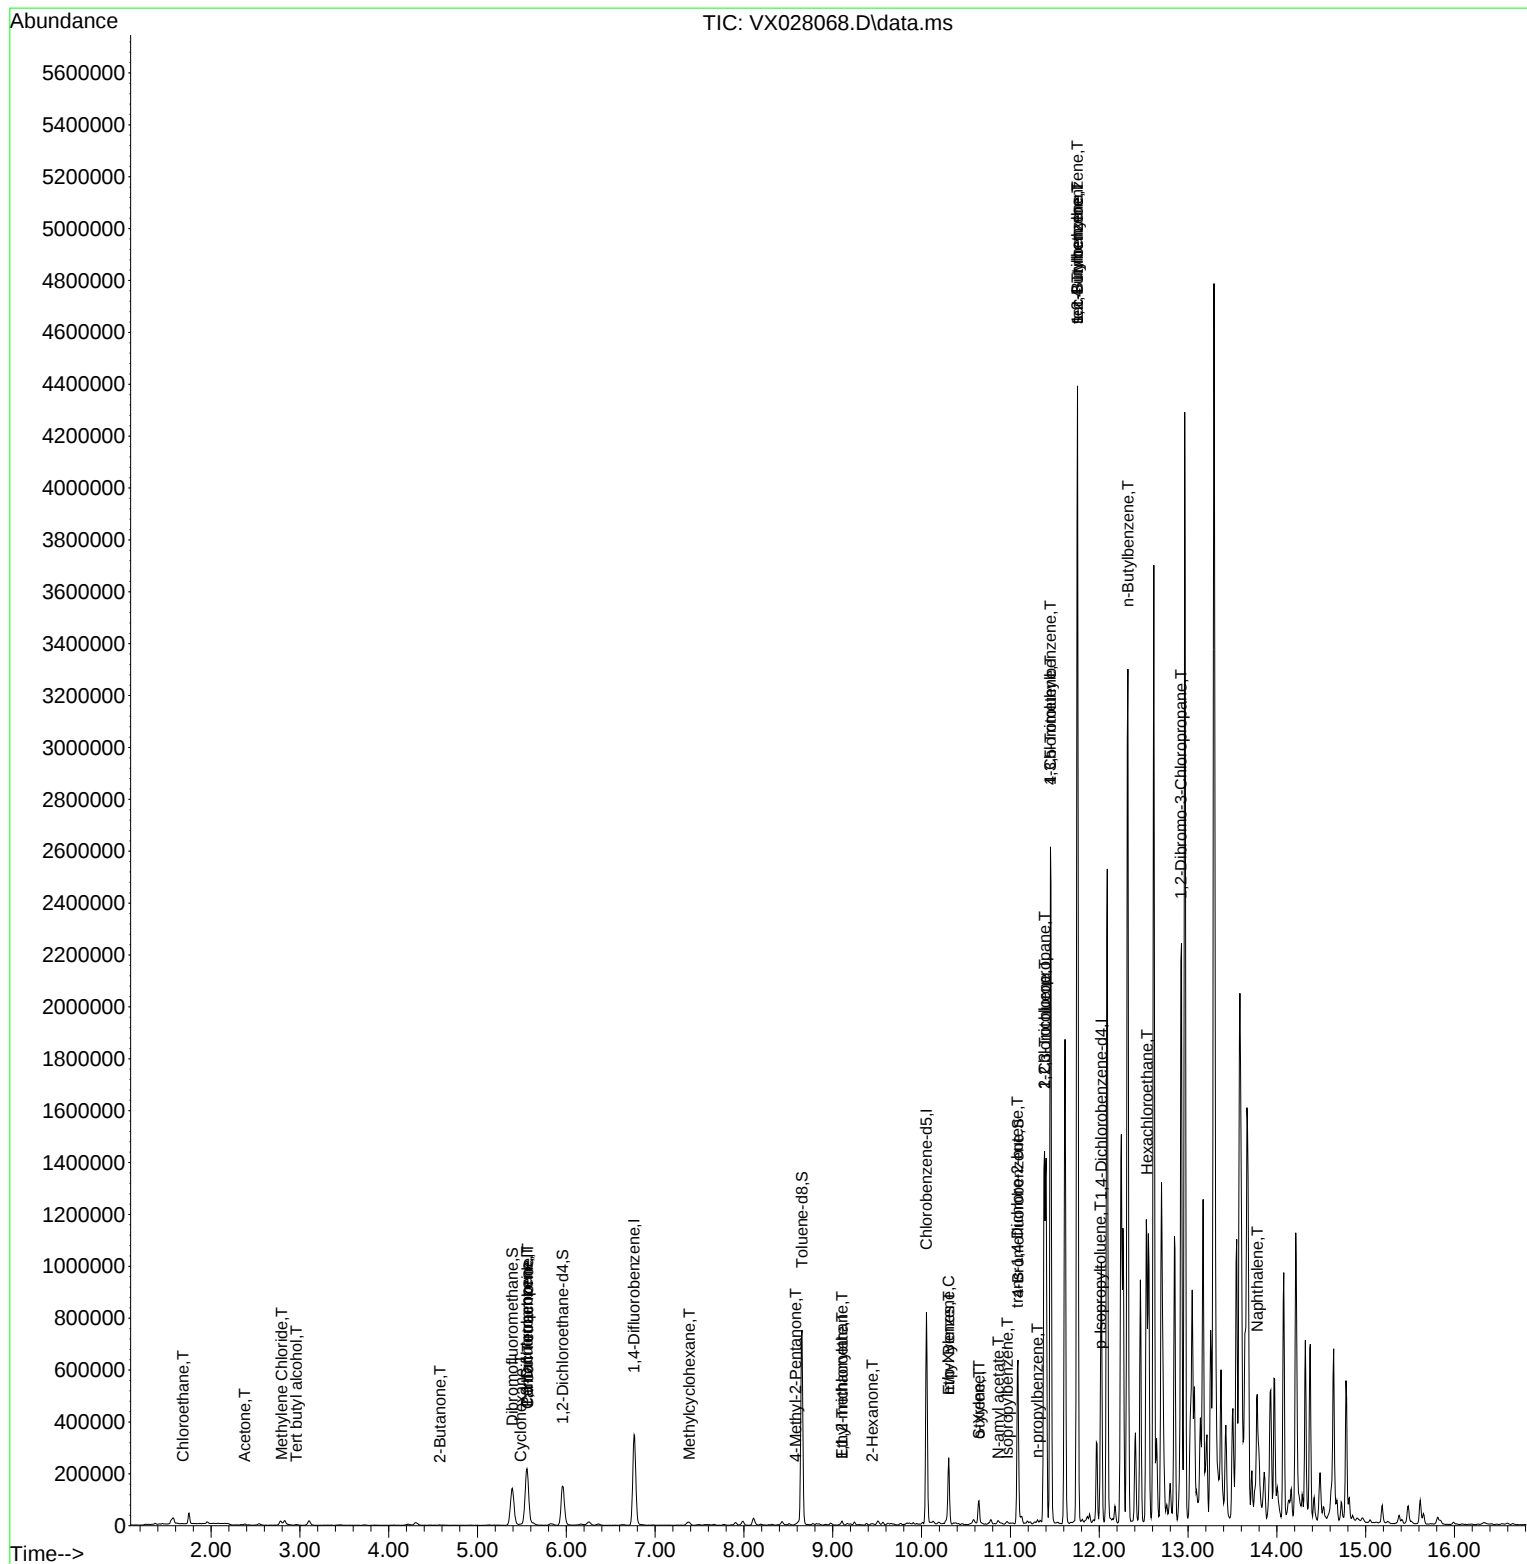




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX028068.D
Acq: 12 Apr 2022 19:53




Instrument :
MSVOA_X
ClientSampleId :
MW-9


Tgt Ion:168 Resp: 207510
Ion Ratio Lower Upper
168 100
99 55.1 41.7 62.5

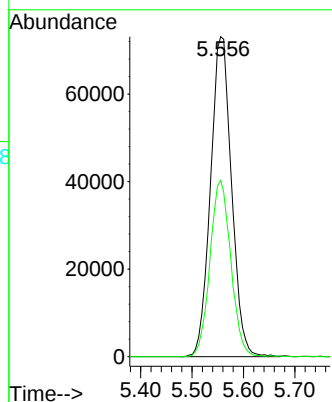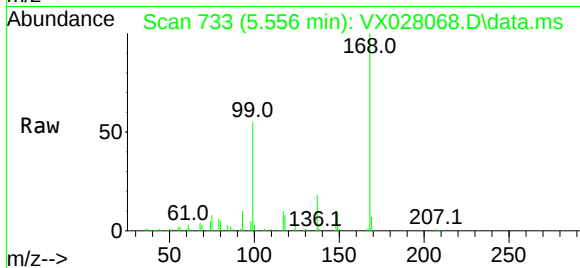

#6
Chloroethane
Concen: 2.622 ug/l
RT: 1.684 min Scan# 98
Delta R.T. 0.005 min
Lab File: VX028068.D
Acq: 12 Apr 2022 19:53

Tgt Ion: 64 Resp: 46
Ion Ratio Lower Upper
64 100
66 14.3 25.3 37.9

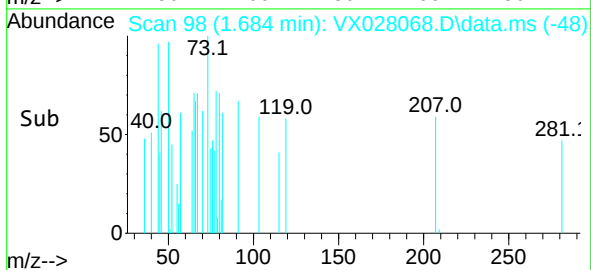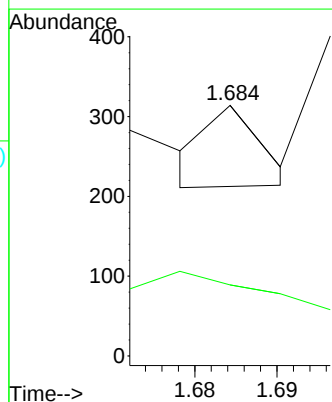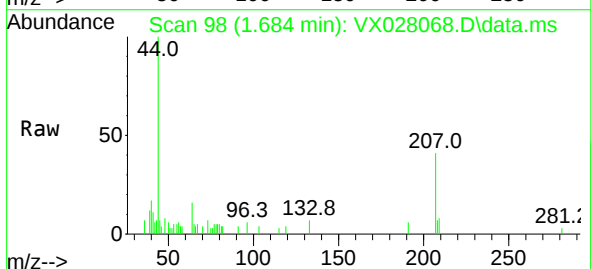

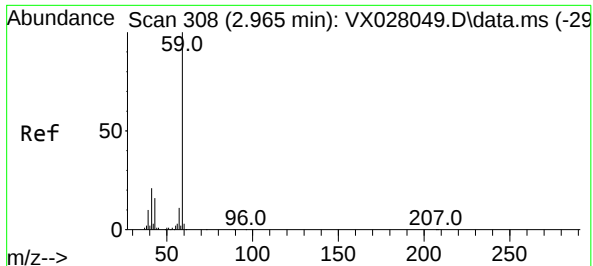

#11

Tert butyl alcohol

Concen: 5.238 ug/l

RT: 2.958 min Scan# 308

Delta R.T. -0.007 min

Lab File: VX028068.D

Acq: 12 Apr 2022 19:53

Instrument :

MSVOA_X

ClientSampleId :





MW-9

Tgt Ion: 59 Resp: 3423

Ion Ratio Lower Upper

59 100

57 11.0 8.3 12.5

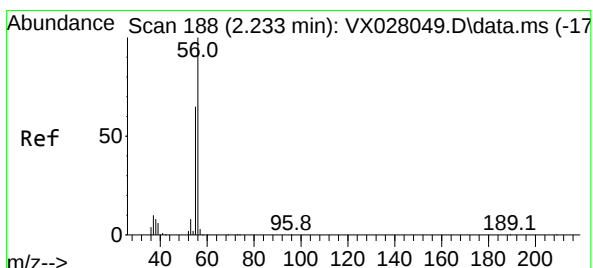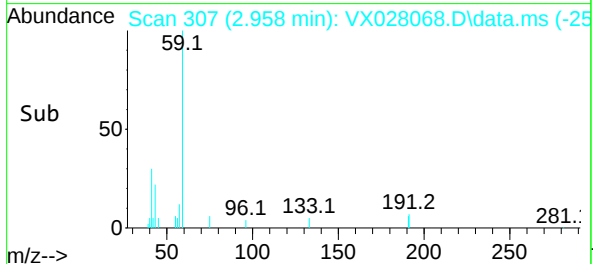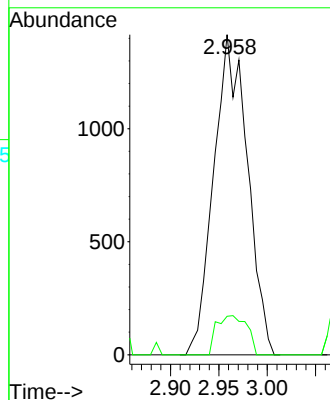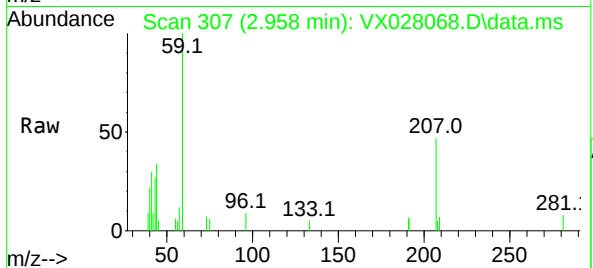

#13

Acrolein

Concen: Below Cal

RT: 2.251 min Scan# 191

Delta R.T. 0.018 min

Lab File: VX028068.D




Acq: 12 Apr 2022 19:53


Tgt Ion: 56 Resp: 84

Ion Ratio Lower Upper

56 100

55 0.0 55.0 82.6#


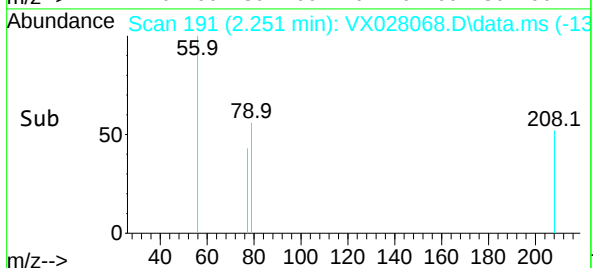
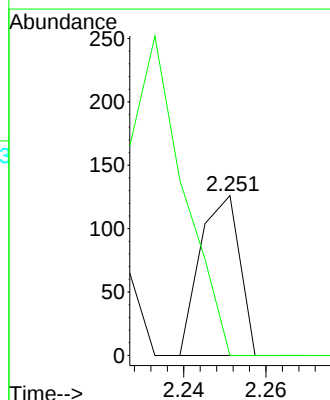
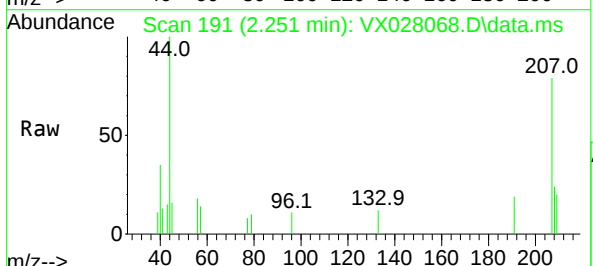




#16
Acetone
Concen: 4.091 ug/l
RT: 2.379 min Scan# 212
Delta R.T. -0.001 min
Lab File: VX028068.D
Acq: 12 Apr 2022 19:53




Instrument :
MSVOA_X
ClientSampleId :
MW-9


Tgt Ion: 43 Resp: 4799
Ion Ratio Lower Upper
43 100
58 31.0 28.8 43.2

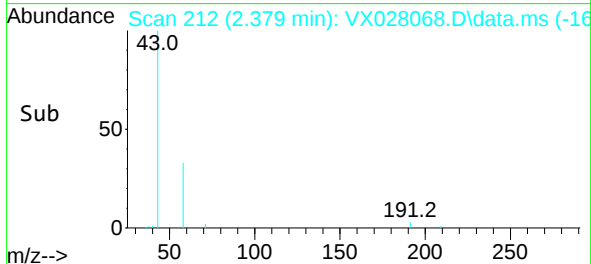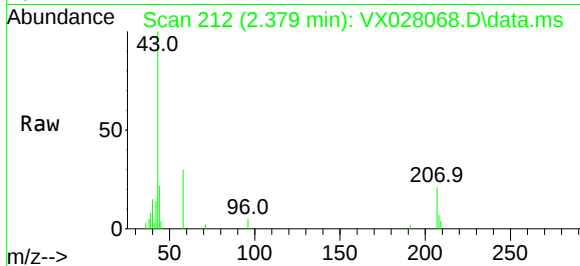

#20
Methylene Chloride
Concen: 0.343 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.006 min
Lab File: VX028068.D
Acq: 12 Apr 2022 19:53

Tgt Ion: 84 Resp: 801
Ion Ratio Lower Upper
84 100
49 110.1 85.5 128.3
51 20.2 26.6 39.8#
86 94.4 51.5 77.3#

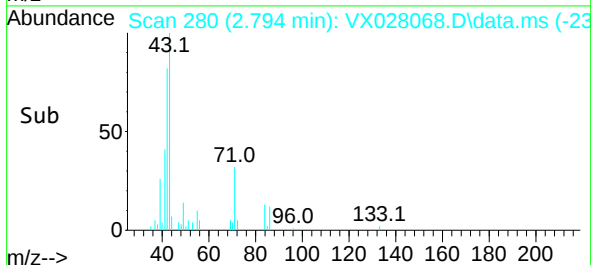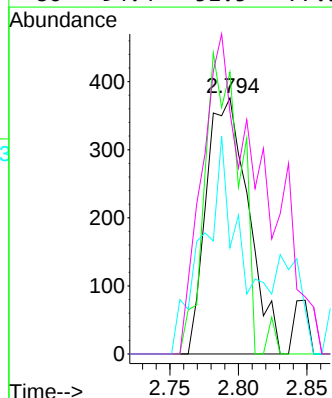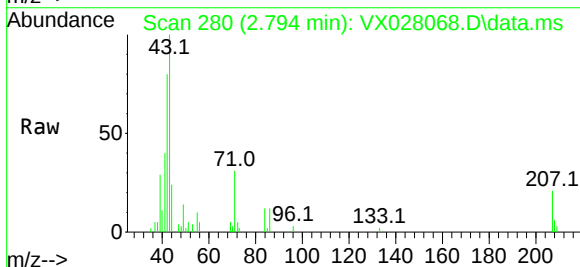



#25

2-Butanone

Concen: 0.470 ug/l

RT: 4.574 min Scan# 51

Delta R.T. 0.018 min

Lab File: VX028068.D

Acq: 12 Apr 2022 19:53

Instrument :

MSVOA_X

ClientSampleId :





MW-9

Tgt Ion: 43 Resp: 953

Ion Ratio Lower Upper

43 100

72 17.0 24.4 36.6#

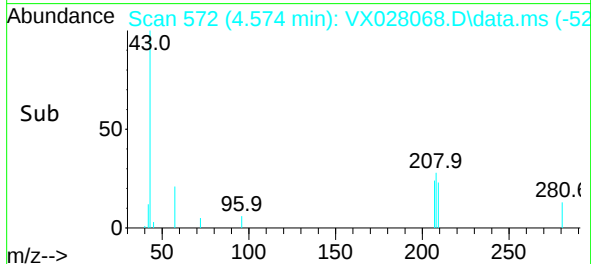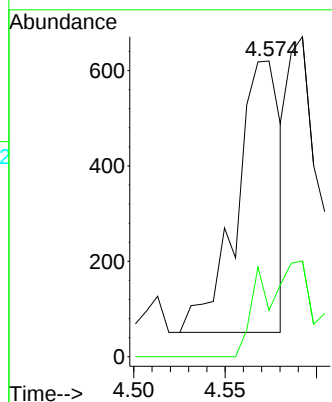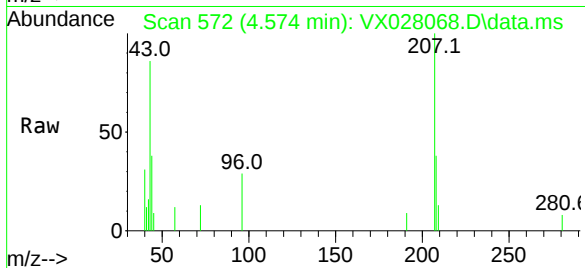

#31

Cyclohexane

Concen: 0.518 ug/l

RT: 5.482 min Scan# 721

Delta R.T. 0.005 min

Lab File: VX028068.D

Acq: 12 Apr 2022 19:53




Tgt Ion: 56 Resp: 2005


Ion Ratio Lower Upper

56 100

69 31.7 26.7 40.1

84 84.1 77.2 115.8

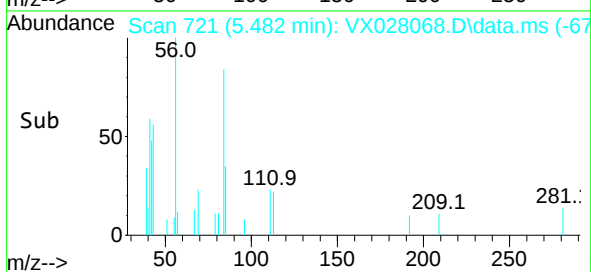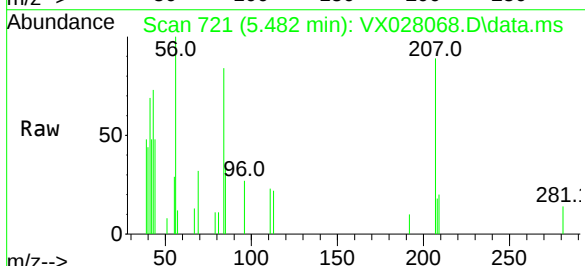



#33

1,2-Dichloroethane-d4

Concen: 49.386 ug/l

RT: 5.958 min Scan# 799

Delta R.T. -0.000 min

Lab File: VX028068.D

Acq: 12 Apr 2022 19:53

Instrument :

MSVOA_X

ClientSampleId :





MW-9

Tgt Ion: 65 Resp: 139033

Ion Ratio Lower Upper

65 100

67 51.6 0.0 107.4

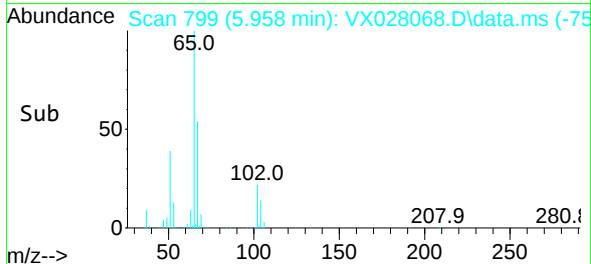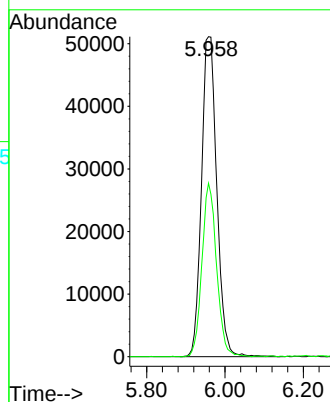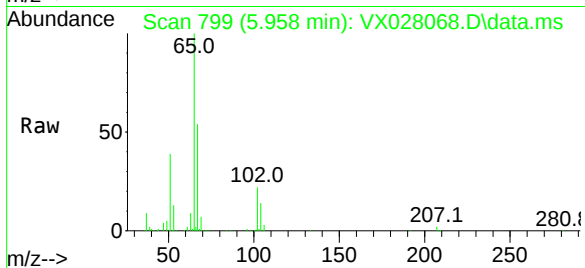

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.000 min

Lab File: VX028068.D

Acq: 12 Apr 2022 19:53




Tgt Ion: 114 Resp: 361376


Ion Ratio Lower Upper

114 100

63 18.7 0.0 36.8

88 14.0 0.0 32.4

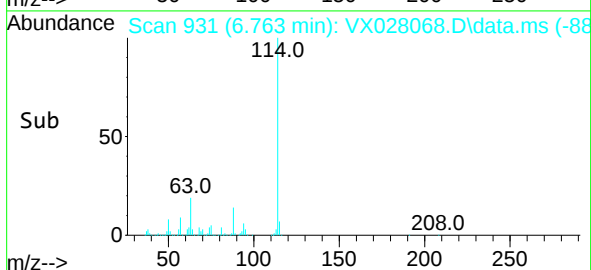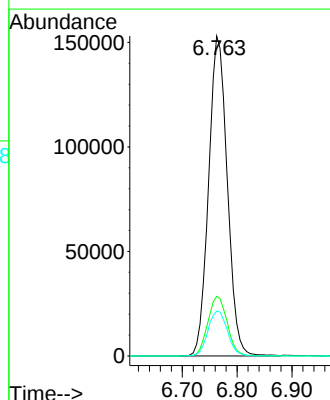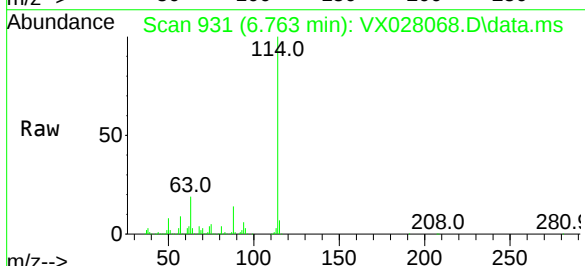

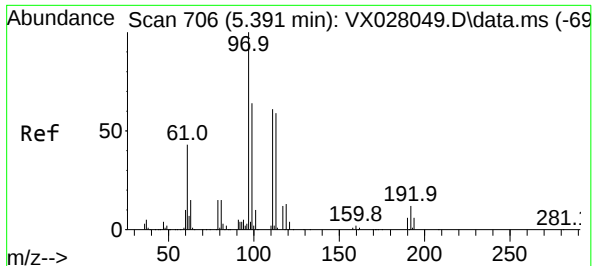

#35

Dibromofluoromethane

Concen: 49.922 ug/l

RT: 5.391 min Scan# 706

Delta R.T. -0.000 min

Lab File: VX028068.D

Acq: 12 Apr 2022 19:53

Instrument :

MSVOA_X

ClientSampleId :

MW-9





Tgt Ion:113 Resp: 118216

Ion Ratio Lower Upper

113 100

111 103.3 82.8 124.2

192 19.7 16.9 25.3

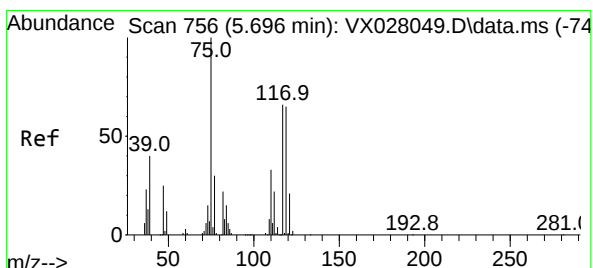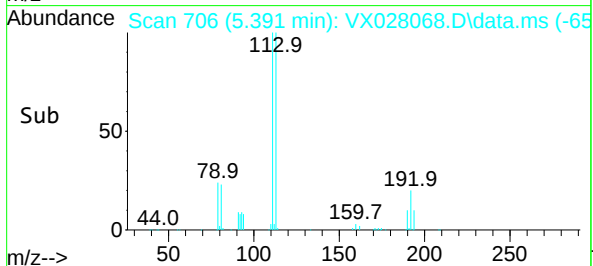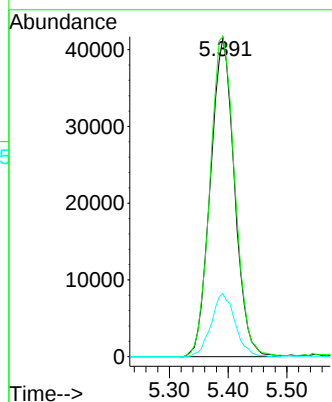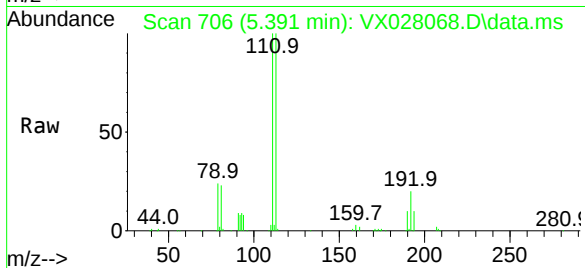

#36

1,1-Dichloropropene

Concen: 4.639 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.140 min

Lab File: VX028068.D

Acq: 12 Apr 2022 19:53




Tgt Ion: 75 Resp: 16766


Ion Ratio Lower Upper

75 100

110 9.9 18.3 54.8#

77 0.0 24.8 37.2#


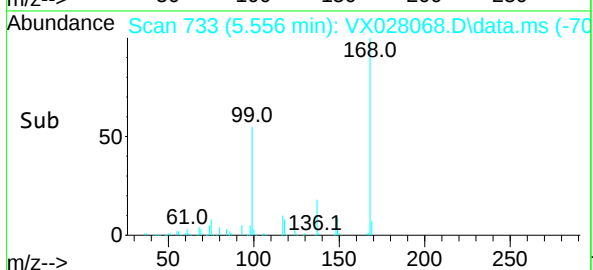

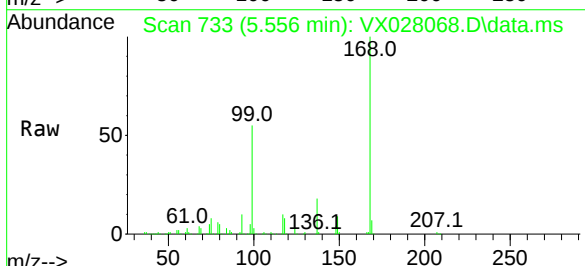




#38
Carbon Tetrachloride
Concen: 5.320 ug/l
RT: 5.562 min Scan# 71
Delta R.T. -0.122 min
Lab File: VX028068.D
Acq: 12 Apr 2022 19:53




Instrument :
MSVOA_X
ClientSampleId :
MW-9


Tgt Ion:117 Resp: 20525
Ion Ratio Lower Upper
117 100
119 4.6 77.3 115.9#
121 0.0 24.2 36.2#

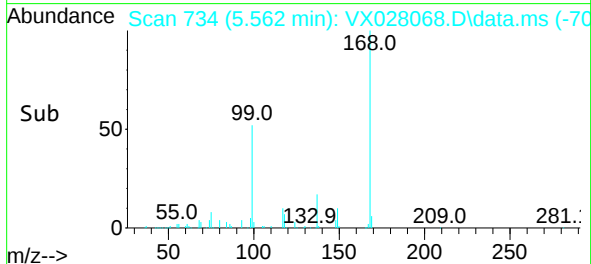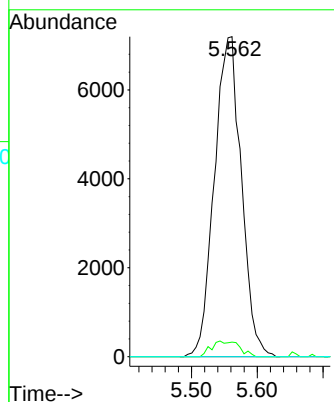

#39
Methylcyclohexane
Concen: 1.117 ug/l
RT: 7.384 min Scan# 1033
Delta R.T. -0.001 min
Lab File: VX028068.D
Acq: 12 Apr 2022 19:53

Tgt Ion: 83 Resp: 4772
Ion Ratio Lower Upper
83 100
55 78.1 54.6 81.8
98 37.3 37.4 56.2#


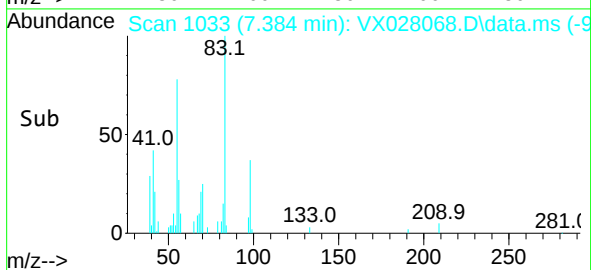
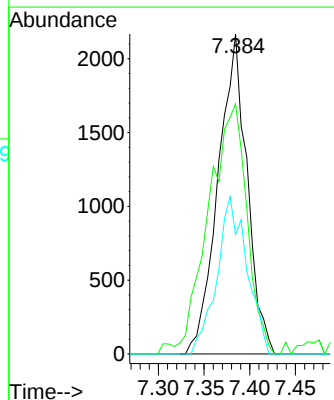
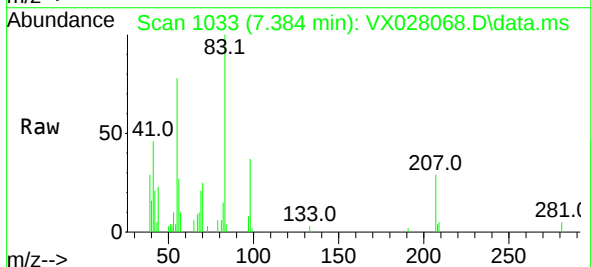




#50
Toluene-d8
Concen: 50.093 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX028068.D
Acq: 12 Apr 2022 19:53




Instrument :
MSVOA_X
ClientSampleId :
MW-9


Tgt Ion: 98 Resp: 442400
Ion Ratio Lower Upper
98 100
100 65.0 52.6 78.8

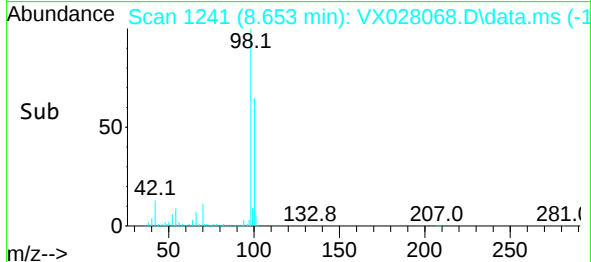

#51
4-Methyl-2-Pentanone
Concen: 0.563 ug/l
RT: 8.579 min Scan# 1229
Delta R.T. 0.005 min
Lab File: VX028068.D
Acq: 12 Apr 2022 19:53

Tgt Ion: 43 Resp: 2516
Ion Ratio Lower Upper
43 100
58 34.9 36.1 54.1#


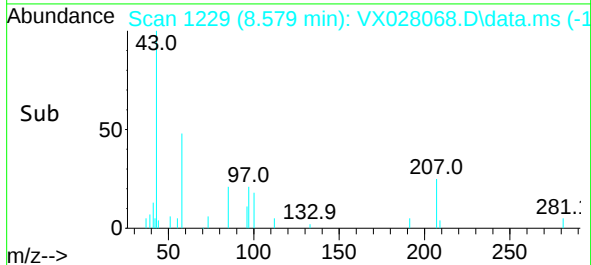

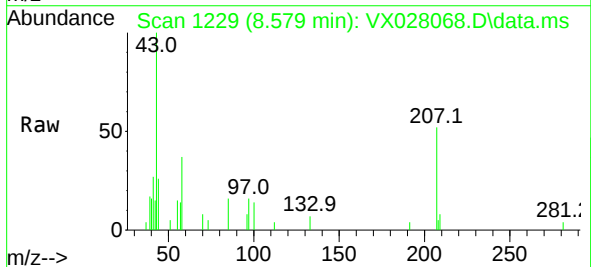


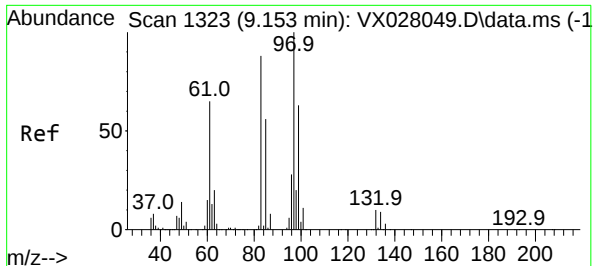

#55
 1,1,2-Trichloroethane
 Concen: 1.659 ug/l
 RT: 9.104 min Scan# 1315
 Delta R.T. -0.049 min
 Lab File: VX028068.D
 Acq: 12 Apr 2022 19:53




Instrument : MSVOA_X
 ClientSampleId : MW-9


Tgt Ion: 97	Resp: 4714
Ion Ratio	Lower Upper
97 100	
83 8.4	66.2 99.4#
85 0.0	42.9 64.3#
99 0.0	49.0 73.6#

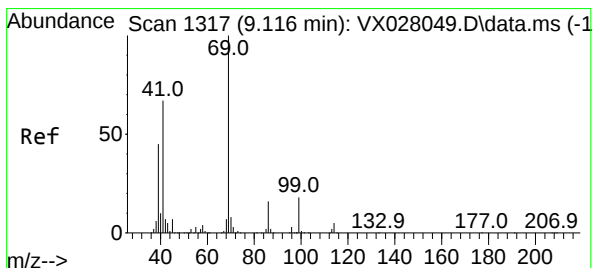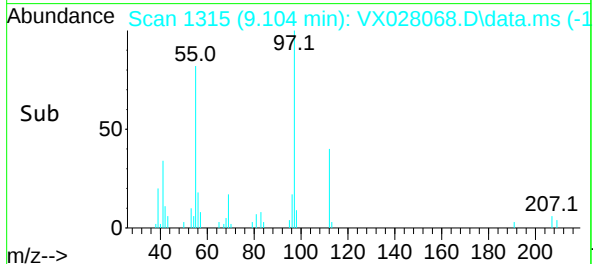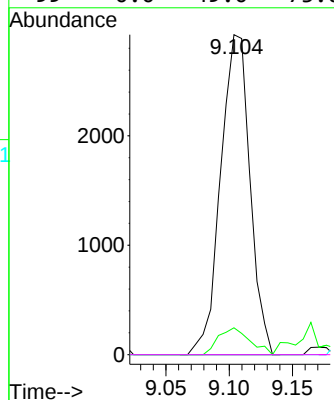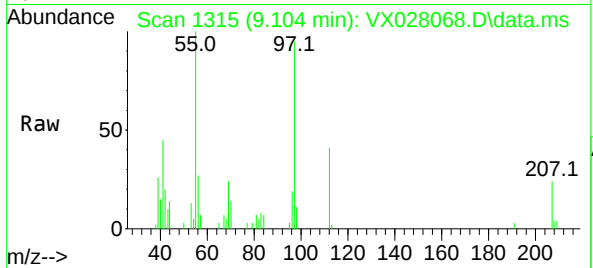

#56
 Ethyl methacrylate
 Concen: 0.290 ug/l
 RT: 9.104 min Scan# 1315
 Delta R.T. -0.012 min
 Lab File: VX028068.D
 Acq: 12 Apr 2022 19:53

Tgt Ion: 69	Resp: 1295
Ion Ratio	Lower Upper
69 100	
41 158.8	43.8 65.6#
39 87.0	22.2 33.2#

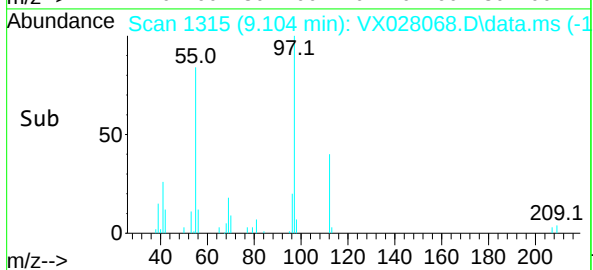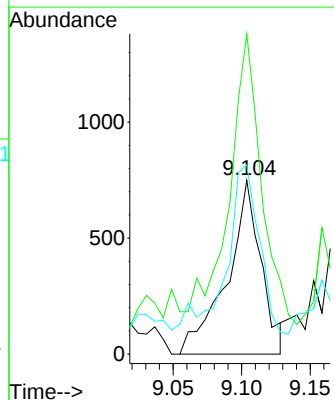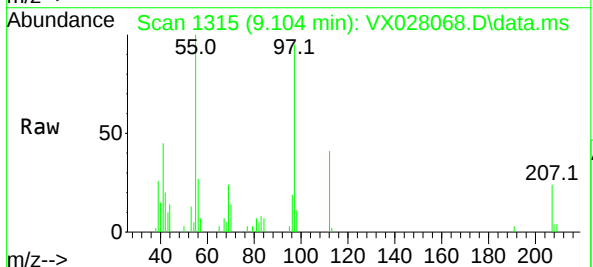



#59

2-Hexanone

Concen: 0.307 ug/l

RT: 9.445 min Scan# 11

Delta R.T. 0.012 min

Lab File: VX028068.D

Acq: 12 Apr 2022 19:53

Instrument :

MSVOA_X

ClientSampleId :





MW-9

Tgt Ion: 43 Resp: 1076

Ion Ratio Lower Upper

43 100

58 60.0 31.9 95.7

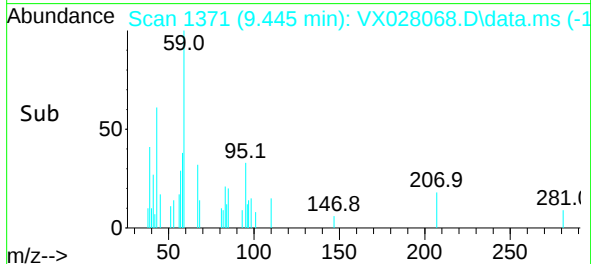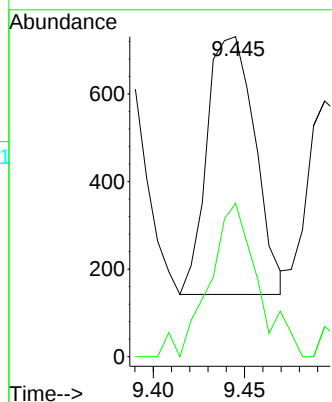

#62

4-Bromofluorobenzene

Concen: 45.571 ug/l

RT: 11.085 min Scan# 1640

Delta R.T. 0.006 min

Lab File: VX028068.D

Acq: 12 Apr 2022 19:53




Tgt Ion: 95 Resp: 150271


Ion Ratio Lower Upper

95 100

174 85.8 0.0 163.0

176 83.2 0.0 155.0


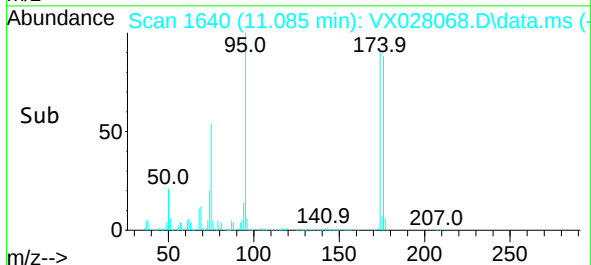

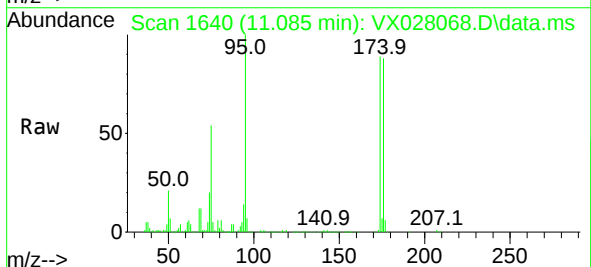


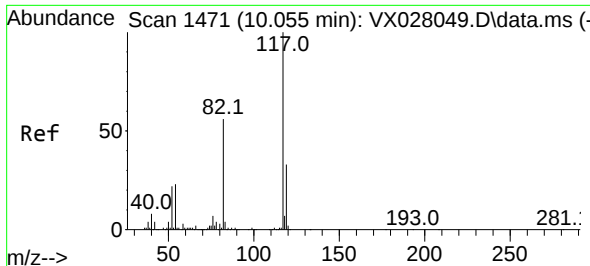

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX028068.D
Acq: 12 Apr 2022 19:53




Instrument :
MSVOA_X
ClientSampleId :
MW-9


Tgt Ion:117 Resp: 340863
Ion Ratio Lower Upper
117 100
82 55.0 41.8 62.8
119 32.4 24.8 37.2

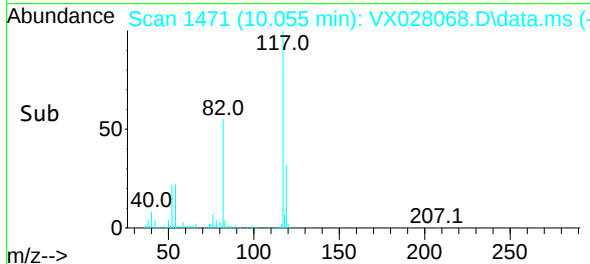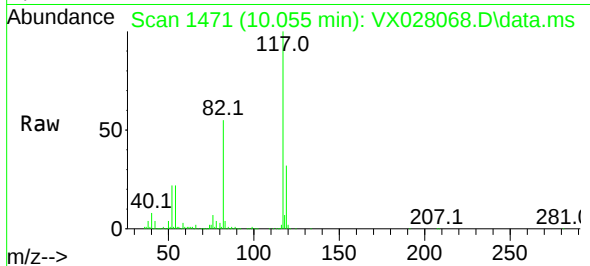

#67
Ethyl Benzene
Concen: 8.269 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.110 min
Lab File: VX028068.D
Acq: 12 Apr 2022 19:53

Tgt Ion: 91 Resp: 108303
Ion Ratio Lower Upper
91 100
106 49.4 24.6 36.8#


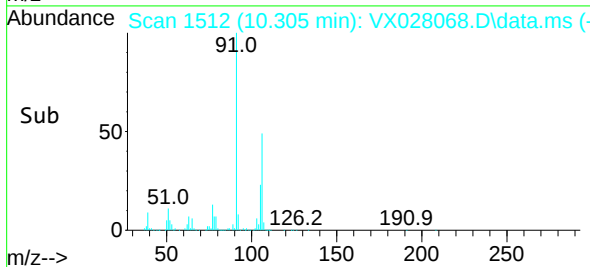

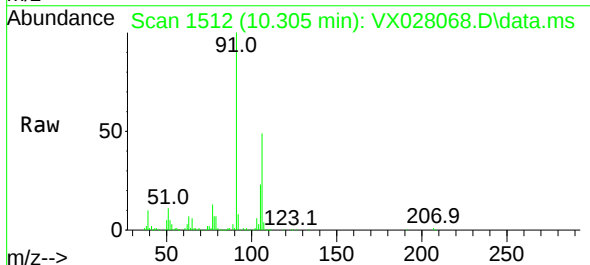




#68
m/p-Xylenes
Concen: 9.649 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX028068.D
Acq: 12 Apr 2022 19:53




Instrument :
MSVOA_X
ClientSampleId :
MW-9


Tgt Ion:106 Resp: 52770
Ion Ratio Lower Upper
106 100
91 205.2 160.4 240.6

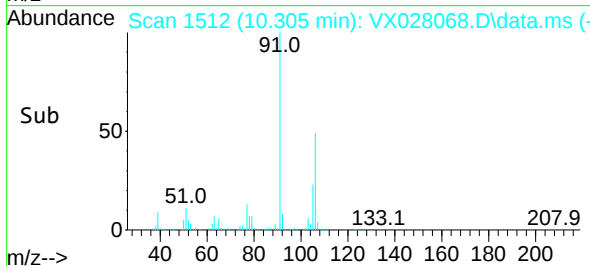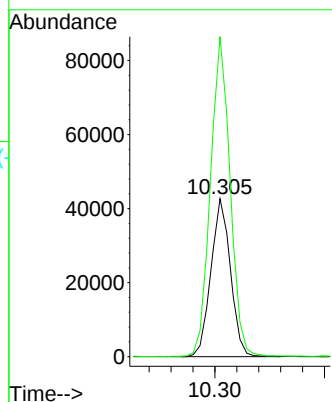

#69
o-Xylene
Concen: 3.868 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.006 min
Lab File: VX028068.D
Acq: 12 Apr 2022 19:53

Tgt Ion:106 Resp: 20561
Ion Ratio Lower Upper
106 100
91 202.6 106.1 318.1


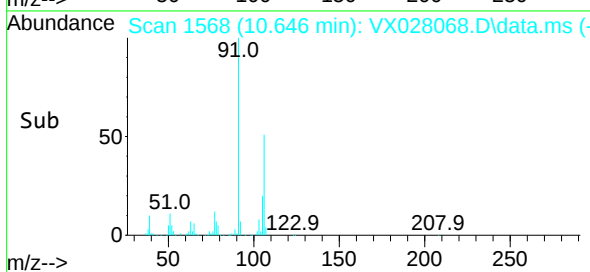
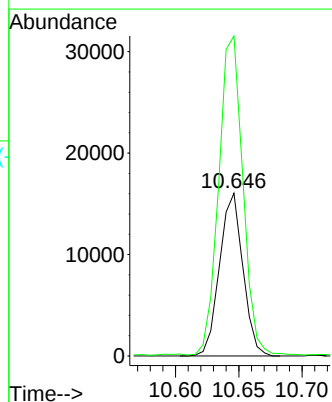
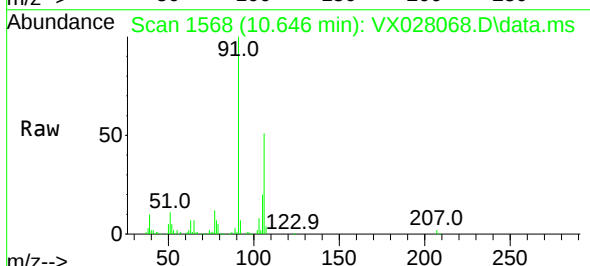


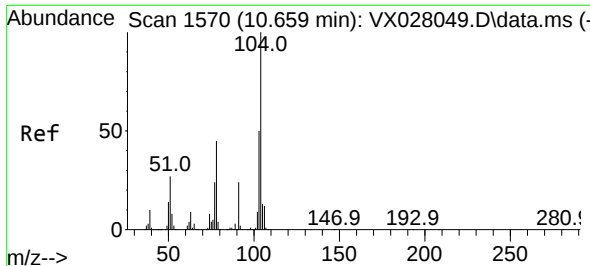

#70
Styrene
Concen: 4.803 ug/l
RT: 10.646 min Scan# 1139
Delta R.T. -0.013 min
Lab File: VX028068.D
Acq: 12 Apr 2022 19:53




Instrument :
MSVOA_X
ClientSampleId :
MW-9


Tgt Ion:104 Resp: 1139
Ion Ratio Lower Upper
104 100
78 278.9 38.6 57.8#
103 285.1 43.8 65.8#

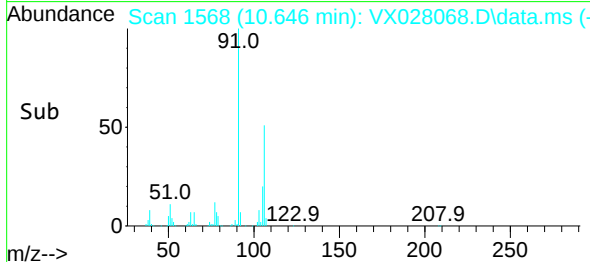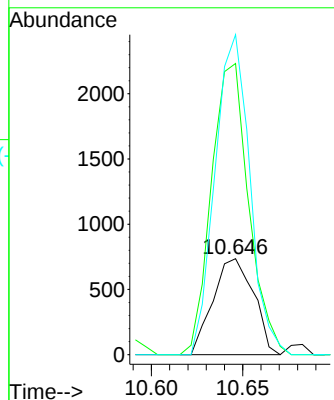

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX028068.D
Acq: 12 Apr 2022 19:53

Tgt Ion:152 Resp: 186600
Ion Ratio Lower Upper
152 100
115 59.7 37.5 112.7
150 157.4 0.0 338.2


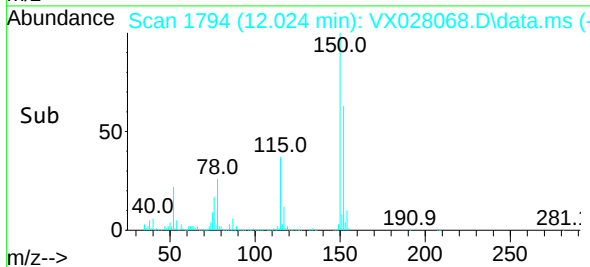
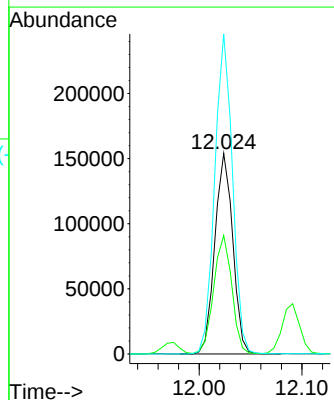
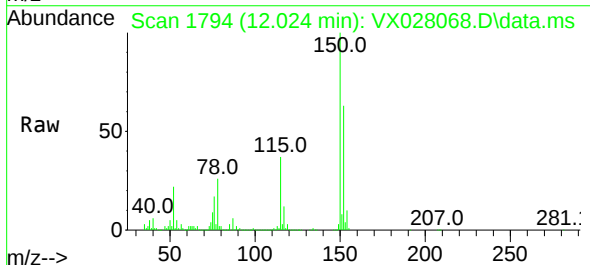




#73
Isopropylbenzene
Concen: 0.284 ug/l
RT: 10.963 min Scan# 1604
Delta R.T. 0.000 min
Lab File: VX028068.D
Acq: 12 Apr 2022 19:53




Instrument :
MSVOA_X
ClientSampleId :
MW-9


Tgt Ion:105 Resp: 3764
Ion Ratio Lower Upper
105 100
120 27.9 13.5 40.5

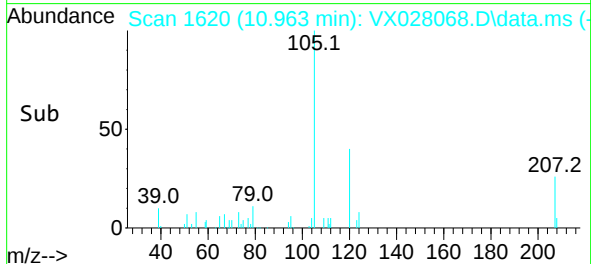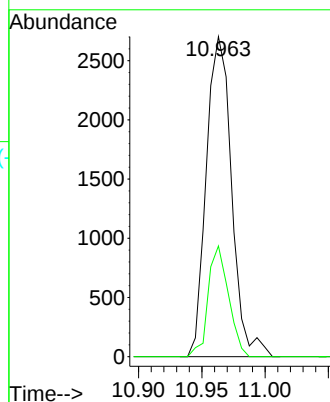

#74
N-ethyl acetate
Concen: 0.204 ug/l
RT: 10.866 min Scan# 1604
Delta R.T. 0.024 min
Lab File: VX028068.D
Acq: 12 Apr 2022 19:53

Tgt Ion: 43 Resp: 1167
Ion Ratio Lower Upper
43 100
70 76.3 42.5 63.7#
55 299.6 23.1 34.7#
61 0.0 22.8 34.2#


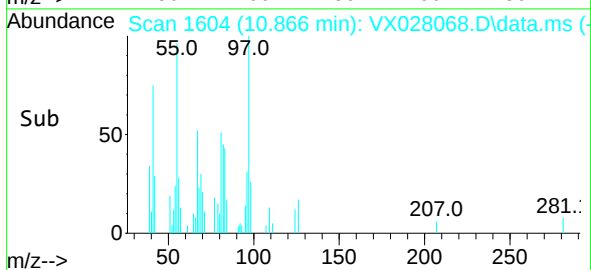
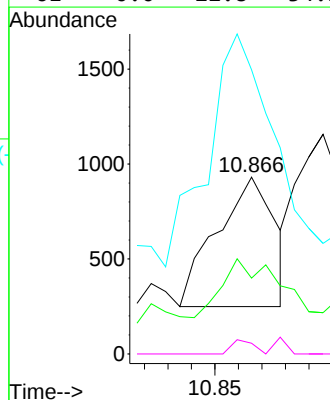
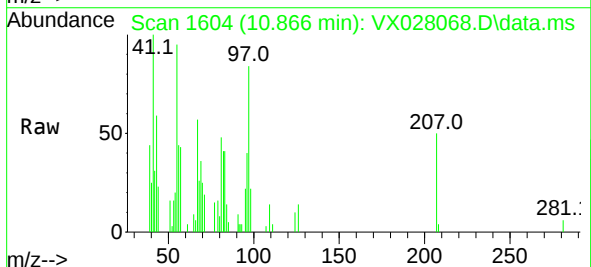




#76
1,2,3-Trichloropropane
Concen: 2.796 ug/l
RT: 11.384 min Scan# 1689
Delta R.T. 0.140 min
Lab File: VX028068.D
Acq: 12 Apr 2022 19:53




Instrument :
MSVOA_X
ClientSampleId :
MW-9


Tgt Ion: 75 Resp: 11615
Ion Ratio Lower Upper
75 100
77 1337.8 19.4 58.2#

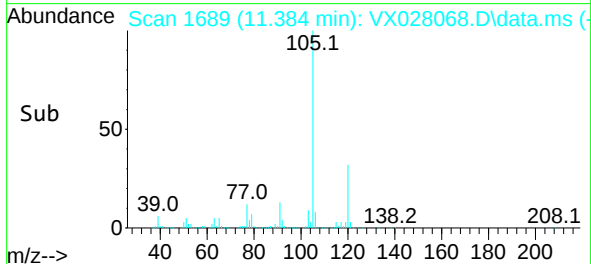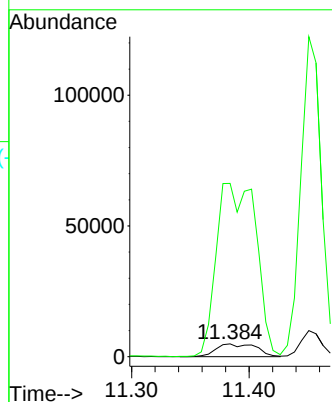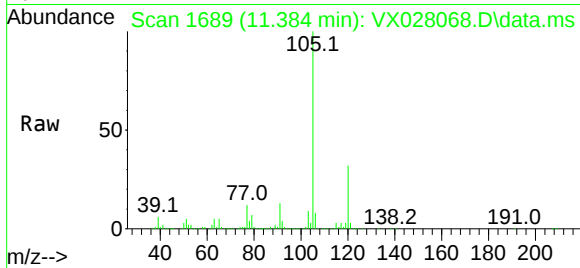

#78
n-propylbenzene
Concen: 0.523 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX028068.D
Acq: 12 Apr 2022 19:53

Tgt Ion: 91 Resp: 8055
Ion Ratio Lower Upper
91 100
120 0.0 11.6 34.8#

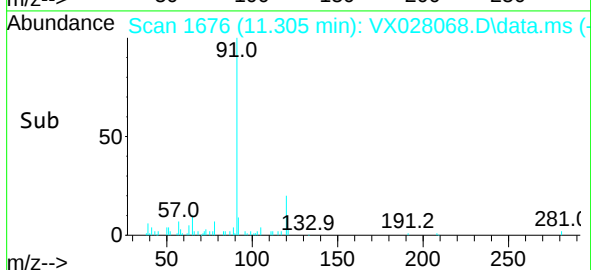

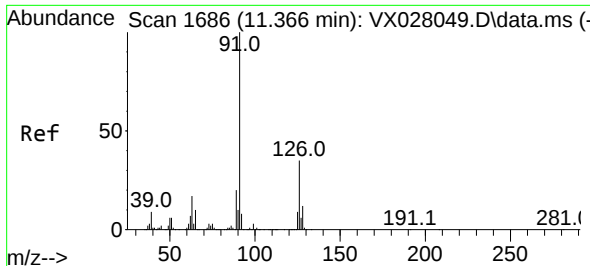

#79

2-Chlorotoluene

Concen: 17.292 ug/l

RT: 11.384 min Scan# 1

Delta R.T. 0.018 min

Lab File: VX028068.D

Acq: 12 Apr 2022 19:53

Instrument :

MSVOA_X

ClientSampleId :





MW-9

Tgt Ion: 91 Resp: 161555

Ion Ratio Lower Upper

91 100

126 0.1 17.3 51.9#

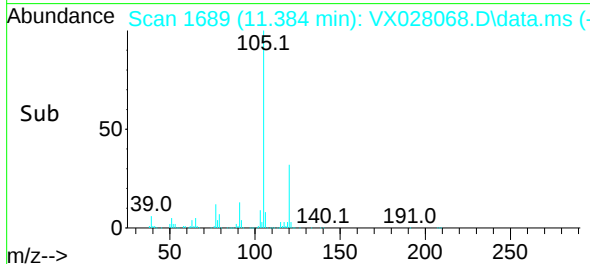

#80

1,3,5-Trimethylbenzene

Concen: 94.911 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. -0.000 min

Lab File: VX028068.D




Acq: 12 Apr 2022 19:53


Tgt Ion: 105 Resp: 1086812

Ion Ratio Lower Upper

105 100

120 50.0 24.3 72.9


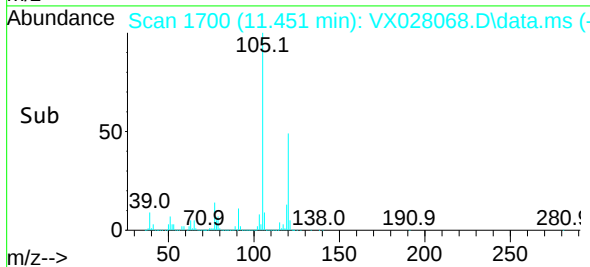

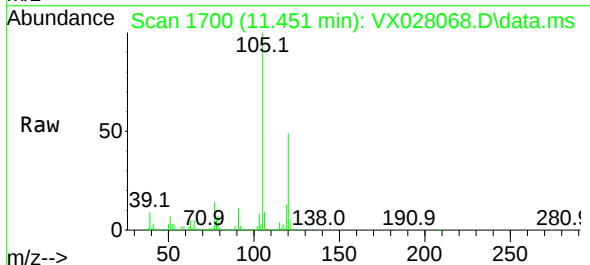


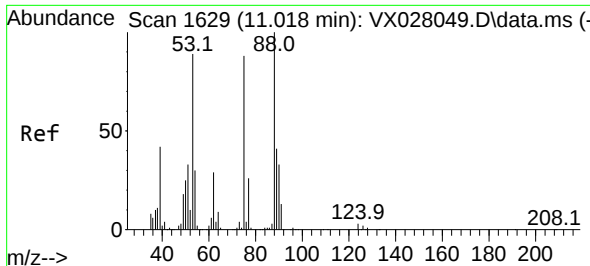

#81
trans-1,4-Dichloro-2-butene
Concen: 57.466 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX028068.D
Acq: 12 Apr 2022 19:53




Instrument :
MSVOA_X
ClientSampleId :
MW-9


Tgt Ion: 75 Resp: 84759
Ion Ratio Lower Upper
75 100
53 0.2 69.0 103.4#
89 0.3 37.0 55.6#

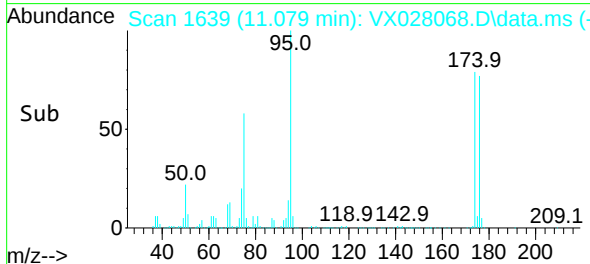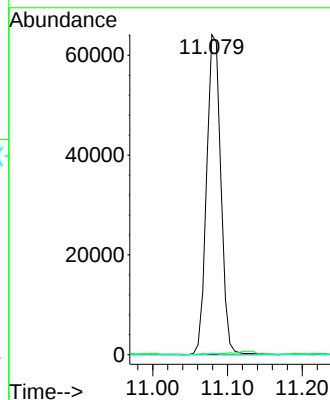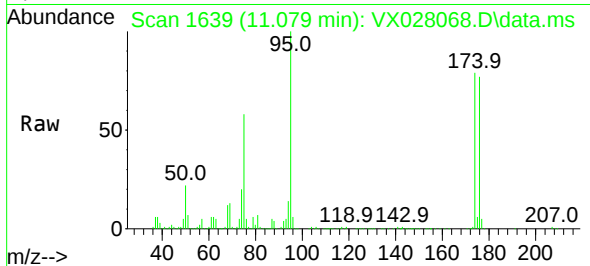

#82
4-Chlorotoluene
Concen: 11.412 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.006 min
Lab File: VX028068.D
Acq: 12 Apr 2022 19:53

Tgt Ion: 91 Resp: 125511
Ion Ratio Lower Upper
91 100
126 0.1 14.9 44.5#


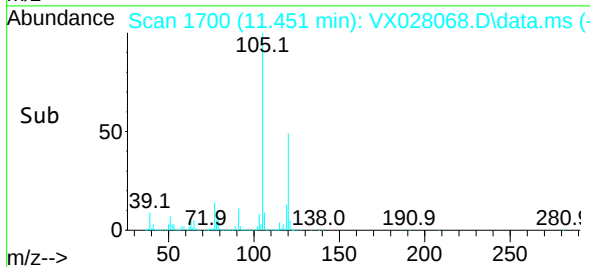
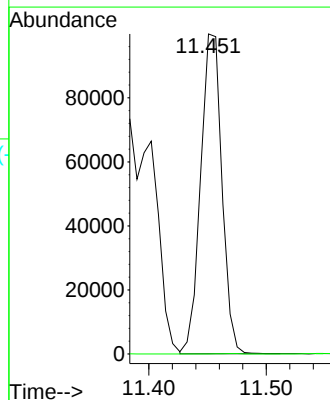
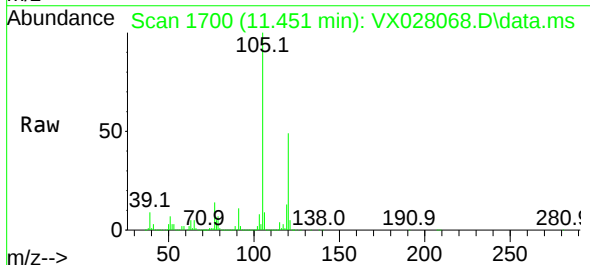




#83
 tert-Butylbenzene
 Concen: 20.296 ug/l
 RT: 11.756 min Scan# 1750
 Delta R.T. 0.043 min
 Lab File: VX028068.D
 Acq: 12 Apr 2022 19:53




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-9


Tgt Ion:119 Resp: 224866
 Ion Ratio Lower Upper
 119 100
 91 90.6 26.9 80.6#
 134 0.0 11.4 34.2#

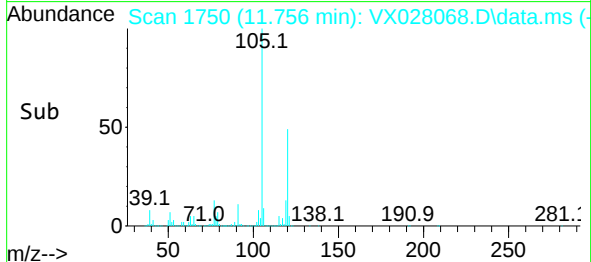

#84
 1,2,4-Trimethylbenzene
 Concen: 160.867 ug/l
 RT: 11.756 min Scan# 1750
 Delta R.T. -0.000 min
 Lab File: VX028068.D
 Acq: 12 Apr 2022 19:53

Tgt Ion:105 Resp: 1803460
 Ion Ratio Lower Upper
 105 100
 120 46.6 22.6 67.8

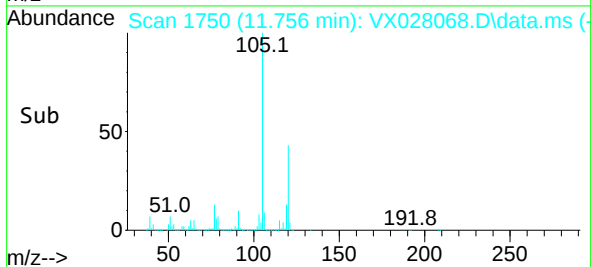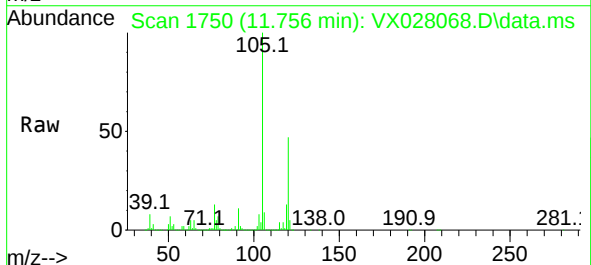



#85

sec-Butylbenzene

Concen: 127.540 ug/l

RT: 11.756 min Scan# 1750

Delta R.T. -0.134 min

Lab File: VX028068.D

Acq: 12 Apr 2022 19:53

Instrument :

MSVOA_X

ClientSampleId :





MW-9

Tgt Ion:105 Resp: 1803460

Ion Ratio Lower Upper

105 100

134 0.0 10.2 30.4#

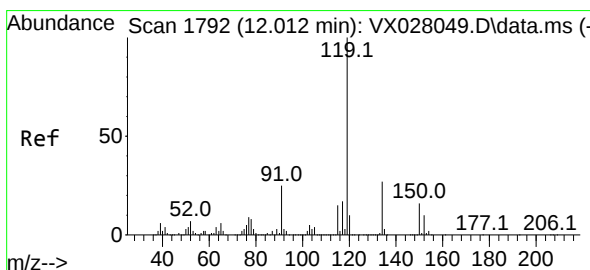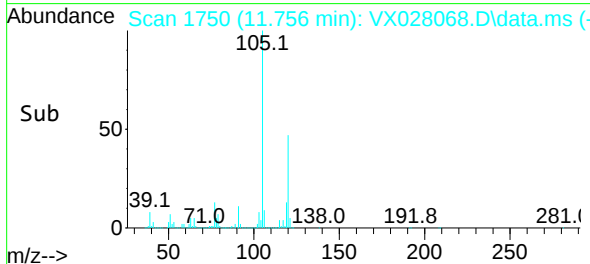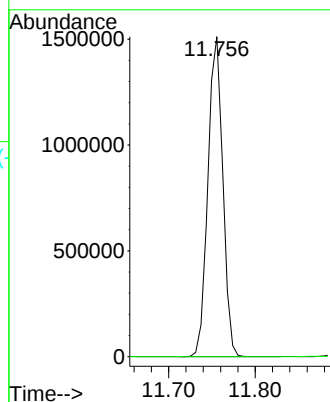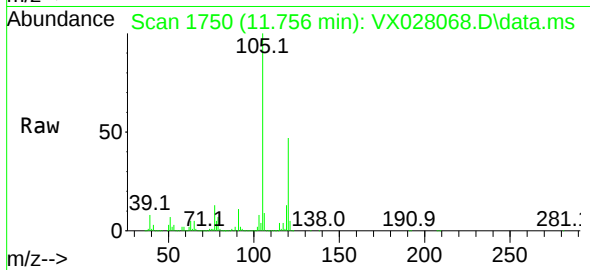

#86

p-Isopropyltoluene

Concen: 2.557 ug/l

RT: 12.012 min Scan# 1792

Delta R.T. -0.000 min

Lab File: VX028068.D

Acq: 12 Apr 2022 19:53




Tgt Ion:119 Resp: 30636


Ion Ratio Lower Upper

119 100

134 26.5 13.0 39.0

91 24.7 11.3 33.9


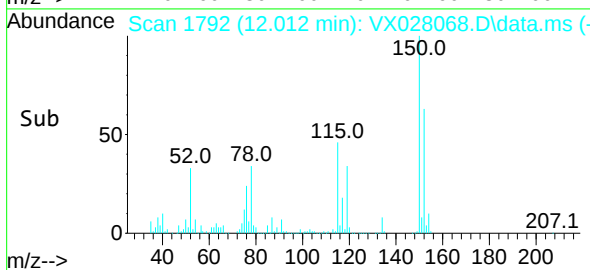
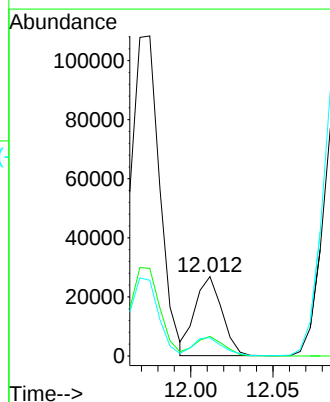
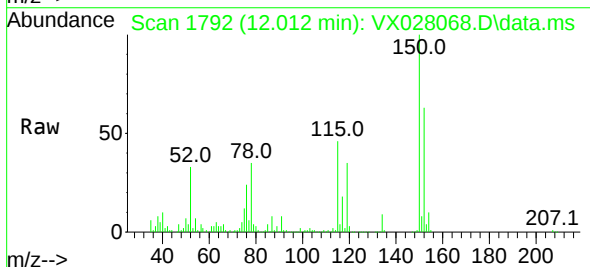


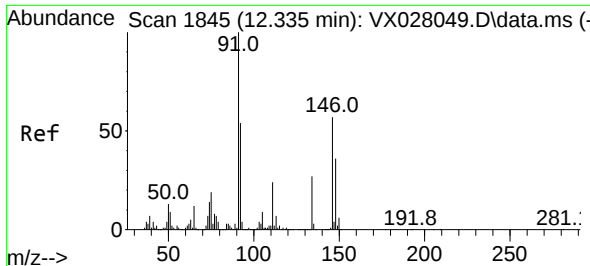

#89
n-Butylbenzene
Concen: 26.457 ug/l
RT: 12.323 min Scan# 1843
Delta R.T. -0.012 min
Lab File: VX028068.D
Acq: 12 Apr 2022 19:53




Instrument :
MSVOA_X
ClientSampleId :
MW-9


Tgt Ion: 91 Resp: 271330
Ion Ratio Lower Upper
91 100
92 13.1 27.8 83.3#
134 171.8 13.3 39.8#

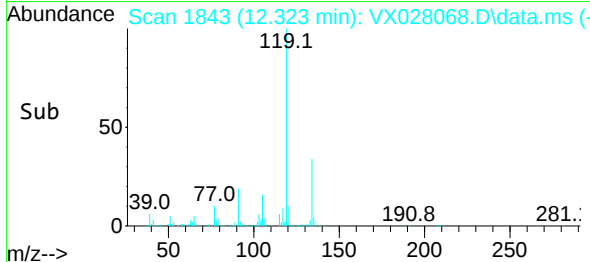

#90
Hexachloroethane
Concen: 24.381 ug/l
RT: 12.536 min Scan# 1878
Delta R.T. -0.006 min
Lab File: VX028068.D
Acq: 12 Apr 2022 19:53

Tgt Ion: 117 Resp: 49083
Ion Ratio Lower Upper
117 100
201 0.0 39.5 118.5#


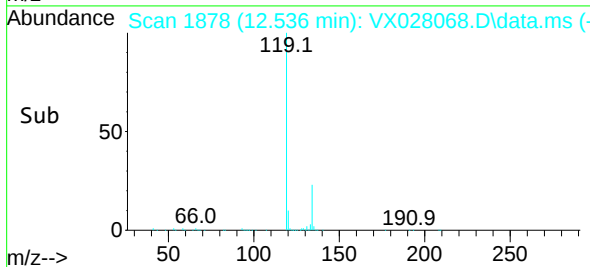

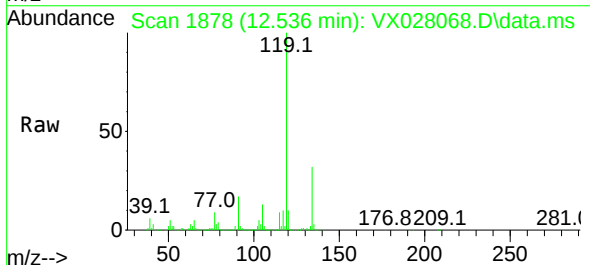




#92
 1,2-Dibromo-3-Chloropropane
 Concen: 7.487 ug/l
 RT: 12.920 min Scan# 1941
 Delta R.T. -0.025 min
 Lab File: VX028068.D
 Acq: 12 Apr 2022 19:53

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-9

Tgt Ion: 75 Resp: 7628
 Ion Ratio Lower Upper
 75 100
 155 0.0 47.0 141.2#
 157 1.5 57.9 173.6#

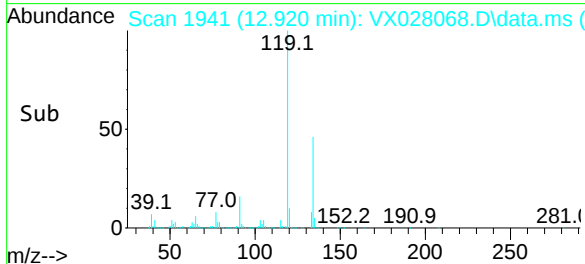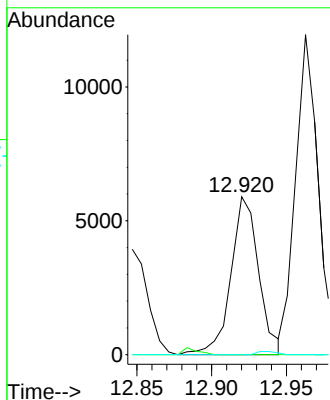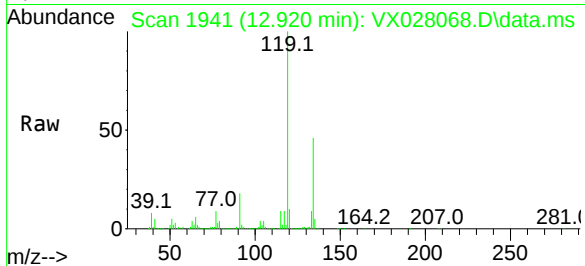

#95
 Naphthalene
 Concen: 23.811 ug/l
 RT: 13.780 min Scan# 2082
 Delta R.T. 0.006 min
 Lab File: VX028068.D
 Acq: 12 Apr 2022 19:53

Tgt Ion: 128 Resp: 293190
 Ion Ratio Lower Upper
 128 100
 127 13.7 10.2 15.4
 129 14.9 8.7 13.1#

