


Bromomethane

Response Ratio

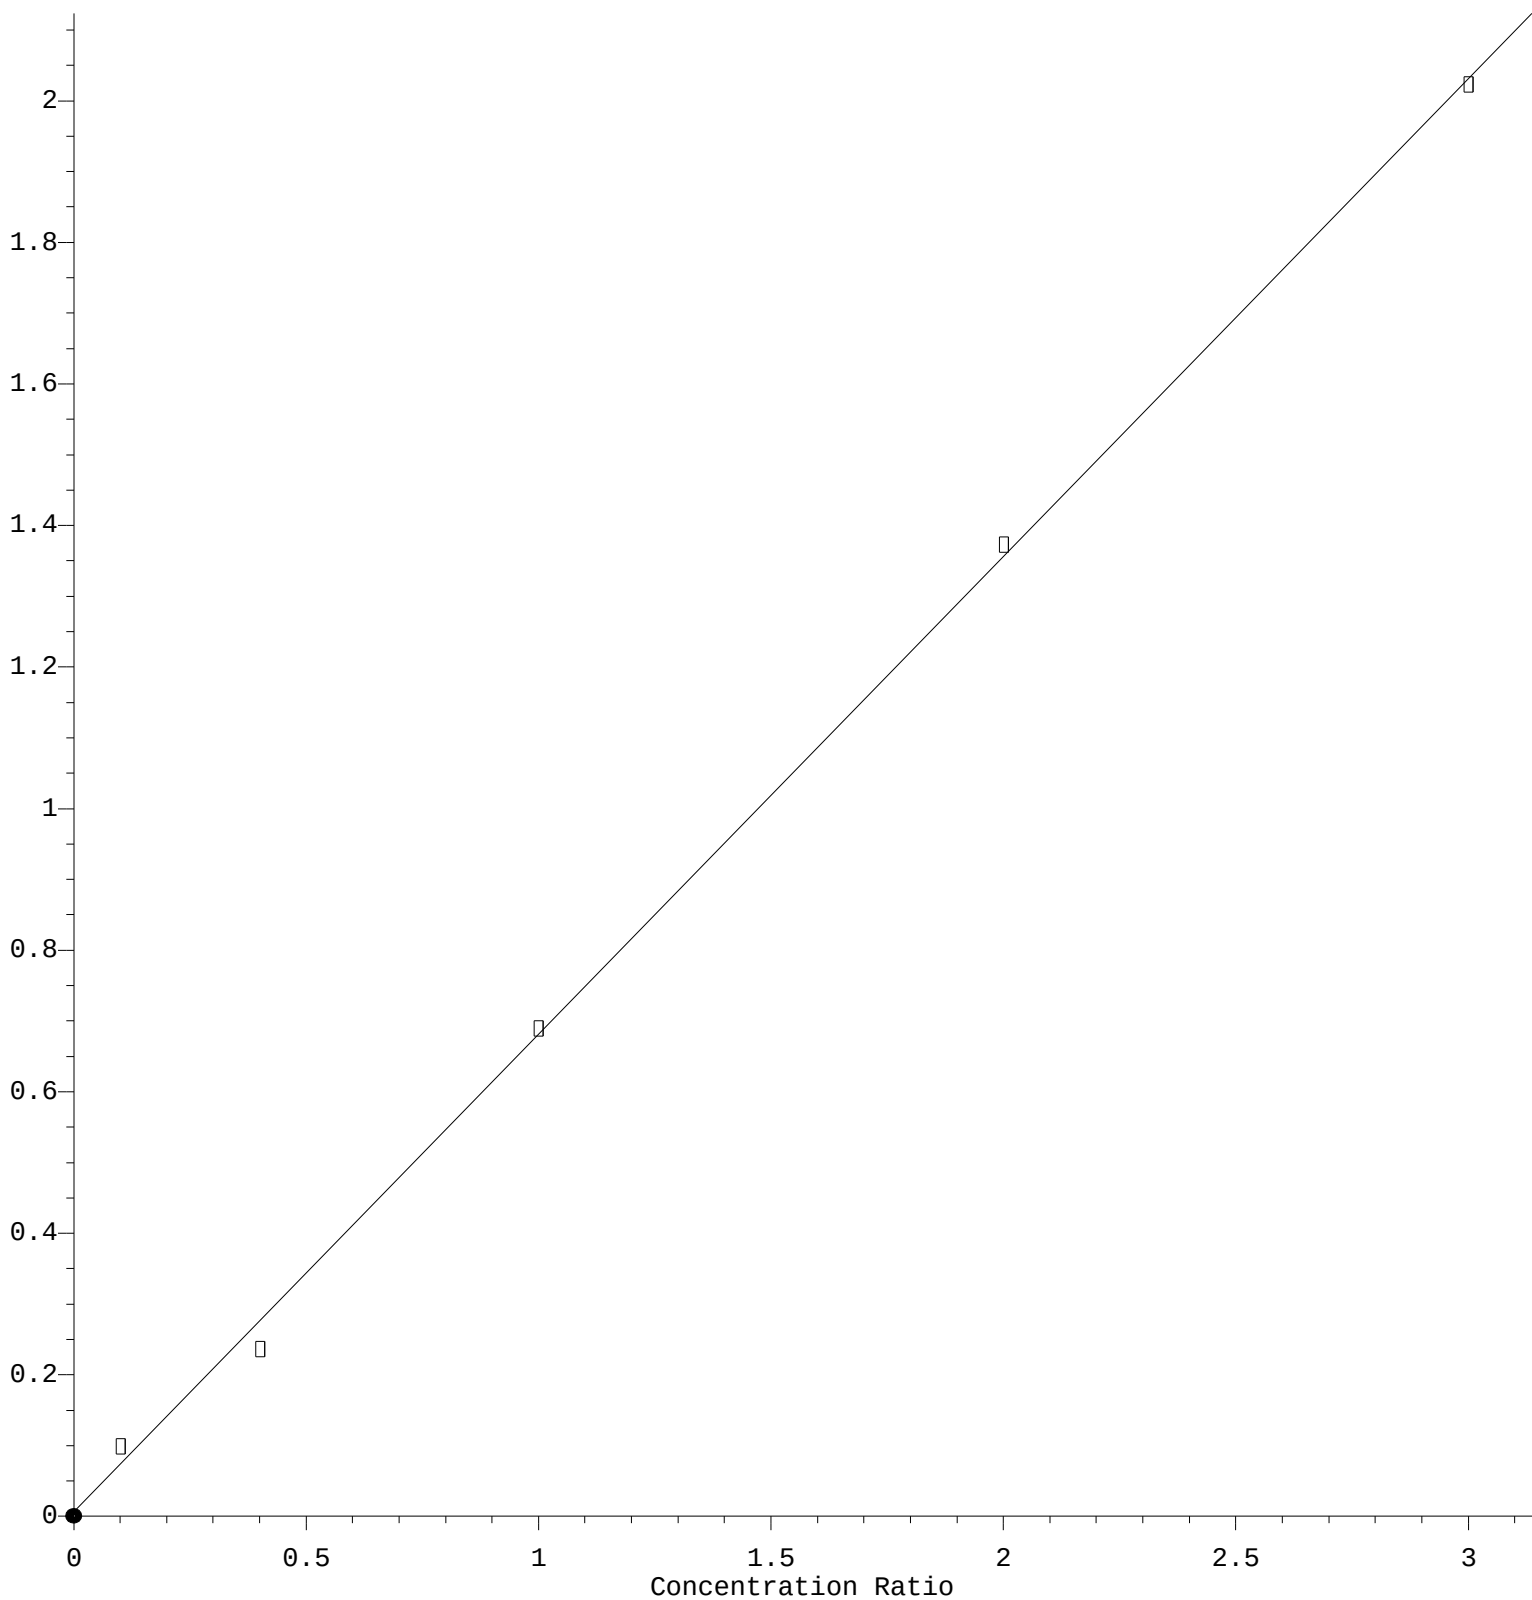

$$\text{Response} = 6.753\text{e-}001 * \text{Amt} + 5.754\text{e-}003$$


Coef of Det (r^2) = 0.998981 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M

Calibration Table Last Updated: Tue Apr 12 22:07:23 2022

Chloroethane

Response Ratio

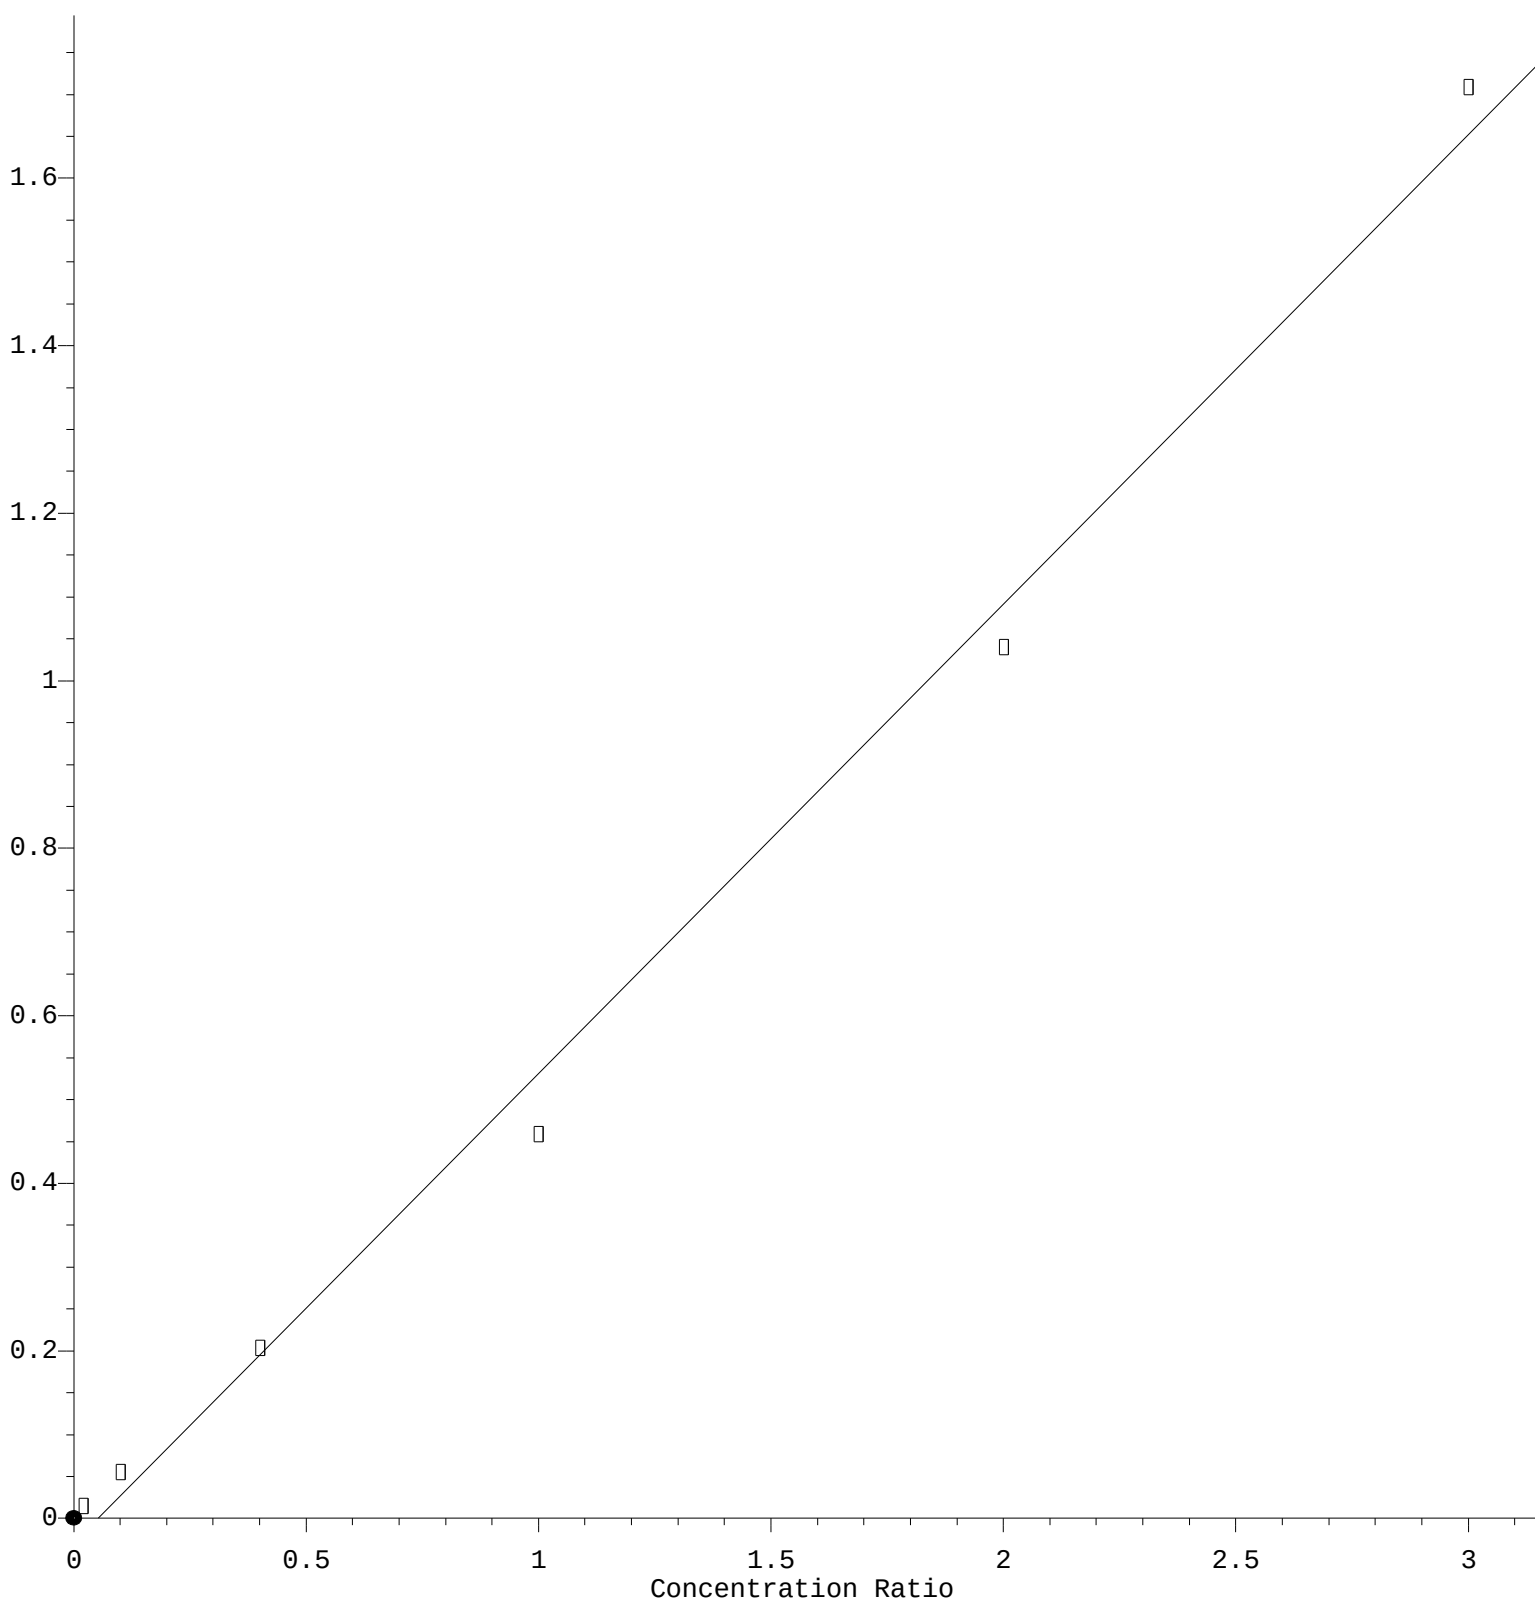

$$\text{Response} = 5.604\text{e-}001 * \text{Amt} - 2.917\text{e-}002$$


Coef of Det (r^2) = 0.994147 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M

Calibration Table Last Updated: Tue Apr 12 22:07:23 2022

Acrolein

Response Ratio

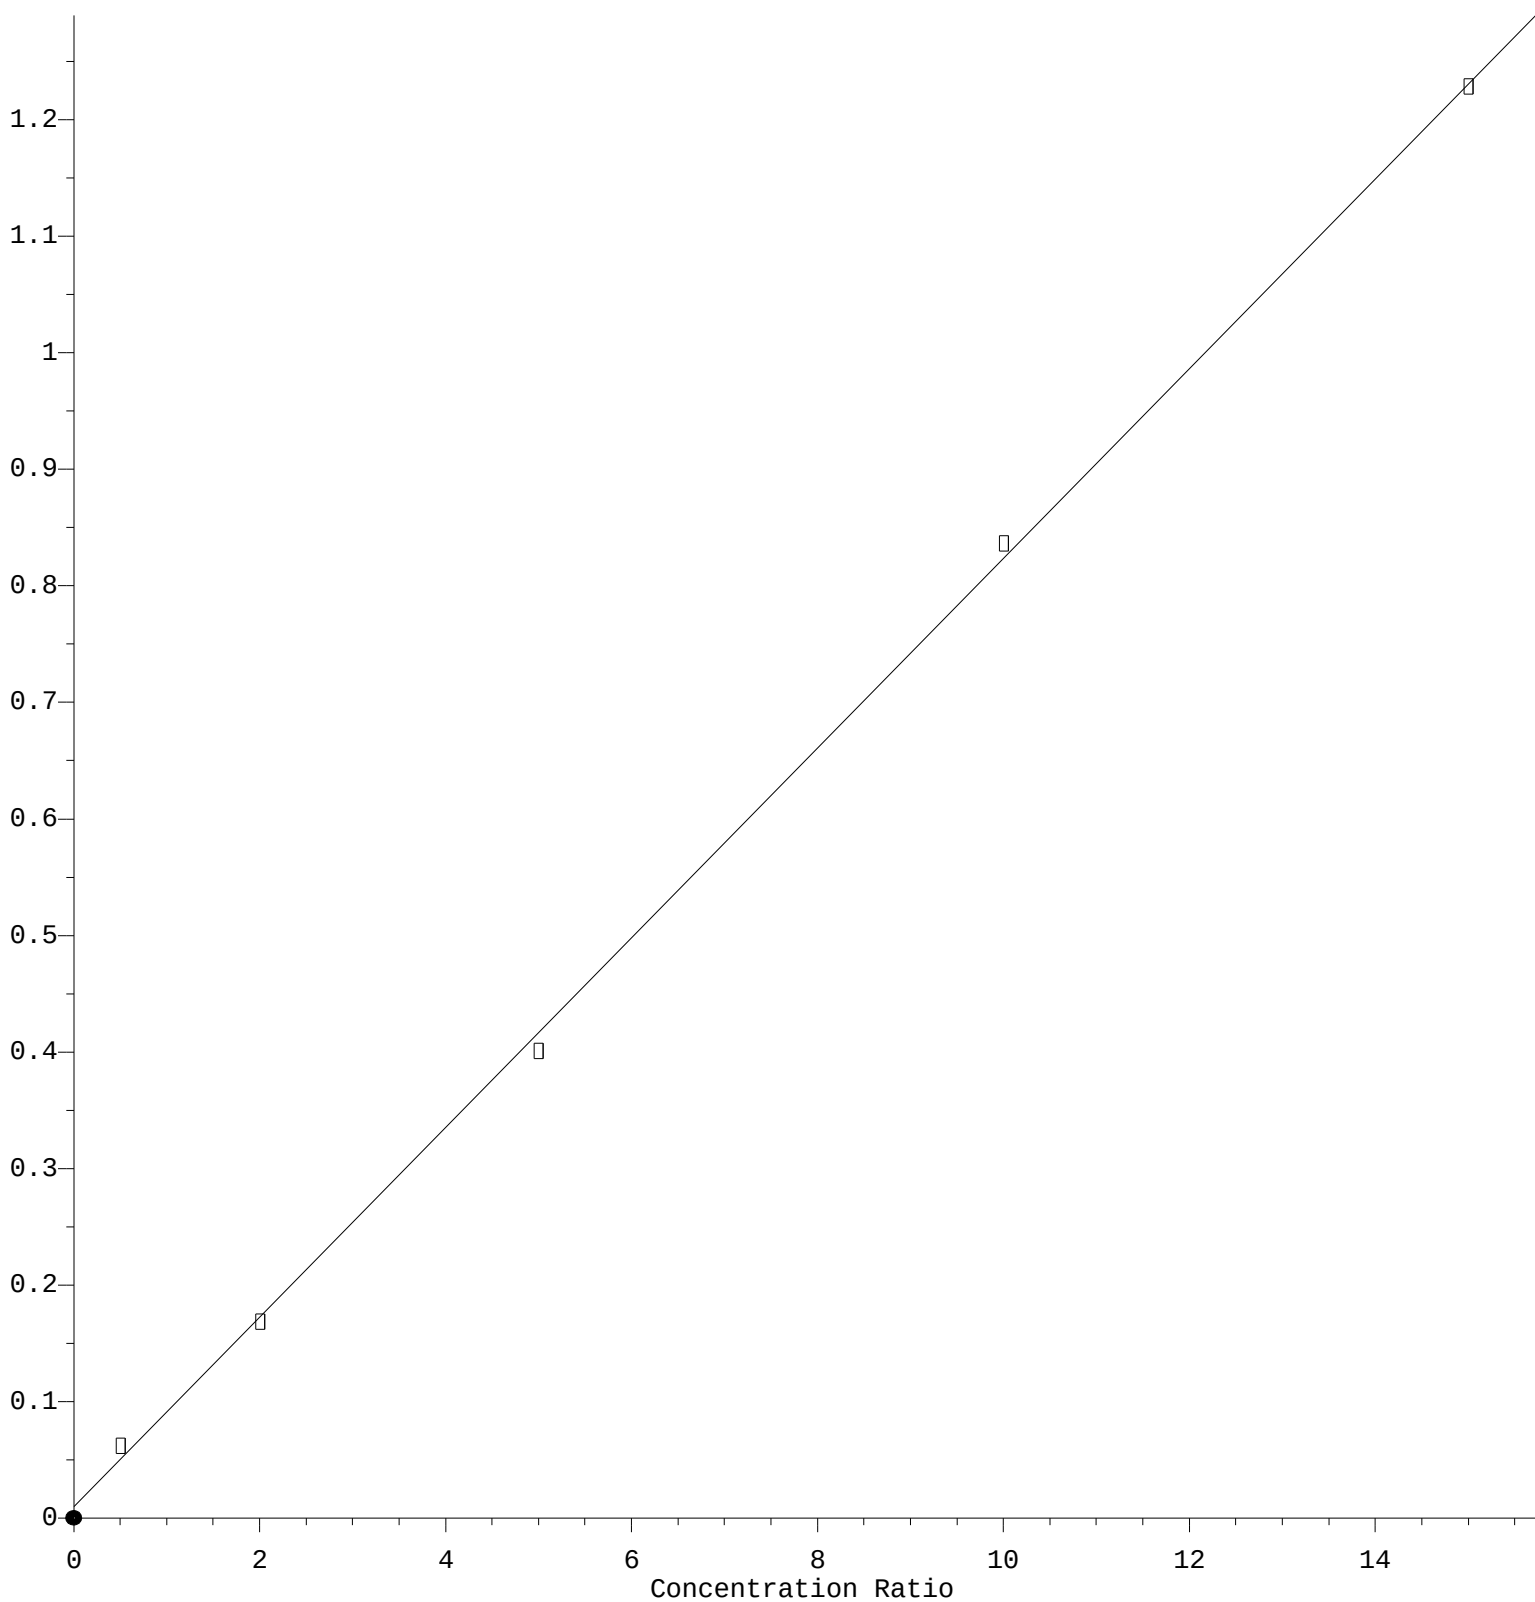

$$\text{Response} = 8.135\text{e-}002 * \text{Amt} + 1.023\text{e-}002$$


Coef of Det (r^2) = 0.999404 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M

Calibration Table Last Updated: Tue Apr 12 22:07:23 2022

Styrene

Response Ratio

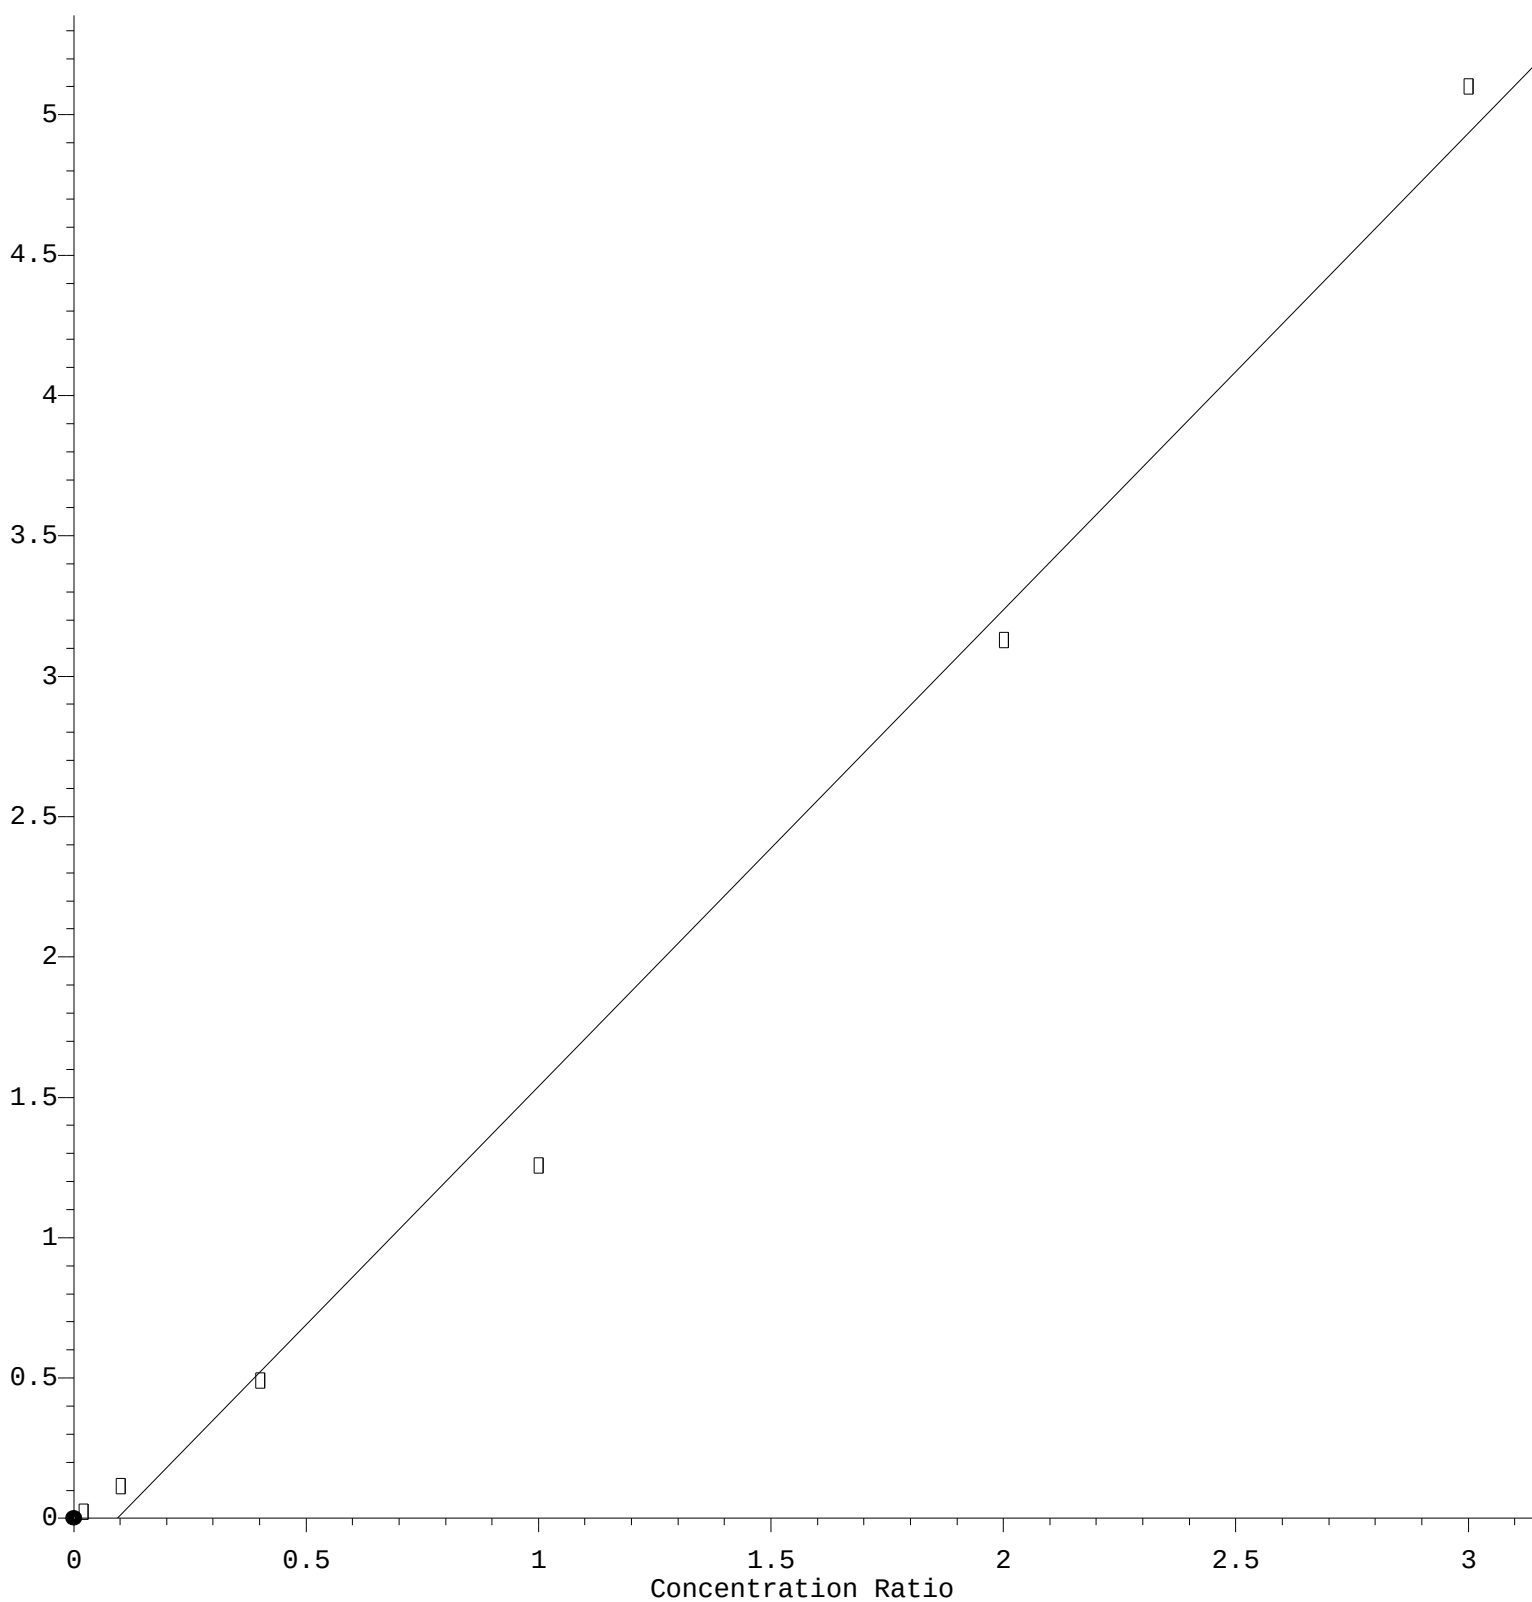

$$\text{Response} = 1.698e+000 * \text{Amt} - 1.597e-001$$


Coef of Det (r^2) = 0.992617 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M

Calibration Table Last Updated: Tue Apr 12 22:07:23 2022

Bromoform

Response Ratio

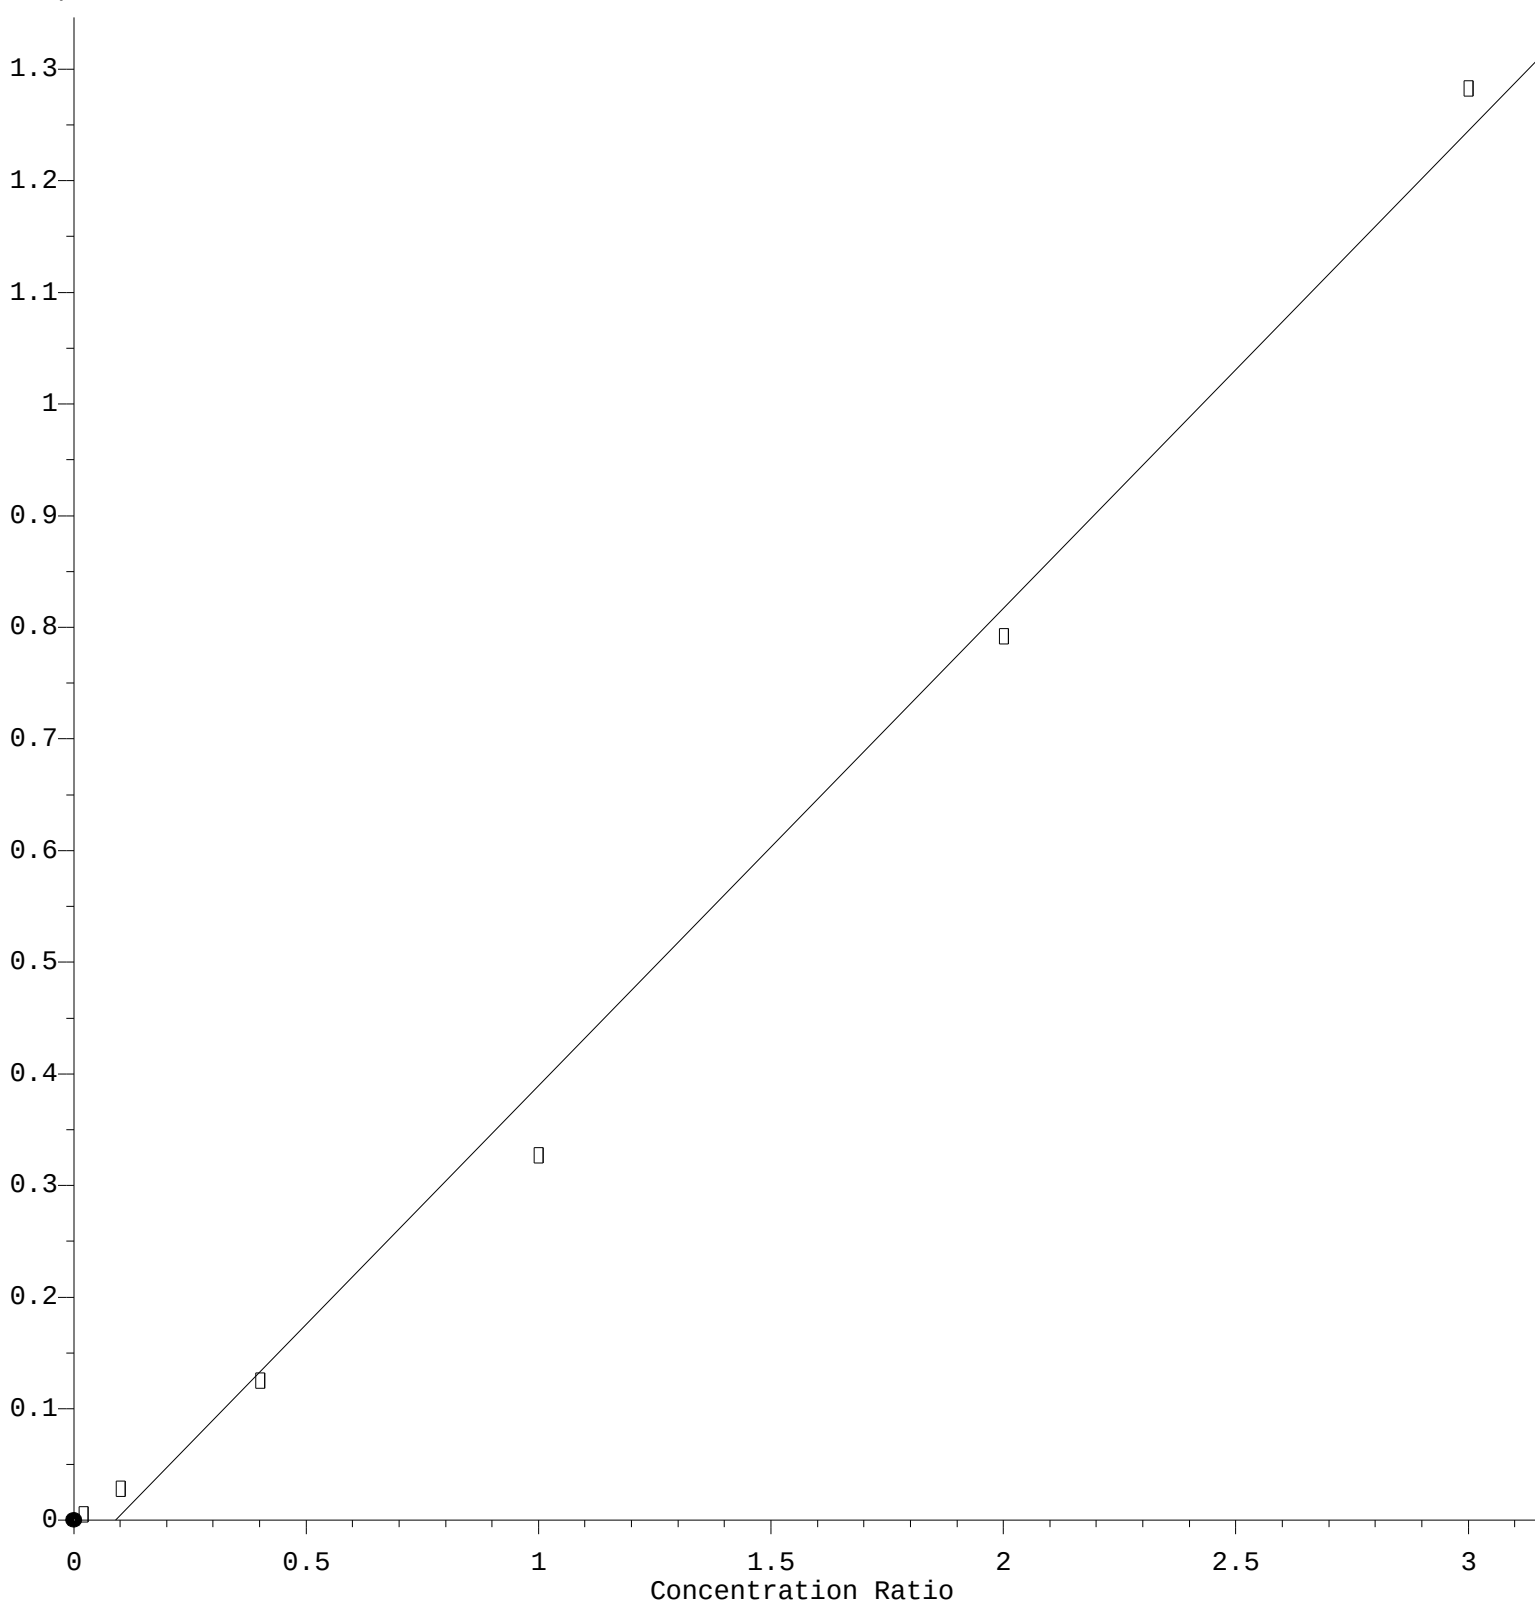

$$\text{Response} = 4.276\text{e-}001 * \text{Amt} - 3.805\text{e-}002$$

Coef of Det (r^2) = 0.993987 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M

Calibration Table Last Updated: Tue Apr 12 22:07:23 2022