

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041222\
 Data File : VX028065.D
 Acq On : 12 Apr 2022 18:43
 Operator : JC/MD
 Sample : N2353-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-5

Quant Time: Apr 13 01:14:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 12 22:07:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	209102	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	366566	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	343961	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	156066	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	140547	49.544	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	99.080%
35) Dibromofluoromethane	5.391	113	118143	49.185	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	98.380%
50) Toluene-d8	8.653	98	449433	50.169	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	100.340%
62) 4-Bromofluorobenzene	11.079	95	147409	44.070	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	88.140%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041222\
Data File : VX028065.D
Acq On : 12 Apr 2022 18:43
Operator : JC/MD
Sample : N2353-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Time: Apr 13 01:14:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 12 22:07:23 2022
Response via : Initial Calibration




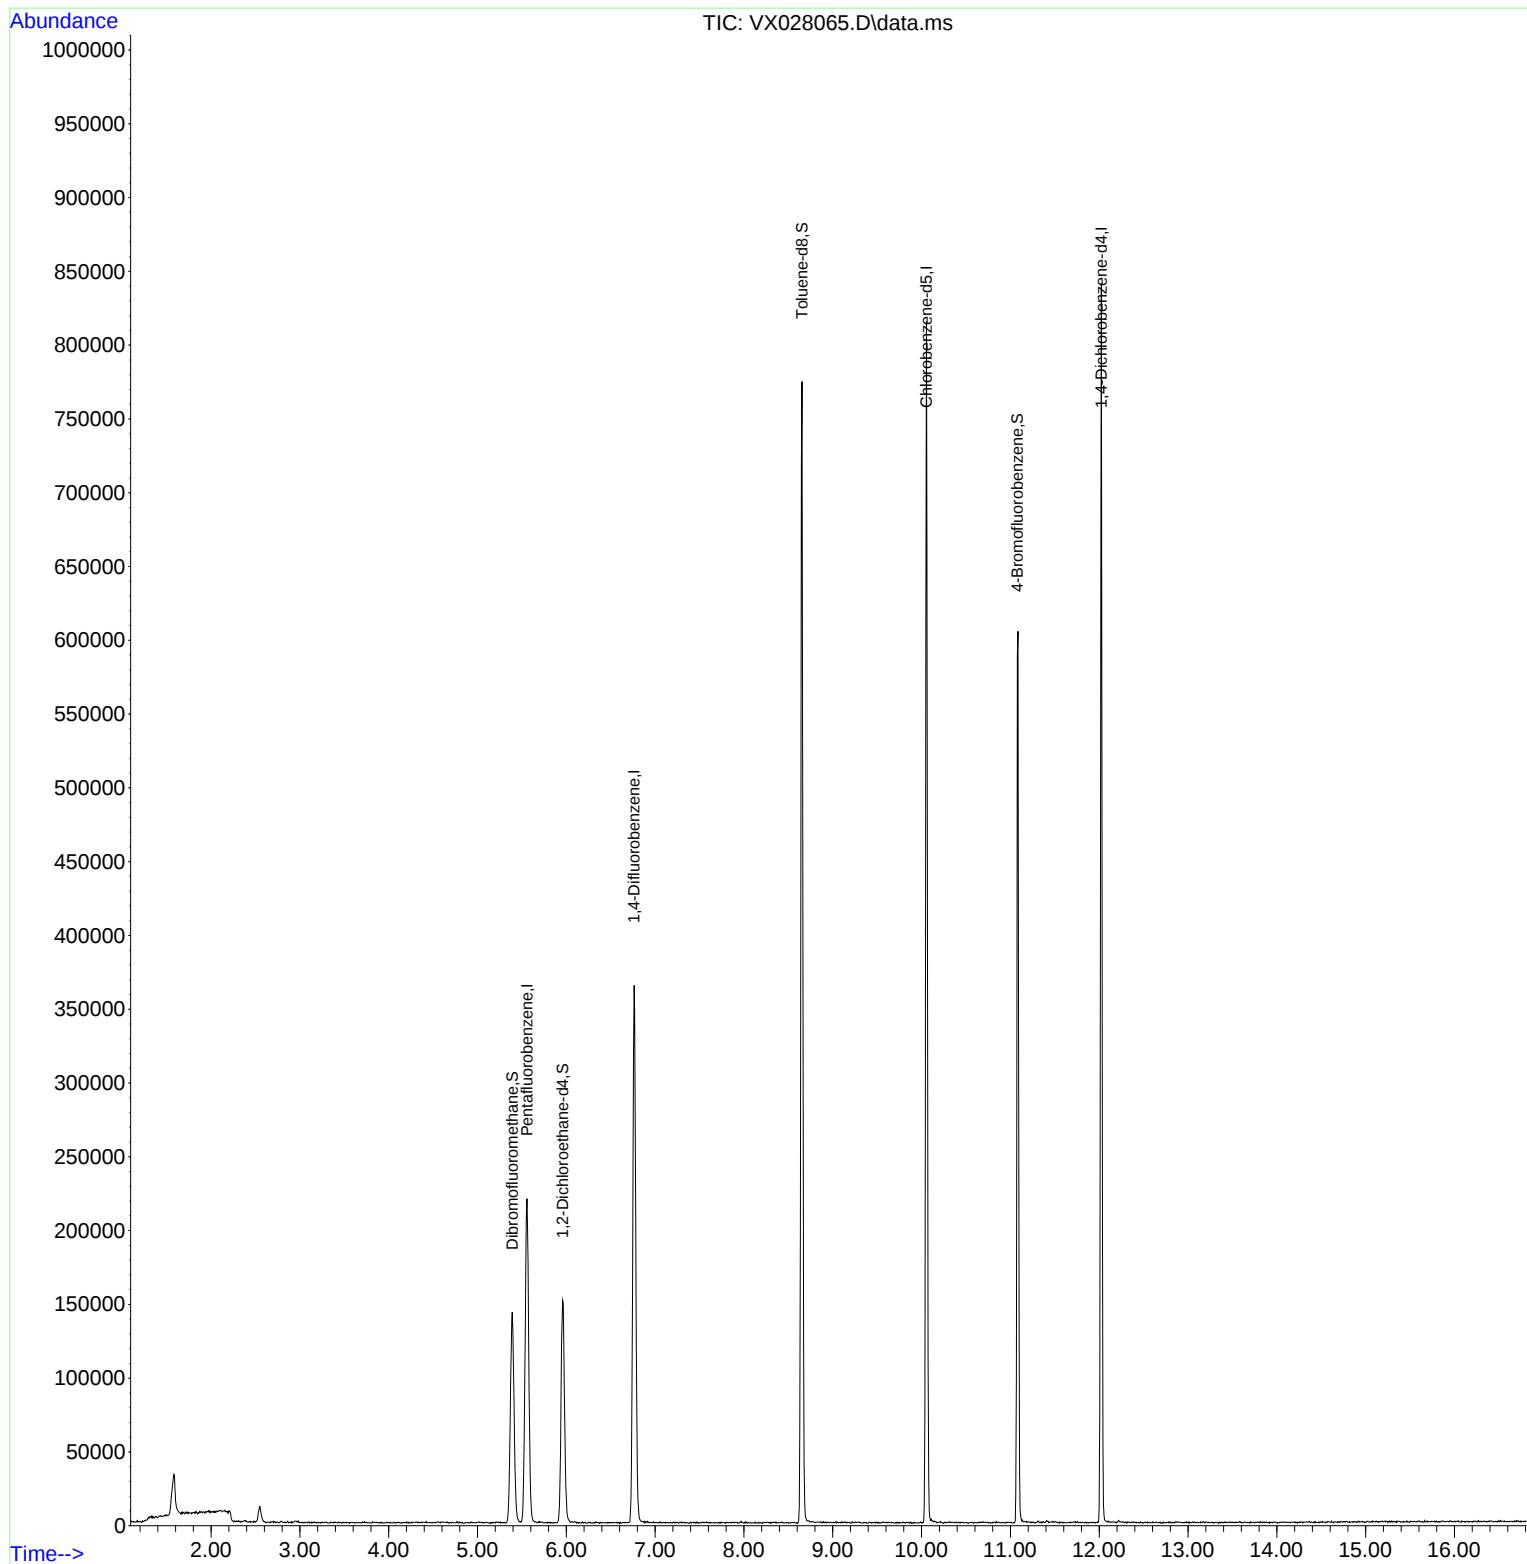




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 713
Delta R.T. -0.000 min
Lab File: VX028065.D
Acq: 12 Apr 2022 18:43




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion:168 Resp: 209102
Ion Ratio Lower Upper
168 100
99 55.7 41.7 62.5

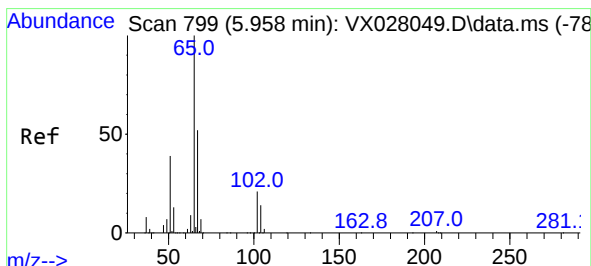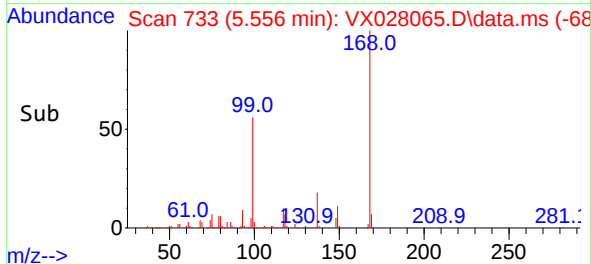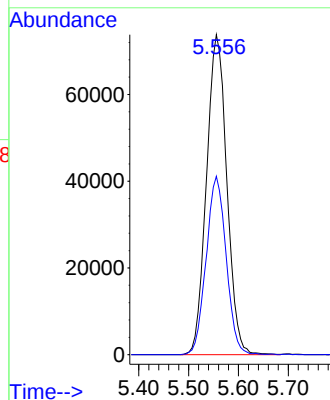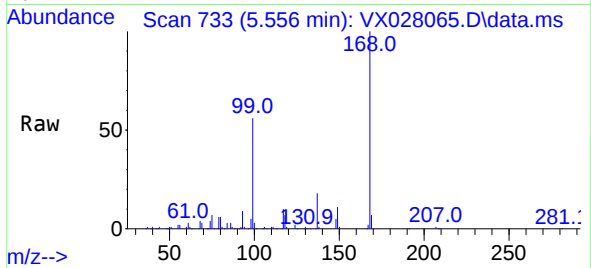

#33
1,2-Dichloroethane-d4
Concen: 49.544 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX028065.D
Acq: 12 Apr 2022 18:43

Tgt Ion: 65 Resp: 140547
Ion Ratio Lower Upper
65 100
67 50.2 0.0 107.4


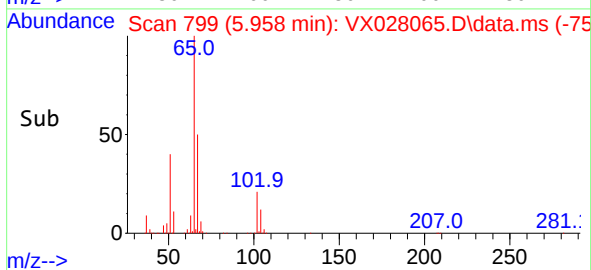
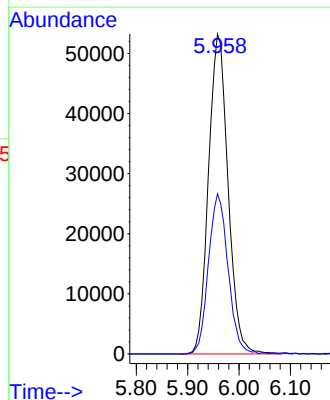
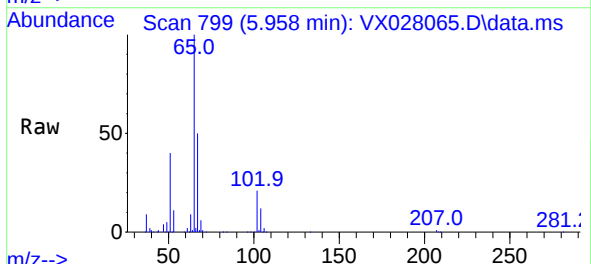


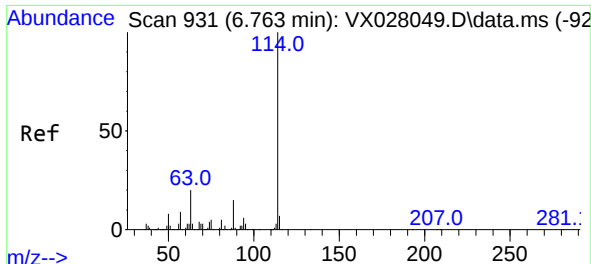

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX028065.D
Acq: 12 Apr 2022 18:43




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion:114 Resp: 366566
Ion Ratio Lower Upper
114 100
63 19.3 0.0 36.8
88 14.8 0.0 32.4

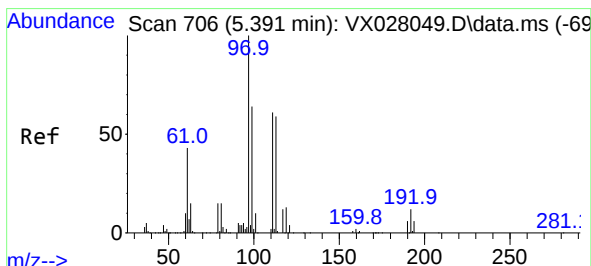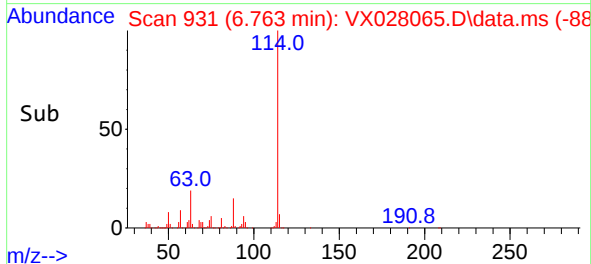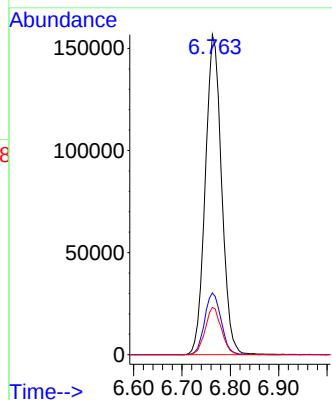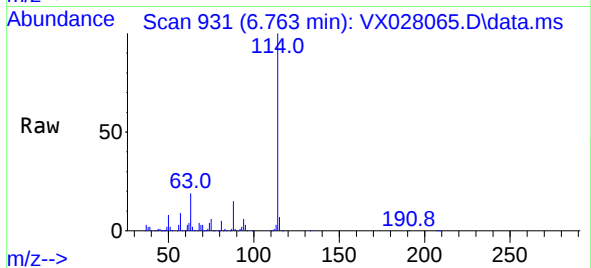

#35
Dibromofluoromethane
Concen: 49.185 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX028065.D
Acq: 12 Apr 2022 18:43

Tgt Ion:113 Resp: 118143
Ion Ratio Lower Upper
113 100
111 103.0 82.8 124.2
192 20.4 16.9 25.3


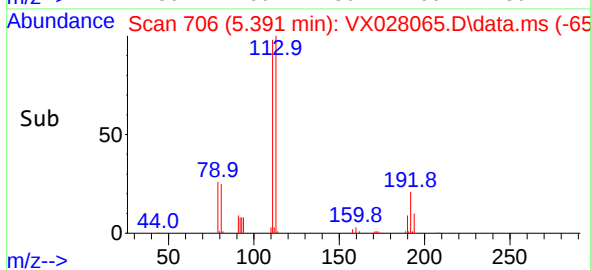
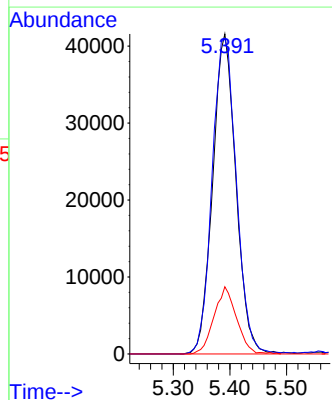
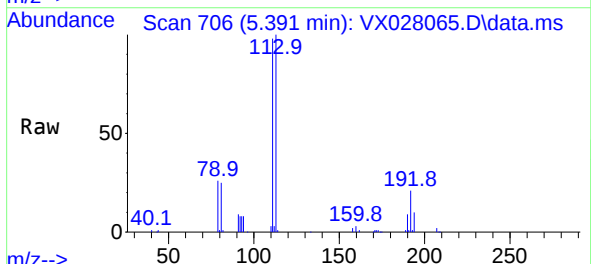


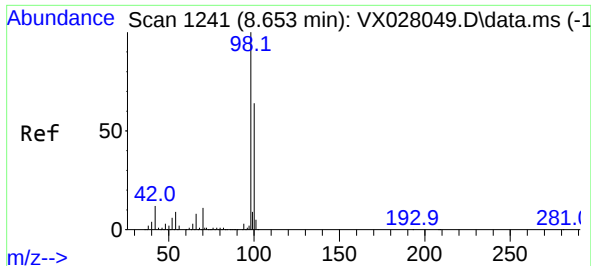

#50
Toluene-d8
Concen: 50.169 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX028065.D
Acq: 12 Apr 2022 18:43




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion: 98 Resp: 449433
Ion Ratio Lower Upper
98 100
100 65.0 52.6 78.8

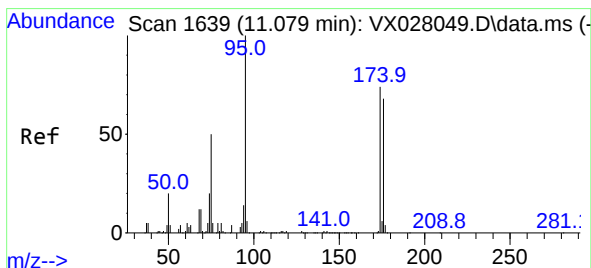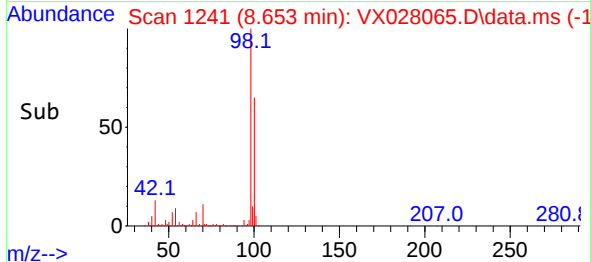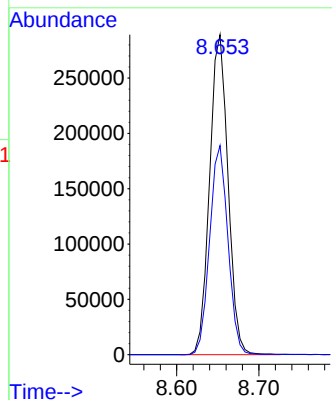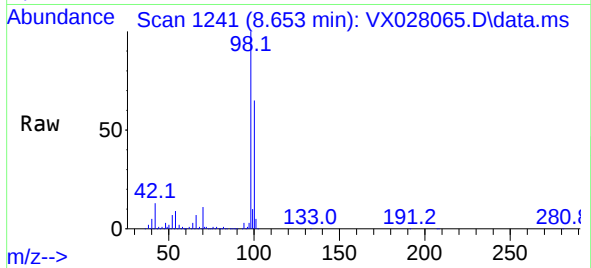

#62
4-Bromofluorobenzene
Concen: 44.070 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX028065.D
Acq: 12 Apr 2022 18:43

Tgt Ion: 95 Resp: 147409
Ion Ratio Lower Upper
95 100
174 87.2 0.0 163.0
176 83.4 0.0 155.0


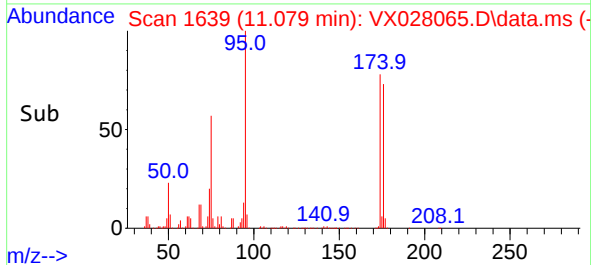
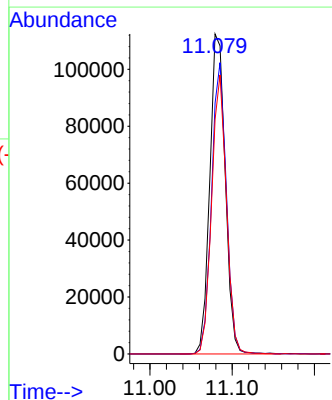
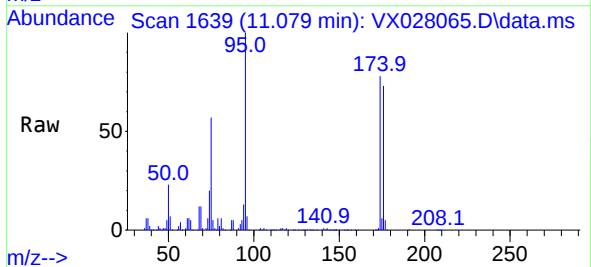


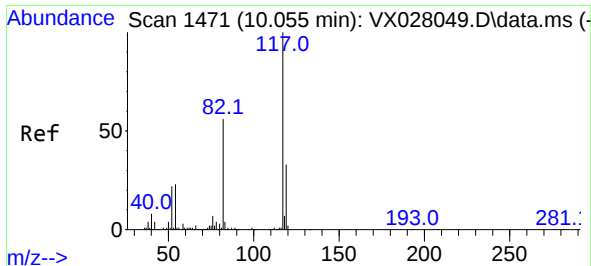

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX028065.D
Acq: 12 Apr 2022 18:43

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Tgt Ion:117	Resp:	343961
Ion	Ratio	Lower Upper
117	100	
82	54.7	41.8 62.8
119	32.6	24.8 37.2

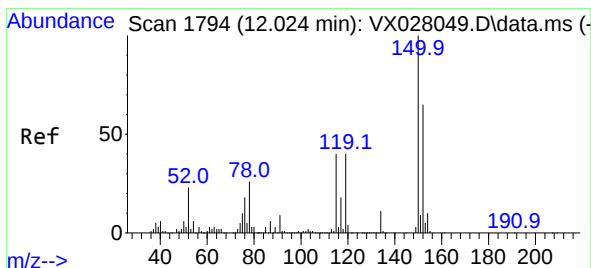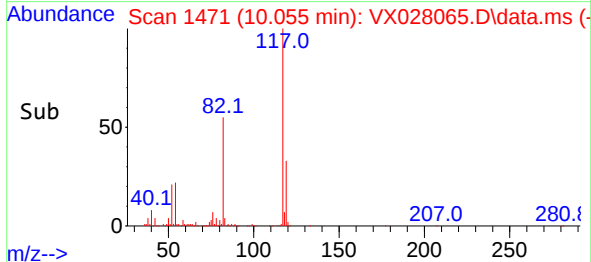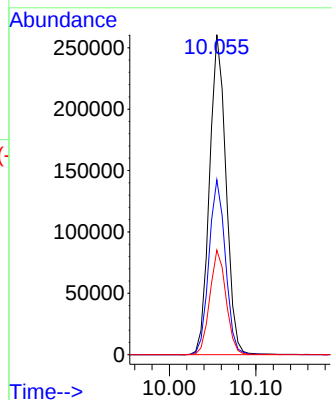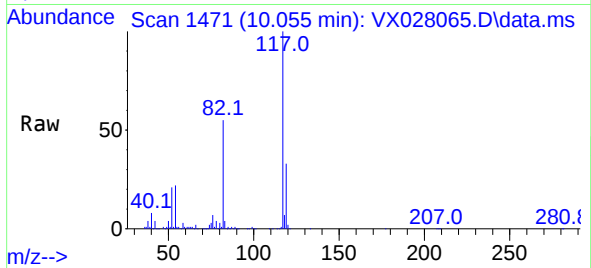

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX028065.D
Acq: 12 Apr 2022 18:43

Tgt Ion:152	Resp:	156066
Ion	Ratio	Lower Upper
152	100	
115	58.0	37.5 112.7
150	158.2	0.0 338.2

