

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041222\
 Data File : VX028062.D
 Acq On : 12 Apr 2022 17:33
 Operator : JC/MD
 Sample : N2334-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FB040522

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M

Title : SW846 8260

Signal : TIC: VX028062.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.581	72	81	93	rBV6	26612	75071	6.07%	1.128%
2	2.544	230	239	250	rBV2	9959	23492	1.90%	0.353%
3	2.947	298	305	312	rBV2	6639	15796	1.28%	0.237%
4	5.391	694	706	721	rBV	145287	427423	34.57%	6.420%
5	5.556	721	733	750	rVB	226087	635135	51.37%	9.540%
6	5.958	788	799	813	rBV	155378	415146	33.58%	6.236%
7	6.763	921	931	947	rBV	371765	878323	71.04%	13.193%
8	8.653	1233	1241	1257	rBV	791294	1236369	100.00%	18.571%
9	10.055	1465	1471	1480	rBV	814070	1102031	89.13%	16.553%
10	11.085	1634	1640	1648	rBV	629204	821795	66.47%	12.344%
11	12.024	1788	1794	1805	rBV	839686	1027037	83.07%	15.426%




Sum of corrected areas: 6657618

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041222\
Data File : VX028062.D
Acq On : 12 Apr 2022 17:33
Operator : JC/MD
Sample : N2334-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB040522

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

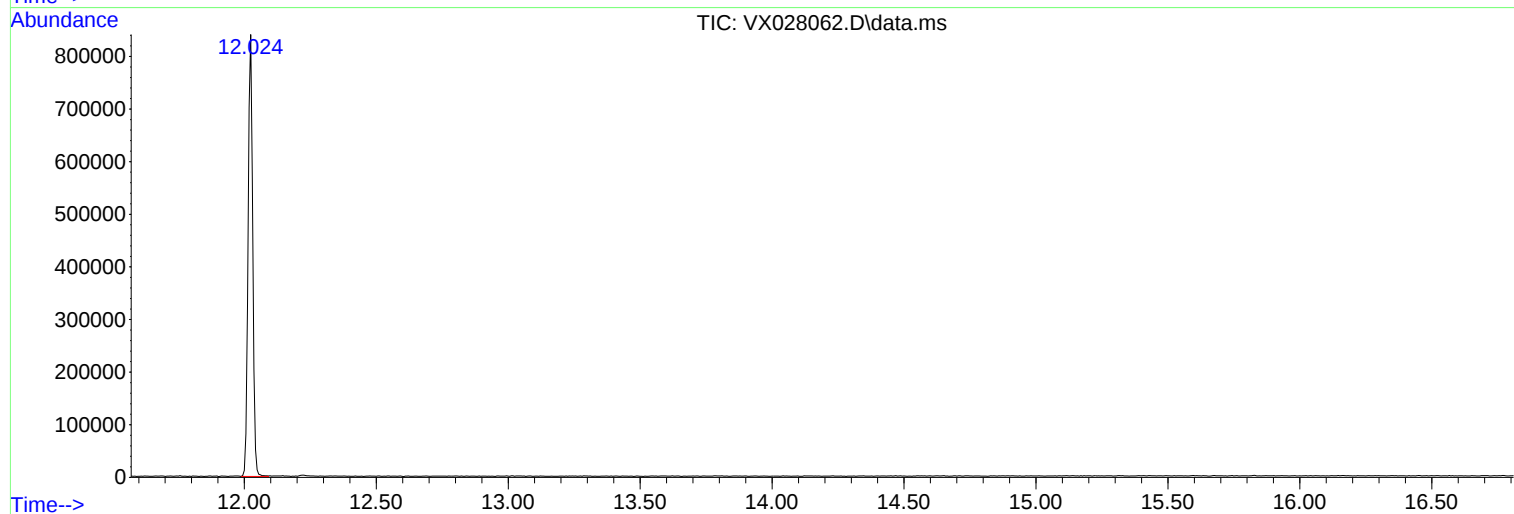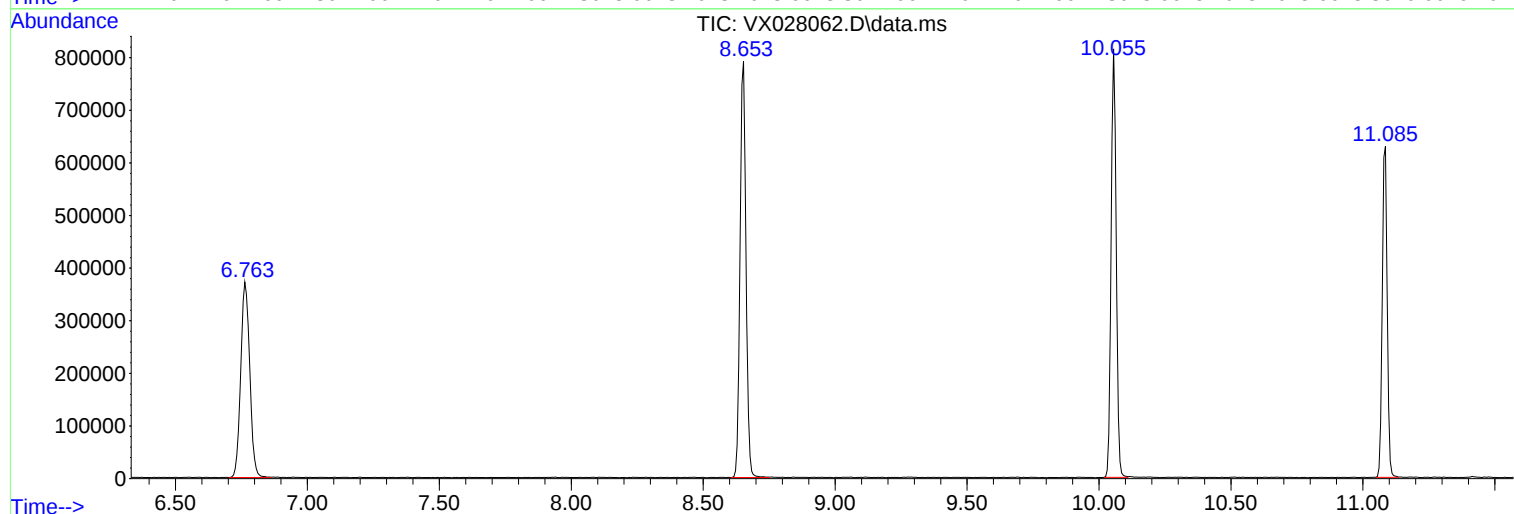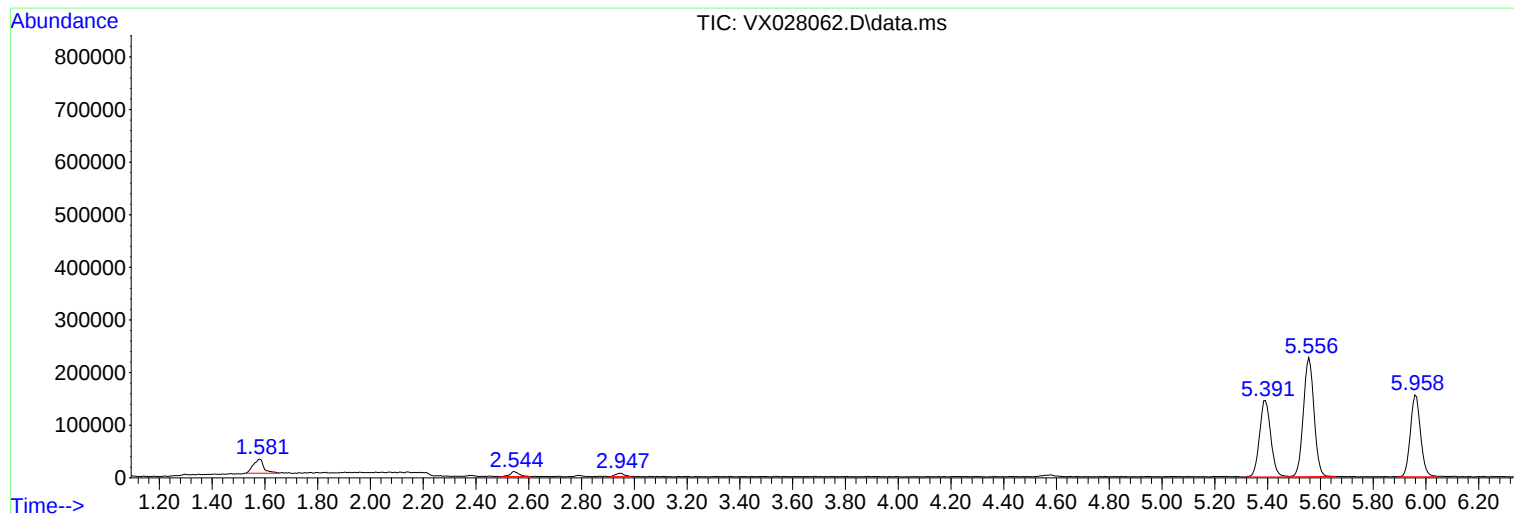

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041222\
Data File : VX028062.D
Acq On : 12 Apr 2022 17:33
Operator : JC/MD
Sample : N2334-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB040522










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown1.581 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.581	5.91 ug/l	75071	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzaldehyde, 2-nitro-, diaminom...	207	C8H9N5O2	102632-31-5	38
2			2-Iodothiostidine	281	C6H8IN3O2	006996-15-2	38
3			Cyclotrisiloxane, hexamethyl-	222	C6H18O3Si3	000541-05-9	27
4			3,3-Dimethyl-4-methylamino-butan...	129	C7H15NO	123528-99-4	18
5			4-APDB	177	C11H15NO	1203342-42-0	18

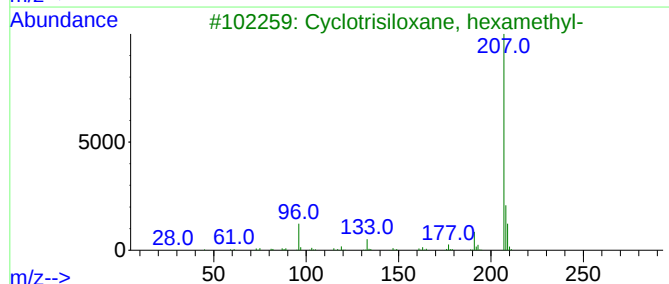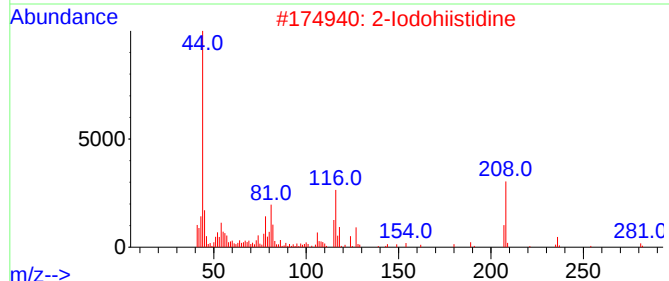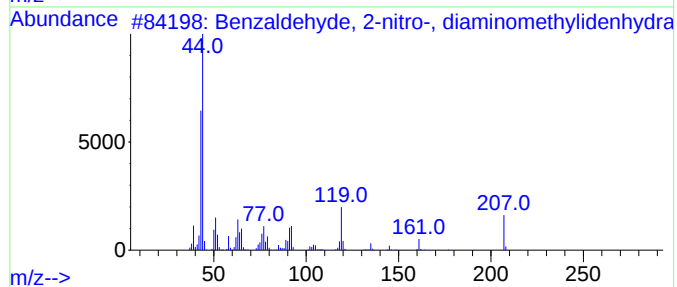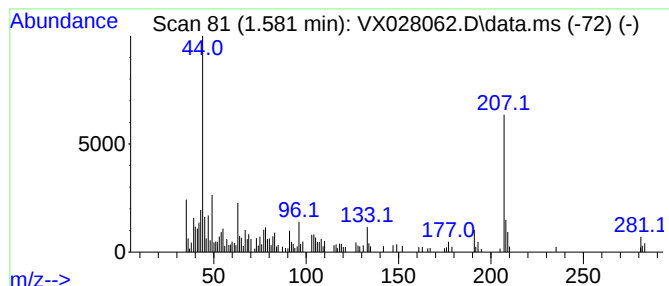

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041222\
Data File : VX028062.D
Acq On : 12 Apr 2022 17:33
Operator : JC/MD
Sample : N2334-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB040522

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown1.581	1.581	5.9	ug/l	75071	1	5.556	635135	50.0