


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041222\
 Data File : VX028054.D
 Acq On : 12 Apr 2022 14:01
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
 Title : SW846 8260
 Last Update : Tue Apr 12 22:07:23 2022

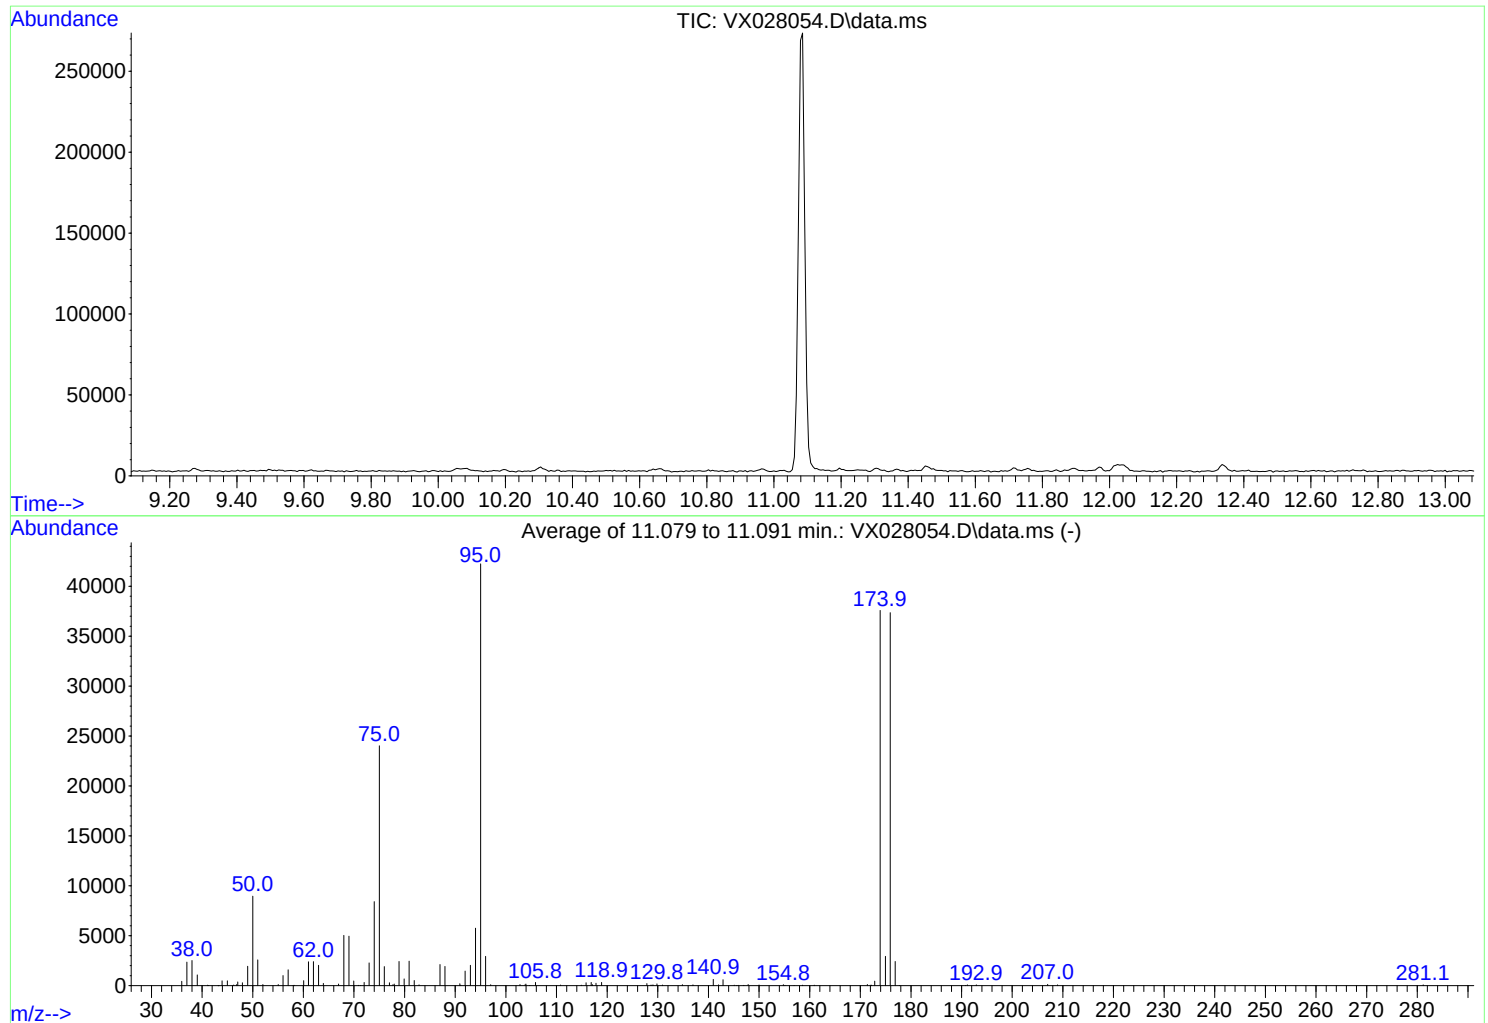

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	8965	PASS
75	95	30	60	56.8	24017	PASS
95	95	100	100	100.0	42248	PASS
96	95	5	9	6.9	2935	PASS
173	174	0.00	2	1.2	444	PASS
174	95	50	100	89.0	37581	PASS
175	174	5	9	7.8	2929	PASS
176	174	95	101	99.4	37363	PASS
177	176	5	9	6.5	2429	PASS