

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041223\
 Data File : VX035021.D
 Acq On : 11 Apr 2023 19:49
 Operator : JC/MD
 Sample : 02272-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-3-040623

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M

Title : SW846 8260

Signal : TIC: VX035021.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	693	705	721	rBV	165584	480370	31.95%	6.111%
2	5.549	721	732	749	rVB	294030	838494	55.77%	10.667%
3	5.958	788	799	818	rBV	195865	526667	35.03%	6.700%
4	6.763	921	931	954	rBV	463757	1117212	74.31%	14.213%
5	8.646	1233	1240	1261	rBV	962407	1503526	100.00%	19.127%
6	10.055	1465	1471	1489	rBV	932815	1276523	84.90%	16.239%
7	11.079	1634	1639	1653	rBV	733258	954209	63.46%	12.139%
8	12.024	1788	1794	1803	rBV	866870	1096128	72.90%	13.945%
9	13.158	1967	1980	1981	rBV9	10934	32901	2.19%	0.419%
10	14.084	2125	2132	2142	rVB9	5383	18685	1.24%	0.238%
11	15.395	2339	2347	2354	rBV9	4990	15924	1.06%	0.203%




Sum of corrected areas: 7860639

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041223\
Data File : VX035021.D
Acq On : 11 Apr 2023 19:49
Operator : JC/MD
Sample : 02272-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3-040623

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

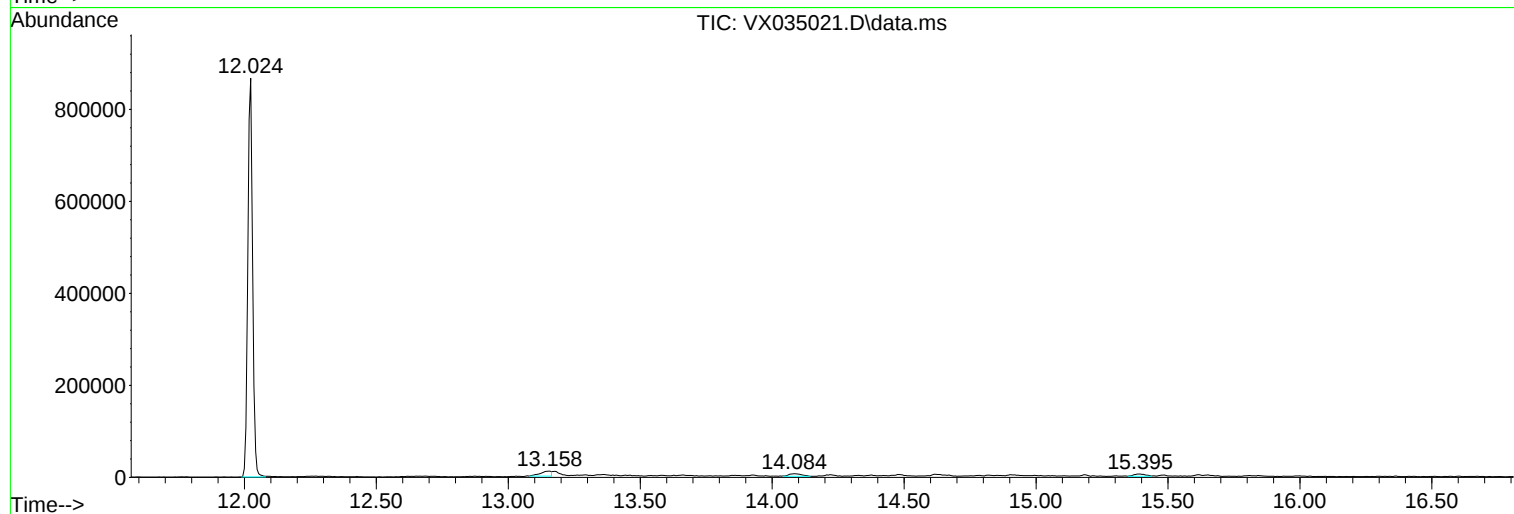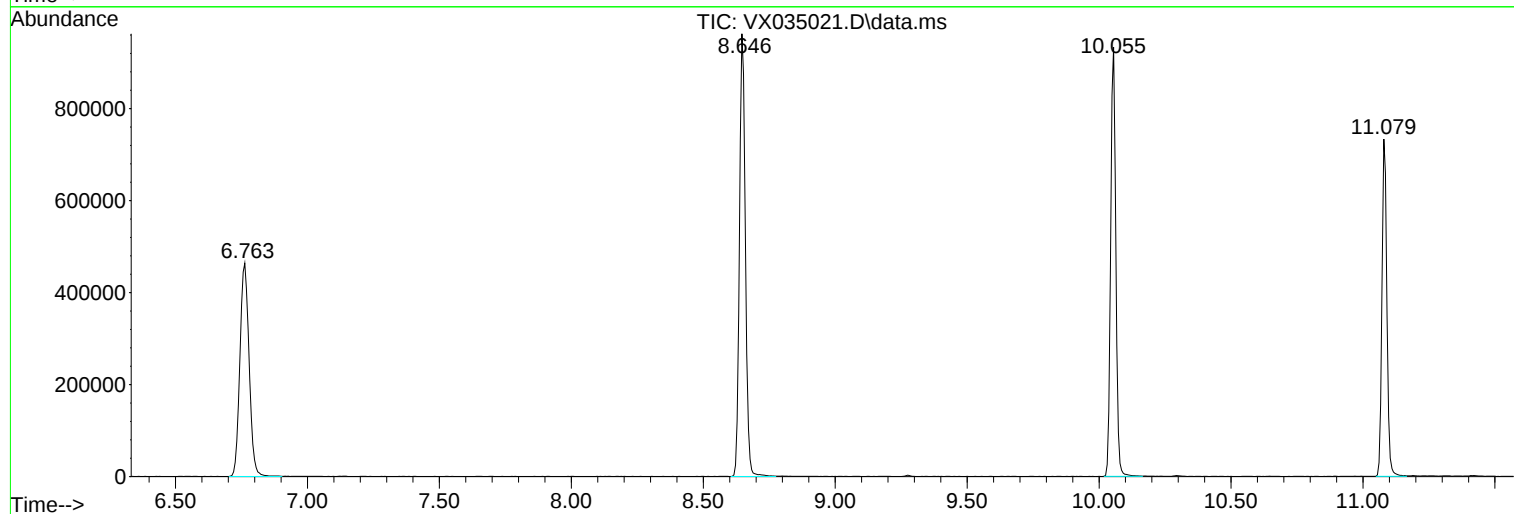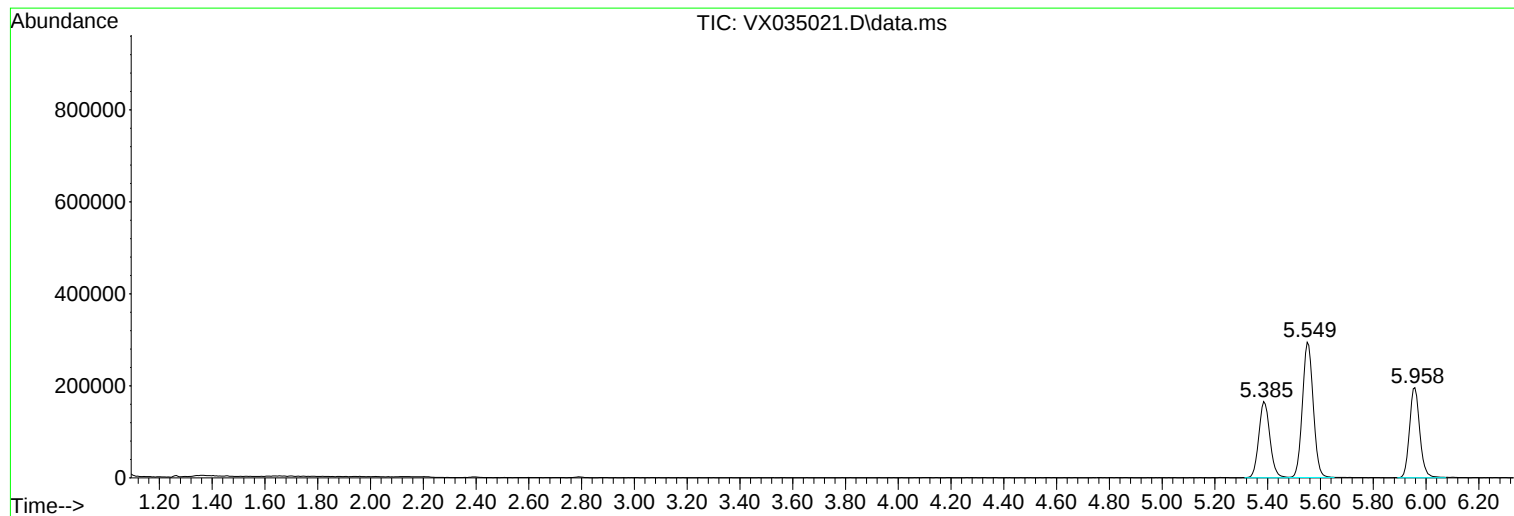

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041223\
Data File : VX035021.D
Acq On : 11 Apr 2023 19:49
Operator : JC/MD
Sample : 02272-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3-040623

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041223\
Data File : VX035021.D
Acq On : 11 Apr 2023 19:49
Operator : JC/MD
Sample : 02272-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3-040623

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------