

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041015.D
 Acq On : 12 Apr 2024 09:23
 Operator : JC/MD
 Sample : VX0412WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Apr 13 01:37:05 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 13 01:36:25 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	295670	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.049	117	277702	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	144228	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	117263	55.760	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	= 111.520%		
7) Chloroethane-d5	1.666	69	93497	54.513	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	= 109.020%		
11) 1,1-Dichloroethene-d2	2.307	65	48524	54.044	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 108.080%		
21) 2-Butanone-d5	4.446	46	140454	122.608	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	= 122.610%		
24) Chloroform-d	5.056	84	196674	50.122	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 100.240%		
26) 1,2-Dichloroethane-d4	5.952	65	129201	50.619	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 101.240%		
32) Benzene-d6	5.971	84	402536	53.393	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 106.780%		
36) 1,2-Dichloropropane-d6	7.306	67	117889	53.615	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	= 107.240%		
41) Toluene-d8	8.647	98	382637	51.951	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 103.900%		
43) trans-1,3-Dichloroprop...	8.946	79	55304	49.981	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 99.960%		
47) 2-Hexanone-d5	9.378	63	98057	105.774	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	= 105.770%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	166471	51.110	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	= 102.220%		
66) 1,2-Dichlorobenzene-d4	12.317	152	158106	54.647	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 109.300%		
Target Compounds						
39) cis-1,3-Dichloropropene	8.324	75	3771	1.238	ug/L	Qvalue 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041015.D
Acq On : 12 Apr 2024 09:23
Operator : JC/MD
Sample : VX0412WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Apr 13 01:37:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 13 01:36:25 2024
Response via : Initial Calibration

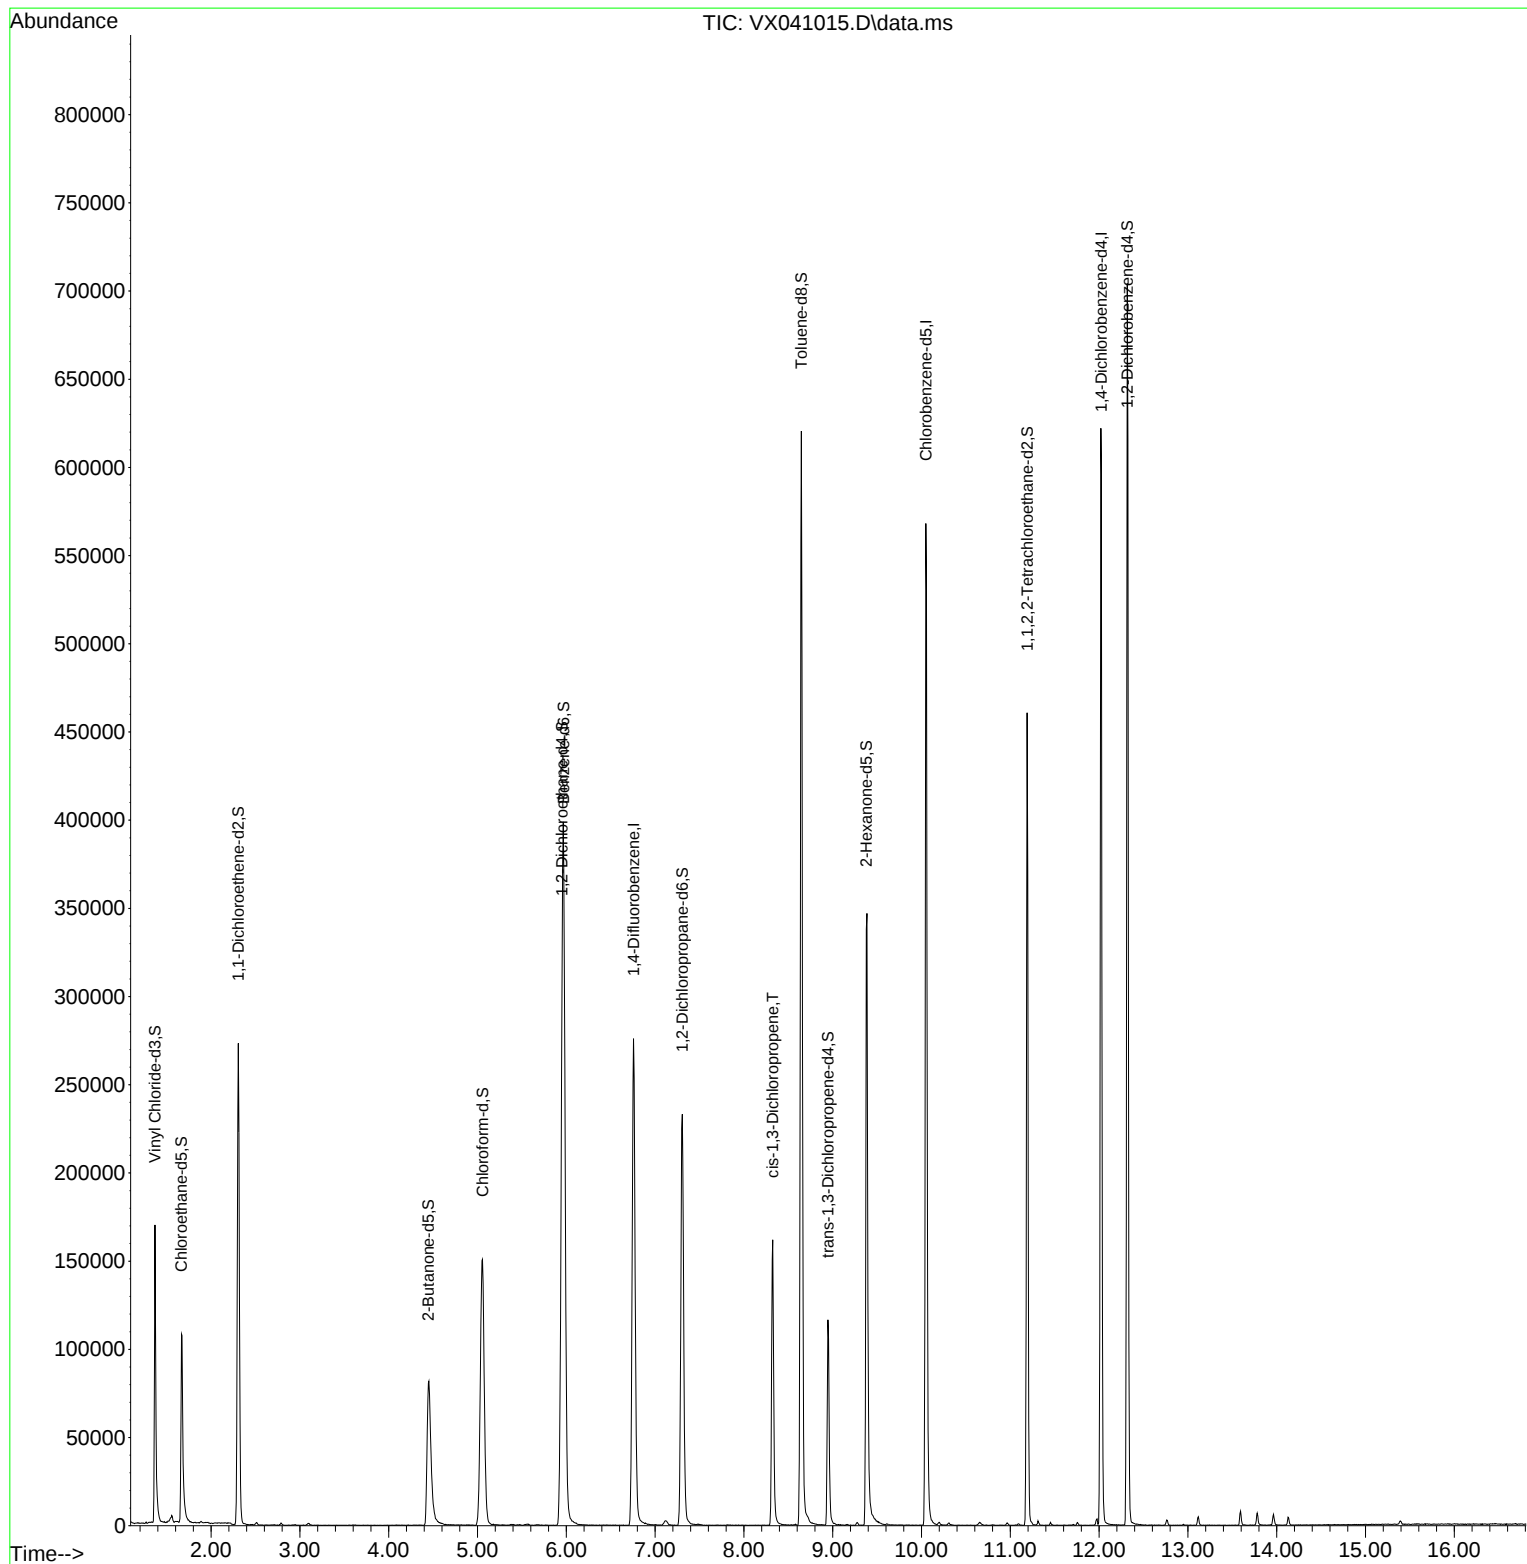

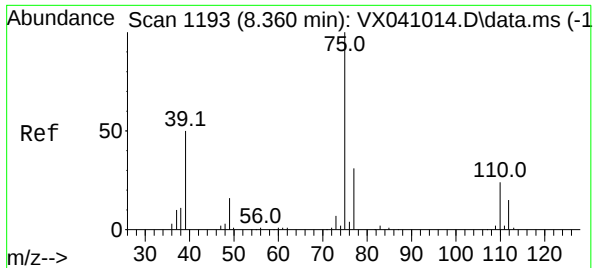

#39
 cis-1,3-Dichloropropene
 Concen: 1.238 ug/L
 RT: 8.324 min Scan# 11
 Delta R.T. -0.036 min
 Lab File: VX041015.D
 Acq: 12 Apr 2024 09:23

Instrument :
 MSVOA_X
 ClientSampleId :

Tgt Ion: 75 Resp: 3771
 Ion Ratio Lower Upper
 75 100
 77 41.9 22.7 42.1

