

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041016.D
 Acq On : 12 Apr 2024 09:51
 Operator : JC/MD
 Sample : P2048-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Apr 13 01:37:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 13 01:36:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	264367	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	251536	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	131526	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	90493	48.125	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 96.260%			
7) Chloroethane-d5	1.672	69	78259	51.031	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 102.060%			
11) 1,1-Dichloroethene-d2	2.306	65	39928	49.736	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 99.480%			
21) 2-Butanone-d5	4.452	46	121184	118.312	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 118.310%			
24) Chloroform-d	5.056	84	173322	49.401	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 98.800%			
26) 1,2-Dichloroethane-d4	5.952	65	115191	50.474	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 100.940%			
32) Benzene-d6	5.970	84	354887	51.969	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 103.940%			
36) 1,2-Dichloropropane-d6	7.306	67	102821	51.627	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 103.260%			
41) Toluene-d8	8.647	98	333792	50.033	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 100.060%			
43) trans-1,3-Dichloroprop...	8.945	79	46648	46.543	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 93.080%			
47) 2-Hexanone-d5	9.384	63	82892	98.717	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 98.720%			
56) 1,1,2,2-Tetrachloroeth...	11.189	84	149167	50.562	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 101.120%			
66) 1,2-Dichlorobenzene-d4	12.317	152	143564	54.413	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 108.820%			
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	8.324	75	3237	1.173	ug/L	# 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041016.D
Acq On : 12 Apr 2024 09:51
Operator : JC/MD
Sample : P2048-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Apr 13 01:37:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 13 01:36:25 2024
Response via : Initial Calibration

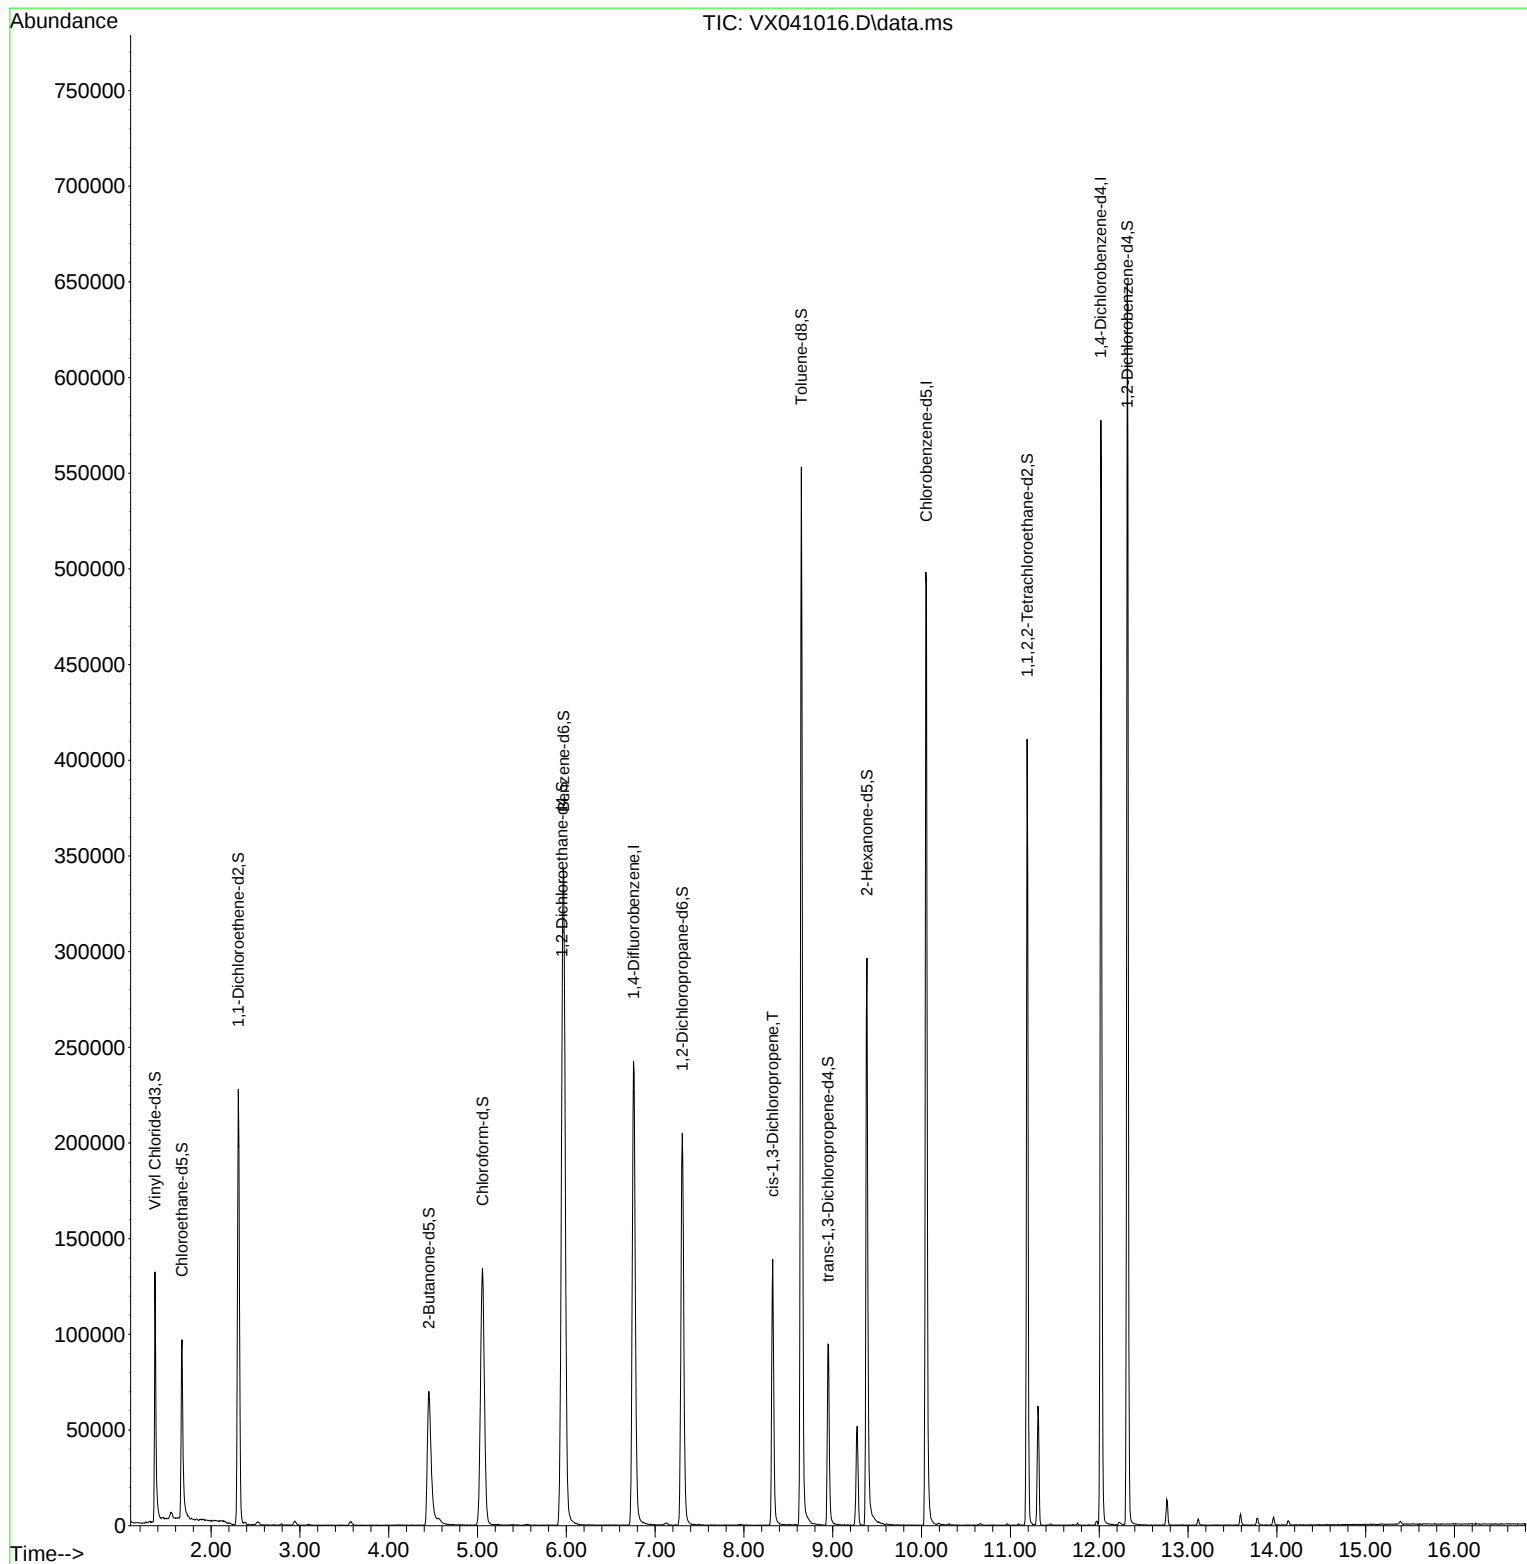

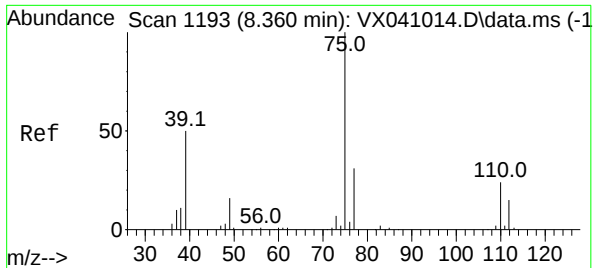

#39
 cis-1,3-Dichloropropene
 Concen: 1.173 ug/L
 RT: 8.324 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VX041016.D
 Acq: 12 Apr 2024 09:51

Instrument :
 MSVOA_X
 ClientSampleId :

Tgt Ion: 75 Resp: 3237
 Ion Ratio Lower Upper
 75 100
 77 50.6 22.7 42.1#

