

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041047.D
 Acq On : 12 Apr 2024 21:42
 Operator : JC/MD
 Sample : P2060-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Apr 13 04:23:21 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 13 04:06:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	245797	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	233317	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	127098	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	90342	51.675	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 103.340%			
7) Chloroethane-d5	1.672	69	74941	52.559	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 105.120%			
11) 1,1-Dichloroethene-d2	2.307	65	36391	48.755	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 97.500%			
21) 2-Butanone-d5	4.459	46	119778	125.774	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 125.770%			
24) Chloroform-d	5.056	84	164138	50.317	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 100.640%			
26) 1,2-Dichloroethane-d4	5.958	65	109353	51.536	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 103.080%			
32) Benzene-d6	5.977	84	328458	51.855	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 103.700%			
36) 1,2-Dichloropropane-d6	7.306	67	97076	52.549	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 105.100%			
41) Toluene-d8	8.647	98	301314	48.692	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 97.380%			
43) trans-1,3-Dichloroprop...	8.952	79	43427	46.713	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 93.420%			
47) 2-Hexanone-d5	9.385	63	83658	107.409	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 107.410%			
56) 1,1,2,2-Tetrachloroeth...	11.189	84	144689	52.873	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 105.740%			
66) 1,2-Dichlorobenzene-d4	12.317	152	137346	53.870	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 107.740%			
Target Compounds						Qvalue
13) Acetone	2.380	43	5585	5.411	ug/L	99
37) 1,2-Dichloropropane	7.306	63	11296	7.209	ug/L #	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041047.D
Acq On : 12 Apr 2024 21:42
Operator : JC/MD
Sample : P2060-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Apr 13 04:23:21 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 13 04:06:48 2024
Response via : Initial Calibration

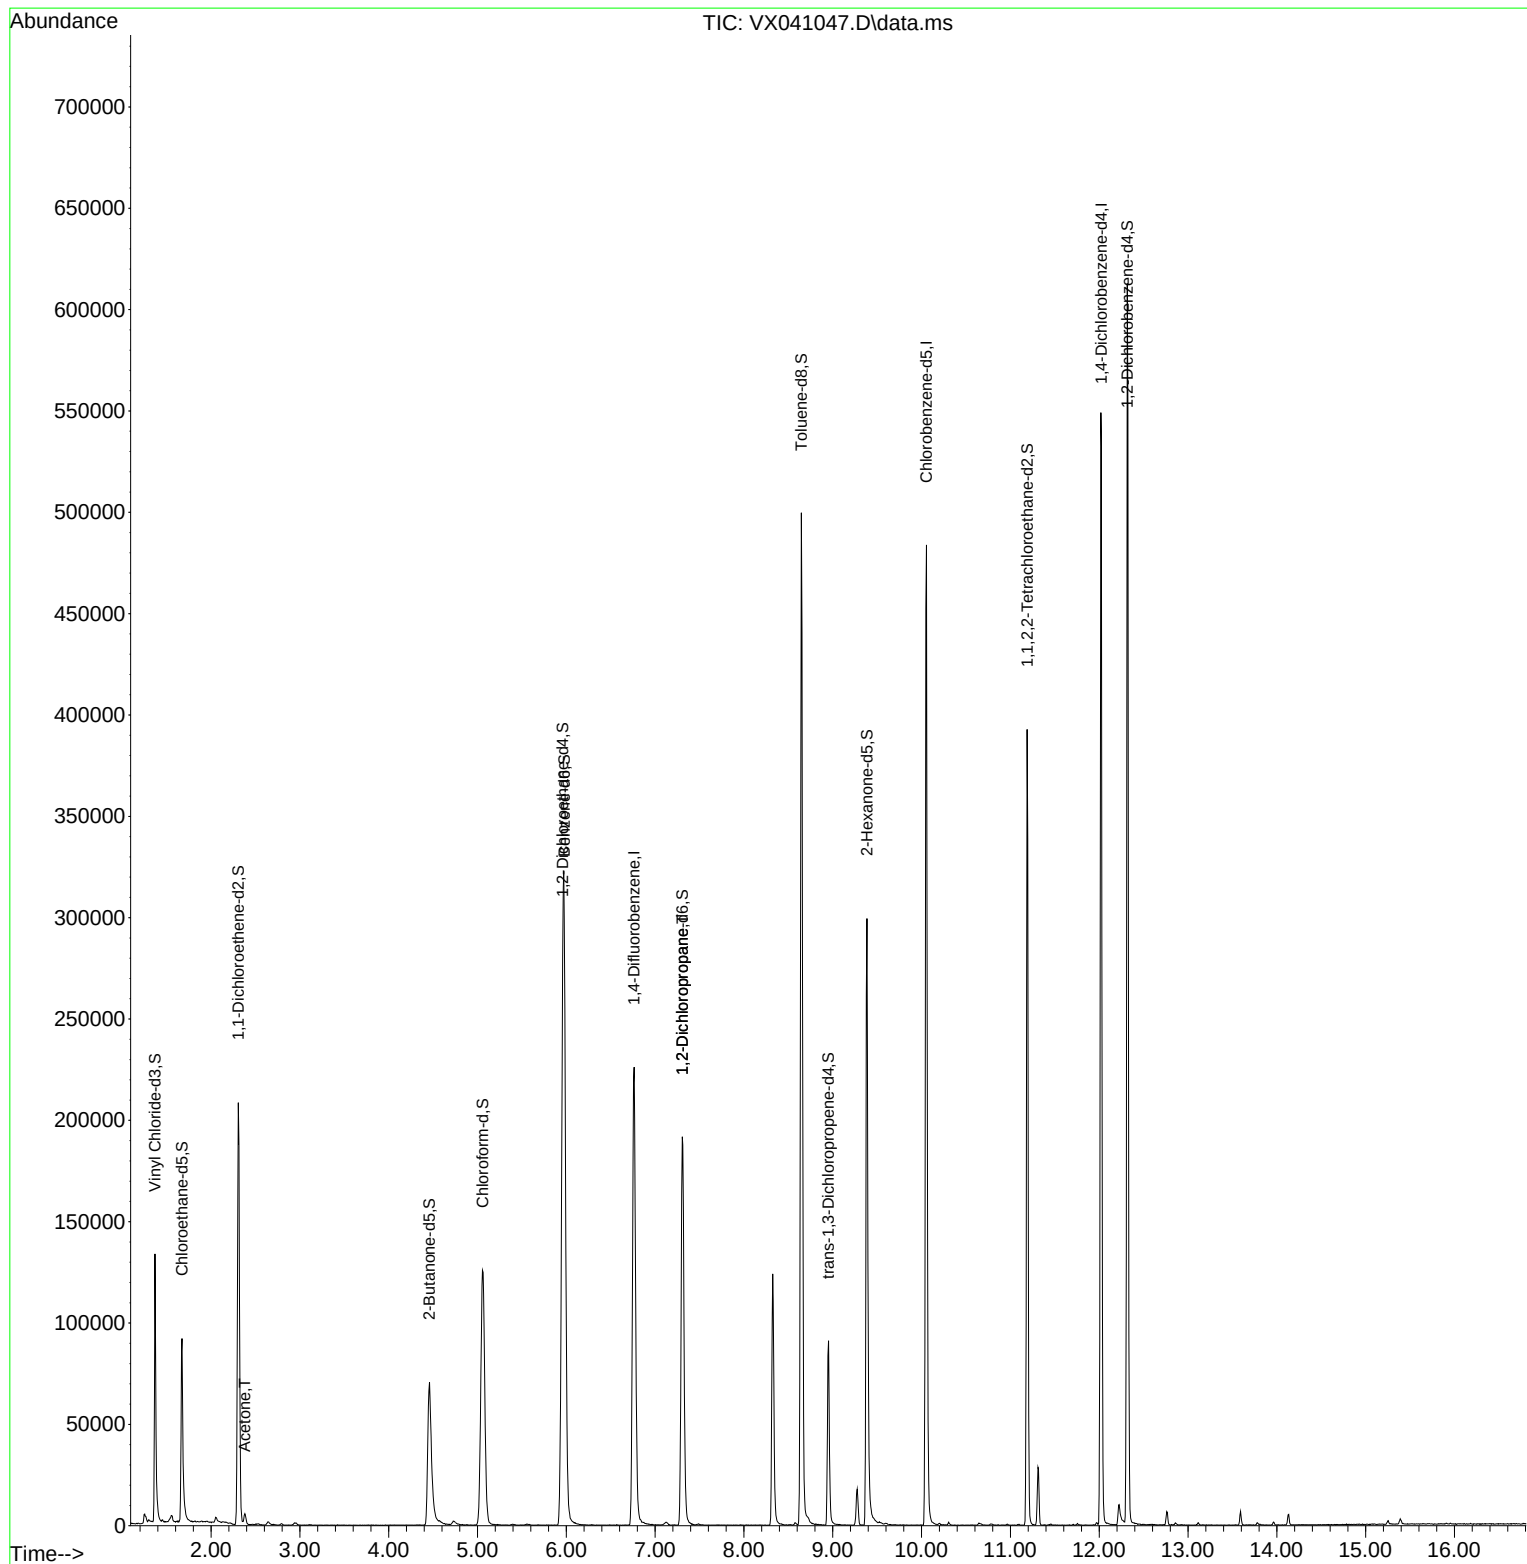

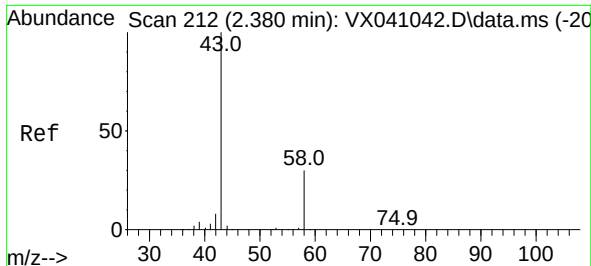

#13

Acetone

Concen: 5.411 ug/L

RT: 2.380 min Scan# 21

Delta R.T. 0.000 min

Lab File: VX041047.D

Acq: 12 Apr 2024 21:42

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 5585

Ion Ratio Lower Upper

43 100

58 30.4 0.0 59.4

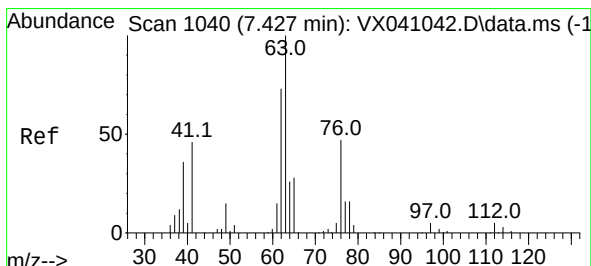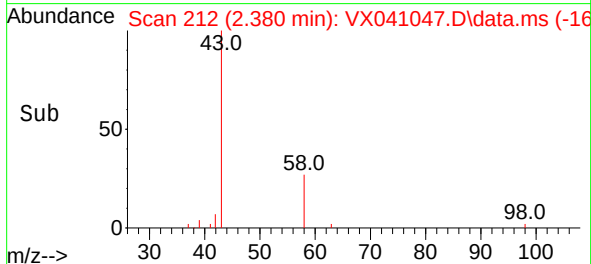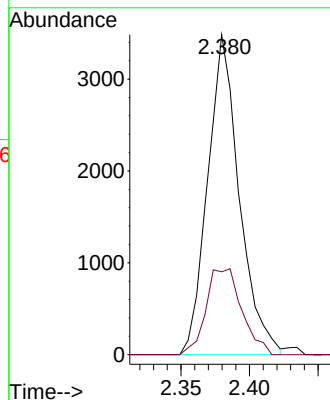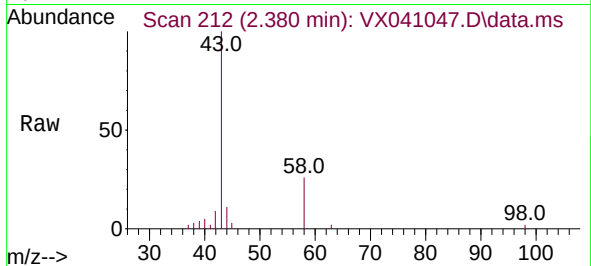

#37

1,2-Dichloropropane

Concen: 7.209 ug/L

RT: 7.306 min Scan# 1020

Delta R.T. -0.122 min

Lab File: VX041047.D

Acq: 12 Apr 2024 21:42

Tgt Ion: 63 Resp: 11296

Ion Ratio Lower Upper

63 100

112 0.0 4.2 6.2#

