

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041052.D
 Acq On : 12 Apr 2024 23:37
 Operator : JC/MD
 Sample : P2098-02 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Apr 13 04:24:28 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 13 04:06:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	265414	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	251086	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	130071	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	93016	49.272	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 98.540%			
7) Chloroethane-d5	1.666	69	77860	50.570	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 101.140%			
11) 1,1-Dichloroethene-d2	2.306	65	39394	48.877	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 97.760%			
21) 2-Butanone-d5	4.452	46	130950	127.343	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 127.340%			
24) Chloroform-d	5.056	84	176751	50.179	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 100.360%			
26) 1,2-Dichloroethane-d4	5.952	65	116408	50.806	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 101.620%			
32) Benzene-d6	5.970	84	351325	51.540	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 103.080%			
36) 1,2-Dichloropropane-d6	7.306	67	104405	52.516	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 105.040%			
41) Toluene-d8	8.647	98	321220	48.235	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 96.480%			
43) trans-1,3-Dichloroprop...	8.952	79	45790	45.769	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 91.540%			
47) 2-Hexanone-d5	9.384	63	91125	108.716	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 108.720%			
56) 1,1,2,2-Tetrachloroeth...	11.189	84	149970	50.925	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 101.840%			
66) 1,2-Dichlorobenzene-d4	12.317	152	138881	53.227	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 106.460%			
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	8.324	75	3257	1.182	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041052.D
Acq On : 12 Apr 2024 23:37
Operator : JC/MD
Sample : P2098-02 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Apr 13 04:24:28 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 13 04:06:48 2024
Response via : Initial Calibration

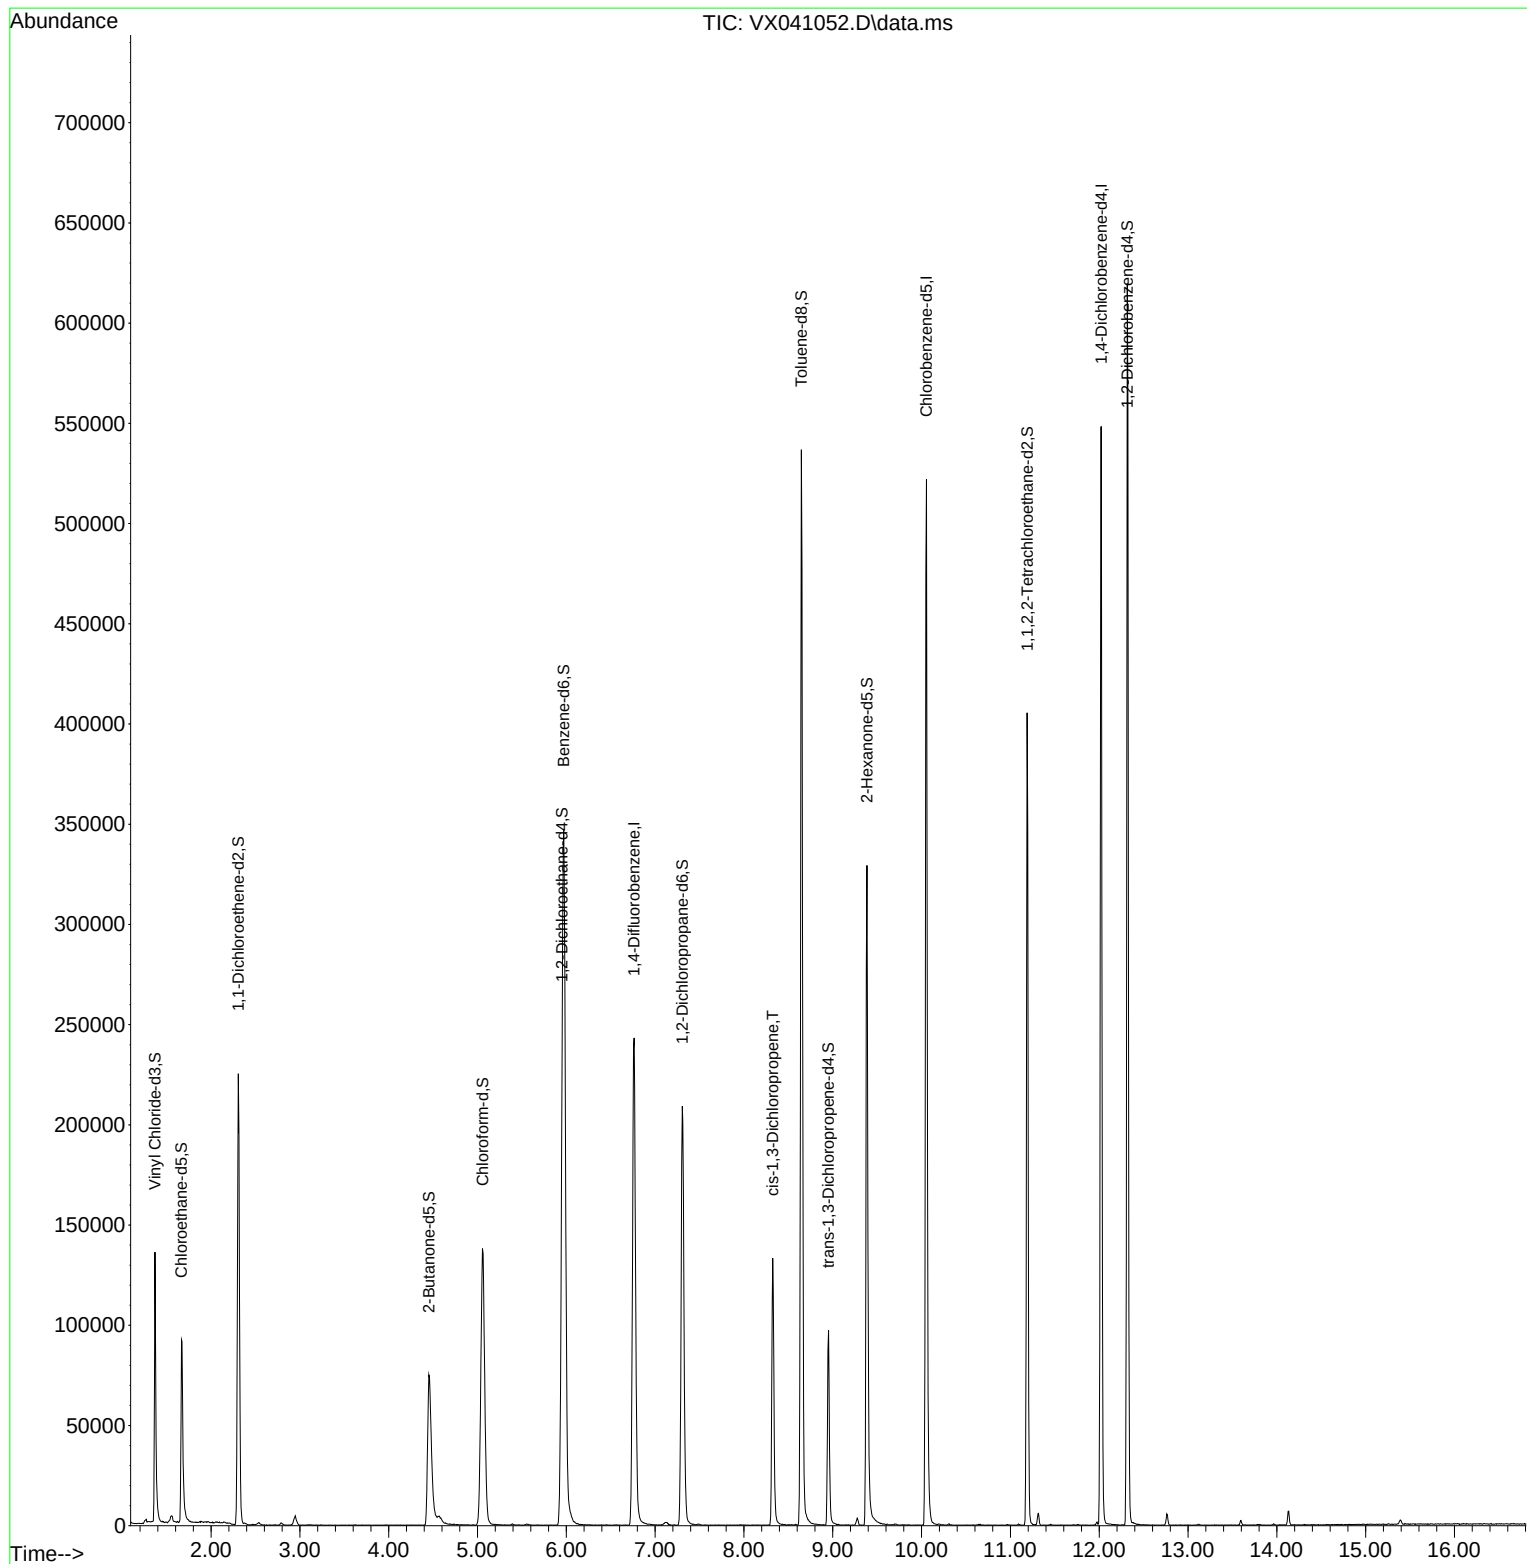

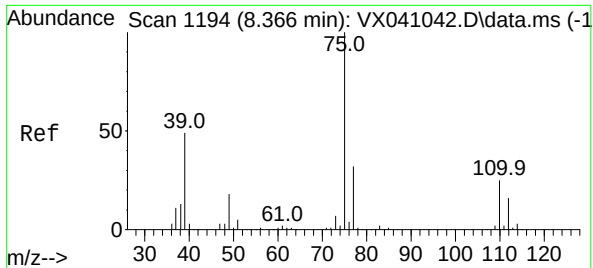

#39
 cis-1,3-Dichloropropene
 Concen: 1.182 ug/L
 RT: 8.324 min Scan# 11
 Delta R.T. -0.043 min
 Lab File: VX041052.D
 Acq: 12 Apr 2024 23:37

Instrument :
 MSVOA_X
 ClientSampleId :

Tgt Ion: 75 Resp: 3257
 Ion Ratio Lower Upper
 75 100
 77 41.4 22.7 42.1

