

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041057.D
 Acq On : 13 Apr 2024 01:32
 Operator : JC/MD
 Sample : P2098-09 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Apr 13 04:25:35 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 13 04:06:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	225012	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	215957	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	112128	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	82250	51.392	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 102.780%			
7) Chloroethane-d5	1.673	69	70595	54.085	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 108.160%			
11) 1,1-Dichloroethene-d2	2.307	65	33326	48.773	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 97.540%			
21) 2-Butanone-d5	4.453	46	124007	142.243	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 142.240%#			
24) Chloroform-d	5.056	84	157813	52.847	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 105.700%			
26) 1,2-Dichloroethane-d4	5.952	65	105819	54.477	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 108.960%			
32) Benzene-d6	5.977	84	309662	52.817	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 105.640%			
36) 1,2-Dichloropropane-d6	7.306	67	93502	54.683	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 109.360%			
41) Toluene-d8	8.647	98	277521	48.452	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 96.900%			
43) trans-1,3-Dichloroprop...	8.952	79	40491	47.056	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 94.120%			
47) 2-Hexanone-d5	9.385	63	87192	120.945	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 120.950%			
56) 1,1,2,2-Tetrachloroeth...	11.189	84	142020	56.070	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 112.140%			
66) 1,2-Dichlorobenzene-d4	12.317	152	125462	55.779	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 111.560%			
Target Compounds			Qvalue			
37) 1,2-Dichloropropane	7.306	63	10866	7.492	ug/L #	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041057.D
Acq On : 13 Apr 2024 01:32
Operator : JC/MD
Sample : P2098-09 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Apr 13 04:25:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 13 04:06:48 2024
Response via : Initial Calibration

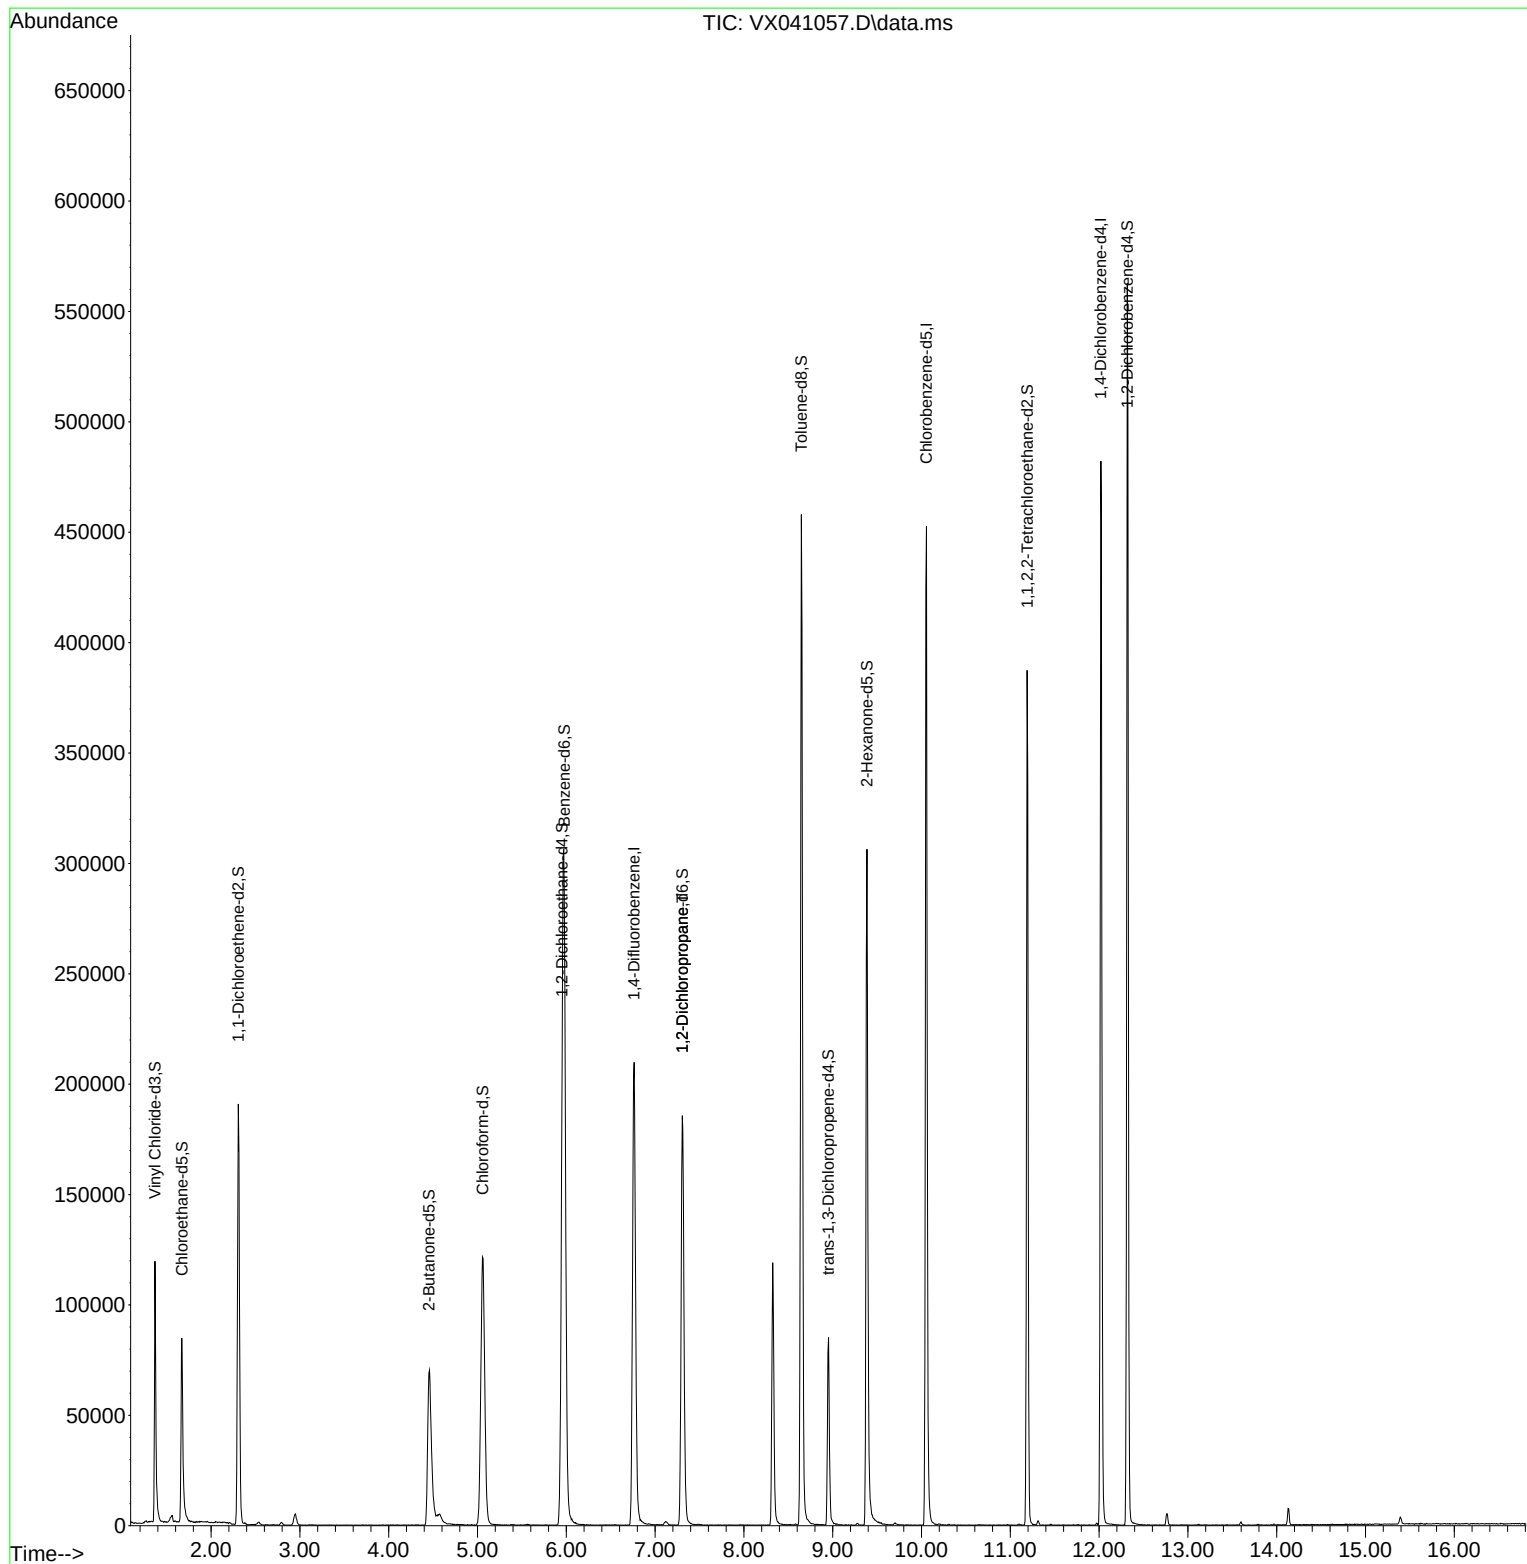

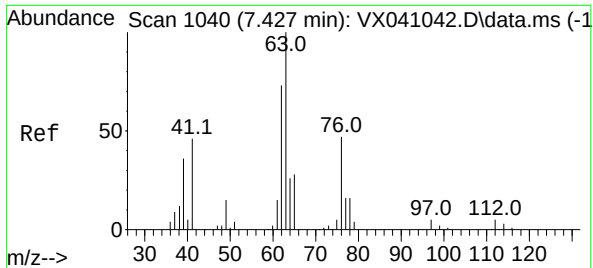

#37
 1,2-Dichloropropane
 Concen: 7.492 ug/L
 RT: 7.306 min Scan# 10
 Delta R.T. -0.122 min
 Lab File: VX041057.D
 Acq: 13 Apr 2024 01:32

Instrument :
 MSVOA_X
 ClientSampleId :

Tgt Ion: 63 Resp: 10866
 Ion Ratio Lower Upper
 63 100
 112 0.0 4.2 6.2#

