

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041020.D
 Acq On : 12 Apr 2024 11:22
 Operator : JC/MD
 Sample : P2048-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R95

Quant Time: Apr 13 01:38:10 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 13 01:36:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	277615	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	259446	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	133114	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	90558	45.862	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	91.720%		
7) Chloroethane-d5	1.672	69	77638	48.210	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	96.420%		
11) 1,1-Dichloroethene-d2	2.306	65	39943	47.380	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	94.760%		
21) 2-Butanone-d5	4.452	46	126070	117.209	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	117.210%		
24) Chloroform-d	5.056	84	175723	47.695	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.380%		
26) 1,2-Dichloroethane-d4	5.958	65	115944	48.379	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.760%		
32) Benzene-d6	5.976	84	352513	50.048	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.100%		
36) 1,2-Dichloropropane-d6	7.305	67	104288	50.767	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	101.540%		
41) Toluene-d8	8.647	98	328347	47.717	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.440%		
43) trans-1,3-Dichloroprop...	8.952	79	46447	44.930	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.860%		
47) 2-Hexanone-d5	9.384	63	84053	97.048	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	97.050%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	146908	48.278	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	96.560%		
66) 1,2-Dichlorobenzene-d4	12.317	152	138980	52.047	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	104.100%		
Target Compounds					Qvalue	
13) Acetone	2.380	43	4441	3.809	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041020.D
Acq On : 12 Apr 2024 11:22
Operator : JC/MD
Sample : P2048-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R95

Quant Time: Apr 13 01:38:10 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041024WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 13 01:36:25 2024
Response via : Initial Calibration

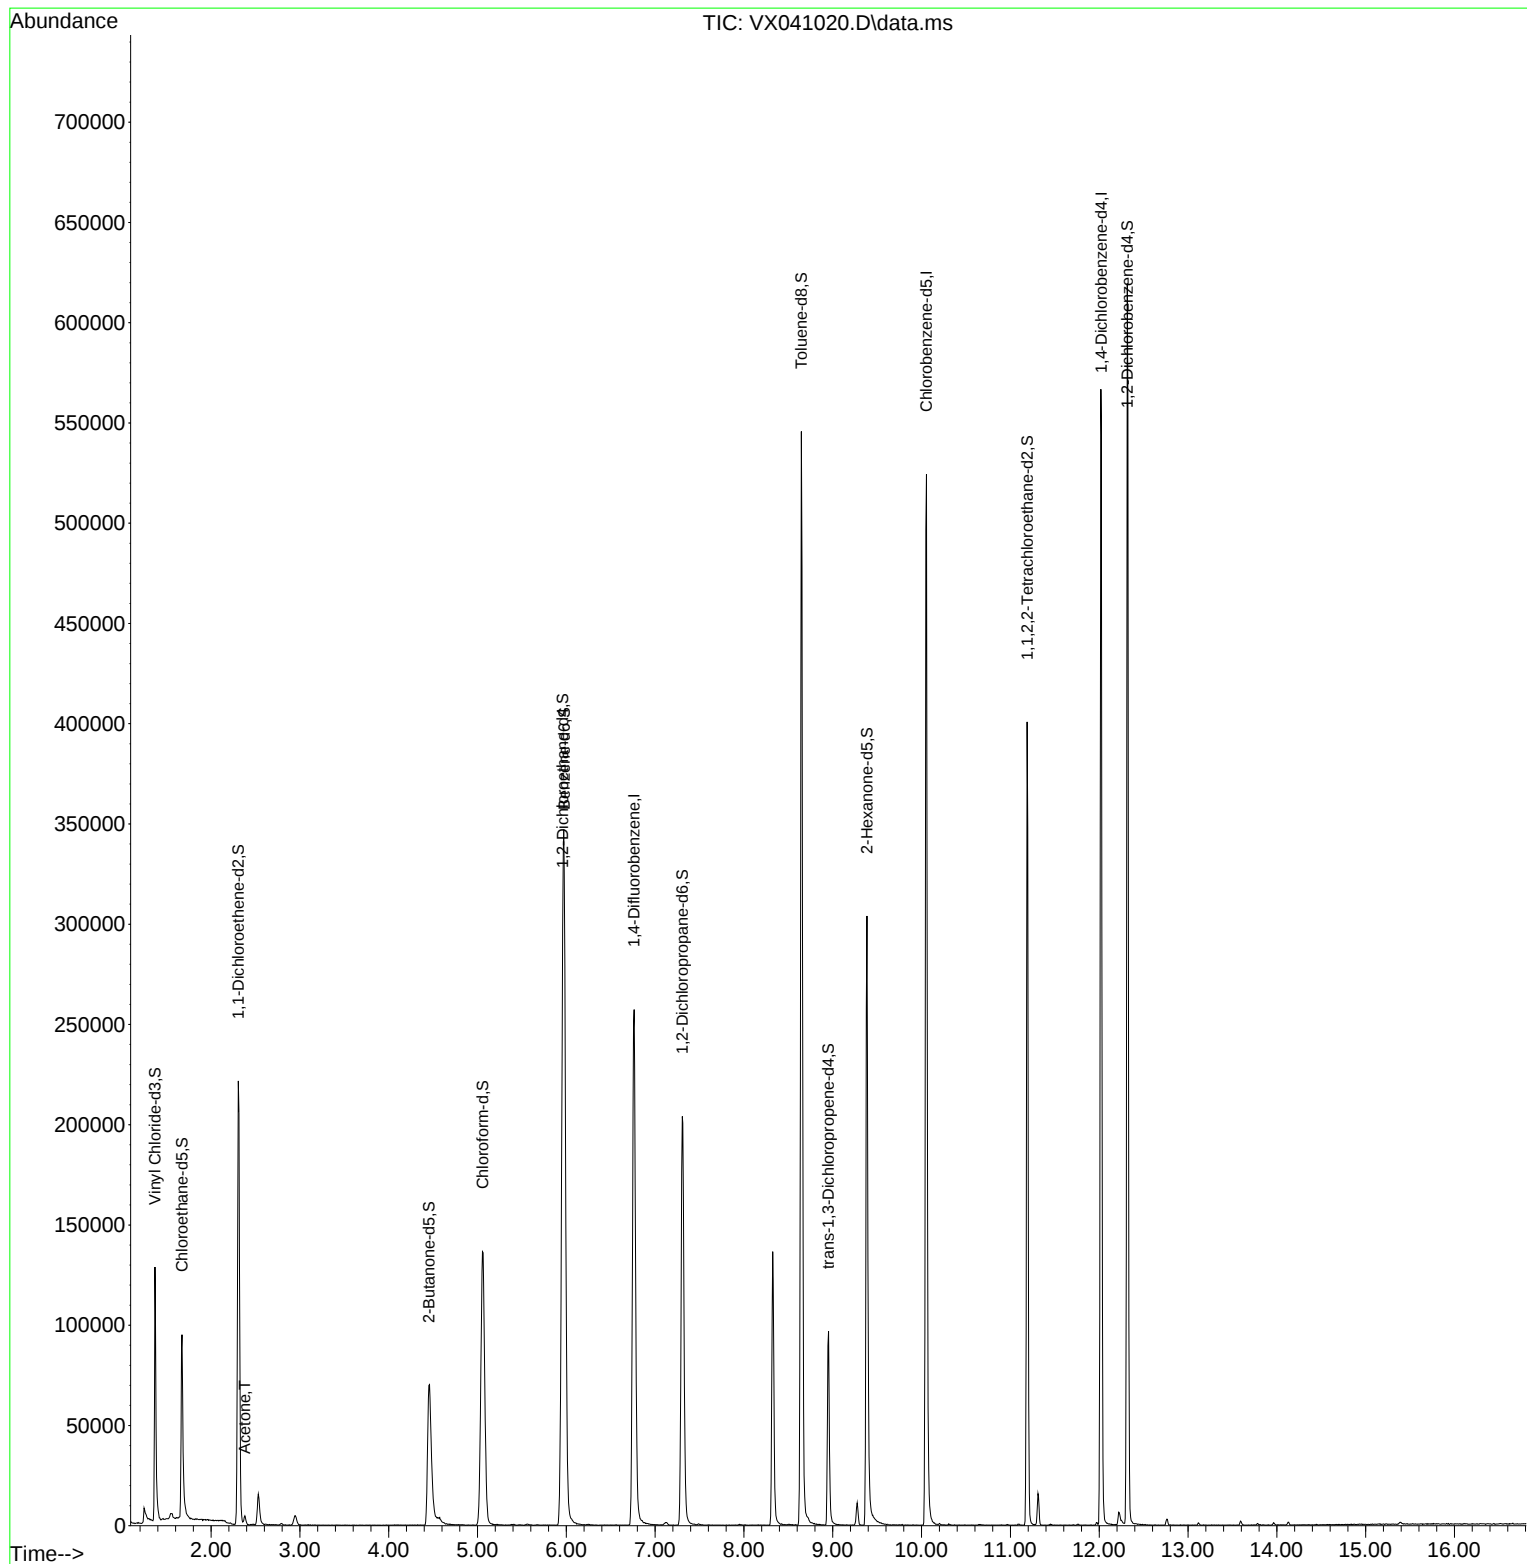

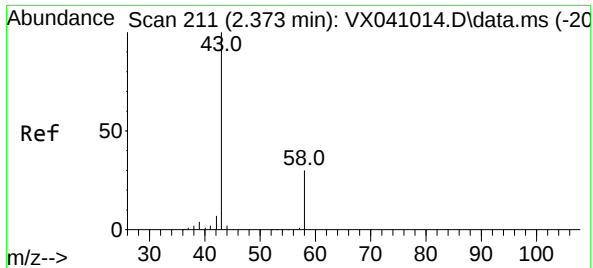

#13
 Acetone
 Concen: 3.809 ug/L
 RT: 2.380 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VX041020.D
 Acq: 12 Apr 2024 11:22

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R95

Tgt Ion: 43 Resp: 4441
 Ion Ratio Lower Upper
 43 100
 58 26.6 0.0 59.4

