

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041045.D
 Acq On : 12 Apr 2024 20:56
 Operator : JC/MD
 Sample : P2060-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1CY9

Quant Time: Apr 13 04:22:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 13 04:06:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	246970	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	235477	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	127717	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	91860	52.294	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	104.580%
7) Chloroethane-d5	1.673	69	75825	52.927	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	105.860%
11) 1,1-Dichloroethene-d2	2.307	65	37983	50.646	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	101.300%
21) 2-Butanone-d5	4.452	46	121465	126.940	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	126.940%
24) Chloroform-d	5.056	84	167362	51.062	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.120%
26) 1,2-Dichloroethane-d4	5.958	65	109858	51.528	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.060%
32) Benzene-d6	5.977	84	333320	52.140	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.280%
36) 1,2-Dichloropropane-d6	7.306	67	98405	52.779	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	105.560%
41) Toluene-d8	8.647	98	308368	49.375	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.740%
43) trans-1,3-Dichloroprop...	8.952	79	45287	48.267	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	96.540%
47) 2-Hexanone-d5	9.385	63	84062	106.938	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	106.940%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	148061	53.609	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	107.220%
66) 1,2-Dichlorobenzene-d4	12.317	152	139396	54.409	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	108.820%
Target Compounds					Qvalue	
13) Acetone	2.380	43	4789	4.618	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041045.D
Acq On : 12 Apr 2024 20:56
Operator : JC/MD
Sample : P2060-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1CY9

Quant Time: Apr 13 04:22:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 13 04:06:48 2024
Response via : Initial Calibration

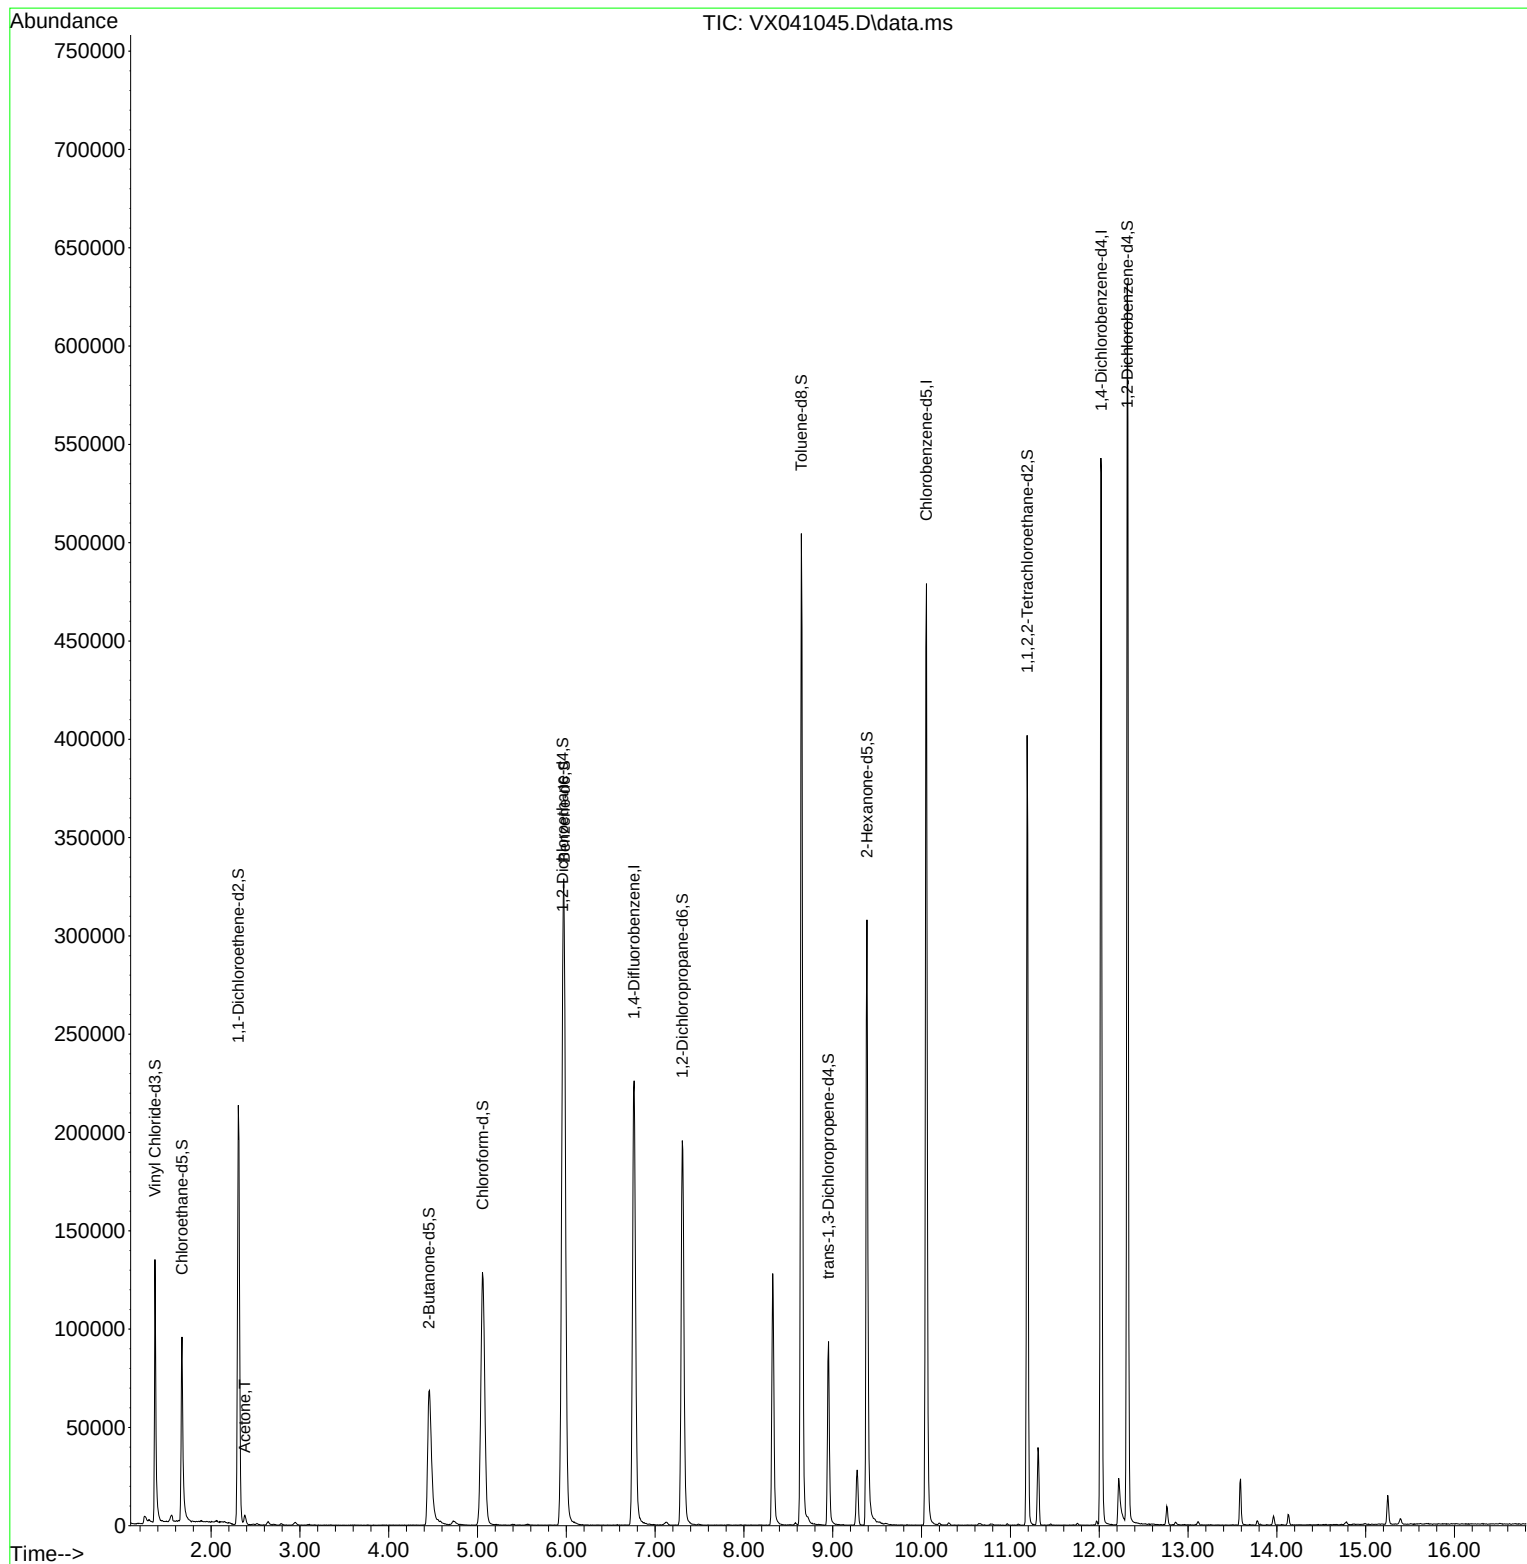

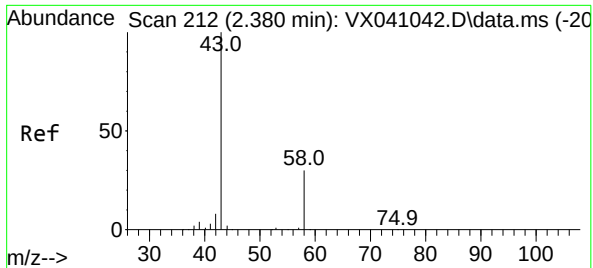

#13

Acetone

Concen: 4.618 ug/L

RT: 2.380 min Scan# 21

Delta R.T. 0.000 min

Lab File: VX041045.D

Acq: 12 Apr 2024 20:56

Instrument :

MSVOA_X

ClientSampleId :

E1CY9

Tgt Ion: 43 Resp: 4789

Ion Ratio Lower Upper

43 100

58 27.5 0.0 59.4

