

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041047.D
 Acq On : 12 Apr 2024 21:42
 Operator : JC/MD
 Sample : P2060-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1D01

Quant Time: Apr 13 04:23:21 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 13 04:06:48 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		6.763	114	245797	50.000	ug/L	0.00
28) Chlorobenzene-d5		10.055	117	233317	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		12.024	152	127098	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.368	65	90342	51.675	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	103.340%	
7) Chloroethane-d5		1.672	69	74941	52.559	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	105.120%	
11) 1,1-Dichloroethene-d2		2.307	65	36391	48.755	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	97.500%	
21) 2-Butanone-d5		4.459	46	119778	125.774	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	125.770%	
24) Chloroform-d		5.056	84	164138	50.317	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.640%	
26) 1,2-Dichloroethane-d4		5.958	65	109353	51.536	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.080%	
32) Benzene-d6		5.977	84	328458	51.855	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.700%	
36) 1,2-Dichloropropane-d6		7.306	67	97076	52.549	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	105.100%	
41) Toluene-d8		8.647	98	301314	48.692	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.380%	
43) trans-1,3-Dichloroprop...		8.952	79	43427	46.713	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.420%	
47) 2-Hexanone-d5		9.385	63	83658	107.409	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	107.410%	
56) 1,1,2,2-Tetrachloroeth...		11.189	84	144689	52.873	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	105.740%	
66) 1,2-Dichlorobenzene-d4		12.317	152	137346	53.870	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.740%	
Target Compounds							
13) Acetone		2.380	43	5585	5.411	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041047.D
Acq On : 12 Apr 2024 21:42
Operator : JC/MD
Sample : P2060-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1D01

Quant Time: Apr 13 04:23:21 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 13 04:06:48 2024
Response via : Initial Calibration

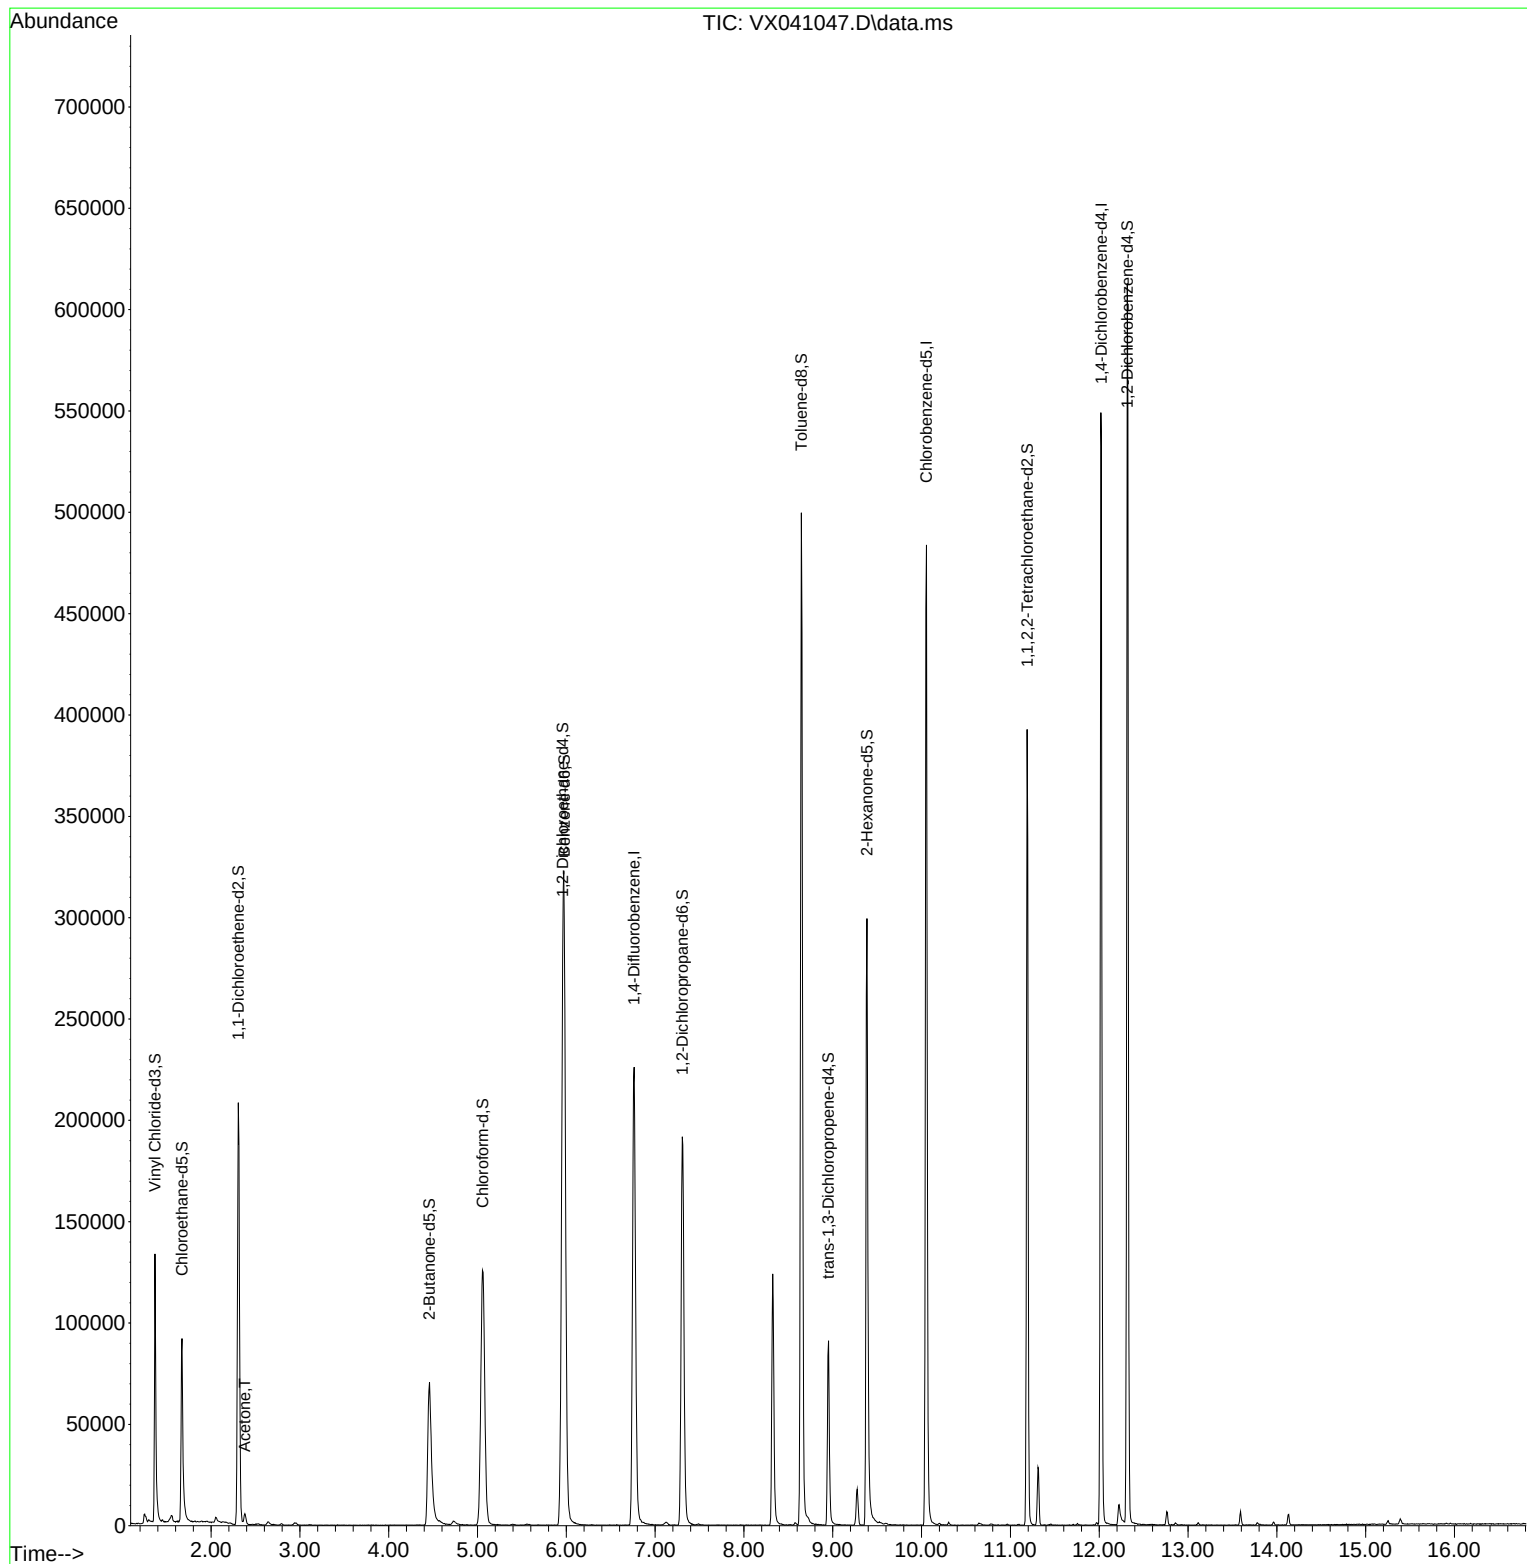

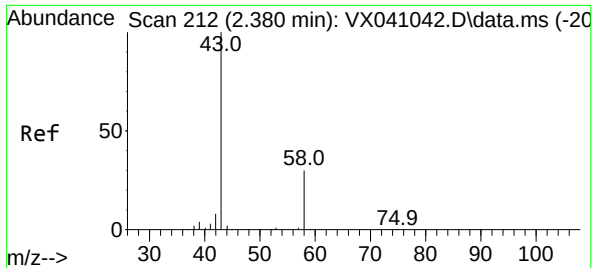

#13

Acetone

Concen: 5.411 ug/L

RT: 2.380 min Scan# 21

Delta R.T. 0.000 min

Lab File: VX041047.D


Acq: 12 Apr 2024 21:42

Instrument :

MSVOA_X

ClientSampleId :

E1D01

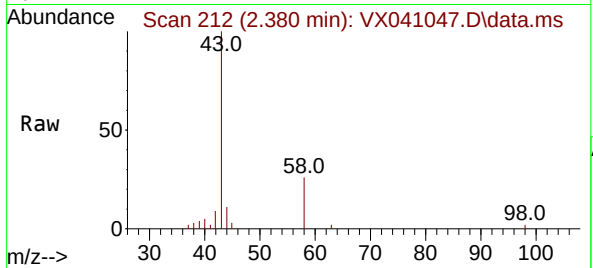

Tgt Ion: 43 Resp: 5585

Ion Ratio Lower Upper

43 100

58 30.4 0.0 59.4

