

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041049.D
 Acq On : 12 Apr 2024 22:28
 Operator : JC/MD
 Sample : P2098-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R87

Quant Time: Apr 13 04:23:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 13 04:06:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	248834	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	235574	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	127609	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	87627	49.510	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	99.020%		
7) Chloroethane-d5	1.673	69	74127	51.354	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	102.700%		
11) 1,1-Dichloroethene-d2	2.307	65	36284	48.018	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	96.040%		
21) 2-Butanone-d5	4.459	46	118312	122.719	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	122.720%		
24) Chloroform-d	5.056	84	163565	49.530	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.060%		
26) 1,2-Dichloroethane-d4	5.958	65	106808	49.722	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.440%		
32) Benzene-d6	5.977	84	322447	50.418	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.840%		
36) 1,2-Dichloropropane-d6	7.312	67	95473	51.186	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	102.380%		
41) Toluene-d8	8.647	98	299616	47.954	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.900%		
43) trans-1,3-Dichloroprop...	8.952	79	43758	46.618	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	93.240%		
47) 2-Hexanone-d5	9.385	63	82376	104.750	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	104.750%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	144243	52.205	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	104.420%		
66) 1,2-Dichlorobenzene-d4	12.317	152	135876	53.080	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	106.160%		
Target Compounds					Qvalue	
13) Acetone	2.380	43	4674	4.473	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041049.D
Acq On : 12 Apr 2024 22:28
Operator : JC/MD
Sample : P2098-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R87

Quant Time: Apr 13 04:23:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 13 04:06:48 2024
Response via : Initial Calibration

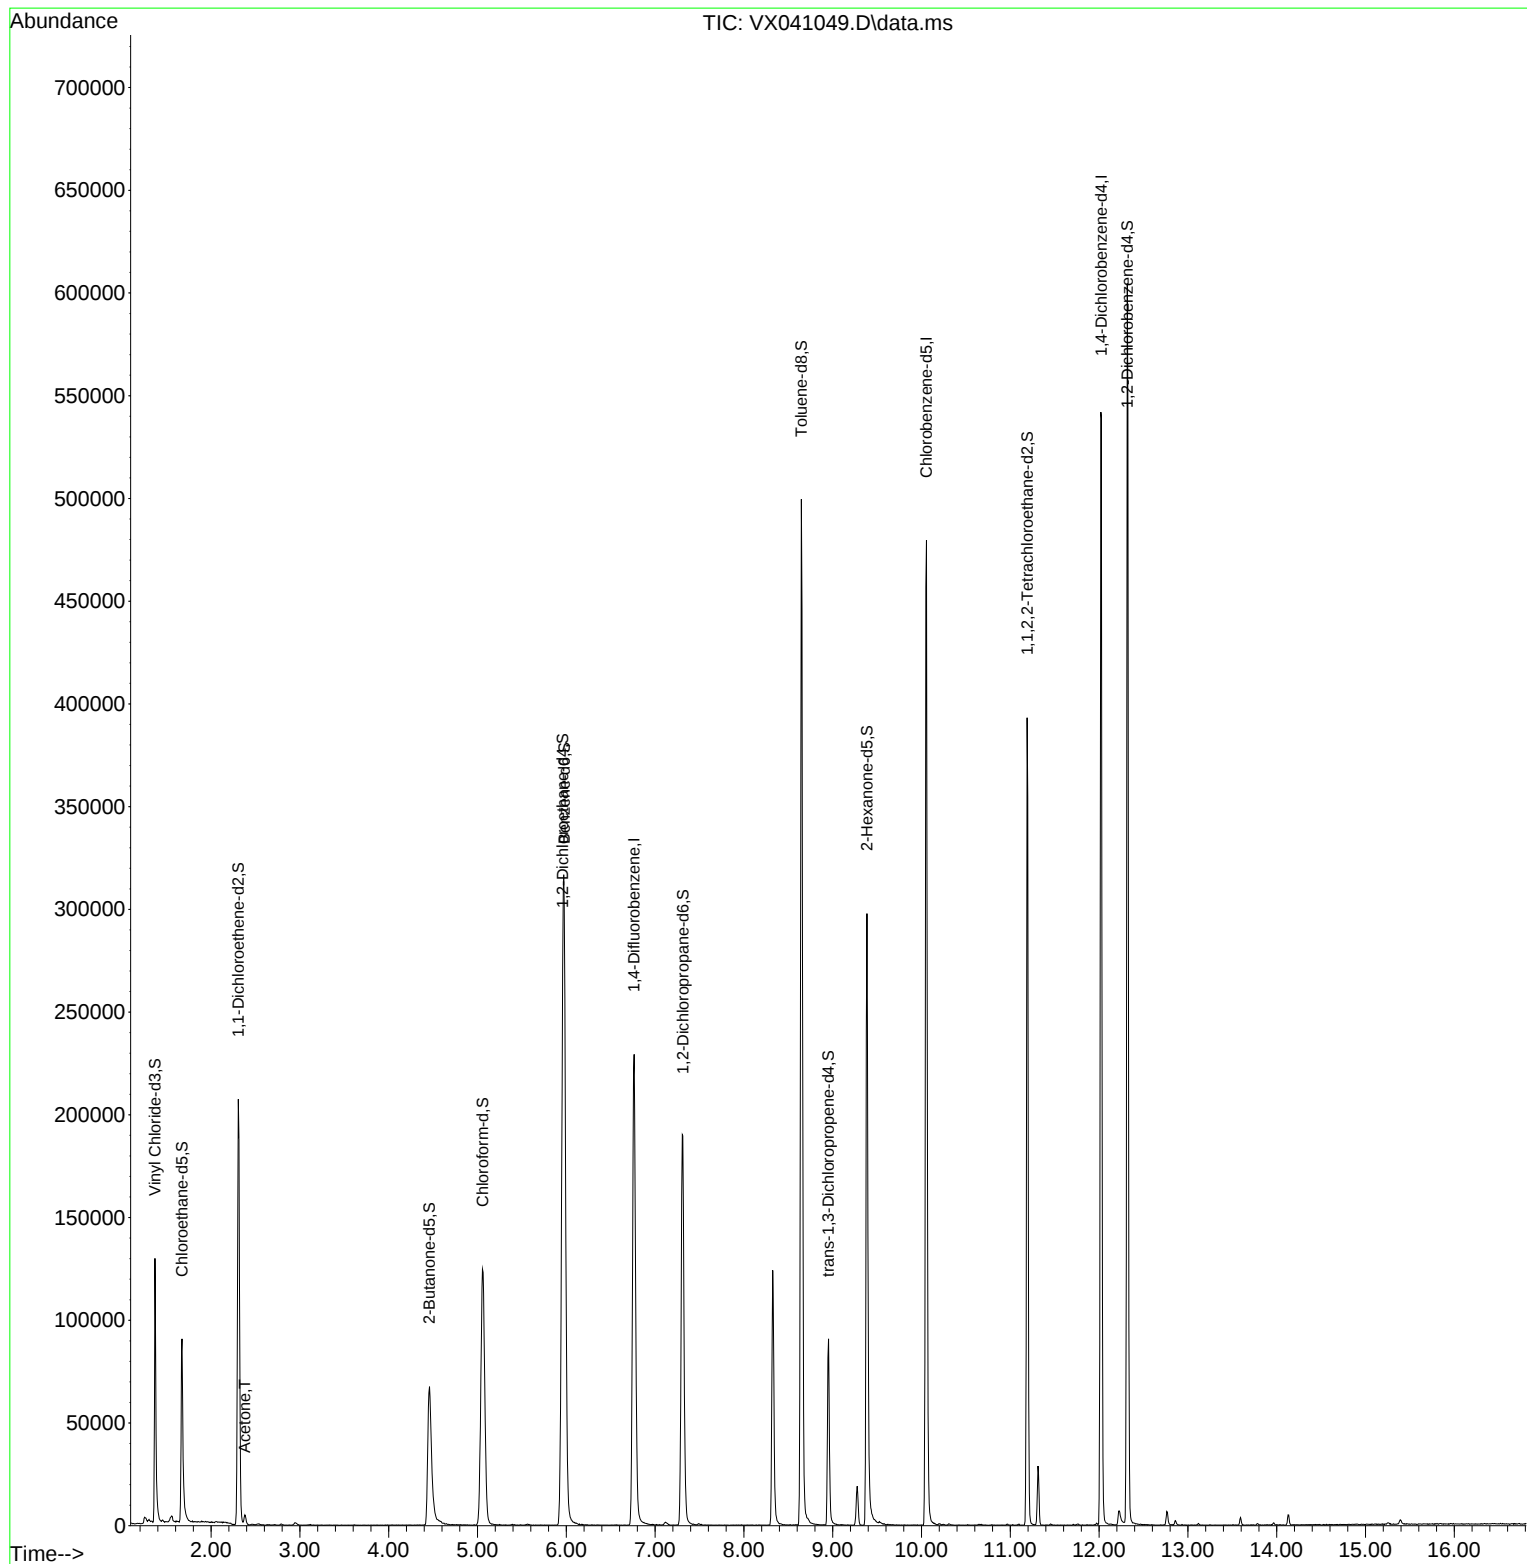

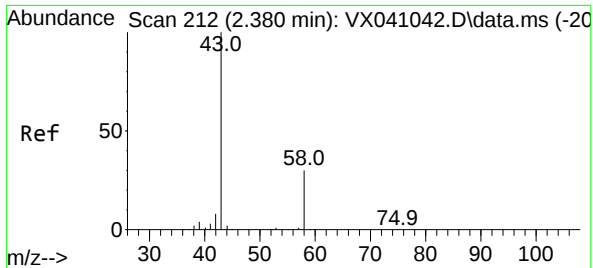

#13
 Acetone
 Concen: 4.473 ug/L
 RT: 2.380 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VX041049.D
 Acq: 12 Apr 2024 22:28

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R87

Tgt Ion: 43 Resp: 4674
 Ion Ratio Lower Upper
 43 100
 58 31.1 0.0 59.4

