

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041050.D
 Acq On : 12 Apr 2024 22:51
 Operator : JC/MD
 Sample : P2049-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MCORE7

Quant Time: Apr 13 04:23:59 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 13 04:06:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	259396	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	243518	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	127255	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	93290	50.564	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	101.120%
7) Chloroethane-d5	1.672	69	76177	50.625	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	101.260%
11) 1,1-Dichloroethene-d2	2.306	65	38985	49.492	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	98.980%
21) 2-Butanone-d5	4.452	46	129809	129.162	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	129.160%
24) Chloroform-d	5.062	84	174978	50.828	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.660%
26) 1,2-Dichloroethane-d4	5.952	65	116069	51.833	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.660%
32) Benzene-d6	5.970	84	346502	52.412	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.820%
36) 1,2-Dichloropropane-d6	7.305	67	102449	53.134	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	106.260%
41) Toluene-d8	8.647	98	318535	49.318	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.640%
43) trans-1,3-Dichloroprop...	8.951	79	45569	46.964	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.920%
47) 2-Hexanone-d5	9.384	63	88685	109.094	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	109.090%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	148876	52.124	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	104.240%
66) 1,2-Dichlorobenzene-d4	12.317	152	137417	53.832	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.660%
Target Compounds						
13) Acetone	2.380	43	3559	3.267	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041050.D
Acq On : 12 Apr 2024 22:51
Operator : JC/MD
Sample : P2049-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RE7

Quant Time: Apr 13 04:23:59 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 13 04:06:48 2024
Response via : Initial Calibration

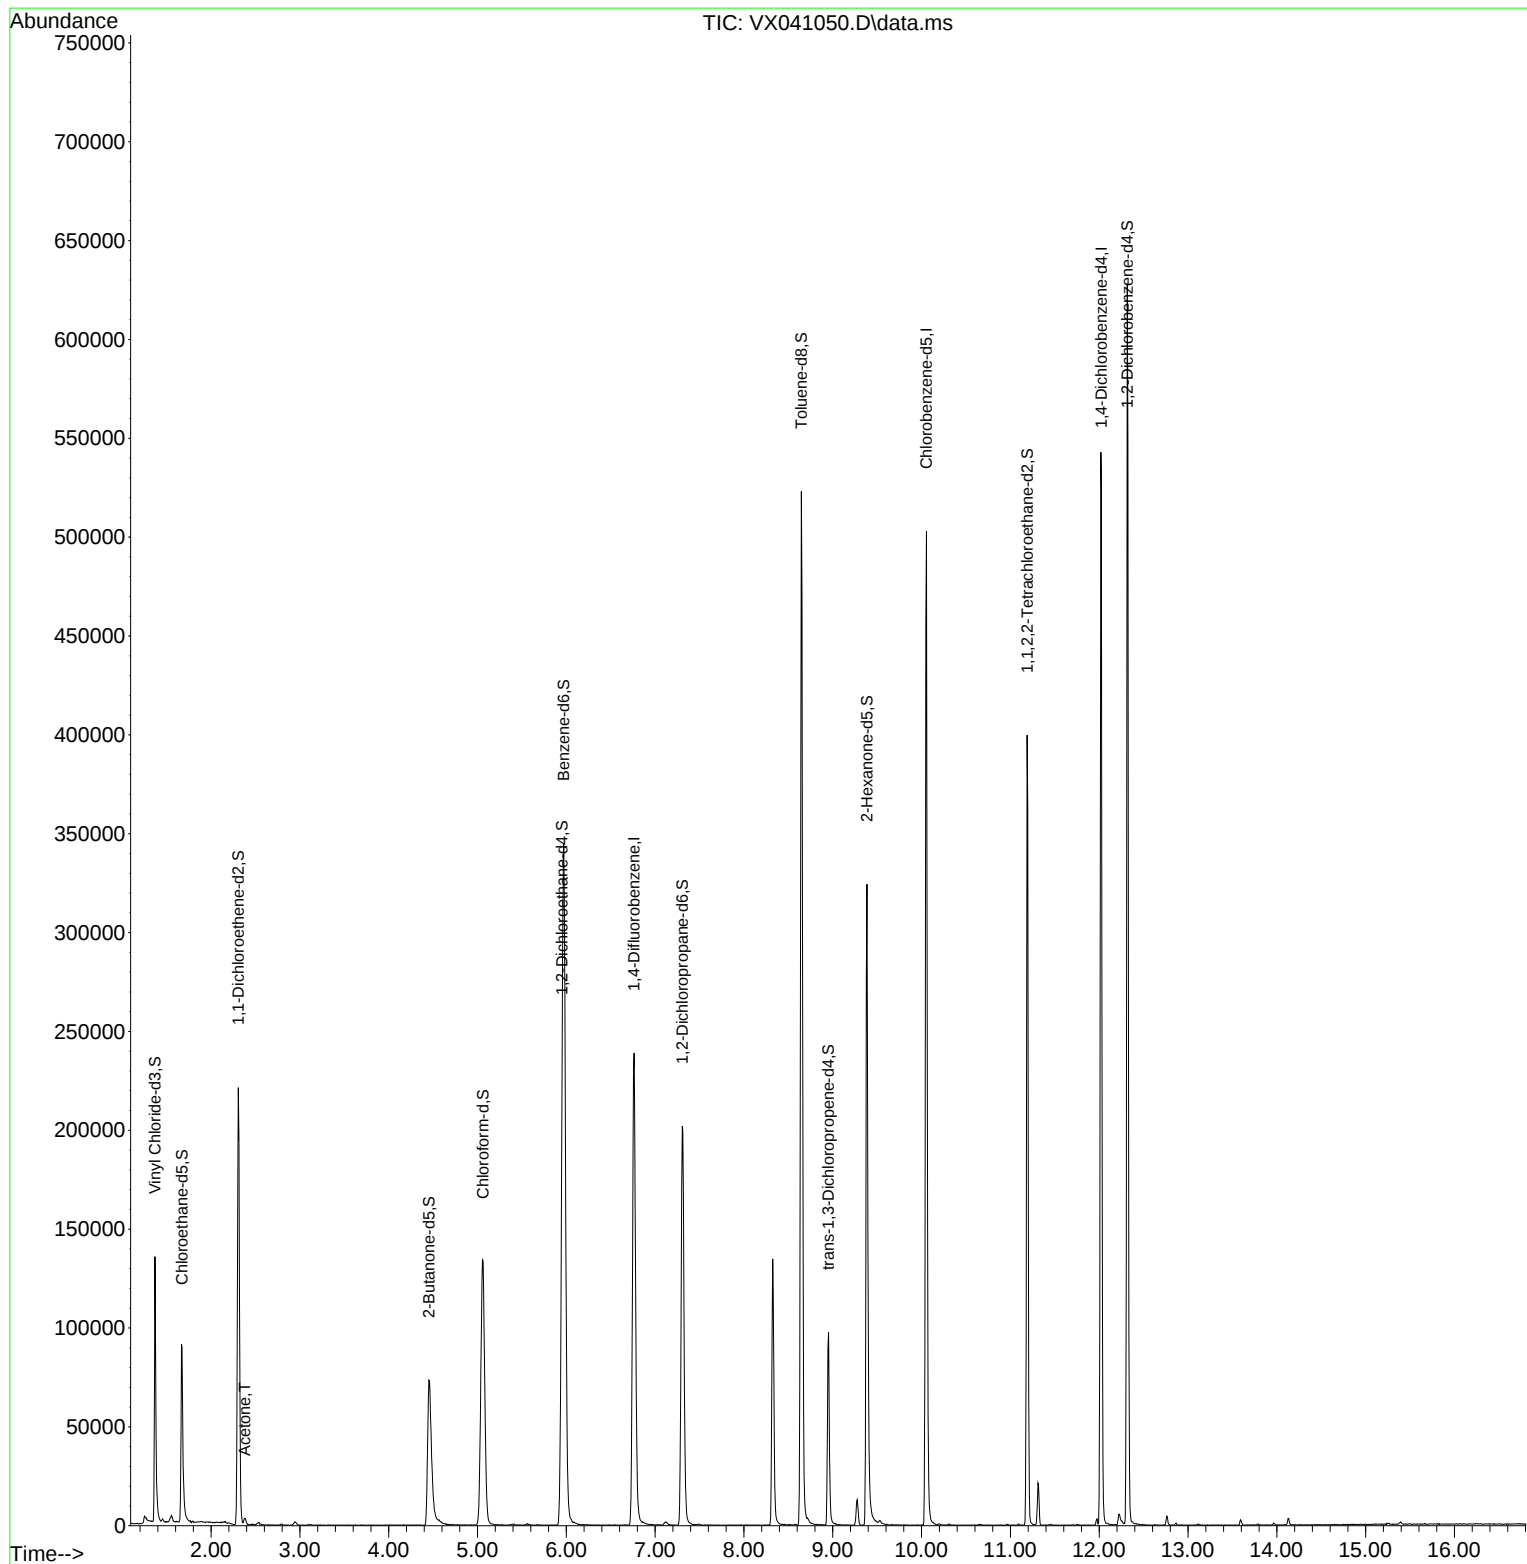

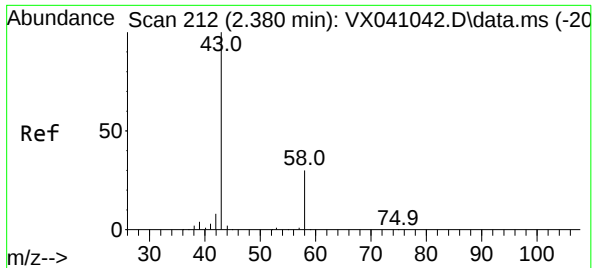

#13
 Acetone
 Concen: 3.267 ug/L
 RT: 2.380 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VX041050.D
 Acq: 12 Apr 2024 22:51

Instrument :
 MSVOA_X
 ClientSampleId :
 MCORE7

Tgt Ion: 43 Resp: 3559
 Ion Ratio Lower Upper
 43 100
 58 28.7 0.0 59.4

