

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041016.D
 Acq On : 12 Apr 2024 09:51
 Operator : JC/MD
 Sample : P2048-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX041016.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	56	rBV	130443	147558	14.29%	1.815%
2	1.672	91	96	111	rVB	93816	142132	13.76%	1.748%
3	2.306	194	200	209	rBV	227363	348408	33.74%	4.285%
4	2.459	224	225	229	rBV2	308	343	0.03%	0.004%
5	2.526	231	236	243	rVB3	1608	3603	0.35%	0.044%
6	2.648	254	256	259	rVB	206	157	0.02%	0.002%
7	2.794	274	280	284	rBV4	677	1406	0.14%	0.017%
8	2.940	298	304	310	rBV2	2094	4119	0.40%	0.051%
9	3.087	323	328	330	rBV3	462	599	0.06%	0.007%
10	3.446	385	387	389	rVB	182	122	0.01%	0.002%
11	3.465	389	390	392	rVB2	173	116	0.01%	0.001%
12	3.489	392	394	396	rBV2	137	161	0.02%	0.002%
13	3.574	401	408	416	rVB3	1982	4448	0.43%	0.055%
14	3.709	426	430	431	rVB2	132	131	0.01%	0.002%
15	3.739	433	435	439	rVB2	121	152	0.01%	0.002%
16	3.788	439	443	445	rBV2	141	243	0.02%	0.003%
17	3.971	471	473	475	rVB2	217	157	0.02%	0.002%
18	4.001	475	478	481	rBV	155	230	0.02%	0.003%
19	4.099	492	494	495	rBV	154	112	0.01%	0.001%
20	4.324	528	531	532	rBV	126	110	0.01%	0.001%
21	4.452	543	552	568	rBV	69882	214709	20.79%	2.641%
22	4.885	619	623	624	rBV2	183	210	0.02%	0.003%
23	5.056	638	651	668	rVV	134362	409613	39.66%	5.038%
24	5.269	685	686	689	rVB	245	177	0.02%	0.002%
25	5.318	692	694	696	rBV2	195	188	0.02%	0.002%
26	5.342	696	698	700	rVB	160	119	0.01%	0.001%
27	5.373	700	703	705	rBV2	276	446	0.04%	0.005%
28	5.550	729	732	740	rVB3	477	1220	0.12%	0.015%
29	5.836	776	779	781	rBV2	133	197	0.02%	0.002%
30	5.964	789	800	822	rBV2	343506	1032721	100.00%	12.702%
31	6.501	886	888	891	rBV	144	149	0.01%	0.002%
32	6.641	910	911	916	rVB2	182	144	0.01%	0.002%
33	6.757	921	930	952	rBV	242585	592865	57.41%	7.292%
34	7.129	985	991	996	rVV4	1091	2686	0.26%	0.033%
35	7.220	1003	1006	1007	rBV	131	172	0.02%	0.002%
36	7.306	1009	1020	1039	rBV	205063	454984	44.06%	5.596%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041016.D
 Acq On : 12 Apr 2024 09:51
 Operator : JC/MD
 Sample : P2048-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	7.446	1041	1043	1047	rVB3	292	228	0.02%	0.003%
38	7.476	1047	1048	1049	rBV	257	168	0.02%	0.002%
39	7.525	1054	1056	1057	rVV2	208	113	0.01%	0.001%
40	7.586	1064	1066	1070	rVB2	127	137	0.01%	0.002%
41	7.623	1070	1072	1073	rBV	159	115	0.01%	0.001%
42	7.933	1121	1123	1124	rBV	164	131	0.01%	0.002%
43	7.946	1124	1125	1128	rVV2	279	325	0.03%	0.004%
44	8.019	1136	1137	1143	rVB2	198	253	0.02%	0.003%
45	8.183	1161	1164	1167	rBV2	112	141	0.01%	0.002%
46	8.324	1181	1187	1200	rBV	138876	227398	22.02%	2.797%
47	8.574	1226	1228	1233	rVB3	440	522	0.05%	0.006%
48	8.647	1233	1240	1259	rBV	553021	871210	84.36%	10.716%
49	8.945	1284	1289	1300	rBV	94544	148855	14.41%	1.831%
50	9.128	1318	1319	1322	rVB	382	267	0.03%	0.003%
51	9.171	1322	1326	1330	rBV2	295	465	0.05%	0.006%
52	9.275	1337	1343	1350	rBV	51826	82094	7.95%	1.010%
53	9.384	1355	1361	1381	rBV	296456	464569	44.98%	5.714%
54	9.732	1416	1418	1421	rVB	198	117	0.01%	0.001%
55	9.799	1427	1429	1430	rVB2	205	117	0.01%	0.001%
56	10.049	1465	1470	1490	rBV	498129	730671	70.75%	8.987%
57	10.311	1509	1513	1517	rVV2	667	1030	0.10%	0.013%
58	10.512	1544	1546	1548	rVB	132	116	0.01%	0.001%
59	10.537	1548	1550	1551	rBV	165	123	0.01%	0.002%
60	10.665	1564	1571	1578	rVB5	846	1990	0.19%	0.024%
61	10.720	1578	1580	1583	rVB2	108	128	0.01%	0.002%
62	10.762	1583	1587	1588	rBV	167	263	0.03%	0.003%
63	10.835	1595	1599	1600	rVB2	134	144	0.01%	0.002%
64	10.963	1616	1620	1626	rVB2	791	1078	0.10%	0.013%
65	11.098	1638	1642	1646	rVV2	720	997	0.10%	0.012%
66	11.189	1652	1657	1667	rVV	410791	518078	50.17%	6.372%
67	11.311	1671	1677	1683	rVV	62187	88966	8.61%	1.094%
68	11.451	1696	1700	1704	rBV3	711	1011	0.10%	0.012%
69	11.604	1723	1725	1728	rVV2	159	131	0.01%	0.002%
70	11.707	1740	1742	1746	rVB3	375	346	0.03%	0.004%
71	11.756	1746	1750	1755	rBV	1150	1301	0.13%	0.016%
72	11.878	1768	1770	1773	rBV	224	184	0.02%	0.002%
73	11.975	1780	1786	1788	rBV3	2094	3130	0.30%	0.038%
74	12.018	1788	1793	1805	rVV	576978	742906	71.94%	9.138%
75	12.225	1824	1827	1834	rVB4	1331	2640	0.26%	0.032%
76	12.317	1837	1842	1865	rVB	648770	824325	79.82%	10.139%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041016.D
 Acq On : 12 Apr 2024 09:51
 Operator : JC/MD
 Sample : P2048-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	12.524	1874	1876	1877	rBV	231	185	0.02%	0.002%
78	12.713	1905	1907	1910	rBV	206	196	0.02%	0.002%
79	12.762	1910	1915	1920	rVV	13359	17783	1.72%	0.219%
80	12.939	1940	1944	1945	rVB2	151	165	0.02%	0.002%
81	13.006	1953	1955	1958	rBV2	115	122	0.01%	0.002%
82	13.085	1966	1968	1969	rBV2	150	148	0.01%	0.002%
83	13.115	1969	1973	1978	rVV2	3306	4125	0.40%	0.051%
84	13.274	1996	1999	2001	rVB2	161	179	0.02%	0.002%
85	13.298	2001	2003	2006	rBV	189	238	0.02%	0.003%
86	13.420	2021	2023	2026	rBV2	158	200	0.02%	0.002%
87	13.530	2038	2041	2043	rVB2	218	195	0.02%	0.002%
88	13.591	2047	2051	2056	rBV2	5886	7642	0.74%	0.094%
89	13.780	2078	2082	2091	rBV2	3647	5704	0.55%	0.070%
90	13.871	2095	2097	2100	rVB2	194	167	0.02%	0.002%
91	13.926	2102	2106	2107	rBV2	168	170	0.02%	0.002%
92	13.963	2107	2112	2118	rBV	4221	5906	0.57%	0.073%
93	14.024	2120	2122	2124	rVB2	176	139	0.01%	0.002%
94	14.054	2124	2127	2128	rBV2	164	148	0.01%	0.002%
95	14.127	2133	2139	2145	rBV	2255	3556	0.34%	0.044%
96	14.298	2166	2167	2170	rBV	243	187	0.02%	0.002%
97	14.365	2176	2178	2179	rBV2	187	173	0.02%	0.002%
98	15.615	2380	2383	2385	rVB3	390	381	0.04%	0.005%
99	15.853	2420	2422	2426	rBV2	414	559	0.05%	0.007%
100	16.011	2446	2448	2449	rBV	396	177	0.02%	0.002%


Sum of corrected areas: 8130135

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041016.D
Acq On : 12 Apr 2024 09:51
Operator : JC/MD
Sample : P2048-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

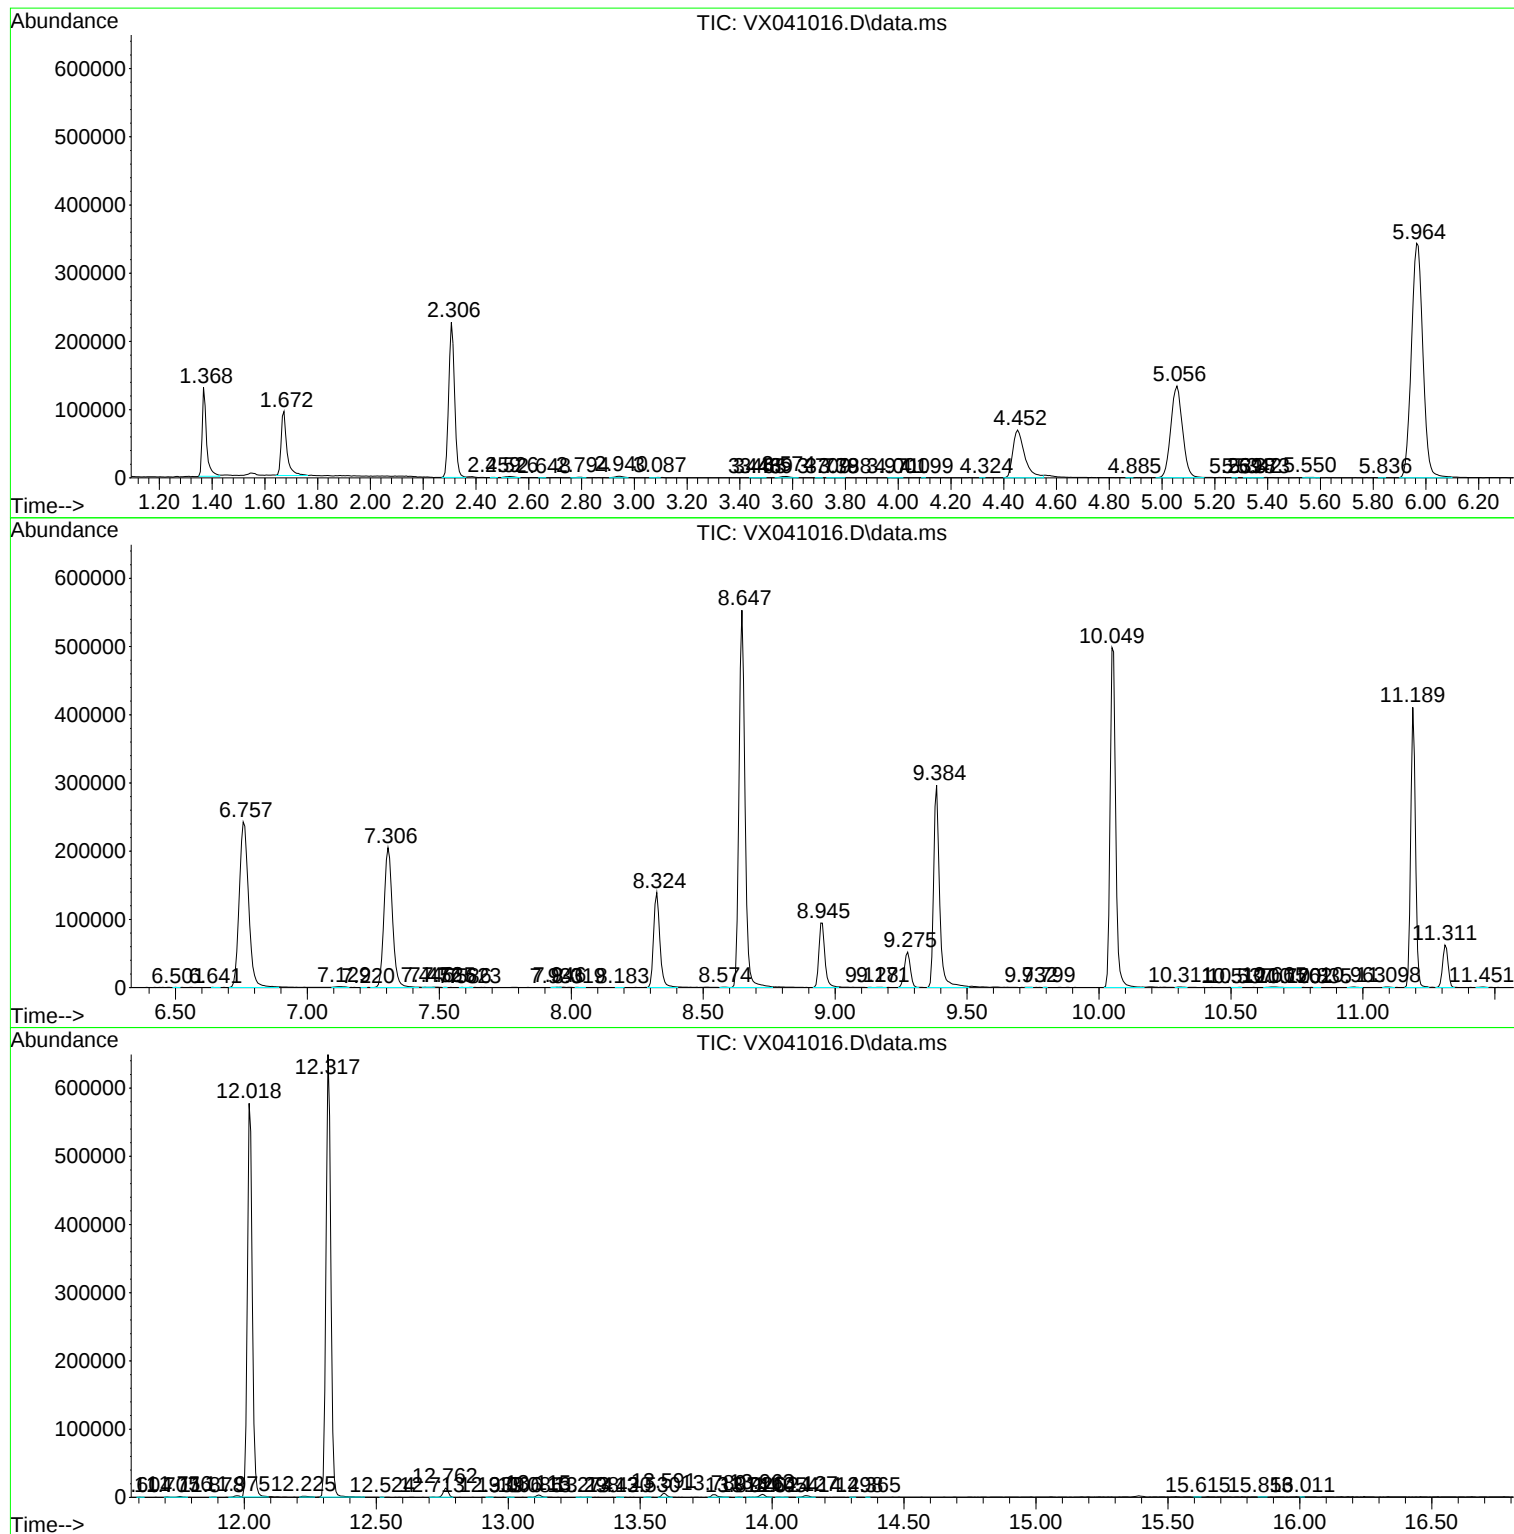

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041016.D
Acq On : 12 Apr 2024 09:51
Operator : JC/MD
Sample : P2048-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041016.D
Acq On : 12 Apr 2024 09:51
Operator : JC/MD
Sample : P2048-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc