

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041023.D
 Acq On : 12 Apr 2024 12:31
 Operator : JC/MD
 Sample : P2048-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX041023.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	33	rBV	8995	15265	1.52%	0.189%
2	1.368	43	46	63	rVB	126590	138767	13.80%	1.719%
3	1.673	91	96	110	rBV	88832	135439	13.47%	1.678%
4	2.307	194	200	209	rBV	216328	332120	33.02%	4.114%
5	2.471	222	227	229	rBV3	465	716	0.07%	0.009%
6	2.532	230	237	260	rVV	108636	210611	20.94%	2.609%
7	2.947	300	305	311	rVB2	1793	3804	0.38%	0.047%
8	3.197	345	346	349	rVB2	136	113	0.01%	0.001%
9	3.264	355	357	359	rBV	252	273	0.03%	0.003%
10	3.306	362	364	366	rBV2	190	172	0.02%	0.002%
11	3.416	379	382	384	rBV	107	117	0.01%	0.001%
12	3.453	387	388	390	rBV2	146	106	0.01%	0.001%
13	3.556	403	405	407	rVB	189	119	0.01%	0.001%
14	3.849	451	453	455	rVB	192	110	0.01%	0.001%
15	3.873	455	457	459	rBV2	137	114	0.01%	0.001%
16	4.007	478	479	483	rVB	162	176	0.02%	0.002%
17	4.172	502	506	509	rBV	256	265	0.03%	0.003%
18	4.453	543	552	576	rBV	73528	230693	22.94%	2.858%
19	4.855	616	618	619	rBV	209	151	0.02%	0.002%
20	5.056	639	651	673	rBV	131142	403475	40.12%	4.998%
21	5.373	701	703	704	rBV2	363	259	0.03%	0.003%
22	5.501	722	724	728	rVV2	132	154	0.02%	0.002%
23	5.562	728	734	741	rVV3	610	1353	0.13%	0.017%
24	5.971	789	801	822	rBV2	337446	1005691	100.00%	12.458%
25	6.355	862	864	865	rVB	191	104	0.01%	0.001%
26	6.409	871	873	876	rBV2	256	204	0.02%	0.003%
27	6.452	878	880	883	rVB2	190	187	0.02%	0.002%
28	6.763	921	931	946	rBV	242502	592730	58.94%	7.343%
29	7.074	980	982	984	rBB	211	138	0.01%	0.002%
30	7.123	984	990	998	rBV6	1343	3255	0.32%	0.040%
31	7.306	1011	1020	1040	rBV	199507	444707	44.22%	5.509%
32	7.434	1040	1041	1042	rVB	307	118	0.01%	0.001%
33	7.482	1047	1049	1053	rBV4	492	712	0.07%	0.009%
34	7.550	1058	1060	1062	rBV	162	160	0.02%	0.002%
35	7.586	1064	1066	1068	rVV	118	98	0.01%	0.001%
36	7.793	1098	1100	1103	rVB2	155	156	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041023.D
 Acq On : 12 Apr 2024 12:31
 Operator : JC/MD
 Sample : P2048-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	7.958	1122	1127	1132	rBV3	338	826	0.08%	0.010%
38	8.153	1155	1159	1162	rVB2	215	315	0.03%	0.004%
39	8.184	1162	1164	1165	rBV2	173	154	0.02%	0.002%
40	8.238	1171	1173	1174	rBV	173	117	0.01%	0.001%
41	8.324	1181	1187	1200	rBV	134106	216811	21.56%	2.686%
42	8.586	1226	1230	1234	rBV2	267	322	0.03%	0.004%
43	8.647	1234	1240	1264	rBV	525788	841481	83.67%	10.424%
44	8.854	1273	1274	1275	rVB	316	115	0.01%	0.001%
45	8.952	1284	1290	1304	rBV	92298	142223	14.14%	1.762%
46	9.129	1317	1319	1321	rVB	242	170	0.02%	0.002%
47	9.202	1328	1331	1334	rVB	217	296	0.03%	0.004%
48	9.226	1334	1335	1337	rBV2	143	132	0.01%	0.002%
49	9.275	1338	1343	1349	rVB	6472	9173	0.91%	0.114%
50	9.330	1349	1352	1355	rBV2	91	116	0.01%	0.001%
51	9.385	1356	1361	1381	rBV2	313164	484769	48.20%	6.005%
52	9.872	1440	1441	1444	rVB2	199	139	0.01%	0.002%
53	10.055	1465	1471	1491	rBV	508216	727455	72.33%	9.012%
54	10.311	1508	1513	1520	rVB3	686	1316	0.13%	0.016%
55	10.360	1520	1521	1524	rVB2	199	141	0.01%	0.002%
56	10.482	1539	1541	1546	rVB2	102	132	0.01%	0.002%
57	10.653	1564	1569	1575	rVV3	435	674	0.07%	0.008%
58	10.732	1581	1582	1586	rBV2	139	174	0.02%	0.002%
59	10.793	1589	1592	1596	rBV2	79	118	0.01%	0.001%
60	10.964	1617	1620	1622	rVV2	402	440	0.04%	0.005%
61	11.000	1624	1626	1627	rVB	170	104	0.01%	0.001%
62	11.018	1627	1629	1631	rBV2	132	133	0.01%	0.002%
63	11.092	1636	1641	1647	rBV4	586	1120	0.11%	0.014%
64	11.189	1652	1657	1669	rVV	406282	520504	51.76%	6.448%
65	11.311	1672	1677	1686	rVB	9580	13688	1.36%	0.170%
66	11.463	1697	1702	1704	rBV3	391	536	0.05%	0.007%
67	11.518	1709	1711	1714	rVV	172	140	0.01%	0.002%
68	11.555	1715	1717	1719	rVB2	212	124	0.01%	0.002%
69	11.665	1734	1735	1738	rBV	122	110	0.01%	0.001%
70	11.713	1738	1743	1746	rVB2	293	379	0.04%	0.005%
71	11.762	1746	1751	1753	rBV3	516	614	0.06%	0.008%
72	11.921	1775	1777	1778	rVB	204	115	0.01%	0.001%
73	11.951	1778	1782	1783	rBV2	149	187	0.02%	0.002%
74	11.976	1783	1786	1788	rBV2	1131	1416	0.14%	0.018%
75	12.018	1788	1793	1805	rVV	571328	738533	73.44%	9.149%
76	12.219	1822	1826	1837	rBV	11184	23075	2.29%	0.286%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041023.D
 Acq On : 12 Apr 2024 12:31
 Operator : JC/MD
 Sample : P2048-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	12.317	1837	1842	1853	rVB	635087	807818	80.32%	10.007%
78	12.658	1896	1898	1900	rBV	217	194	0.02%	0.002%
79	12.725	1908	1909	1911	rBV	232	152	0.02%	0.002%
80	12.762	1911	1915	1921	rVB	2098	2717	0.27%	0.034%
81	12.847	1926	1929	1933	rBV2	199	307	0.03%	0.004%
82	12.902	1936	1938	1941	rBV2	197	258	0.03%	0.003%
83	12.988	1951	1952	1954	rVB	234	130	0.01%	0.002%
84	13.012	1954	1956	1957	rBV	131	113	0.01%	0.001%
85	13.049	1960	1962	1964	rBV	140	155	0.02%	0.002%
86	13.122	1970	1974	1981	rBV3	819	996	0.10%	0.012%
87	13.451	2026	2028	2030	rBV2	133	136	0.01%	0.002%
88	13.591	2048	2051	2058	rVB3	1601	2443	0.24%	0.030%
89	13.695	2067	2068	2074	rVB2	203	281	0.03%	0.003%
90	13.737	2074	2075	2078	rBV2	198	126	0.01%	0.002%
91	13.780	2078	2082	2087	rBV3	585	1045	0.10%	0.013%
92	13.896	2099	2101	2102	rBV	167	121	0.01%	0.001%
93	13.963	2110	2112	2116	rVB2	1083	1078	0.11%	0.013%
94	14.054	2125	2127	2131	rBV3	177	234	0.02%	0.003%
95	14.128	2135	2139	2145	rBV2	1483	1913	0.19%	0.024%
96	14.189	2148	2149	2152	rBV2	214	184	0.02%	0.002%
97	14.219	2152	2154	2157	rBV2	212	323	0.03%	0.004%
98	14.335	2171	2173	2175	rBV	147	143	0.01%	0.002%
99	14.640	2221	2223	2226	rVB	338	264	0.03%	0.003%
100	14.737	2238	2239	2240	rBV	368	208	0.02%	0.003%




Sum of corrected areas: 8072358

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041023.D
Acq On : 12 Apr 2024 12:31
Operator : JC/MD
Sample : P2048-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R98

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

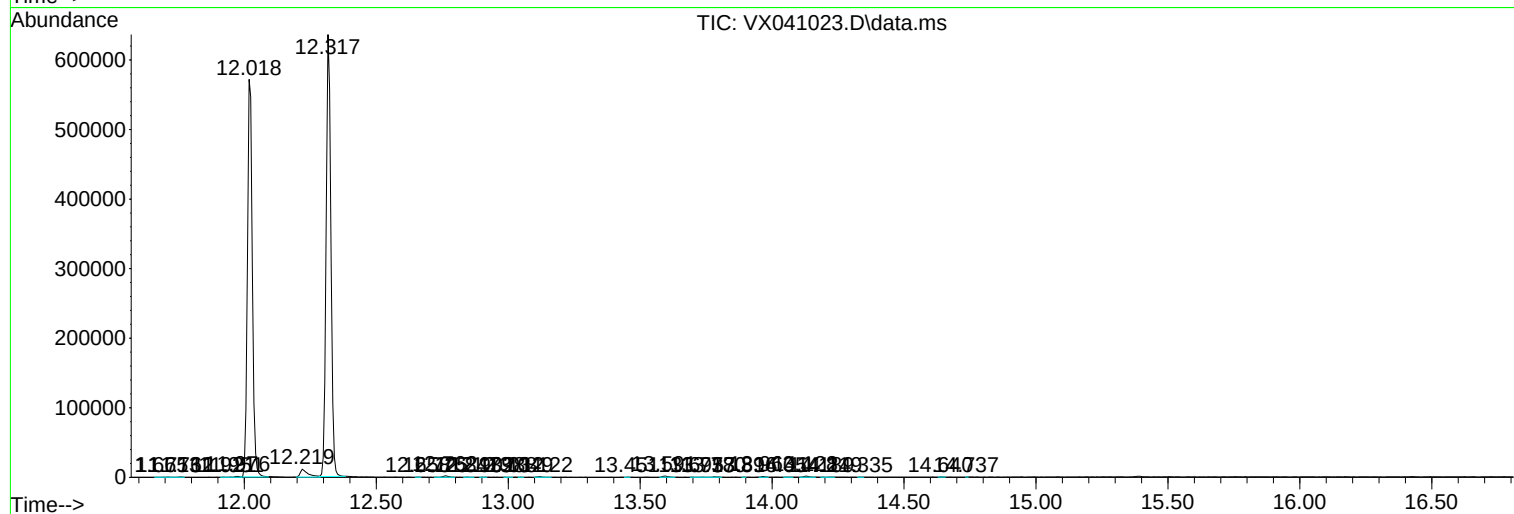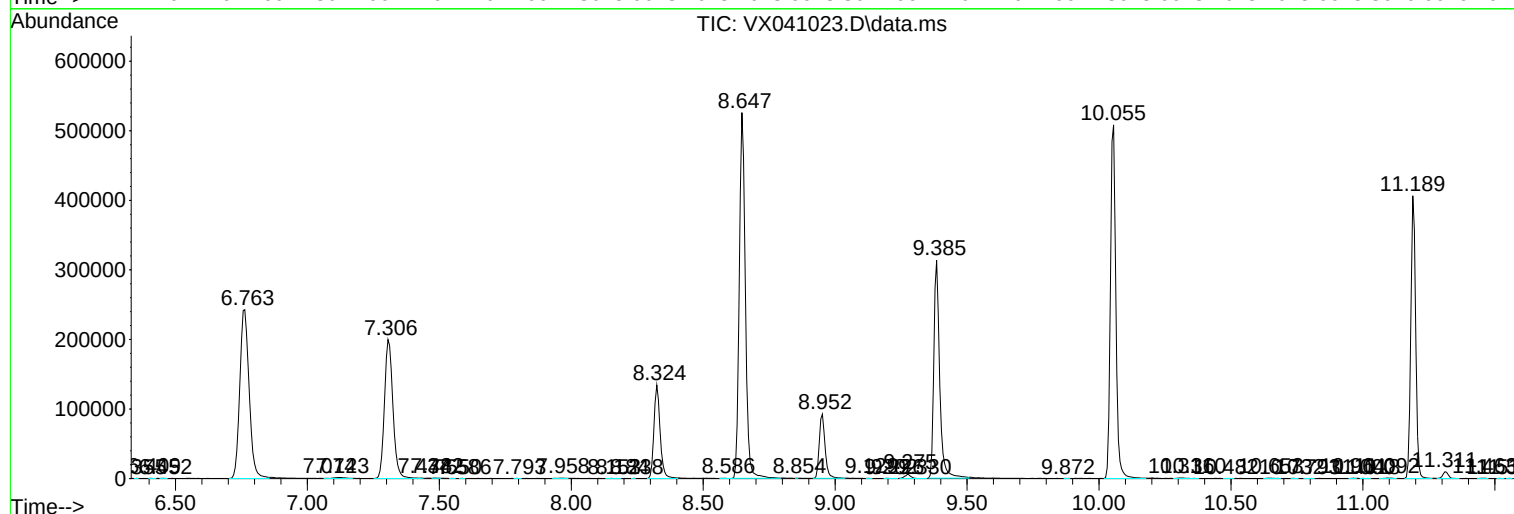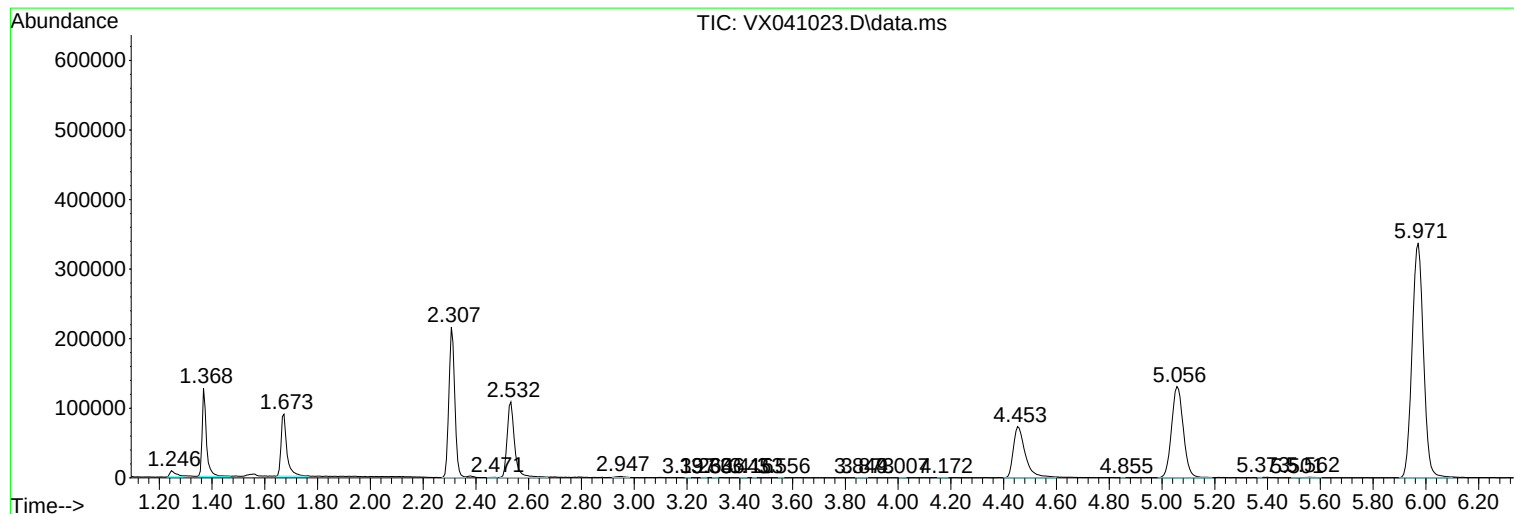

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041023.D
Acq On : 12 Apr 2024 12:31
Operator : JC/MD
Sample : P2048-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R98










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.532	17.77 ug/L	210611	1,4-Difluorobenzene	6.763

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	83
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
4			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
5			Isopropyl Alcohol	60	C3H8O	000067-63-0	64

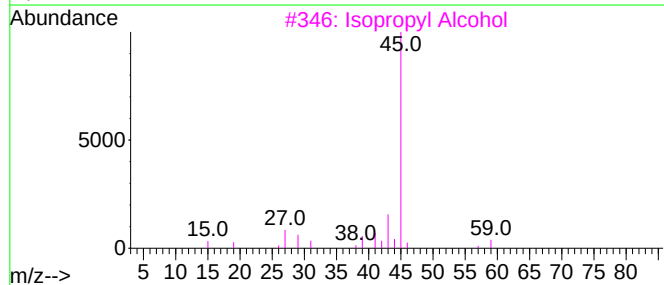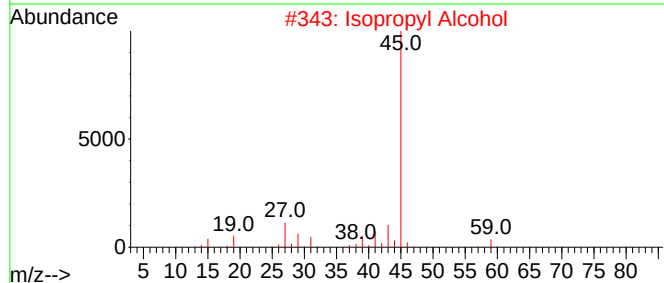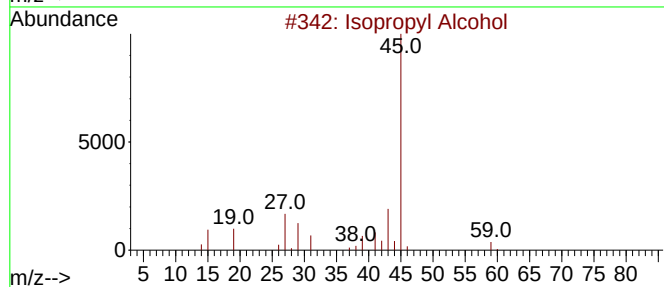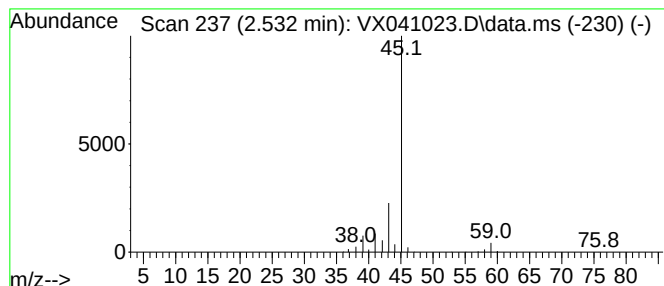

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041023.D
Acq On : 12 Apr 2024 12:31
Operator : JC/MD
Sample : P2048-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R98

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.532	17.8	ug/L	210611	1	6.763	592730	50.0