

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041026.D
 Acq On : 12 Apr 2024 13:40
 Operator : JC/MD
 Sample : P2048-03DL 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R47DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M

Title : VOC Analysis

Signal : TIC: VX041026.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	33	rBV	8908	14969	1.39%	0.173%
2	1.368	43	46	57	rBV	146428	164192	15.22%	1.897%
3	1.672	91	96	110	rVB	99396	149172	13.83%	1.723%
4	2.306	194	200	211	rBV	238529	374385	34.71%	4.325%
5	2.532	231	237	245	rVB4	802	2086	0.19%	0.024%
6	2.666	257	259	261	rBV	216	170	0.02%	0.002%
7	2.703	263	265	267	rBV2	223	194	0.02%	0.002%
8	2.794	273	280	286	rBV5	761	1614	0.15%	0.019%
9	2.855	288	290	294	rBV2	106	150	0.01%	0.002%
10	2.941	297	304	314	rVB	5097	11440	1.06%	0.132%
11	3.093	327	329	330	rBV	227	170	0.02%	0.002%
12	3.154	338	339	341	rBV	141	117	0.01%	0.001%
13	3.227	347	351	352	rBV2	140	152	0.01%	0.002%
14	3.465	388	390	392	rVV2	163	149	0.01%	0.002%
15	3.599	409	412	416	rVB2	169	217	0.02%	0.003%
16	3.678	423	425	427	rVB2	109	117	0.01%	0.001%
17	3.764	436	439	440	rBV2	152	116	0.01%	0.001%
18	3.800	444	445	450	rBV2	148	186	0.02%	0.002%
19	3.849	450	453	454	rBV	156	150	0.01%	0.002%
20	3.940	466	468	470	rBV2	121	119	0.01%	0.001%
21	3.983	474	475	478	rVV2	158	128	0.01%	0.001%
22	4.111	495	496	500	rBV2	195	243	0.02%	0.003%
23	4.202	510	511	514	rBV2	149	144	0.01%	0.002%
24	4.282	522	524	526	rVB2	166	110	0.01%	0.001%
25	4.452	544	552	568	rBV	74900	232304	21.54%	2.684%
26	4.855	616	618	621	rBV3	125	162	0.02%	0.002%
27	5.056	638	651	670	rBV	136347	423042	39.22%	4.887%
28	5.288	688	689	694	rBV2	168	222	0.02%	0.003%
29	5.324	694	695	699	rVB2	121	150	0.01%	0.002%
30	5.379	702	704	705	rBV	419	292	0.03%	0.003%
31	5.617	742	743	746	rBV2	112	139	0.01%	0.002%
32	5.879	784	786	787	rBV2	131	117	0.01%	0.001%
33	5.970	789	801	807	rBV2	358252	1078660	100.00%	12.460%
34	6.263	847	849	850	rBV	317	147	0.01%	0.002%
35	6.379	865	868	871	rBV2	189	207	0.02%	0.002%
36	6.653	911	913	917	rBV2	107	136	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041026.D
 Acq On : 12 Apr 2024 13:40
 Operator : JC/MD
 Sample : P2048-03DL 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R47DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	6.763	921	931	954	rBV	250263	602633	55.87%	6.962%
38	7.110	984	988	989	rBV2	1103	1171	0.11%	0.014%
39	7.306	1011	1020	1034	rBV	208768	463657	42.98%	5.356%
40	7.488	1046	1050	1056	rVB5	609	1176	0.11%	0.014%
41	7.604	1067	1069	1071	rVV	171	124	0.01%	0.001%
42	7.976	1127	1130	1131	rVB2	161	142	0.01%	0.002%
43	7.988	1131	1132	1135	rVB	226	144	0.01%	0.002%
44	8.025	1137	1138	1141	rBV	149	117	0.01%	0.001%
45	8.153	1158	1159	1163	rVB	132	124	0.01%	0.001%
46	8.324	1180	1187	1201	rBV	139976	234916	21.78%	2.714%
47	8.647	1234	1240	1266	rBV	558637	884560	82.01%	10.218%
48	8.952	1284	1290	1302	rBV	99803	153822	14.26%	1.777%
49	9.122	1316	1318	1319	rBV2	181	136	0.01%	0.002%
50	9.159	1322	1324	1328	rVV2	156	168	0.02%	0.002%
51	9.275	1338	1343	1348	rBV2	1949	3057	0.28%	0.035%
52	9.384	1355	1361	1373	rBV	329385	496883	46.06%	5.740%
53	9.701	1410	1413	1419	rVB4	637	1097	0.10%	0.013%
54	9.787	1425	1427	1429	rVB	236	183	0.02%	0.002%
55	9.872	1440	1441	1443	rBV2	186	161	0.01%	0.002%
56	10.055	1465	1471	1473	rBV	551381	846243	78.45%	9.776%
57	10.311	1507	1513	1517	rBV2	735	1190	0.11%	0.014%
58	10.396	1525	1527	1531	rBV2	111	109	0.01%	0.001%
59	10.500	1542	1544	1546	rVB2	175	147	0.01%	0.002%
60	10.518	1546	1547	1549	rBV2	128	123	0.01%	0.001%
61	10.646	1565	1568	1574	rBV2	318	580	0.05%	0.007%
62	10.756	1585	1586	1589	rVB	168	111	0.01%	0.001%
63	10.793	1589	1592	1594	rBV	130	164	0.02%	0.002%
64	10.848	1599	1601	1605	rBV	106	131	0.01%	0.002%
65	10.963	1618	1620	1626	rBV3	503	668	0.06%	0.008%
66	11.024	1628	1630	1632	rBV	109	128	0.01%	0.001%
67	11.091	1638	1641	1645	rBV2	650	761	0.07%	0.009%
68	11.189	1652	1657	1669	rBV	427235	539297	50.00%	6.230%
69	11.317	1673	1678	1683	rVB2	4588	6806	0.63%	0.079%
70	11.384	1688	1689	1691	rBV	148	117	0.01%	0.001%
71	11.457	1698	1701	1706	rVB2	356	509	0.05%	0.006%
72	11.646	1731	1732	1735	rBV	193	172	0.02%	0.002%
73	11.713	1739	1743	1745	rBV2	642	638	0.06%	0.007%
74	11.756	1746	1750	1754	rVV3	443	646	0.06%	0.007%
75	11.829	1759	1762	1767	rVB2	130	196	0.02%	0.002%
76	11.872	1767	1769	1772	rBV	142	170	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041026.D
 Acq On : 12 Apr 2024 13:40
 Operator : JC/MD
 Sample : P2048-03DL 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R47DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041024WMA.M
 Title : VOC Analysis

77	11.969	1781	1785	1789	rBV	8929	11281	1.05%	0.130%
78	12.024	1789	1794	1804	rVB2	608790	962200	89.20%	11.115%
79	12.152	1814	1815	1822	rVB4	339	376	0.03%	0.004%
80	12.238	1827	1829	1832	rVB3	224	237	0.02%	0.003%
81	12.317	1837	1842	1859	rBV2	678966	963731	89.35%	11.133%
82	12.567	1881	1883	1884	rBV	158	112	0.01%	0.001%
83	12.762	1911	1915	1920	rVB	4507	5376	0.50%	0.062%
84	13.116	1970	1973	1978	rVB2	513	618	0.06%	0.007%
85	13.414	2020	2022	2024	rVB2	114	108	0.01%	0.001%
86	13.542	2042	2043	2047	rVB2	133	108	0.01%	0.001%
87	13.591	2047	2051	2063	rBV	3535	5126	0.48%	0.059%
88	13.682	2065	2066	2070	rBV2	250	271	0.03%	0.003%
89	13.731	2072	2074	2076	rBV	224	185	0.02%	0.002%
90	13.786	2080	2083	2086	rBV3	506	774	0.07%	0.009%
91	13.884	2096	2099	2102	rBV	216	208	0.02%	0.002%
92	13.932	2105	2107	2109	rBV2	158	167	0.02%	0.002%
93	13.969	2109	2113	2114	rBV2	527	466	0.04%	0.005%
94	14.036	2122	2124	2126	rVB2	262	245	0.02%	0.003%
95	14.073	2128	2130	2132	rVB2	210	129	0.01%	0.001%
96	14.134	2135	2140	2146	rVB	2726	3765	0.35%	0.043%
97	14.262	2160	2161	2164	rVB	246	180	0.02%	0.002%
98	14.457	2190	2193	2195	rBV	250	283	0.03%	0.003%
99	14.707	2233	2234	2236	rBV	219	113	0.01%	0.001%
100	15.389	2343	2346	2352	rVB4	801	1348	0.12%	0.016%




Sum of corrected areas: 8656652

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041026.D
Acq On : 12 Apr 2024 13:40
Operator : JC/MD
Sample : P2048-03DL 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R47DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

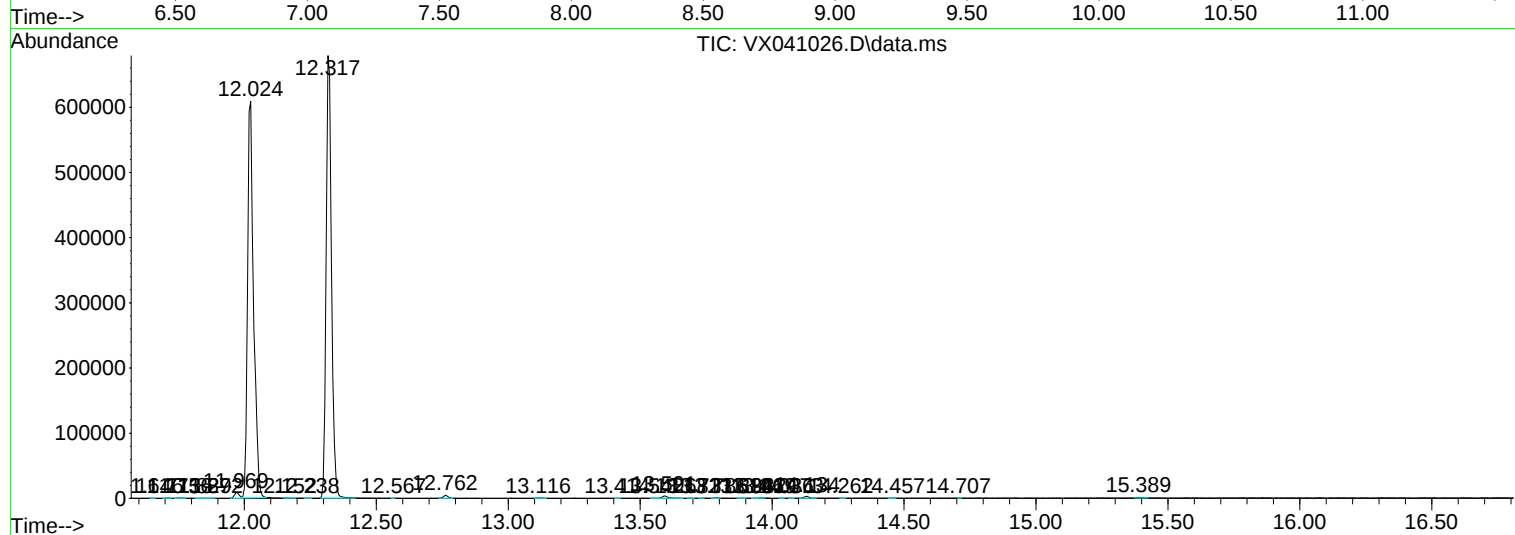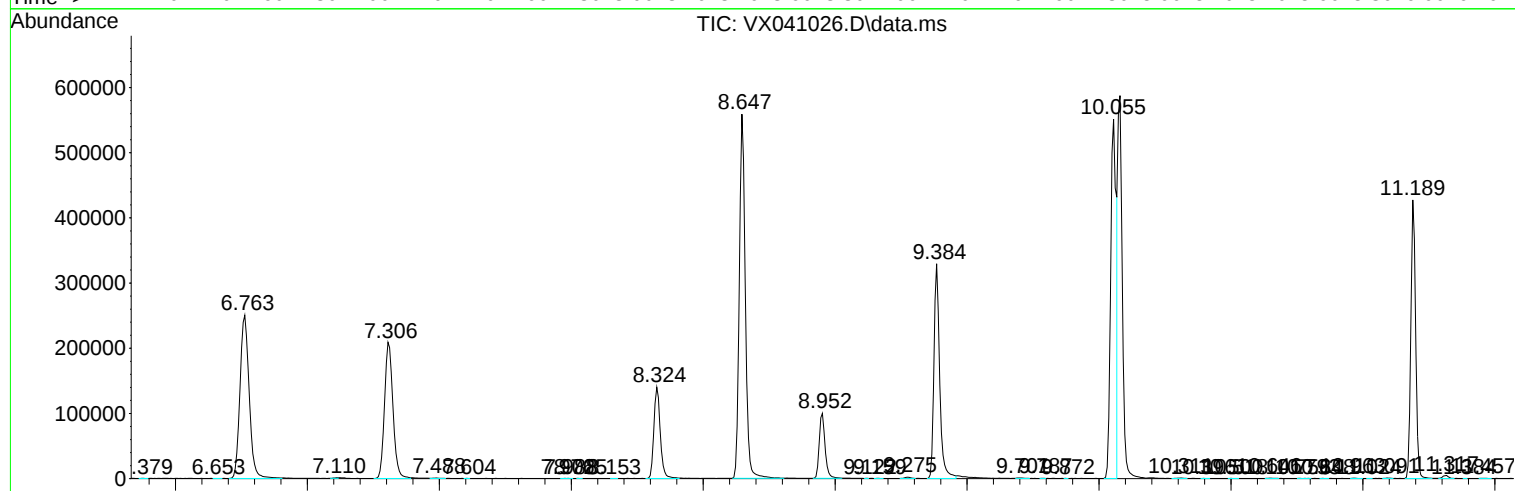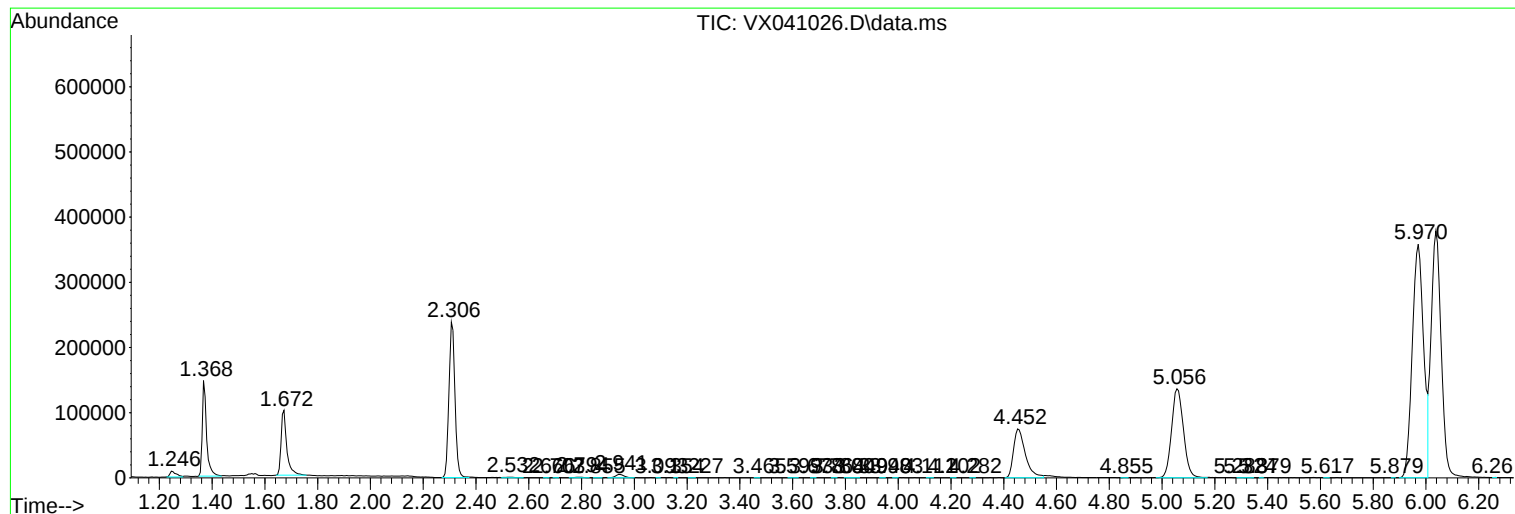

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041026.D
Acq On : 12 Apr 2024 13:40
Operator : JC/MD
Sample : P2048-03DL 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R47DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041026.D
Acq On : 12 Apr 2024 13:40
Operator : JC/MD
Sample : P2048-03DL 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R47DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------