

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041027.D
 Acq On : 12 Apr 2024 14:03
 Operator : JC/MD
 Sample : P2048-04DL 500X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R51DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX041027.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	23	27	35	rBV	7232	15424	0.51%	0.112%
2	1.367	43	46	58	rVB	142943	163191	5.35%	1.181%
3	1.672	91	96	112	rVB	98959	149792	4.91%	1.084%
4	2.306	194	200	211	rBV	236838	370096	12.13%	2.679%
5	2.459	222	225	228	rBV3	382	618	0.02%	0.004%
6	2.636	249	254	256	rBV3	193	289	0.01%	0.002%
7	2.709	264	266	270	rVB2	217	211	0.01%	0.002%
8	2.745	270	272	274	rBV	104	118	0.00%	0.001%
9	2.794	275	280	286	rVV3	971	1674	0.05%	0.012%
10	2.946	298	305	313	rVB	3978	9255	0.30%	0.067%
11	3.020	315	317	320	rVB	147	135	0.00%	0.001%
12	3.099	328	330	333	rBV2	280	389	0.01%	0.003%
13	3.148	336	338	342	rVB2	131	125	0.00%	0.001%
14	3.379	373	376	378	rVV2	143	132	0.00%	0.001%
15	3.605	411	413	418	rVB	170	222	0.01%	0.002%
16	3.696	425	428	430	rVB2	143	140	0.00%	0.001%
17	3.739	434	435	437	rBV	123	117	0.00%	0.001%
18	3.898	458	461	464	rBV2	100	159	0.01%	0.001%
19	3.983	473	475	476	rBV2	132	125	0.00%	0.001%
20	4.190	507	509	513	rVB2	168	146	0.00%	0.001%
21	4.227	513	515	516	rBV	202	115	0.00%	0.001%
22	4.452	544	552	580	rBV	72262	236424	7.75%	1.712%
23	4.672	587	588	590	rVB	399	208	0.01%	0.002%
24	4.879	618	622	623	rBV2	163	206	0.01%	0.001%
25	5.056	638	651	671	rBV	136118	422190	13.83%	3.056%
26	5.391	703	706	707	rBV2	259	307	0.01%	0.002%
27	5.544	729	731	732	rBV	358	299	0.01%	0.002%
28	5.739	761	763	767	rVB2	153	183	0.01%	0.001%
29	5.781	767	770	772	rBV	126	184	0.01%	0.001%
30	5.970	788	801	806	rBV2	356952	1059738	34.72%	7.672%
31	6.037	807	812	844	rVB	939318	2393052	78.41%	17.324%
32	6.537	892	894	897	rBV	230	290	0.01%	0.002%
33	6.580	899	901	904	rVB3	142	156	0.01%	0.001%
34	6.763	921	931	949	rBV	253081	615193	20.16%	4.454%
35	7.110	984	988	996	rVB7	1579	3793	0.12%	0.027%
36	7.171	996	998	1000	rVB	267	175	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041027.D
 Acq On : 12 Apr 2024 14:03
 Operator : JC/MD
 Sample : P2048-04DL 500X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R51DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	7.196	1000	1002	1004	rVB	370	218	0.01%	0.002%
38	7.305	1012	1020	1038	rBV	207022	461193	15.11%	3.339%
39	7.494	1048	1051	1055	rVB4	528	718	0.02%	0.005%
40	7.659	1074	1078	1079	rVB	181	189	0.01%	0.001%
41	7.781	1095	1098	1099	rBV2	121	125	0.00%	0.001%
42	8.177	1162	1163	1167	rVB2	135	134	0.00%	0.001%
43	8.324	1181	1187	1202	rBV	140019	231867	7.60%	1.679%
44	8.537	1216	1222	1225	rVB2	181	342	0.01%	0.002%
45	8.580	1225	1229	1232	rBV3	618	694	0.02%	0.005%
46	8.647	1234	1240	1264	rVV	560260	879612	28.82%	6.368%
47	8.952	1284	1290	1307	rBV	101446	153588	5.03%	1.112%
48	9.171	1325	1326	1331	rBV	213	345	0.01%	0.002%
49	9.275	1337	1343	1348	rBV4	1038	1596	0.05%	0.012%
50	9.384	1355	1361	1381	rBV	322447	497737	16.31%	3.603%
51	9.701	1409	1413	1418	rVV3	605	1049	0.03%	0.008%
52	9.781	1424	1426	1428	rBV	196	139	0.00%	0.001%
53	9.848	1436	1437	1440	rVB	320	190	0.01%	0.001%
54	9.878	1440	1442	1443	rBV2	168	127	0.00%	0.001%
55	10.006	1462	1463	1465	rBV	125	120	0.00%	0.001%
56	10.079	1465	1475	1493	rBV2	1686975	3052124	100.00%	22.095%
57	10.311	1507	1513	1519	rVB4	682	1315	0.04%	0.010%
58	10.494	1542	1543	1547	rVV	171	139	0.00%	0.001%
59	10.652	1565	1569	1572	rBV3	470	741	0.02%	0.005%
60	10.707	1576	1578	1579	rBV2	198	148	0.00%	0.001%
61	10.933	1613	1615	1617	rBV2	111	132	0.00%	0.001%
62	10.963	1618	1620	1624	rVB2	608	580	0.02%	0.004%
63	11.091	1637	1641	1646	rBV3	551	789	0.03%	0.006%
64	11.189	1652	1657	1669	rBV	412191	529892	17.36%	3.836%
65	11.317	1674	1678	1682	rVB2	2153	2976	0.10%	0.022%
66	11.421	1694	1695	1698	rBV	110	128	0.00%	0.001%
67	11.457	1698	1701	1705	rVV3	462	659	0.02%	0.005%
68	11.524	1710	1712	1713	rVB	231	138	0.00%	0.001%
69	11.536	1713	1714	1716	rBV	156	129	0.00%	0.001%
70	11.707	1740	1742	1745	rVB2	338	287	0.01%	0.002%
71	11.756	1747	1750	1754	rBV3	425	591	0.02%	0.004%
72	11.872	1766	1769	1770	rBV	231	225	0.01%	0.002%
73	11.969	1781	1785	1789	rBV	13481	18080	0.59%	0.131%
74	12.024	1789	1794	1810	rVB2	675051	1316538	43.14%	9.531%
75	12.323	1837	1843	1855	rBV2	713895	1184436	38.81%	8.575%
76	12.494	1869	1871	1875	rVV2	266	250	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041027.D
 Acq On : 12 Apr 2024 14:03
 Operator : JC/MD
 Sample : P2048-04DL 500X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R51DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	12.548	1878	1880	1882	rBV2	241	132	0.00%	0.001%
78	12.762	1911	1915	1921	rVB2	3422	4745	0.16%	0.034%
79	12.804	1921	1922	1924	rBV	196	147	0.00%	0.001%
80	12.963	1943	1948	1951	rBV3	134	271	0.01%	0.002%
81	13.109	1968	1972	1978	rBV3	1582	2353	0.08%	0.017%
82	13.317	2005	2006	2008	rBV2	177	120	0.00%	0.001%
83	13.408	2018	2021	2022	rBV2	126	122	0.00%	0.001%
84	13.475	2028	2032	2036	rVB3	222	367	0.01%	0.003%
85	13.591	2047	2051	2061	rVB2	6236	9021	0.30%	0.065%
86	13.664	2061	2063	2065	rBV2	119	131	0.00%	0.001%
87	13.786	2080	2083	2084	rBV2	371	432	0.01%	0.003%
88	13.835	2089	2091	2094	rBV2	210	284	0.01%	0.002%
89	13.938	2106	2108	2109	rBV2	171	120	0.00%	0.001%
90	13.963	2109	2112	2117	rVV3	963	1292	0.04%	0.009%
91	14.048	2124	2126	2128	rBV2	201	180	0.01%	0.001%
92	14.073	2128	2130	2133	rVV	122	129	0.00%	0.001%
93	14.127	2135	2139	2144	rVB	3479	4535	0.15%	0.033%
94	14.201	2149	2151	2154	rBV2	193	205	0.01%	0.001%
95	14.322	2169	2171	2174	rBV2	165	129	0.00%	0.001%
96	14.536	2204	2206	2209	rBV2	230	210	0.01%	0.002%
97	14.591	2213	2215	2217	rBV2	252	211	0.01%	0.002%
98	14.798	2245	2249	2251	rBV2	270	378	0.01%	0.003%
99	15.304	2330	2332	2333	rBV	431	201	0.01%	0.001%
100	15.389	2343	2346	2353	rVB4	1323	2475	0.08%	0.018%




Sum of corrected areas: 13813341

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041027.D
Acq On : 12 Apr 2024 14:03
Operator : JC/MD
Sample : P2048-04DL 500X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R51DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

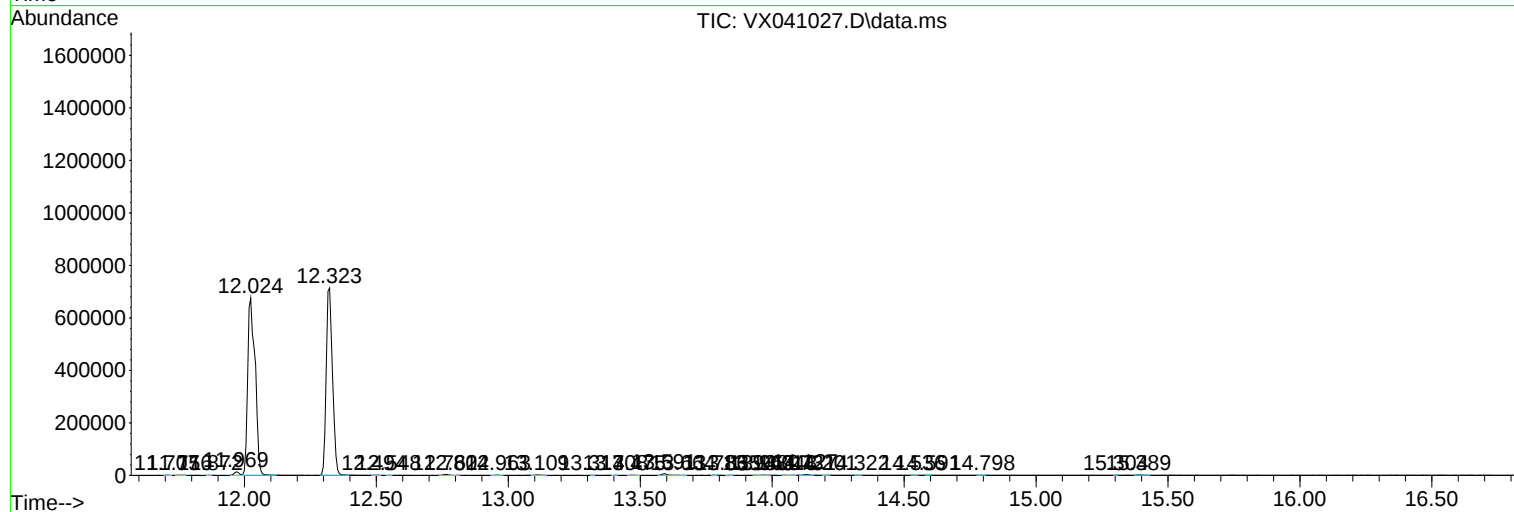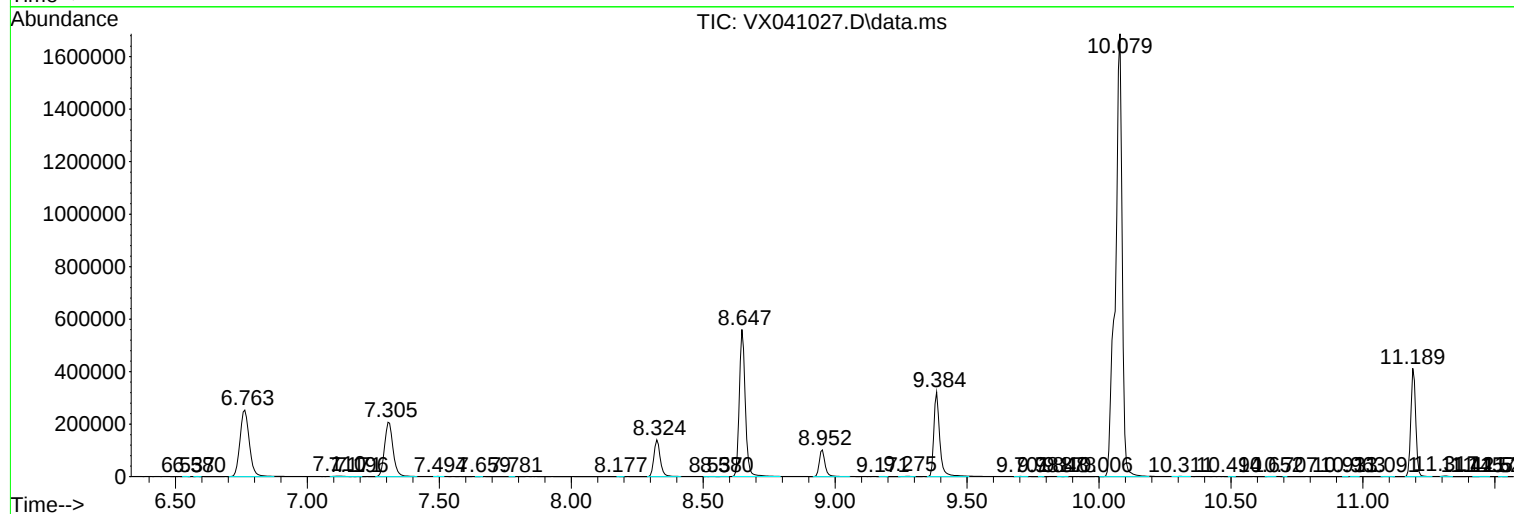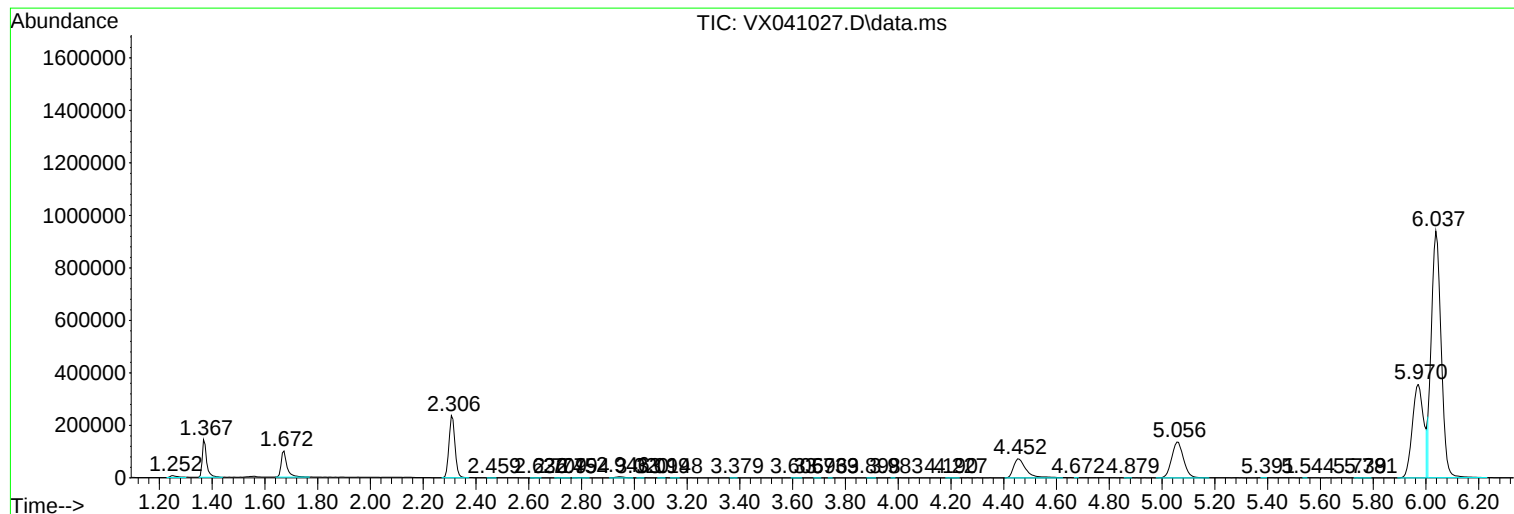

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041027.D
Acq On : 12 Apr 2024 14:03
Operator : JC/MD
Sample : P2048-04DL 500X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R51DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041027.D
Acq On : 12 Apr 2024 14:03
Operator : JC/MD
Sample : P2048-04DL 500X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R51DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------