

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041028.D
 Acq On : 12 Apr 2024 14:26
 Operator : JC/MD
 Sample : P2048-21
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX041028.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	23	27	35	rBV	5856	13230	1.18%	0.153%
2	1.368	43	46	59	rVB	154396	173952	15.48%	2.017%
3	1.672	91	96	111	rBV	102063	158177	14.08%	1.834%
4	2.306	194	200	218	rVB	255092	399360	35.54%	4.631%
5	2.465	222	226	230	rBV	568	855	0.08%	0.010%
6	2.703	262	265	272	rVB3	291	546	0.05%	0.006%
7	2.782	275	278	285	rVB4	884	1725	0.15%	0.020%
8	2.837	285	287	288	rBV2	184	138	0.01%	0.002%
9	2.947	297	305	315	rBV	4433	9749	0.87%	0.113%
10	3.032	318	319	322	rVB2	173	119	0.01%	0.001%
11	3.099	327	330	333	rBV3	325	609	0.05%	0.007%
12	3.282	359	360	364	rVB	145	129	0.01%	0.001%
13	3.587	407	410	411	rBV2	100	120	0.01%	0.001%
14	3.696	425	428	430	rBB2	138	138	0.01%	0.002%
15	3.727	430	433	437	rBV2	103	163	0.01%	0.002%
16	4.184	506	508	510	rBV	130	124	0.01%	0.001%
17	4.330	530	532	533	rBV	174	118	0.01%	0.001%
18	4.361	533	537	539	rVB2	157	233	0.02%	0.003%
19	4.452	544	552	568	rBV2	77097	239587	21.32%	2.778%
20	4.775	601	605	608	rBV3	224	342	0.03%	0.004%
21	4.824	612	613	617	rVB2	215	215	0.02%	0.002%
22	4.855	617	618	622	rBV2	205	207	0.02%	0.002%
23	5.056	638	651	669	rBV	145925	444336	39.54%	5.152%
24	5.275	685	687	690	rVB	301	248	0.02%	0.003%
25	5.324	693	695	698	rVB2	155	147	0.01%	0.002%
26	5.391	703	706	710	rVB2	336	571	0.05%	0.007%
27	5.489	720	722	723	rBV	138	117	0.01%	0.001%
28	5.556	727	733	735	rBV2	518	880	0.08%	0.010%
29	5.605	739	741	744	rBV	120	143	0.01%	0.002%
30	5.635	744	746	749	rVB2	177	184	0.02%	0.002%
31	5.678	749	753	759	rBV3	277	544	0.05%	0.006%
32	5.733	759	762	765	rVB2	145	151	0.01%	0.002%
33	5.970	789	801	828	rBV2	373347	1123794	100.00%	13.031%
34	6.324	855	859	860	rBV2	172	209	0.02%	0.002%
35	6.342	860	862	863	rBV2	121	123	0.01%	0.001%
36	6.415	872	874	875	rBV2	142	121	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041028.D
 Acq On : 12 Apr 2024 14:26
 Operator : JC/MD
 Sample : P2048-21
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	6.513	888	890	892	rBV	107	122	0.01%	0.001%
38	6.763	921	931	951	rBV	260716	636980	56.68%	7.386%
39	7.123	983	990	992	rBV6	1774	3737	0.33%	0.043%
40	7.306	1012	1020	1039	rBV	225157	489237	43.53%	5.673%
41	7.690	1081	1083	1085	rVV	202	174	0.02%	0.002%
42	7.830	1104	1106	1111	rVB2	252	323	0.03%	0.004%
43	7.879	1111	1114	1117	rVB2	139	122	0.01%	0.001%
44	7.952	1125	1126	1129	rBV2	154	207	0.02%	0.002%
45	8.061	1140	1144	1147	rBV2	147	162	0.01%	0.002%
46	8.208	1165	1168	1170	rBV2	115	176	0.02%	0.002%
47	8.324	1181	1187	1202	rBV	148951	246767	21.96%	2.861%
48	8.580	1226	1229	1233	rVB2	739	1005	0.09%	0.012%
49	8.647	1234	1240	1264	rVV	594084	936148	83.30%	10.855%
50	8.952	1284	1290	1306	rBV	104918	161605	14.38%	1.874%
51	9.116	1314	1317	1319	rBV3	152	197	0.02%	0.002%
52	9.238	1335	1337	1340	rBV2	145	201	0.02%	0.002%
53	9.275	1340	1343	1349	rVB3	1096	1471	0.13%	0.017%
54	9.330	1349	1352	1353	rBV2	186	181	0.02%	0.002%
55	9.384	1355	1361	1381	rBV	333570	518277	46.12%	6.010%
56	9.695	1410	1412	1416	rVB3	634	838	0.07%	0.010%
57	9.811	1428	1431	1434	rBV3	153	211	0.02%	0.002%
58	9.970	1456	1457	1462	rBV2	93	142	0.01%	0.002%
59	10.055	1465	1471	1490	rBV	551468	791969	70.47%	9.183%
60	10.305	1509	1512	1521	rVB4	805	1319	0.12%	0.015%
61	10.585	1554	1558	1559	rBV	172	148	0.01%	0.002%
62	10.652	1565	1569	1572	rBV4	432	829	0.07%	0.010%
63	10.970	1617	1621	1625	rVB2	459	703	0.06%	0.008%
64	11.098	1638	1642	1646	rVV3	550	664	0.06%	0.008%
65	11.189	1652	1657	1670	rVV	421309	546418	48.62%	6.336%
66	11.311	1673	1677	1685	rVB2	1933	2832	0.25%	0.033%
67	11.451	1696	1700	1705	rBV3	490	733	0.07%	0.008%
68	11.707	1740	1742	1745	rVV2	307	244	0.02%	0.003%
69	11.762	1747	1751	1753	rVV3	535	644	0.06%	0.007%
70	11.969	1782	1785	1788	rBV	872	1103	0.10%	0.013%
71	12.018	1788	1793	1812	rVV	614405	809295	72.01%	9.384%
72	12.317	1837	1842	1854	rBV	685726	879440	78.26%	10.197%
73	12.481	1867	1869	1872	rVB	180	141	0.01%	0.002%
74	12.646	1895	1896	1901	rBV2	189	257	0.02%	0.003%
75	12.762	1911	1915	1920	rBV2	3567	4957	0.44%	0.057%
76	12.853	1927	1930	1934	rVB2	189	267	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041028.D
 Acq On : 12 Apr 2024 14:26
 Operator : JC/MD
 Sample : P2048-21
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	12.902	1934	1938	1939	rBV2	187	204	0.02%	0.002%
78	12.926	1941	1942	1947	rVB2	170	120	0.01%	0.001%
79	12.963	1947	1948	1952	rVB2	211	182	0.02%	0.002%
80	13.115	1971	1973	1978	rVB2	612	689	0.06%	0.008%
81	13.176	1982	1983	1985	rBV	230	147	0.01%	0.002%
82	13.256	1993	1996	1999	rVB2	216	240	0.02%	0.003%
83	13.426	2021	2024	2025	rBV2	174	161	0.01%	0.002%
84	13.481	2030	2033	2034	rVB2	130	122	0.01%	0.001%
85	13.500	2034	2036	2038	rBV2	173	146	0.01%	0.002%
86	13.542	2042	2043	2046	rVV2	152	152	0.01%	0.002%
87	13.597	2046	2052	2057	rVV3	1058	1500	0.13%	0.017%
88	13.646	2058	2060	2063	rVV2	180	132	0.01%	0.002%
89	13.670	2063	2064	2069	rVB2	122	168	0.01%	0.002%
90	13.786	2078	2083	2086	rBV3	433	820	0.07%	0.010%
91	13.823	2088	2089	2091	rVB	229	174	0.02%	0.002%
92	13.963	2108	2112	2116	rVB2	628	830	0.07%	0.010%
93	14.042	2123	2125	2129	rVB2	213	232	0.02%	0.003%
94	14.079	2129	2131	2133	rBV3	215	230	0.02%	0.003%
95	14.134	2135	2140	2144	rVB	4111	4968	0.44%	0.058%
96	14.560	2208	2210	2212	rBV2	260	299	0.03%	0.003%
97	14.670	2226	2228	2231	rBV2	220	261	0.02%	0.003%
98	14.725	2233	2237	2238	rBV3	181	257	0.02%	0.003%
99	14.816	2250	2252	2254	rBV	250	287	0.03%	0.003%
100	16.511	2528	2530	2531	rBV2	367	187	0.02%	0.002%

Sum of corrected areas: 8624158




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041028.D
Acq On : 12 Apr 2024 14:26
Operator : JC/MD
Sample : P2048-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

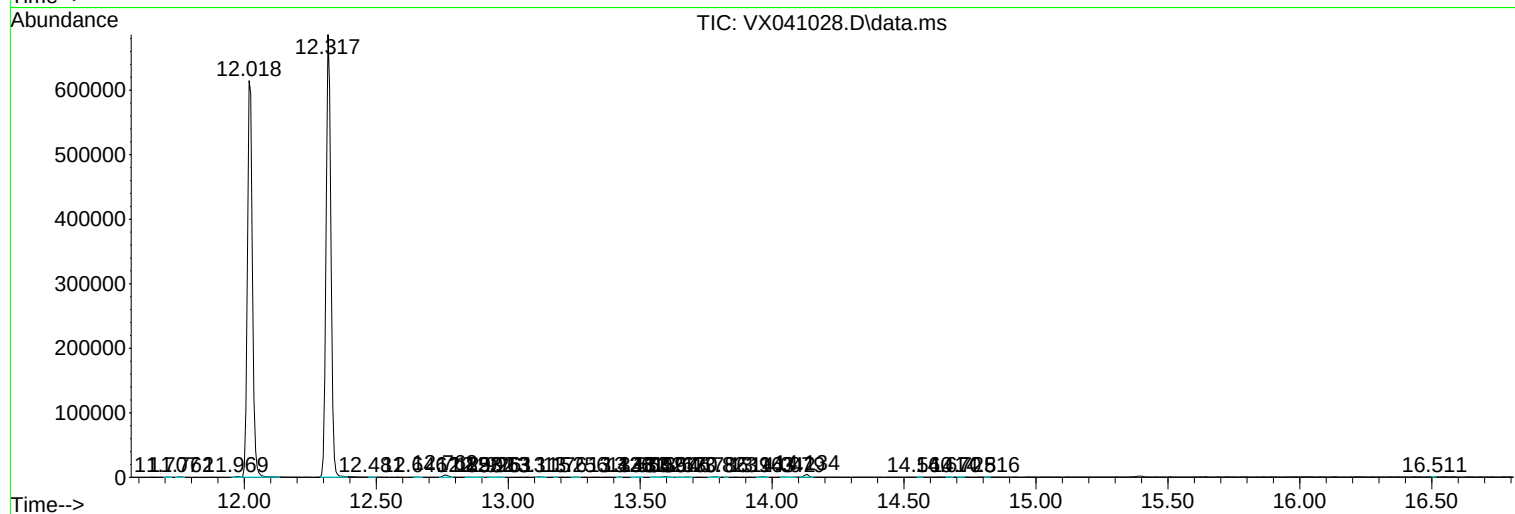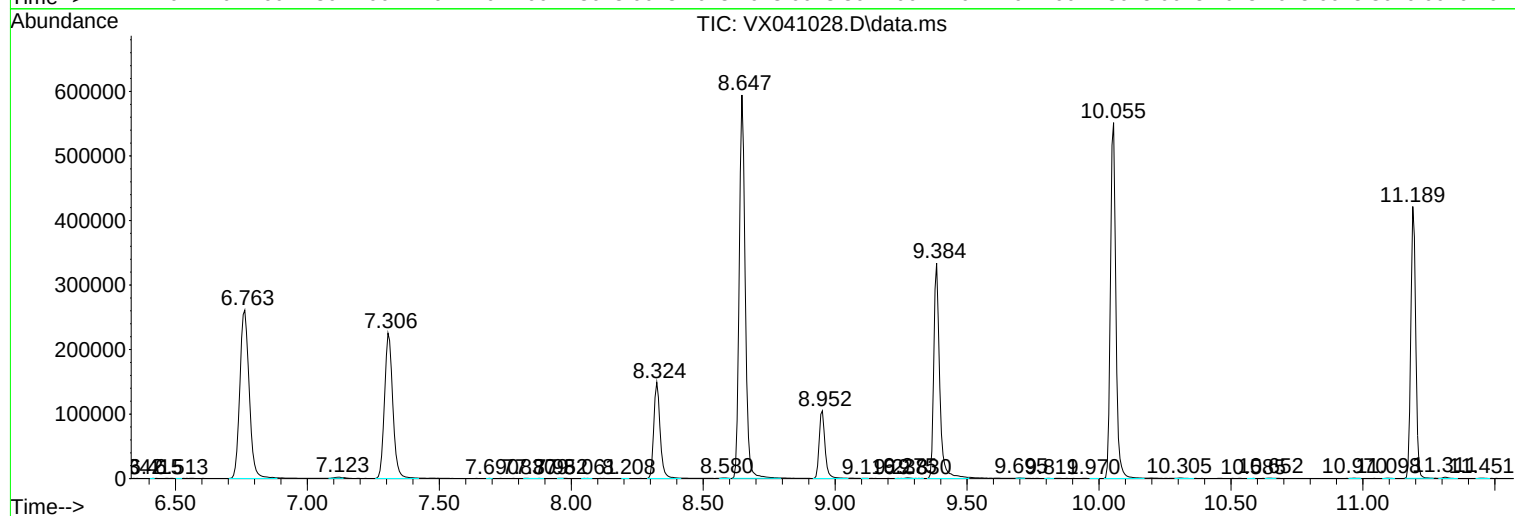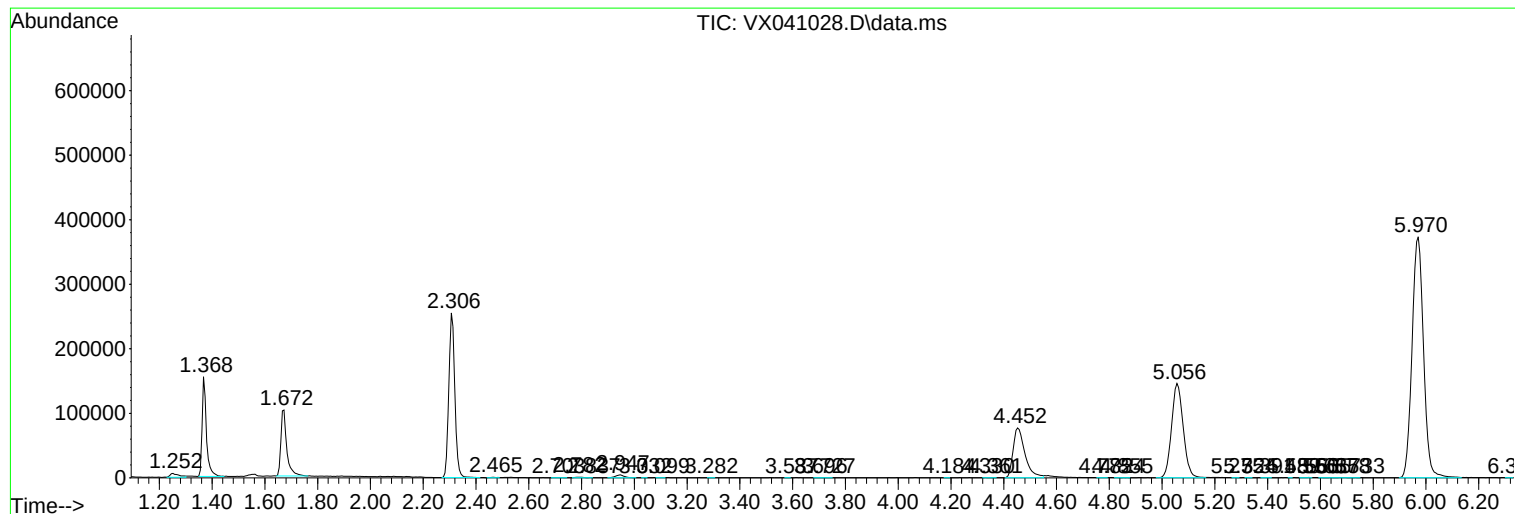

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041028.D
Acq On : 12 Apr 2024 14:26
Operator : JC/MD
Sample : P2048-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041028.D
Acq On : 12 Apr 2024 14:26
Operator : JC/MD
Sample : P2048-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------