

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041035.D
 Acq On : 12 Apr 2024 17:06
 Operator : JC/MD
 Sample : P2049-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CORH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX041035.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	32	rBV	8713	15308	1.43%	0.187%
2	1.368	43	46	61	rVB	146267	162859	15.22%	1.994%
3	1.673	91	96	111	rVB	97867	148280	13.86%	1.816%
4	2.307	194	200	210	rBV	240257	376817	35.22%	4.615%
5	2.483	222	229	230	rBV4	337	677	0.06%	0.008%
6	2.532	230	237	250	rVV	14921	29138	2.72%	0.357%
7	2.794	275	280	283	rBV4	730	1128	0.11%	0.014%
8	2.947	299	305	309	rBV2	1162	2407	0.23%	0.029%
9	3.075	325	326	329	rVV	128	123	0.01%	0.002%
10	3.099	329	330	334	rVV3	251	284	0.03%	0.003%
11	3.154	337	339	343	rVB2	119	135	0.01%	0.002%
12	3.197	343	346	348	rBV	162	139	0.01%	0.002%
13	3.441	384	386	387	rBV	160	131	0.01%	0.002%
14	3.599	411	412	414	rBV2	115	118	0.01%	0.001%
15	3.849	451	453	457	rVB2	144	125	0.01%	0.002%
16	3.940	464	468	471	rBV	119	166	0.02%	0.002%
17	4.075	488	490	492	rVB	193	134	0.01%	0.002%
18	4.142	499	501	502	rBV	167	130	0.01%	0.002%
19	4.239	515	517	520	rVV2	109	132	0.01%	0.002%
20	4.459	543	553	569	rBV	72306	224662	21.00%	2.751%
21	4.916	625	628	632	rVB2	162	185	0.02%	0.002%
22	5.056	638	651	668	rBV	138396	424561	39.69%	5.199%
23	5.239	679	681	683	rVB2	371	311	0.03%	0.004%
24	5.318	692	694	696	rVB2	215	182	0.02%	0.002%
25	5.349	696	699	700	rBV2	124	139	0.01%	0.002%
26	5.373	701	703	704	rBV2	364	265	0.02%	0.003%
27	5.556	728	733	737	rBV3	450	980	0.09%	0.012%
28	5.684	751	754	757	rBV2	301	343	0.03%	0.004%
29	5.806	772	774	777	rBV	107	164	0.02%	0.002%
30	5.971	788	801	830	rBV2	352932	1069746	100.00%	13.101%
31	6.288	852	853	856	rVB2	277	144	0.01%	0.002%
32	6.342	861	862	866	rVB	211	130	0.01%	0.002%
33	6.672	913	916	919	rBV2	140	224	0.02%	0.003%
34	6.763	921	931	951	rBV	241822	593126	55.45%	7.264%
35	7.226	1004	1007	1009	rBV2	210	253	0.02%	0.003%
36	7.306	1011	1020	1032	rBV	206231	462513	43.24%	5.664%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041035.D
 Acq On : 12 Apr 2024 17:06
 Operator : JC/MD
 Sample : P2049-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CORH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	7.842	1105	1108	1110	rBV	114	172	0.02%	0.002%
38	8.080	1145	1147	1151	rVB2	105	130	0.01%	0.002%
39	8.324	1181	1187	1205	rBV	139436	230613	21.56%	2.824%
40	8.580	1225	1229	1233	rBV2	308	511	0.05%	0.006%
41	8.647	1234	1240	1260	rVV	564173	886647	82.88%	10.858%
42	8.952	1284	1290	1305	rBV	97604	150652	14.08%	1.845%
43	9.177	1324	1327	1328	rBV	210	219	0.02%	0.003%
44	9.208	1330	1332	1337	rBV2	147	278	0.03%	0.003%
45	9.275	1337	1343	1348	rBV	16116	25415	2.38%	0.311%
46	9.385	1356	1361	1383	rBV	314906	483358	45.18%	5.919%
47	9.738	1417	1419	1420	rBV	175	156	0.01%	0.002%
48	9.854	1436	1438	1441	rBV2	146	174	0.02%	0.002%
49	9.921	1445	1449	1453	rVV	132	155	0.01%	0.002%
50	10.055	1465	1471	1490	rBV	501769	722799	67.57%	8.852%
51	10.311	1510	1513	1516	rBV3	486	708	0.07%	0.009%
52	10.360	1520	1521	1523	rBV2	132	126	0.01%	0.002%
53	10.610	1559	1562	1565	rBV	138	183	0.02%	0.002%
54	10.653	1565	1569	1572	rBV2	432	588	0.05%	0.007%
55	10.738	1581	1583	1584	rBV2	132	124	0.01%	0.002%
56	10.897	1608	1609	1612	rBV2	189	186	0.02%	0.002%
57	10.927	1612	1614	1616	rVV	240	173	0.02%	0.002%
58	10.964	1616	1620	1625	rVV2	375	708	0.07%	0.009%
59	11.018	1628	1629	1632	rBV2	125	139	0.01%	0.002%
60	11.049	1632	1634	1635	rVV2	144	122	0.01%	0.001%
61	11.092	1639	1641	1647	rVB2	540	692	0.06%	0.008%
62	11.146	1647	1650	1652	rBV	112	116	0.01%	0.001%
63	11.189	1652	1657	1669	rVV	396925	516181	48.25%	6.321%
64	11.311	1672	1677	1684	rVB	28802	40230	3.76%	0.493%
65	11.396	1689	1691	1693	rVV	113	117	0.01%	0.001%
66	11.451	1698	1700	1705	rVV3	540	627	0.06%	0.008%
67	11.494	1705	1707	1710	rVV2	214	185	0.02%	0.002%
68	11.604	1723	1725	1726	rVV	163	119	0.01%	0.001%
69	11.707	1741	1742	1746	rVB2	342	304	0.03%	0.004%
70	11.750	1746	1749	1755	rBV4	496	779	0.07%	0.010%
71	11.805	1755	1758	1761	rBV2	124	149	0.01%	0.002%
72	11.841	1763	1764	1767	rVB2	177	121	0.01%	0.001%
73	11.976	1782	1786	1788	rBV2	1035	1210	0.11%	0.015%
74	12.018	1788	1793	1806	rBV	570295	739783	69.16%	9.060%
75	12.226	1823	1827	1834	rBV5	1421	2843	0.27%	0.035%
76	12.317	1837	1842	1859	rVB	657967	820369	76.69%	10.047%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041035.D
 Acq On : 12 Apr 2024 17:06
 Operator : JC/MD
 Sample : P2049-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0RH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	12.506	1871	1873	1875	rVB	270	195	0.02%	0.002%
78	12.573	1883	1884	1886	rBV2	163	118	0.01%	0.001%
79	12.591	1886	1887	1889	rVV	210	123	0.01%	0.002%
80	12.695	1902	1904	1905	rBV2	186	125	0.01%	0.002%
81	12.762	1911	1915	1922	rVB2	6609	8539	0.80%	0.105%
82	12.884	1933	1935	1936	rBV	207	156	0.01%	0.002%
83	13.055	1961	1963	1965	rBV2	145	124	0.01%	0.002%
84	13.116	1970	1973	1979	rBV3	461	642	0.06%	0.008%
85	13.323	2006	2007	2010	rVB	239	166	0.02%	0.002%
86	13.500	2034	2036	2039	rVB2	154	159	0.01%	0.002%
87	13.548	2041	2044	2047	rVV2	138	187	0.02%	0.002%
88	13.591	2047	2051	2060	rVB3	2958	4498	0.42%	0.055%
89	13.725	2071	2073	2076	rVB2	200	157	0.01%	0.002%
90	13.762	2076	2079	2080	rBV2	154	155	0.01%	0.002%
91	13.786	2080	2083	2087	rVV2	403	477	0.04%	0.006%
92	13.908	2101	2103	2106	rBV2	245	294	0.03%	0.004%
93	13.939	2106	2108	2109	rVV	178	118	0.01%	0.001%
94	13.963	2109	2112	2117	rVB3	831	1121	0.10%	0.014%
95	14.091	2130	2133	2135	rBV3	141	171	0.02%	0.002%
96	14.128	2135	2139	2146	rVB	1441	2038	0.19%	0.025%
97	14.201	2146	2151	2154	rBV2	301	432	0.04%	0.005%
98	14.280	2162	2164	2166	rBV2	234	295	0.03%	0.004%
99	14.341	2173	2174	2176	rBV	266	215	0.02%	0.003%
100	15.390	2344	2346	2353	rVB4	758	803	0.08%	0.010%




Sum of corrected areas: 8165628

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041035.D
Acq On : 12 Apr 2024 17:06
Operator : JC/MD
Sample : P2049-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CORH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

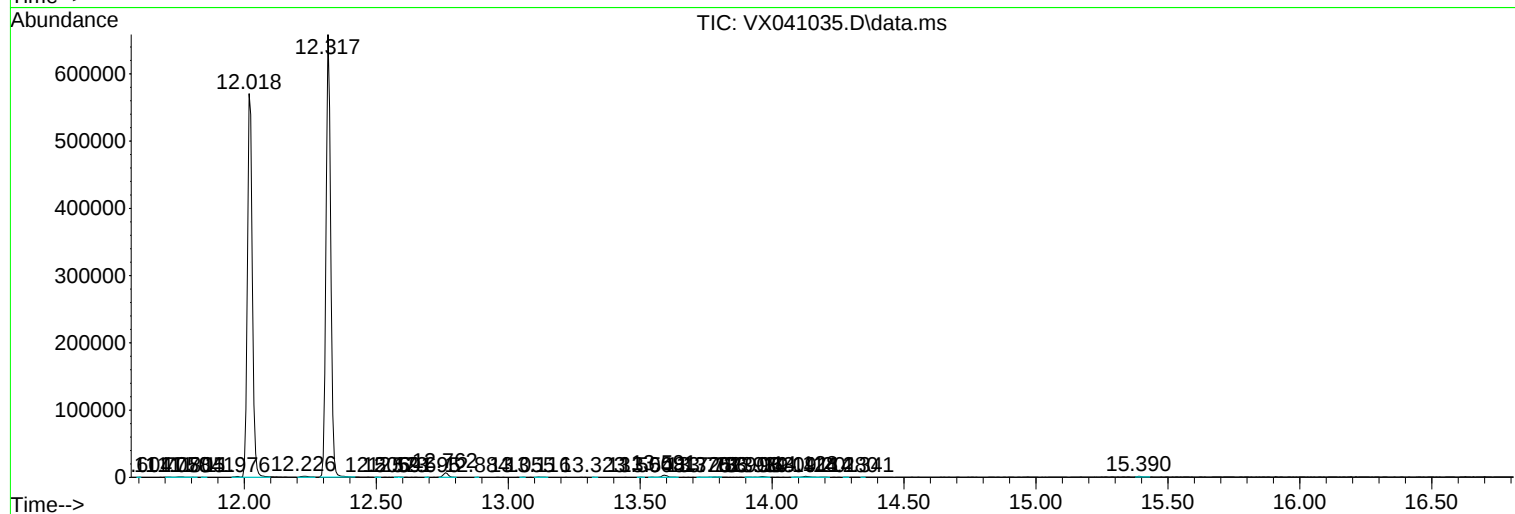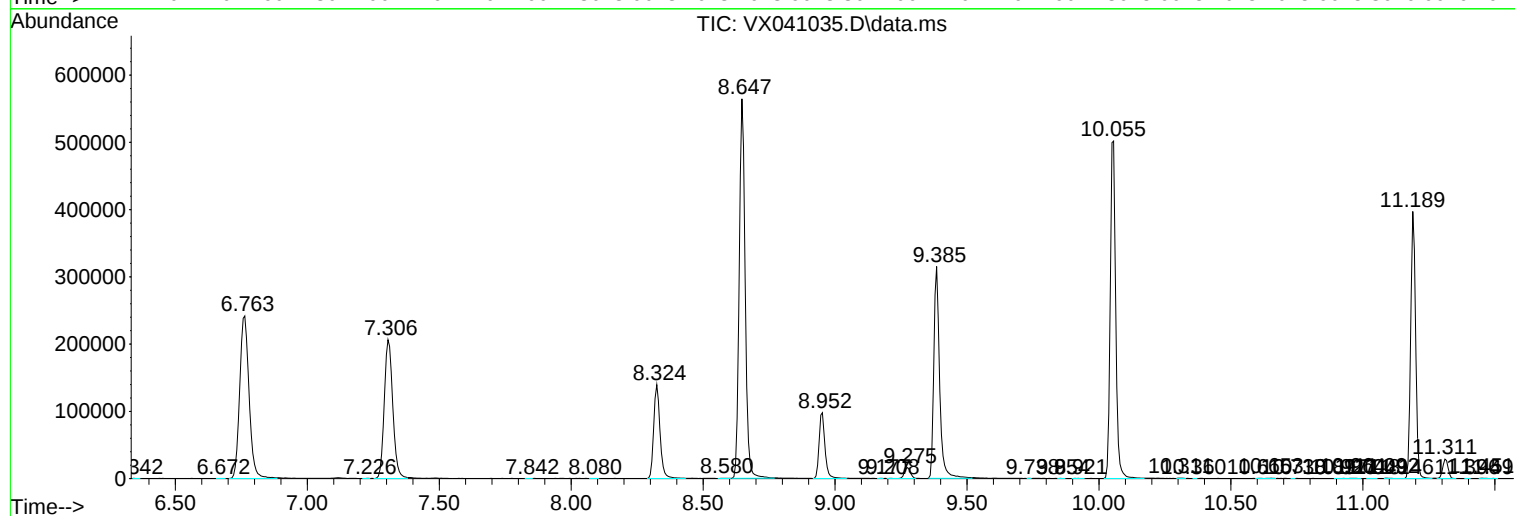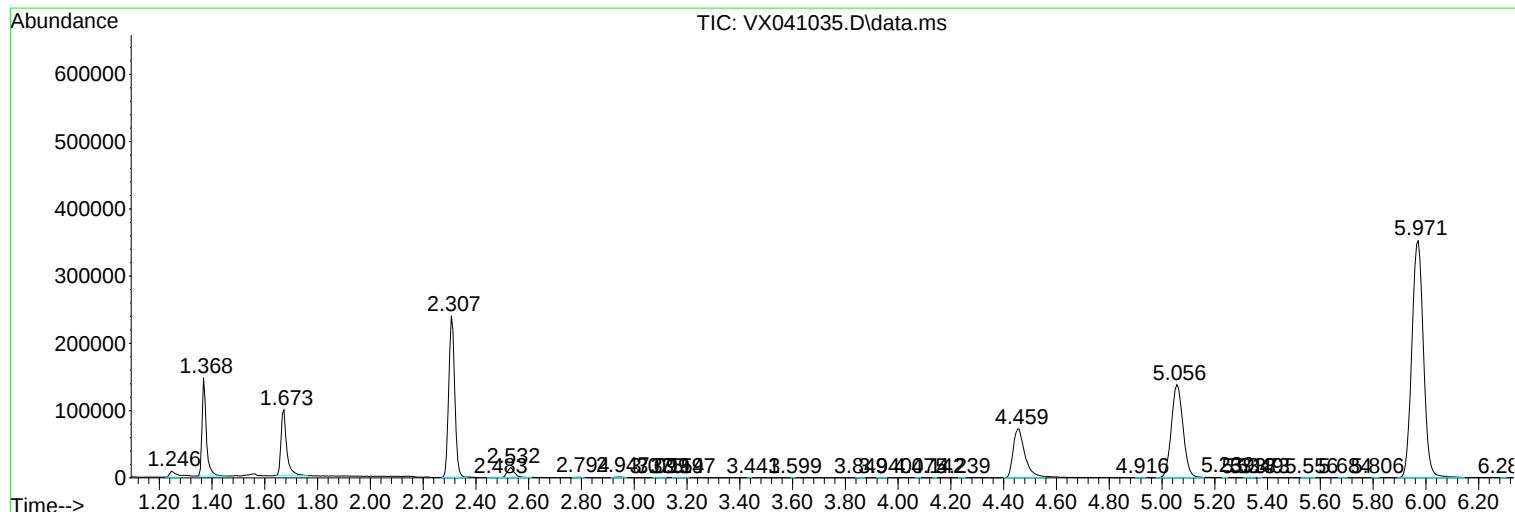

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041035.D
Acq On : 12 Apr 2024 17:06
Operator : JC/MD
Sample : P2049-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0RH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041035.D
Acq On : 12 Apr 2024 17:06
Operator : JC/MD
Sample : P2049-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0RH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc