

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041039.D
 Acq On : 12 Apr 2024 18:38
 Operator : JC/MD
 Sample : P2049-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CORJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M

Title : VOC Analysis

Signal : TIC: VX041039.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	23	27	33	rBV	6300	12229	1.19%	0.156%
2	1.368	43	46	57	rBV	134135	152296	14.85%	1.946%
3	1.666	91	95	114	rBV	92060	146857	14.32%	1.876%
4	2.306	194	200	209	rBV	225544	345703	33.70%	4.417%
5	2.471	225	227	230	rBV	273	320	0.03%	0.004%
6	2.532	232	237	246	rVV	4575	8614	0.84%	0.110%
7	2.617	249	251	253	rVB2	282	224	0.02%	0.003%
8	2.642	253	255	258	rVB2	239	267	0.03%	0.003%
9	2.672	258	260	263	rBV2	256	304	0.03%	0.004%
10	2.794	273	280	287	rBV4	1049	2028	0.20%	0.026%
11	2.947	297	305	314	rVV	8145	18325	1.79%	0.234%
12	3.105	328	331	332	rVV	124	138	0.01%	0.002%
13	3.117	332	333	335	rVV	250	154	0.02%	0.002%
14	3.203	345	347	350	rBV2	109	146	0.01%	0.002%
15	3.428	381	384	389	rBV2	165	279	0.03%	0.004%
16	3.556	402	405	407	rBV2	150	185	0.02%	0.002%
17	3.885	457	459	461	rBV	200	129	0.01%	0.002%
18	3.952	466	470	472	rBV2	185	226	0.02%	0.003%
19	4.312	528	529	533	rBV2	144	185	0.02%	0.002%
20	4.458	543	553	567	rBV	74113	231072	22.53%	2.952%
21	4.775	603	605	606	rBV2	232	191	0.02%	0.002%
22	4.873	619	621	626	rVB4	215	267	0.03%	0.003%
23	5.056	638	651	666	rBV	133153	410263	39.99%	5.242%
24	5.214	675	677	678	rBV	343	247	0.02%	0.003%
25	5.263	683	685	688	rVB3	294	251	0.02%	0.003%
26	5.294	688	690	692	rBV	250	129	0.01%	0.002%
27	5.318	692	694	697	rVB2	148	141	0.01%	0.002%
28	5.385	702	705	706	rBV	310	296	0.03%	0.004%
29	5.556	726	733	737	rBV3	505	1180	0.12%	0.015%
30	5.684	750	754	755	rVB2	126	126	0.01%	0.002%
31	5.775	768	769	772	rBV2	188	146	0.01%	0.002%
32	5.970	787	801	816	rBV2	342430	1025833	100.00%	13.107%
33	6.178	833	835	838	rVB2	384	393	0.04%	0.005%
34	6.354	862	864	866	rVB	213	133	0.01%	0.002%
35	6.647	910	912	915	rVB	214	165	0.02%	0.002%
36	6.696	915	920	922	rBV2	131	236	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041039.D
 Acq On : 12 Apr 2024 18:38
 Operator : JC/MD
 Sample : P2049-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CORJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	6.763	922	931	952	rBV	231556	555920	54.19%	7.103%
38	7.123	984	990	996	rVB4	1040	2329	0.23%	0.030%
39	7.306	1012	1020	1035	rBV	204952	453121	44.17%	5.790%
40	7.482	1044	1049	1050	rBV2	467	626	0.06%	0.008%
41	7.952	1120	1126	1128	rBV2	126	196	0.02%	0.003%
42	7.970	1128	1129	1132	rVB2	248	183	0.02%	0.002%
43	8.007	1132	1135	1137	rVB	159	169	0.02%	0.002%
44	8.025	1137	1138	1141	rBV	140	148	0.01%	0.002%
45	8.104	1149	1151	1153	rBV2	102	126	0.01%	0.002%
46	8.324	1181	1187	1205	rBV	135177	224737	21.91%	2.872%
47	8.507	1215	1217	1218	rBV	235	165	0.02%	0.002%
48	8.580	1225	1229	1234	rBV4	593	902	0.09%	0.012%
49	8.647	1234	1240	1262	rVV	520930	833408	81.24%	10.649%
50	8.915	1283	1284	1285	rBV	212	131	0.01%	0.002%
51	8.952	1285	1290	1305	rVV	95403	148052	14.43%	1.892%
52	9.153	1319	1323	1327	rBV2	200	281	0.03%	0.004%
53	9.275	1337	1343	1349	rBV3	3937	6153	0.60%	0.079%
54	9.384	1355	1361	1388	rBV	331988	503221	49.05%	6.430%
55	9.647	1402	1404	1406	rVB	286	148	0.01%	0.002%
56	9.793	1426	1428	1429	rVB	228	136	0.01%	0.002%
57	9.848	1436	1437	1442	rBV	251	326	0.03%	0.004%
58	9.884	1442	1443	1447	rVV2	205	155	0.02%	0.002%
59	10.055	1465	1471	1492	rBV	473842	681889	66.47%	8.713%
60	10.195	1492	1494	1500	rVB3	605	898	0.09%	0.011%
61	10.311	1510	1513	1516	rBV	471	575	0.06%	0.007%
62	10.366	1520	1522	1526	rVB	190	205	0.02%	0.003%
63	10.445	1534	1535	1538	rBV2	118	138	0.01%	0.002%
64	10.646	1566	1568	1570	rVV2	208	188	0.02%	0.002%
65	10.762	1586	1587	1590	rBV	167	141	0.01%	0.002%
66	10.969	1617	1621	1625	rBV3	408	601	0.06%	0.008%
67	11.098	1638	1642	1645	rBV2	493	649	0.06%	0.008%
68	11.189	1652	1657	1671	rVV	407252	521694	50.86%	6.666%
69	11.311	1673	1677	1682	rVB	4578	6290	0.61%	0.080%
70	11.366	1682	1686	1689	rVB2	125	173	0.02%	0.002%
71	11.463	1696	1702	1705	rBV3	375	638	0.06%	0.008%
72	11.579	1719	1721	1725	rBV2	141	203	0.02%	0.003%
73	11.713	1739	1743	1745	rVV3	314	380	0.04%	0.005%
74	11.756	1747	1750	1754	rBV4	394	543	0.05%	0.007%
75	11.969	1781	1785	1788	rBV2	2070	2361	0.23%	0.030%
76	12.018	1788	1793	1805	rVV	526859	696124	67.86%	8.895%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041039.D
 Acq On : 12 Apr 2024 18:38
 Operator : JC/MD
 Sample : P2049-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CORJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	12.317	1837	1842	1853	rBV	626783	799302	77.92%	10.213%
78	12.616	1889	1891	1895	rBV	131	135	0.01%	0.002%
79	12.762	1911	1915	1919	rVV3	702	1137	0.11%	0.015%
80	12.853	1928	1930	1932	rBV2	198	159	0.02%	0.002%
81	13.213	1988	1989	1993	rBV2	168	196	0.02%	0.003%
82	13.359	2011	2013	2015	rVB2	198	132	0.01%	0.002%
83	13.414	2018	2022	2024	rBV2	219	299	0.03%	0.004%
84	13.524	2038	2040	2042	rBV	151	128	0.01%	0.002%
85	13.591	2047	2051	2058	rVV2	4980	7208	0.70%	0.092%
86	13.762	2076	2079	2080	rVV	168	150	0.01%	0.002%
87	13.792	2080	2084	2087	rVB3	353	506	0.05%	0.006%
88	13.835	2089	2091	2092	rBV	225	128	0.01%	0.002%
89	13.963	2108	2112	2119	rVB2	1880	2727	0.27%	0.035%
90	14.048	2124	2126	2128	rBV2	192	219	0.02%	0.003%
91	14.127	2135	2139	2144	rBV	3962	5568	0.54%	0.071%
92	14.274	2160	2163	2164	rBV3	220	253	0.02%	0.003%
93	14.304	2166	2168	2169	rVV	259	148	0.01%	0.002%
94	14.341	2173	2174	2175	rBV	244	138	0.01%	0.002%
95	14.524	2202	2204	2205	rBV2	273	193	0.02%	0.002%
96	14.859	2257	2259	2262	rBV2	256	309	0.03%	0.004%
97	15.389	2344	2346	2352	rVB3	2045	2750	0.27%	0.035%
98	15.609	2380	2382	2383	rBV	330	217	0.02%	0.003%
99	16.237	2484	2485	2487	rBV	375	192	0.02%	0.002%
100	16.712	2561	2563	2564	rBV	356	145	0.01%	0.002%




Sum of corrected areas: 7826340

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041039.D
Acq On : 12 Apr 2024 18:38
Operator : JC/MD
Sample : P2049-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CORJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

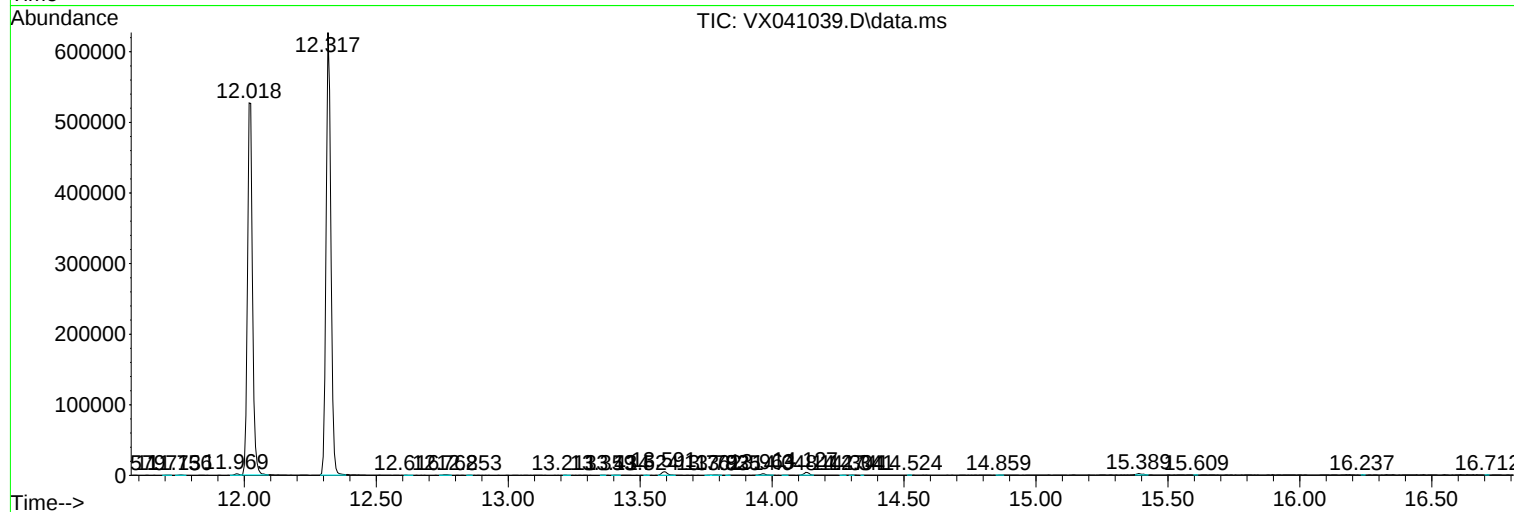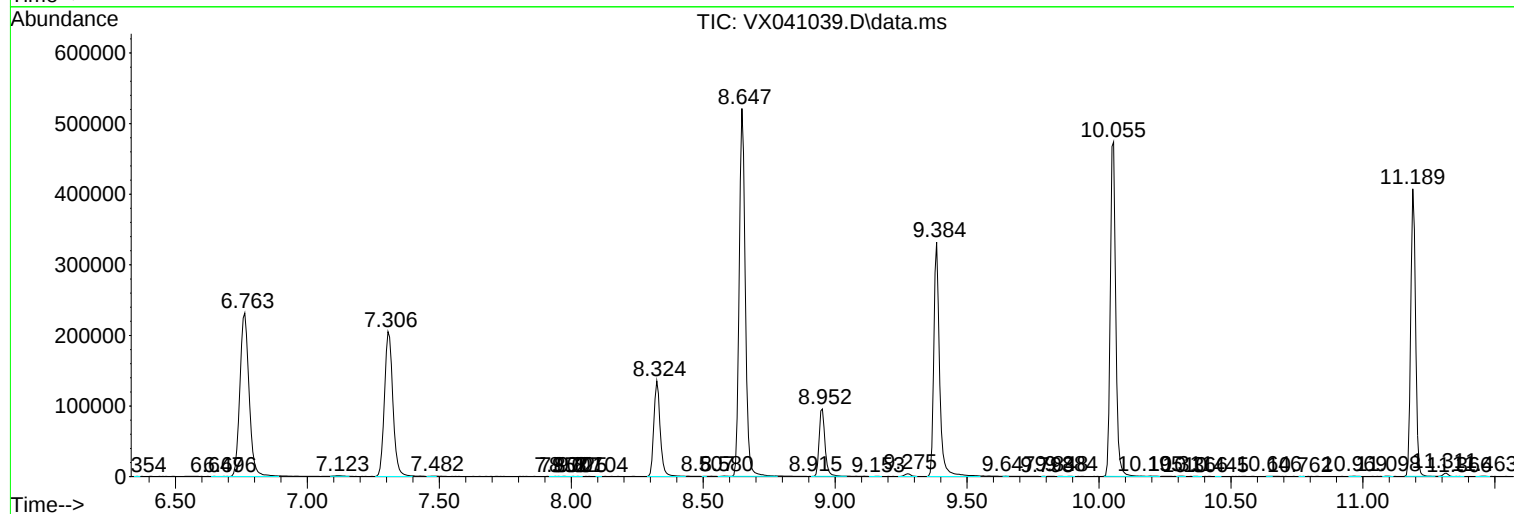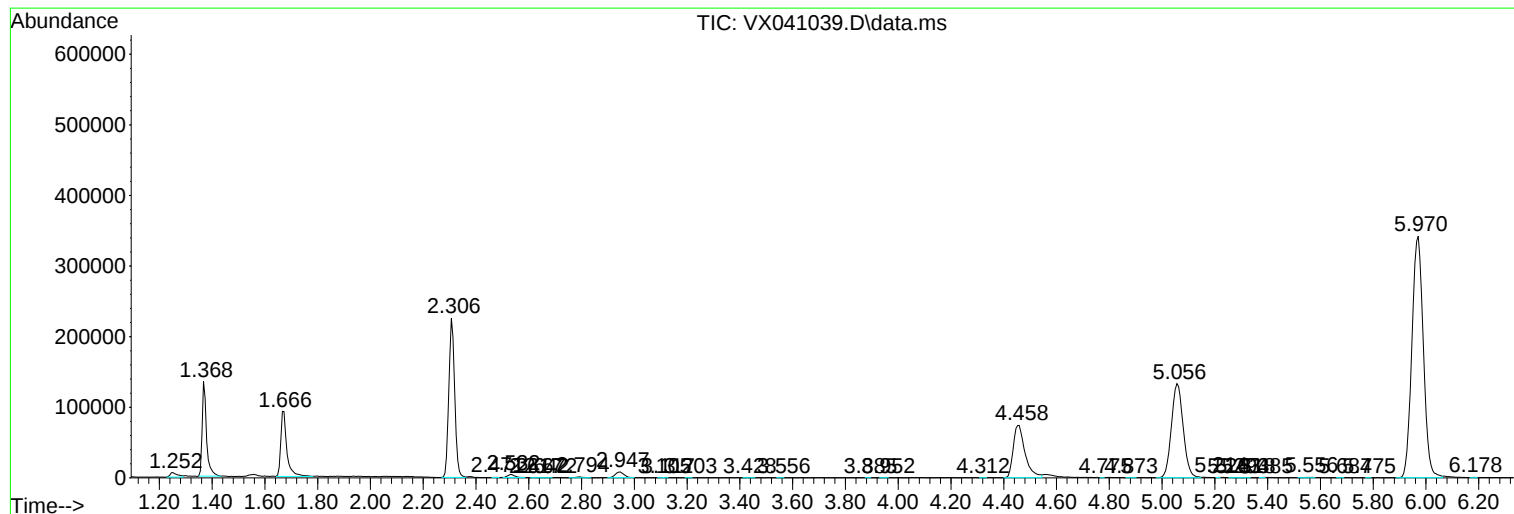

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041039.D
Acq On : 12 Apr 2024 18:38
Operator : JC/MD
Sample : P2049-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0RJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041039.D
Acq On : 12 Apr 2024 18:38
Operator : JC/MD
Sample : P2049-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0RJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------