

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041043.D
 Acq On : 12 Apr 2024 20:10
 Operator : JC/MD
 Sample : VX0412WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK670

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX041043.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.251	23	27	32	rBV	5162	9953	0.93%	0.122%
2	1.367	43	46	63	rVB	145804	167235	15.55%	2.042%
3	1.672	91	96	112	rBV	100354	154725	14.38%	1.889%
4	2.306	194	200	210	rBV	236563	371803	34.56%	4.540%
5	2.513	230	234	241	rVB3	2204	3938	0.37%	0.048%
6	2.654	254	257	258	rBV	106	106	0.01%	0.001%
7	2.788	275	279	286	rVB3	1351	2621	0.24%	0.032%
8	2.904	296	298	299	rBV	157	114	0.01%	0.001%
9	2.946	299	305	314	rVB2	2141	4945	0.46%	0.060%
10	3.093	325	329	330	rBV3	1394	1491	0.14%	0.018%
11	3.312	364	365	367	rBV	144	108	0.01%	0.001%
12	3.379	374	376	380	rBV2	158	212	0.02%	0.003%
13	3.428	383	384	388	rVB2	191	134	0.01%	0.002%
14	3.489	391	394	395	rBV	146	145	0.01%	0.002%
15	3.617	409	415	417	rBV4	347	616	0.06%	0.008%
16	3.702	427	429	430	rVB	183	116	0.01%	0.001%
17	3.714	430	431	433	rBV	242	182	0.02%	0.002%
18	3.800	443	445	449	rVB2	307	273	0.03%	0.003%
19	3.867	454	456	459	rVB	189	157	0.01%	0.002%
20	3.964	468	472	473	rBV2	166	181	0.02%	0.002%
21	4.452	544	552	578	rBV	76601	245124	22.79%	2.993%
22	4.964	635	636	638	rBV	226	135	0.01%	0.002%
23	5.062	639	652	667	rBV	137502	426945	39.69%	5.213%
24	5.306	691	692	697	rVB2	238	228	0.02%	0.003%
25	5.354	699	700	701	rBV	227	109	0.01%	0.001%
26	5.391	701	706	714	rVB4	936	1994	0.19%	0.024%
27	5.470	714	719	727	rVB5	652	1579	0.15%	0.019%
28	5.556	727	733	734	rBV	743	1238	0.12%	0.015%
29	5.677	751	753	759	rVB3	453	673	0.06%	0.008%
30	5.781	768	770	771	rBV2	149	148	0.01%	0.002%
31	5.970	788	801	834	rBV2	358732	1075708	100.00%	13.135%
32	6.342	858	862	863	rBV	205	237	0.02%	0.003%
33	6.409	870	873	874	rBV2	134	119	0.01%	0.001%
34	6.427	874	876	878	rVV2	208	200	0.02%	0.002%
35	6.464	880	882	884	rBV2	229	194	0.02%	0.002%
36	6.763	921	931	954	rBV	242989	597074	55.51%	7.290%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041043.D
 Acq On : 12 Apr 2024 20:10
 Operator : JC/MD
 Sample : VX0412WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK670

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	7.122	983	990	999	rVB6	2727	7580	0.70%	0.093%
38	7.208	1003	1004	1008	rBV	193	220	0.02%	0.003%
39	7.305	1011	1020	1038	rBV	211146	471969	43.88%	5.763%
40	7.671	1078	1080	1082	rBV2	139	111	0.01%	0.001%
41	7.830	1102	1106	1111	rVB3	399	678	0.06%	0.008%
42	7.921	1119	1121	1122	rBV	207	110	0.01%	0.001%
43	7.951	1122	1126	1129	rVV2	128	190	0.02%	0.002%
44	8.037	1136	1140	1142	rBV2	221	216	0.02%	0.003%
45	8.086	1145	1148	1150	rBV2	153	133	0.01%	0.002%
46	8.104	1150	1151	1155	rVV	150	111	0.01%	0.001%
47	8.323	1181	1187	1206	rBV	137748	233354	21.69%	2.849%
48	8.585	1224	1230	1234	rBV3	1150	1936	0.18%	0.024%
49	8.646	1234	1240	1250	rBV	536588	854429	79.43%	10.433%
50	8.951	1284	1290	1304	rBV	100753	155217	14.43%	1.895%
51	9.159	1320	1324	1329	rVB4	640	1103	0.10%	0.013%
52	9.213	1329	1333	1334	rBV	199	125	0.01%	0.002%
53	9.244	1337	1338	1339	rBV	249	147	0.01%	0.002%
54	9.274	1339	1343	1348	rVB3	2952	4224	0.39%	0.052%
55	9.384	1356	1361	1381	rBV	338795	513128	47.70%	6.265%
56	9.604	1394	1397	1399	rBV3	519	701	0.07%	0.009%
57	9.658	1404	1406	1409	rVB2	342	240	0.02%	0.003%
58	9.701	1409	1413	1417	rBV3	601	929	0.09%	0.011%
59	10.055	1465	1471	1489	rBV	502296	717660	66.72%	8.763%
60	10.201	1491	1495	1500	rVB	2264	3408	0.32%	0.042%
61	10.305	1507	1512	1519	rBV4	2144	3458	0.32%	0.042%
62	10.390	1524	1526	1527	rVB2	191	126	0.01%	0.002%
63	10.542	1547	1551	1555	rVV	205	406	0.04%	0.005%
64	10.622	1562	1564	1565	rVV2	132	119	0.01%	0.001%
65	10.658	1565	1570	1578	rVV4	2553	5787	0.54%	0.071%
66	10.799	1590	1593	1596	rVV2	329	421	0.04%	0.005%
67	10.829	1596	1598	1600	rVB	197	126	0.01%	0.002%
68	10.853	1600	1602	1606	rBV	104	159	0.01%	0.002%
69	10.963	1617	1620	1626	rVB2	2389	3353	0.31%	0.041%
70	11.085	1638	1640	1647	rVB5	634	735	0.07%	0.009%
71	11.189	1652	1657	1673	rVV	412559	539609	50.16%	6.589%
72	11.311	1674	1677	1685	rVB	2175	2960	0.28%	0.036%
73	11.378	1685	1688	1689	rBV2	247	227	0.02%	0.003%
74	11.396	1689	1691	1694	rVV2	124	150	0.01%	0.002%
75	11.451	1696	1700	1708	rVB	2108	3160	0.29%	0.039%
76	11.573	1718	1720	1722	rBV	173	142	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041043.D
 Acq On : 12 Apr 2024 20:10
 Operator : JC/MD
 Sample : VX0412WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK670

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041024WMA.M
 Title : VOC Analysis

77	11.603	1722	1725	1728	rVB	206	176	0.02%	0.002%
78	11.640	1728	1731	1733	rBV2	104	120	0.01%	0.001%
79	11.713	1739	1743	1746	rBV3	324	446	0.04%	0.005%
80	11.756	1746	1750	1754	rVV2	2411	3105	0.29%	0.038%
81	11.969	1781	1785	1788	rBV	4905	6465	0.60%	0.079%
82	12.024	1788	1794	1806	rVB	546167	720370	66.97%	8.796%
83	12.317	1837	1842	1854	rBV	615864	803687	74.71%	9.813%
84	12.762	1910	1915	1921	rVB2	3702	5013	0.47%	0.061%
85	12.865	1929	1932	1935	rBV2	143	202	0.02%	0.002%
86	12.902	1935	1938	1939	rVV	131	135	0.01%	0.002%
87	12.944	1942	1945	1949	rVB4	467	569	0.05%	0.007%
88	13.115	1968	1973	1981	rVB	5837	7529	0.70%	0.092%
89	13.487	2032	2034	2035	rBV2	141	116	0.01%	0.001%
90	13.591	2046	2051	2056	rBV	9138	11468	1.07%	0.140%
91	13.688	2065	2067	2070	rBV	273	214	0.02%	0.003%
92	13.731	2072	2074	2077	rBV	213	286	0.03%	0.003%
93	13.780	2077	2082	2087	rBV	7917	10685	0.99%	0.130%
94	13.963	2108	2112	2122	rVB	8174	10390	0.97%	0.127%
95	14.133	2135	2140	2146	rVB	4428	5736	0.53%	0.070%
96	14.237	2156	2157	2161	rBV2	231	165	0.02%	0.002%
97	14.292	2163	2166	2168	rBV2	207	252	0.02%	0.003%
98	14.639	2221	2223	2226	rVB2	360	259	0.02%	0.003%
99	14.670	2226	2228	2230	rBV	217	175	0.02%	0.002%
100	15.395	2344	2347	2353	rVB4	1871	2734	0.25%	0.033%

Sum of corrected areas: 8189914




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041043.D
Acq On : 12 Apr 2024 20:10
Operator : JC/MD
Sample : VX0412WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK670

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

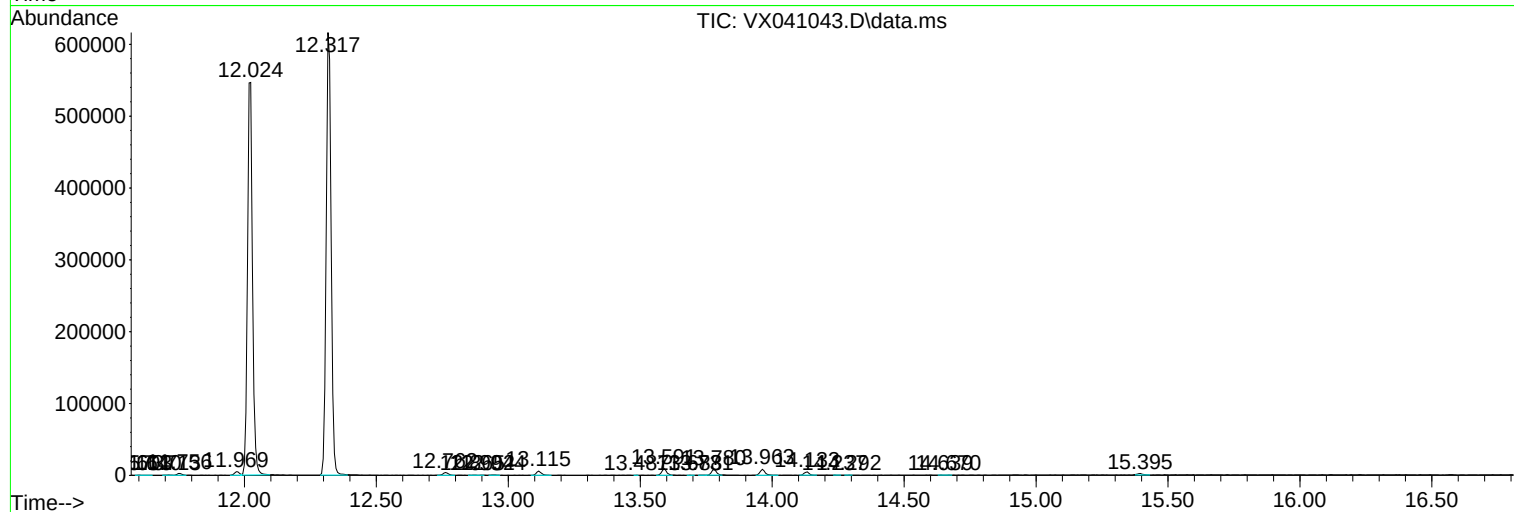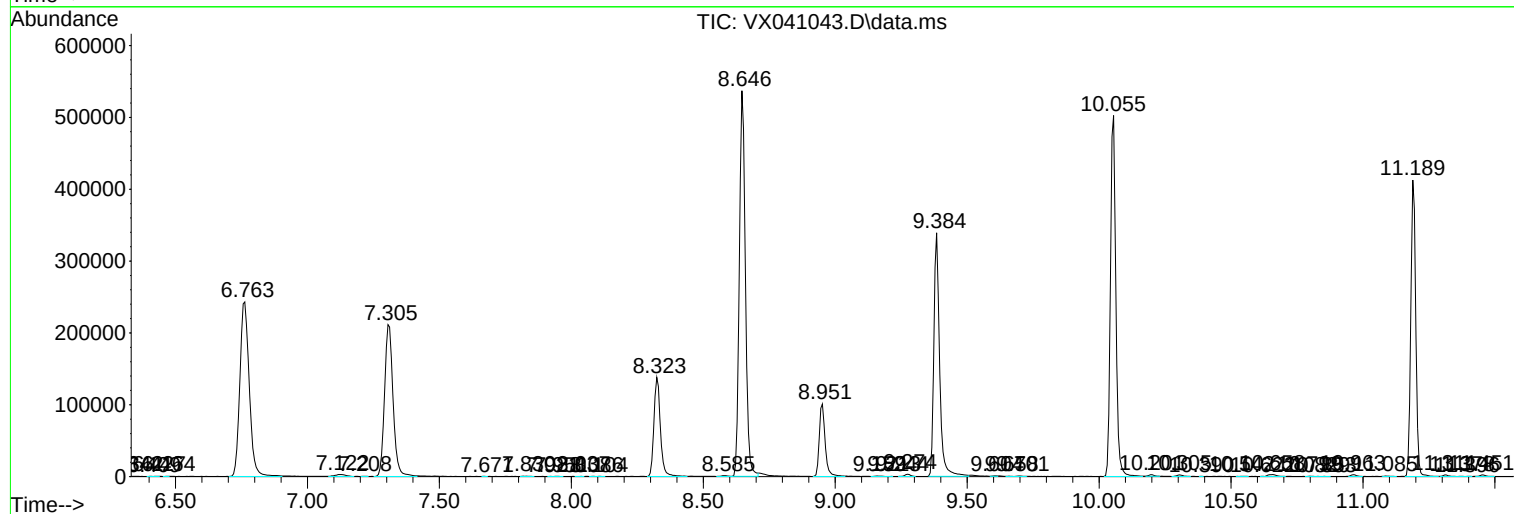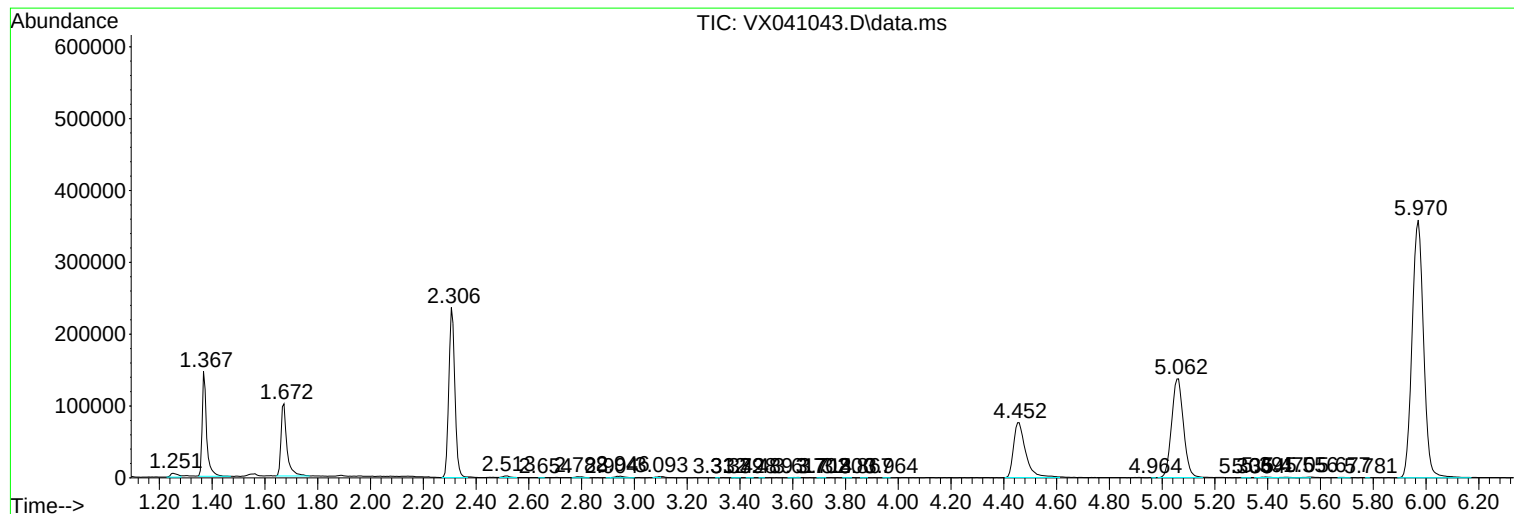

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041043.D
Acq On : 12 Apr 2024 20:10
Operator : JC/MD
Sample : VX0412WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK670

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041043.D
Acq On : 12 Apr 2024 20:10
Operator : JC/MD
Sample : VX0412WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK670

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------