

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041044.D
 Acq On : 12 Apr 2024 20:33
 Operator : JC/MD
 Sample : P2049-18 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0RB9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX041044.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	23	27	32	rBV2	4285	8183	0.50%	0.069%
2	1.368	42	46	59	rBV	138937	153947	9.48%	1.297%
3	1.666	91	95	111	rVB	93073	142241	8.76%	1.198%
4	2.264	191	193	194	rBV	242	159	0.01%	0.001%
5	2.307	194	200	210	rVV	229728	355302	21.88%	2.994%
6	2.447	222	223	224	rBV	250	132	0.01%	0.001%
7	2.624	250	252	254	rVB2	217	168	0.01%	0.001%
8	2.739	269	271	272	rBV	125	109	0.01%	0.001%
9	2.794	276	280	286	rVB5	746	1541	0.09%	0.013%
10	2.947	296	305	315	rBV2	10416	24005	1.48%	0.202%
11	3.050	320	322	324	rBV	161	136	0.01%	0.001%
12	3.093	326	329	335	rBV3	580	872	0.05%	0.007%
13	3.172	341	342	346	rBV2	151	183	0.01%	0.002%
14	3.434	383	385	387	rVB2	164	135	0.01%	0.001%
15	3.489	392	394	396	rVB	185	120	0.01%	0.001%
16	3.611	411	414	417	rVV2	189	249	0.02%	0.002%
17	3.642	417	419	422	rVB	130	109	0.01%	0.001%
18	3.678	422	425	427	rBV2	128	119	0.01%	0.001%
19	3.758	436	438	441	rVV	203	147	0.01%	0.001%
20	3.788	441	443	445	rVB2	160	125	0.01%	0.001%
21	3.825	447	449	451	rBV2	192	161	0.01%	0.001%
22	4.020	480	481	486	rBV2	139	188	0.01%	0.002%
23	4.196	508	510	514	rBV2	122	158	0.01%	0.001%
24	4.294	524	526	529	rVB2	122	116	0.01%	0.001%
25	4.453	544	552	568	rBV	77517	242856	14.96%	2.046%
26	5.056	639	651	669	rBV	137626	424978	26.17%	3.581%
27	5.355	699	700	702	rBV2	164	169	0.01%	0.001%
28	5.391	702	706	708	rVV3	577	813	0.05%	0.007%
29	5.550	728	732	733	rBV	604	701	0.04%	0.006%
30	5.672	747	752	753	rBV2	250	300	0.02%	0.003%
31	5.782	767	770	773	rBV2	134	158	0.01%	0.001%
32	5.971	789	801	827	rBV2	350122	1048949	64.60%	8.838%
33	6.355	863	864	866	rBV	177	169	0.01%	0.001%
34	6.470	881	883	885	rVB2	133	111	0.01%	0.001%
35	6.666	912	915	916	rBV2	143	161	0.01%	0.001%
36	6.763	921	931	955	rBV	258609	628117	38.68%	5.292%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041044.D
 Acq On : 12 Apr 2024 20:33
 Operator : JC/MD
 Sample : P2049-18 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0RB9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	7.123	983	990	997	rVB7	1459	4012	0.25%	0.034%
38	7.184	997	1000	1002	rBV2	134	137	0.01%	0.001%
39	7.306	1012	1020	1037	rBV	210075	465309	28.66%	3.921%
40	7.482	1047	1049	1050	rBV2	288	293	0.02%	0.002%
41	7.659	1076	1078	1081	rVB	210	155	0.01%	0.001%
42	7.818	1102	1104	1105	rBV	146	117	0.01%	0.001%
43	7.964	1124	1128	1129	rBV2	200	255	0.02%	0.002%
44	8.104	1148	1151	1152	rBV2	117	127	0.01%	0.001%
45	8.147	1156	1158	1161	rVB2	111	126	0.01%	0.001%
46	8.177	1161	1163	1164	rBV	130	114	0.01%	0.001%
47	8.196	1164	1166	1169	rVB2	120	123	0.01%	0.001%
48	8.324	1181	1187	1205	rBV	139810	232052	14.29%	1.955%
49	8.488	1211	1214	1215	rBV	187	178	0.01%	0.001%
50	8.586	1226	1230	1233	rVB2	639	672	0.04%	0.006%
51	8.647	1234	1240	1262	rVV	554656	861360	53.05%	7.257%
52	8.952	1284	1290	1303	rBV	99544	151200	9.31%	1.274%
53	9.275	1338	1343	1348	rVB3	2006	2826	0.17%	0.024%
54	9.324	1349	1351	1354	rVB	227	139	0.01%	0.001%
55	9.385	1356	1361	1377	rBV	337258	507312	31.24%	4.274%
56	9.695	1410	1412	1416	rVB2	289	259	0.02%	0.002%
57	9.903	1445	1446	1450	rBV	130	124	0.01%	0.001%
58	9.964	1454	1456	1459	rBV2	205	197	0.01%	0.002%
59	10.055	1465	1471	1491	rBV2	541468	923839	56.90%	7.784%
60	10.201	1492	1495	1500	rVB	1255	1580	0.10%	0.013%
61	10.305	1508	1512	1518	rBV2	1112	1697	0.10%	0.014%
62	10.409	1526	1529	1530	rBV	173	146	0.01%	0.001%
63	10.512	1544	1546	1547	rBV	149	140	0.01%	0.001%
64	10.659	1564	1570	1579	rVB4	1083	2672	0.16%	0.023%
65	10.836	1597	1599	1601	rVV	173	141	0.01%	0.001%
66	10.964	1617	1620	1626	rBB	1198	1326	0.08%	0.011%
67	11.092	1638	1641	1645	rBV3	567	788	0.05%	0.007%
68	11.189	1652	1657	1671	rBV	419659	528472	32.55%	4.453%
69	11.317	1674	1678	1682	rVV3	1233	1819	0.11%	0.015%
70	11.451	1696	1700	1707	rVB3	981	1322	0.08%	0.011%
71	11.537	1711	1714	1715	rVB	167	151	0.01%	0.001%
72	11.567	1715	1719	1721	rBV2	127	178	0.01%	0.001%
73	11.646	1730	1732	1734	rBV2	133	115	0.01%	0.001%
74	11.671	1734	1736	1739	rVB	141	123	0.01%	0.001%
75	11.707	1739	1742	1745	rVB3	223	272	0.02%	0.002%
76	11.756	1746	1750	1755	rVB	1209	1568	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041044.D
 Acq On : 12 Apr 2024 20:33
 Operator : JC/MD
 Sample : P2049-18 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0RB9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041024WMA.M
 Title : VOC Analysis

77	11.915	1774	1776	1778	rBV	151	119	0.01%	0.001%
78	11.969	1780	1785	1789	rBV	50895	62796	3.87%	0.529%
79	12.024	1789	1794	1812	rVB2	634964	1093982	67.38%	9.217%
80	12.323	1837	1843	1863	rVB2	864298	1584640	97.60%	13.352%
81	12.658	1895	1898	1899	rBV2	159	128	0.01%	0.001%
82	12.762	1910	1915	1920	rBV2	4132	5478	0.34%	0.046%
83	12.927	1940	1942	1945	rBV	484	516	0.03%	0.004%
84	12.975	1948	1950	1953	rVB	139	117	0.01%	0.001%
85	13.006	1953	1955	1958	rBV2	105	112	0.01%	0.001%
86	13.116	1969	1973	1977	rBV2	3673	4818	0.30%	0.041%
87	13.195	1983	1986	1989	rVB2	193	250	0.02%	0.002%
88	13.244	1992	1994	1998	rVB2	206	255	0.02%	0.002%
89	13.585	2045	2050	2068	rBV	1387815	1623683	100.00%	13.681%
90	13.780	2078	2082	2087	rVB2	4159	5320	0.33%	0.045%
91	13.963	2106	2112	2123	rBV	166725	216875	13.36%	1.827%
92	14.128	2135	2139	2148	rVB2	6365	9214	0.57%	0.078%
93	14.268	2160	2162	2165	rVB2	289	156	0.01%	0.001%
94	14.384	2177	2181	2188	rBV3	1514	2167	0.13%	0.018%
95	14.634	2220	2222	2223	rVV2	264	137	0.01%	0.001%
96	14.652	2223	2225	2227	rVB2	270	195	0.01%	0.002%
97	14.780	2239	2246	2257	rVB	39458	80730	4.97%	0.680%
98	15.249	2317	2323	2333	rBV	316731	433801	26.72%	3.655%
99	15.390	2342	2346	2352	rVB3	3073	5052	0.31%	0.043%
100	16.511	2525	2530	2537	rVB2	4847	8528	0.53%	0.072%




Sum of corrected areas: 11868592

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041044.D
Acq On : 12 Apr 2024 20:33
Operator : JC/MD
Sample : P2049-18 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MCORB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

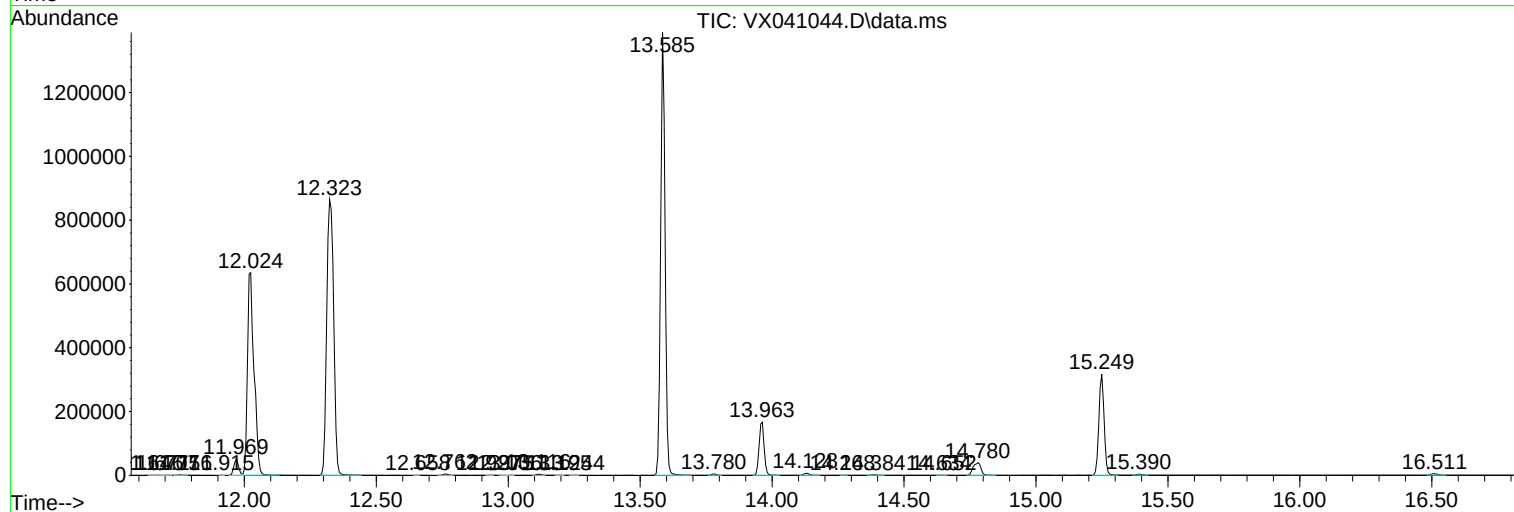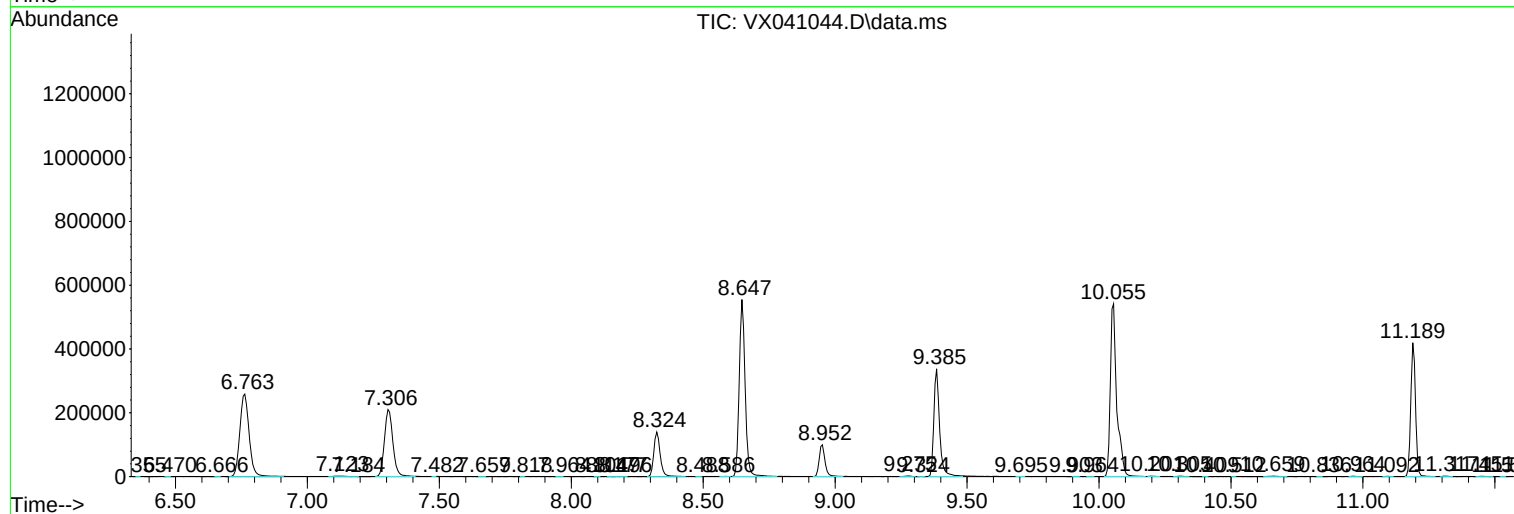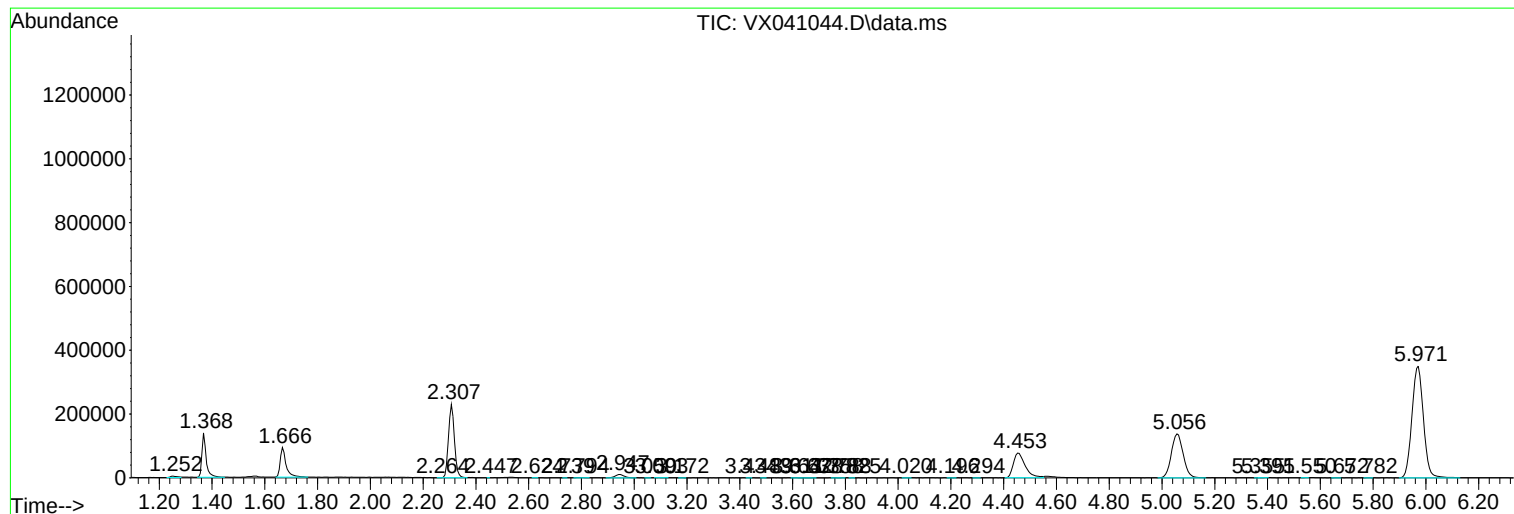

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041044.D
Acq On : 12 Apr 2024 20:33
Operator : JC/MD
Sample : P2049-18 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041044.D
Acq On : 12 Apr 2024 20:33
Operator : JC/MD
Sample : P2049-18 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------