

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041046.D
 Acq On : 12 Apr 2024 21:19
 Operator : JC/MD
 Sample : P2060-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1D13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX041046.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	24	27	32	rBV2	3067	6254	0.66%	0.083%
2	1.368	43	46	57	rVB	128243	142490	14.98%	1.883%
3	1.672	91	96	110	rBV	92197	134700	14.16%	1.780%
4	2.307	194	200	208	rBV	206850	322648	33.91%	4.264%
5	2.380	208	212	218	rVB	5567	9490	1.00%	0.125%
6	2.447	222	223	224	rBV	348	190	0.02%	0.003%
7	2.642	250	255	262	rBV	1666	3207	0.34%	0.042%
8	2.788	275	279	286	rVB3	916	1415	0.15%	0.019%
9	2.947	298	305	315	rBV3	1142	2788	0.29%	0.037%
10	3.087	326	328	329	rBV	213	129	0.01%	0.002%
11	3.105	329	331	333	rVB2	309	219	0.02%	0.003%
12	3.379	374	376	379	rVB	153	130	0.01%	0.002%
13	3.587	405	410	413	rBV2	120	202	0.02%	0.003%
14	3.654	420	421	424	rBV2	102	116	0.01%	0.002%
15	3.867	452	456	457	rBV2	103	128	0.01%	0.002%
16	3.977	470	474	475	rVB	151	153	0.02%	0.002%
17	4.160	500	504	508	rBV2	152	229	0.02%	0.003%
18	4.245	515	518	519	rBV2	167	155	0.02%	0.002%
19	4.282	522	524	527	rVB2	152	150	0.02%	0.002%
20	4.459	544	553	573	rBV	67970	211900	22.27%	2.800%
21	4.678	587	589	590	rBV2	236	131	0.01%	0.002%
22	4.885	621	623	627	rBV3	146	170	0.02%	0.002%
23	5.056	639	651	673	rBV	124159	386546	40.63%	5.108%
24	5.434	712	713	715	rBV	162	111	0.01%	0.001%
25	5.471	715	719	721	rBV	120	166	0.02%	0.002%
26	5.538	728	730	731	rBV2	286	208	0.02%	0.003%
27	5.684	750	754	755	rBV	208	147	0.02%	0.002%
28	5.970	789	801	817	rBV2	319565	951445	100.00%	12.573%
29	6.214	839	841	846	rVB2	230	333	0.03%	0.004%
30	6.294	853	854	857	rVB	279	178	0.02%	0.002%
31	6.647	910	912	913	rBV	170	131	0.01%	0.002%
32	6.702	918	921	922	rBV	150	135	0.01%	0.002%
33	6.763	922	931	953	rBV	221971	540098	56.77%	7.137%
34	7.123	983	990	999	rVB6	1497	3831	0.40%	0.051%
35	7.239	1007	1009	1012	rBV2	184	265	0.03%	0.004%
36	7.306	1012	1020	1038	rVV	188167	423985	44.56%	5.603%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041046.D
 Acq On : 12 Apr 2024 21:19
 Operator : JC/MD
 Sample : P2060-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1D13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	7.482	1046	1049	1055	rVB4	440	823	0.09%	0.011%
38	7.830	1104	1106	1109	rVB	257	200	0.02%	0.003%
39	7.866	1109	1112	1114	rBV	121	177	0.02%	0.002%
40	7.964	1126	1128	1131	rVB2	199	179	0.02%	0.002%
41	8.007	1131	1135	1137	rVB2	155	140	0.01%	0.002%
42	8.324	1181	1187	1200	rBV	127191	209052	21.97%	2.762%
43	8.501	1212	1216	1217	rBV	172	143	0.02%	0.002%
44	8.519	1217	1219	1220	rBV	188	176	0.02%	0.002%
45	8.580	1225	1229	1234	rVB2	1176	1636	0.17%	0.022%
46	8.647	1234	1240	1264	rBV	507527	789483	82.98%	10.432%
47	8.952	1285	1290	1304	rBV	88995	135473	14.24%	1.790%
48	9.202	1329	1331	1332	rVB	190	113	0.01%	0.001%
49	9.275	1337	1343	1349	rBV	23629	37747	3.97%	0.499%
50	9.385	1356	1361	1373	rBV	299718	453669	47.68%	5.995%
51	9.823	1431	1433	1434	rBV2	137	113	0.01%	0.001%
52	9.897	1441	1445	1449	rBV2	165	277	0.03%	0.004%
53	10.055	1465	1471	1488	rBV	479862	669697	70.39%	8.849%
54	10.195	1492	1494	1500	rVB	849	1228	0.13%	0.016%
55	10.305	1506	1512	1517	rBV3	1151	2017	0.21%	0.027%
56	10.372	1520	1523	1525	rBV	127	203	0.02%	0.003%
57	10.646	1564	1568	1576	rVV6	977	2026	0.21%	0.027%
58	10.781	1583	1590	1592	rBV2	884	1394	0.15%	0.018%
59	10.963	1617	1620	1624	rVB2	569	807	0.08%	0.011%
60	11.000	1624	1626	1627	rVB	193	118	0.01%	0.002%
61	11.024	1627	1630	1633	rBV2	178	252	0.03%	0.003%
62	11.085	1638	1640	1646	rVB3	593	929	0.10%	0.012%
63	11.189	1652	1657	1672	rVV	383037	499293	52.48%	6.598%
64	11.311	1672	1677	1684	rVB	40664	55620	5.85%	0.735%
65	11.457	1697	1701	1704	rVB3	643	853	0.09%	0.011%
66	11.616	1726	1727	1729	rBV	209	150	0.02%	0.002%
67	11.707	1738	1742	1746	rBV2	390	400	0.04%	0.005%
68	11.756	1746	1750	1758	rVB3	777	1188	0.12%	0.016%
69	11.969	1782	1785	1788	rBV	1472	1676	0.18%	0.022%
70	12.024	1788	1794	1803	rBV	538951	700962	73.67%	9.263%
71	12.225	1822	1827	1837	rBV2	9416	20835	2.19%	0.275%
72	12.317	1837	1842	1852	rVB	622366	779469	81.92%	10.300%
73	12.524	1874	1876	1877	rBV	214	131	0.01%	0.002%
74	12.597	1886	1888	1889	rBV2	314	255	0.03%	0.003%
75	12.677	1899	1901	1903	rBV2	181	164	0.02%	0.002%
76	12.762	1911	1915	1920	rVB2	8715	11568	1.22%	0.153%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041046.D
 Acq On : 12 Apr 2024 21:19
 Operator : JC/MD
 Sample : P2060-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1D13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	12.859	1926	1931	1938	rVB3	1473	2161	0.23%	0.029%
78	13.006	1952	1955	1961	rBV2	220	435	0.05%	0.006%
79	13.109	1969	1972	1979	rVB4	1179	1658	0.17%	0.022%
80	13.207	1986	1988	1991	rBV	145	131	0.01%	0.002%
81	13.286	1999	2001	2003	rVV	191	172	0.02%	0.002%
82	13.591	2047	2051	2062	rVB	9801	12679	1.33%	0.168%
83	13.701	2067	2069	2070	rVB	190	137	0.01%	0.002%
84	13.725	2070	2073	2075	rBV3	276	358	0.04%	0.005%
85	13.780	2079	2082	2091	rVB	1471	2246	0.24%	0.030%
86	13.932	2104	2107	2108	rBV2	227	261	0.03%	0.003%
87	13.963	2108	2112	2116	rVV3	2243	2814	0.30%	0.037%
88	14.091	2130	2133	2135	rBV2	204	260	0.03%	0.003%
89	14.134	2135	2140	2145	rVB2	5694	7662	0.81%	0.101%
90	14.243	2156	2158	2161	rVB2	270	309	0.03%	0.004%
91	14.353	2174	2176	2181	rBV3	246	292	0.03%	0.004%
92	14.518	2202	2203	2206	rBV2	144	154	0.02%	0.002%
93	14.579	2211	2213	2215	rBV2	219	183	0.02%	0.002%
94	14.640	2222	2223	2225	rBV	180	115	0.01%	0.002%
95	15.042	2288	2289	2291	rBV	358	214	0.02%	0.003%
96	15.127	2301	2303	2305	rBV	327	257	0.03%	0.003%
97	15.249	2319	2323	2329	rVB	4287	5786	0.61%	0.076%
98	15.390	2343	2346	2353	rVB3	2341	3701	0.39%	0.049%
99	15.463	2356	2358	2360	rBV	343	237	0.02%	0.003%
100	15.694	2394	2396	2397	rBV	399	230	0.02%	0.003%


Sum of corrected areas: 7567661

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041046.D
Acq On : 12 Apr 2024 21:19
Operator : JC/MD
Sample : P2060-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1D13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

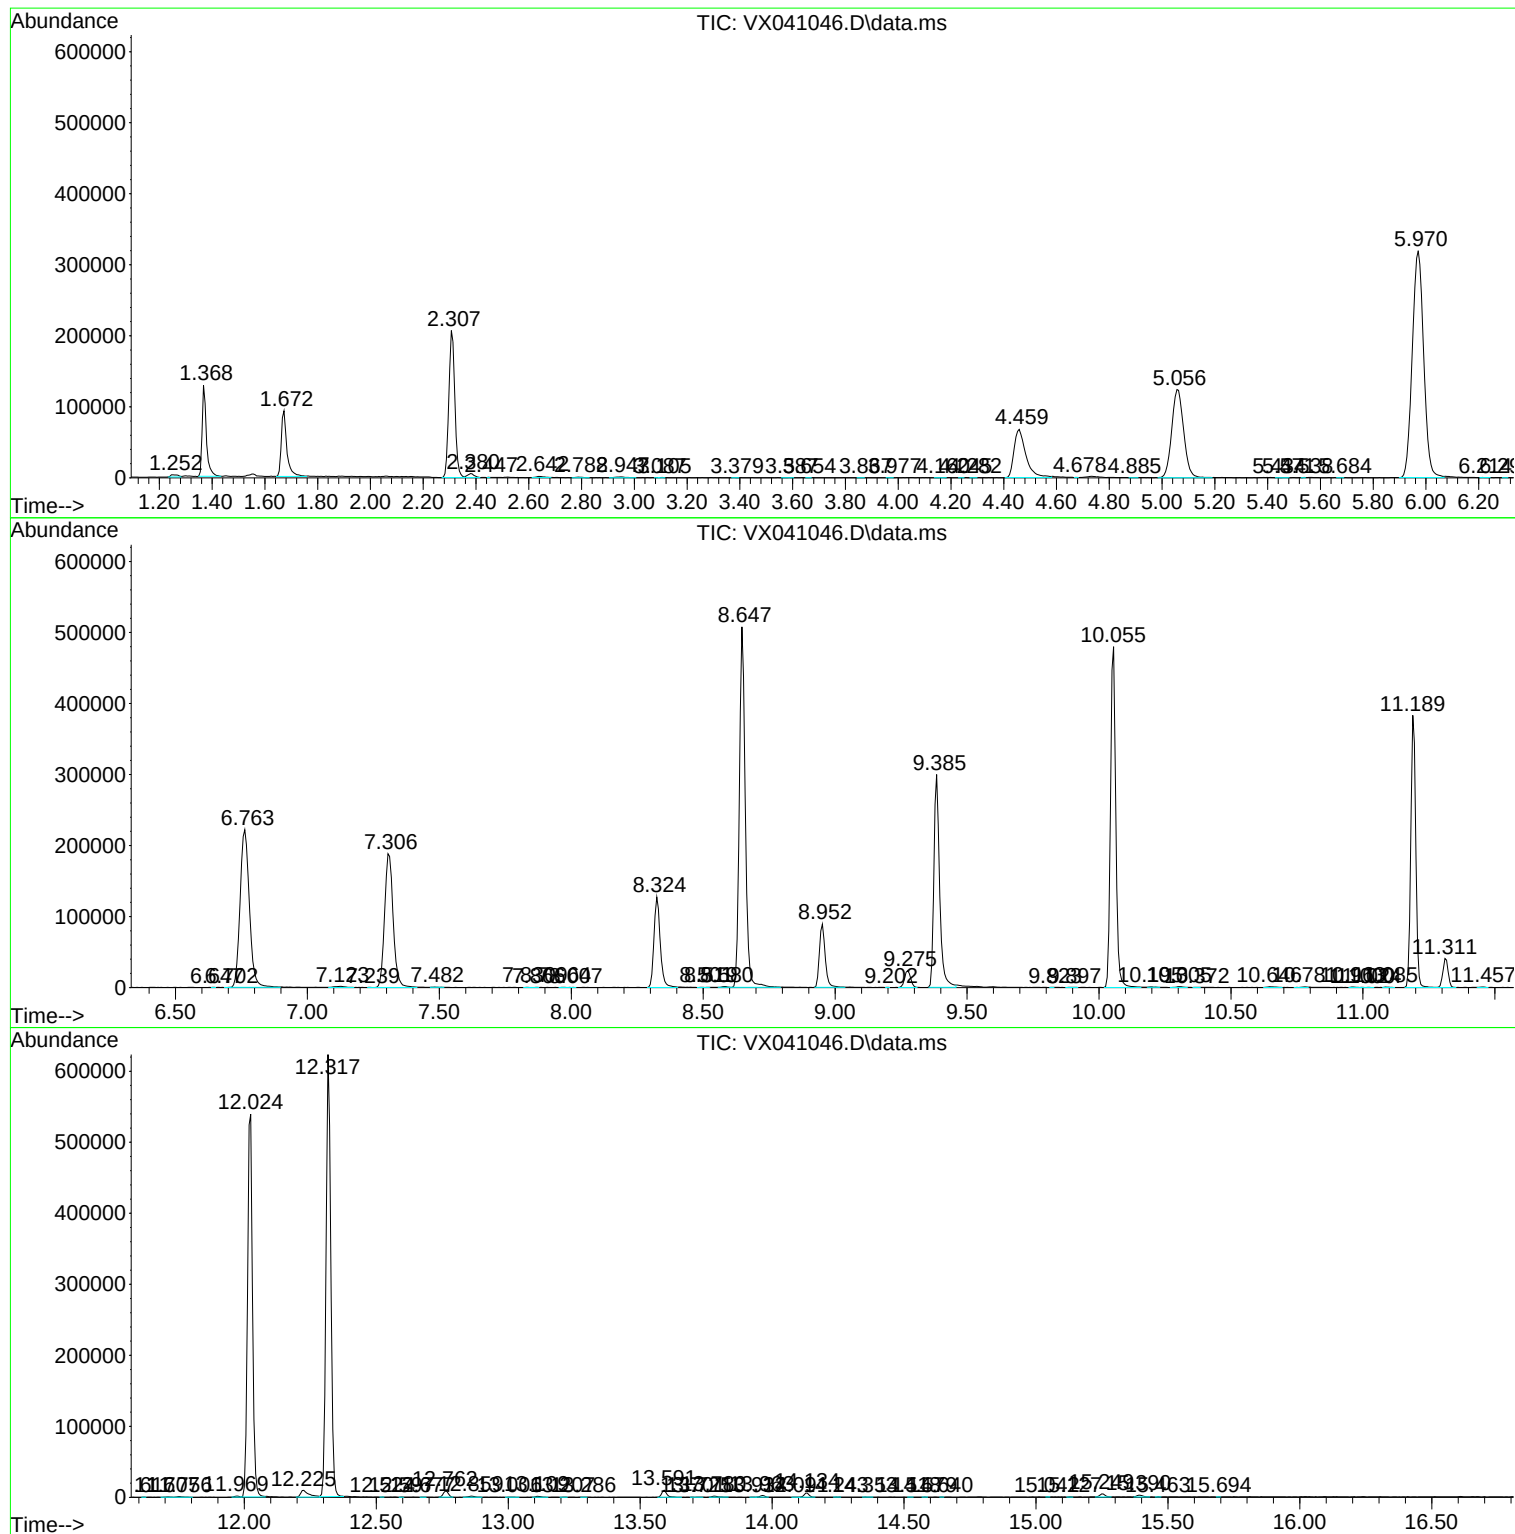

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041046.D
Acq On : 12 Apr 2024 21:19
Operator : JC/MD
Sample : P2060-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1D13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041046.D
Acq On : 12 Apr 2024 21:19
Operator : JC/MD
Sample : P2060-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1D13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
