

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041047.D
 Acq On : 12 Apr 2024 21:42
 Operator : JC/MD
 Sample : P2060-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1D01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX041047.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	23	27	32	rBV2	4550	8324	0.86%	0.109%
2	1.368	43	46	58	rVB	131943	143140	14.83%	1.881%
3	1.672	91	96	113	rVB	90316	134728	13.96%	1.771%
4	2.050	156	158	169	rVB2	2615	4705	0.49%	0.062%
5	2.307	194	200	208	rBV	208154	323977	33.56%	4.258%
6	2.380	209	212	220	rVB	5343	8677	0.90%	0.114%
7	2.642	249	255	262	rBV3	1521	3477	0.36%	0.046%
8	2.794	276	280	284	rVB4	740	1057	0.11%	0.014%
9	2.873	292	293	297	rBV2	148	150	0.02%	0.002%
10	2.941	298	304	305	rBV3	1071	1371	0.14%	0.018%
11	3.069	323	325	328	rBV	147	156	0.02%	0.002%
12	3.105	328	331	333	rVV	317	311	0.03%	0.004%
13	3.123	333	334	337	rVB	315	200	0.02%	0.003%
14	3.343	368	370	373	rBV	129	181	0.02%	0.002%
15	3.422	381	383	388	rVB2	231	181	0.02%	0.002%
16	3.495	394	395	398	rVB	165	123	0.01%	0.002%
17	3.703	427	429	432	rBV2	152	172	0.02%	0.002%
18	3.904	461	462	465	rBV2	92	117	0.01%	0.002%
19	4.459	544	553	570	rBV	70623	214794	22.25%	2.823%
20	4.727	593	597	605	rBV3	1503	3449	0.36%	0.045%
21	4.879	620	622	623	rVB	205	109	0.01%	0.001%
22	4.916	626	628	633	rVB2	111	159	0.02%	0.002%
23	5.056	638	651	670	rBV	125784	392948	40.70%	5.164%
24	5.276	685	687	690	rBV	100	123	0.01%	0.002%
25	5.391	700	706	715	rBV4	458	1290	0.13%	0.017%
26	5.483	720	721	723	rVB	168	122	0.01%	0.002%
27	5.556	727	733	737	rBV2	549	1164	0.12%	0.015%
28	5.684	752	754	755	rBV	187	141	0.01%	0.002%
29	5.782	767	770	771	rBV	129	135	0.01%	0.002%
30	5.867	780	784	785	rBV	132	128	0.01%	0.002%
31	5.971	789	801	825	rBV2	322671	965365	100.00%	12.687%
32	6.288	851	853	854	rVB	259	143	0.01%	0.002%
33	6.568	897	899	904	rVB2	316	316	0.03%	0.004%
34	6.605	904	905	908	rVB	174	121	0.01%	0.002%
35	6.629	908	909	911	rBV	173	132	0.01%	0.002%
36	6.659	913	914	917	rBV2	166	162	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041047.D
 Acq On : 12 Apr 2024 21:42
 Operator : JC/MD
 Sample : P2060-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1D01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	6.763	922	931	946	rBV	225837	548978	56.87%	7.215%
38	7.037	972	976	977	rBV	142	166	0.02%	0.002%
39	7.123	983	990	998	rVB5	1416	3659	0.38%	0.048%
40	7.214	1003	1005	1008	rVB2	175	193	0.02%	0.003%
41	7.306	1012	1020	1037	rBV	191599	428362	44.37%	5.629%
42	7.909	1117	1119	1121	rVV2	133	110	0.01%	0.001%
43	7.958	1123	1127	1129	rBV	302	310	0.03%	0.004%
44	8.031	1135	1139	1140	rBV2	176	258	0.03%	0.003%
45	8.080	1146	1147	1150	rBV2	131	119	0.01%	0.002%
46	8.324	1181	1187	1201	rBV	123983	208852	21.63%	2.745%
47	8.507	1216	1217	1219	rBV	262	235	0.02%	0.003%
48	8.574	1223	1228	1234	rBV	1165	2008	0.21%	0.026%
49	8.647	1234	1240	1260	rBV	499273	790435	81.88%	10.388%
50	8.952	1284	1290	1305	rBV	90956	138010	14.30%	1.814%
51	9.275	1336	1343	1350	rBB	17684	27708	2.87%	0.364%
52	9.385	1356	1361	1381	rBV2	299182	465186	48.19%	6.113%
53	9.763	1419	1423	1425	rBV3	224	173	0.02%	0.002%
54	9.793	1425	1428	1433	rVV2	144	212	0.02%	0.003%
55	9.994	1459	1461	1463	rVB	180	113	0.01%	0.001%
56	10.055	1465	1471	1492	rBV	483701	679678	70.41%	8.932%
57	10.201	1492	1495	1500	rVB2	726	954	0.10%	0.013%
58	10.305	1509	1512	1521	rVB	1494	1862	0.19%	0.024%
59	10.439	1532	1534	1536	rBV	111	116	0.01%	0.002%
60	10.646	1564	1568	1574	rBV4	1063	2080	0.22%	0.027%
61	10.781	1586	1590	1597	rBV4	582	1143	0.12%	0.015%
62	10.848	1599	1601	1602	rBV	161	131	0.01%	0.002%
63	10.909	1607	1611	1613	rBV	146	213	0.02%	0.003%
64	10.964	1617	1620	1625	rVB	490	543	0.06%	0.007%
65	11.098	1637	1642	1644	rBV3	456	684	0.07%	0.009%
66	11.189	1652	1657	1667	rBV	392495	500319	51.83%	6.575%
67	11.311	1672	1677	1686	rVB	28530	40030	4.15%	0.526%
68	11.433	1693	1697	1698	rBV2	244	299	0.03%	0.004%
69	11.457	1698	1701	1705	rVB2	584	730	0.08%	0.010%
70	11.530	1711	1713	1715	rBV	167	121	0.01%	0.002%
71	11.707	1738	1742	1744	rBV2	472	448	0.05%	0.006%
72	11.756	1747	1750	1752	rBV	810	787	0.08%	0.010%
73	11.854	1763	1766	1768	rBV2	182	212	0.02%	0.003%
74	11.933	1777	1779	1781	rVB	168	127	0.01%	0.002%
75	11.969	1781	1785	1788	rBV2	1145	1539	0.16%	0.020%
76	12.018	1788	1793	1804	rBV	548543	708041	73.34%	9.305%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041047.D
 Acq On : 12 Apr 2024 21:42
 Operator : JC/MD
 Sample : P2060-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1D01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	12.225	1822	1827	1837	rBV	10096	22929	2.38%	0.301%
78	12.317	1837	1842	1856	rVB	612046	779309	80.73%	10.242%
79	12.725	1907	1909	1911	rBV	297	297	0.03%	0.004%
80	12.762	1911	1915	1920	rVV	6680	9204	0.95%	0.121%
81	12.817	1922	1924	1926	rVV	315	244	0.03%	0.003%
82	12.841	1926	1928	1929	rVV2	362	330	0.03%	0.004%
83	12.860	1929	1931	1935	rVV3	1147	1408	0.15%	0.019%
84	12.927	1938	1942	1945	rVB2	279	470	0.05%	0.006%
85	12.957	1945	1947	1949	rBV	188	169	0.02%	0.002%
86	13.000	1952	1954	1955	rBV	180	117	0.01%	0.002%
87	13.116	1968	1973	1977	rBV3	1208	1672	0.17%	0.022%
88	13.591	2046	2051	2056	rBV2	6758	8065	0.84%	0.106%
89	13.628	2056	2057	2059	rVB	247	109	0.01%	0.001%
90	13.658	2059	2062	2065	rBV2	191	315	0.03%	0.004%
91	13.737	2073	2075	2076	rBV	181	121	0.01%	0.002%
92	13.780	2079	2082	2086	rVV2	1063	1297	0.13%	0.017%
93	13.878	2096	2098	2099	rBV	256	162	0.02%	0.002%
94	13.963	2109	2112	2116	rVB2	1478	1807	0.19%	0.024%
95	14.091	2130	2133	2134	rBV	169	138	0.01%	0.002%
96	14.134	2134	2140	2146	rVV	5221	7365	0.76%	0.097%
97	14.469	2191	2195	2196	rBV	259	369	0.04%	0.005%
98	14.963	2275	2276	2278	rVB2	360	210	0.02%	0.003%
99	15.255	2319	2324	2327	rBV2	1853	2416	0.25%	0.032%
100	15.390	2342	2346	2350	rBV3	2562	3757	0.39%	0.049%




Sum of corrected areas: 7609272

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041047.D
Acq On : 12 Apr 2024 21:42
Operator : JC/MD
Sample : P2060-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1D01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

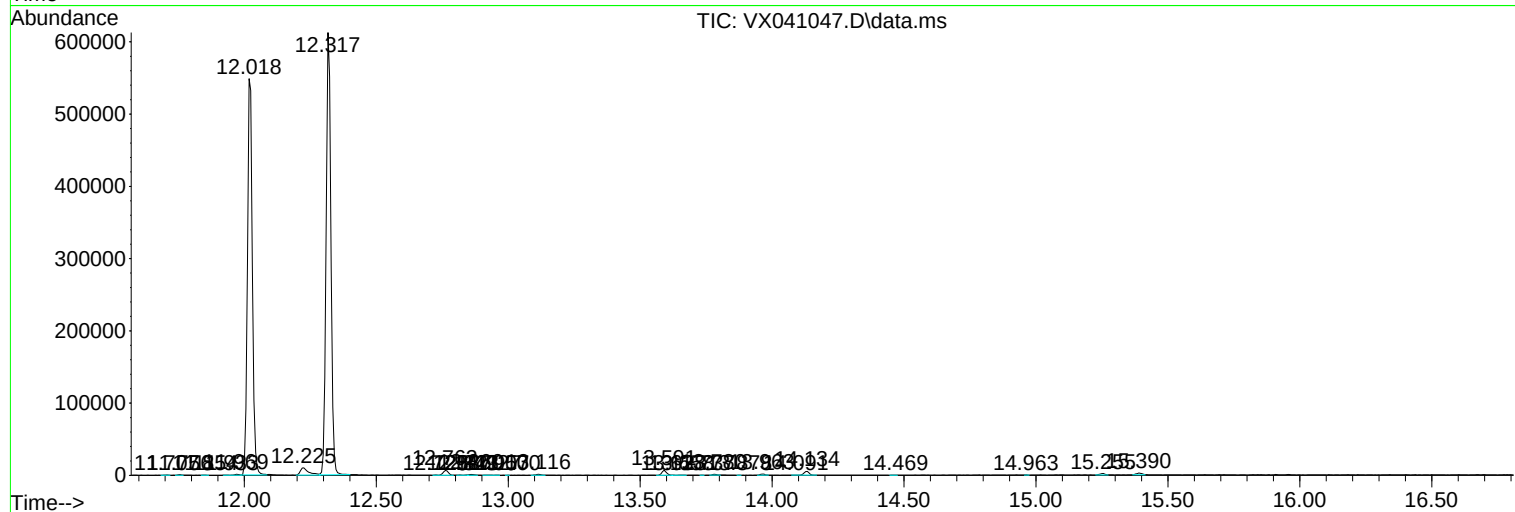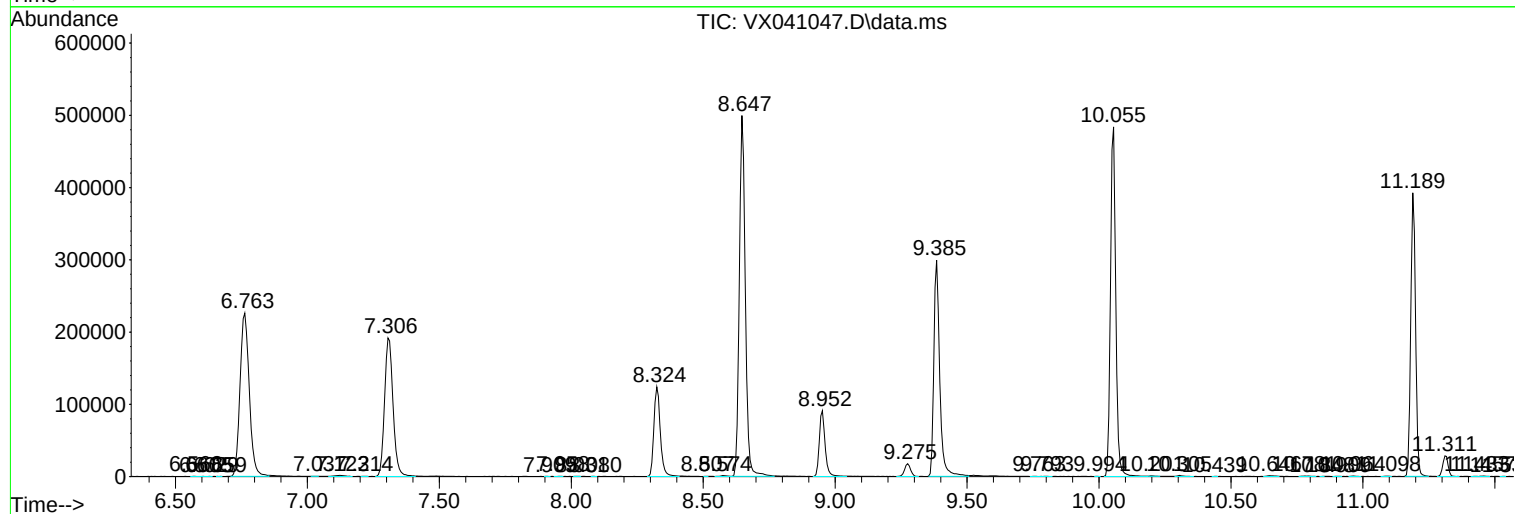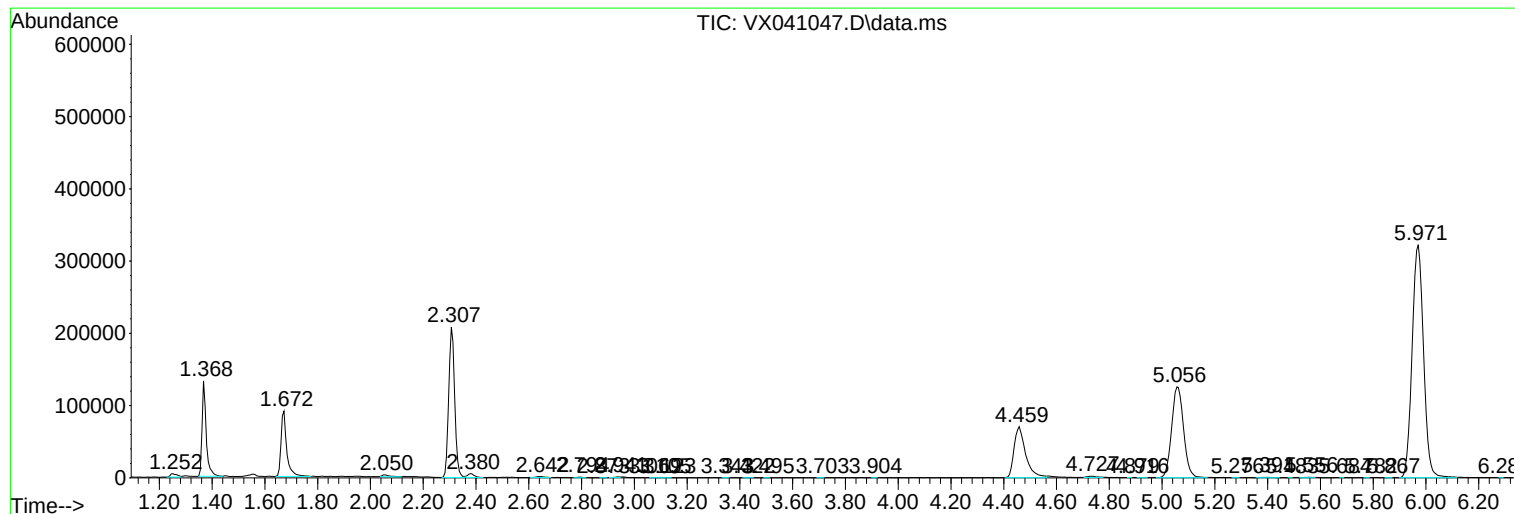

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041047.D
Acq On : 12 Apr 2024 21:42
Operator : JC/MD
Sample : P2060-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1D01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041047.D
Acq On : 12 Apr 2024 21:42
Operator : JC/MD
Sample : P2060-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1D01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------